

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041024\
 Data File : PL088974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2024 19:48
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA1251

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 05:00:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 04:57:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.633	2.851	13221024	7245012	4.934	4.882
27)	SA Decachlor...	9.298	8.077	26686653	17839631	10.559	10.878
Target Compounds							
2)	A alpha-BHC	4.098	3.364	17999202	9337494	4.606	4.493
3)	MA gamma-BHC...	4.436	3.701	17670957	9164008	4.729	4.590
4)	MA Heptachlor	5.036	4.049	19476342	9689541	4.971	4.800
9)	A Endosulfan I	6.205	5.220	16473499	8232327	5.099	4.857
13)	MA Dieldrin	6.484	5.490	32622638	17518142	9.698	9.228
14)	MA Endrin	6.716	5.769	27637772	15887048	9.876	9.442
16)	A 4,4'-DDD	6.851	5.918	24687205	12737127	9.760	9.232
17)	MA 4,4'-DDT	7.169	6.173	26853711	15123796	9.776	9.329
20)	A Methoxychlor	7.650	6.757	79570808	47498512	52.146	52.407

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041024\
Data File : PL088974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 19:48
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 05:00:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 04:57:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

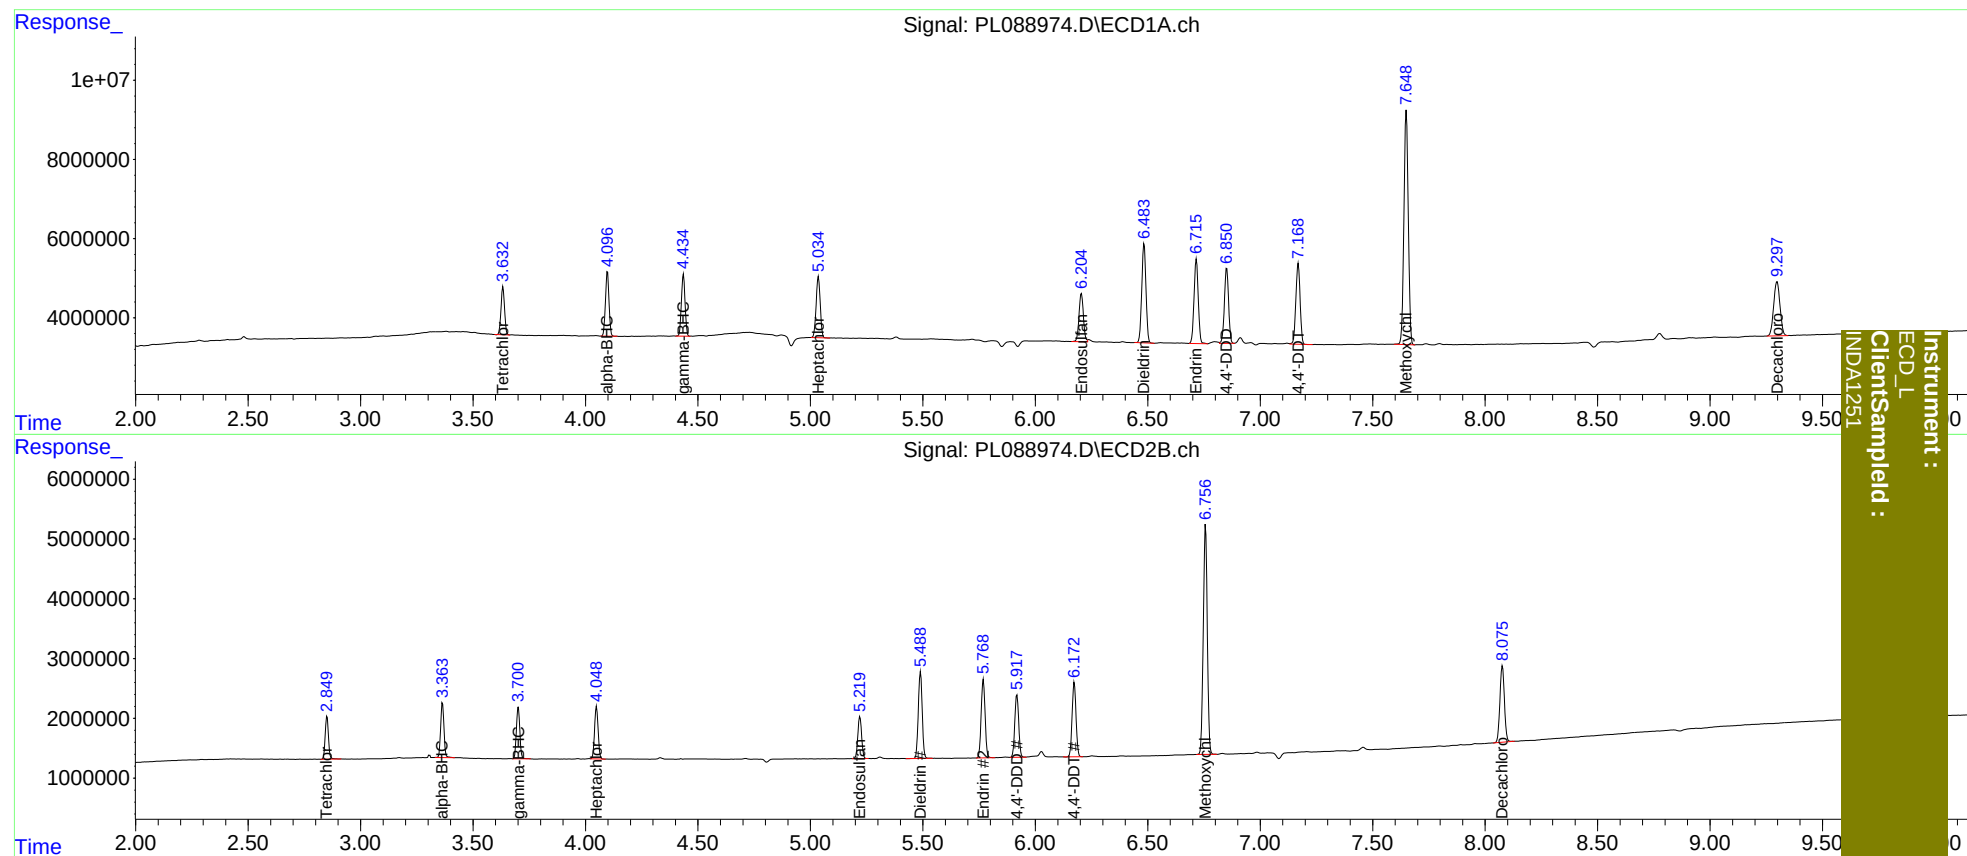


Instrument :
ECD_L
ClientSampled :
INDA1251

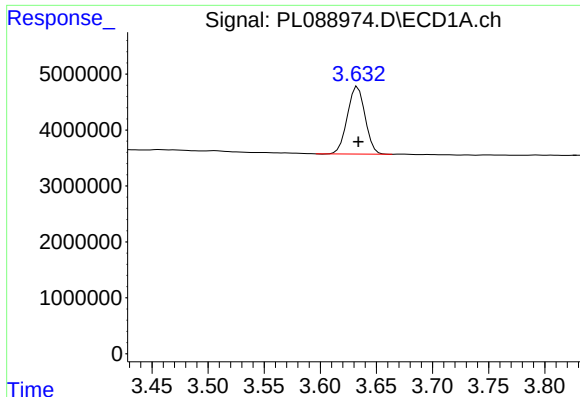

#1 Tetrachloro-m-xylene


R.T.: 3.633 min
Delta R.T.: 0.000 min
Response: 13221024
Conc: 4.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA1251

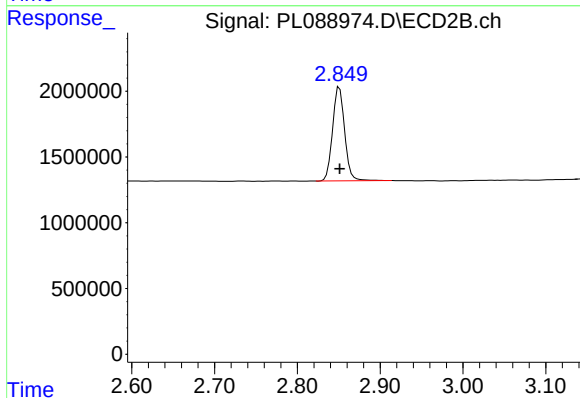


#1 Tetrachloro-m-xylene

R.T.: 2.851 min
Delta R.T.: 0.000 min
Response: 7245012
Conc: 4.88 ng/ml

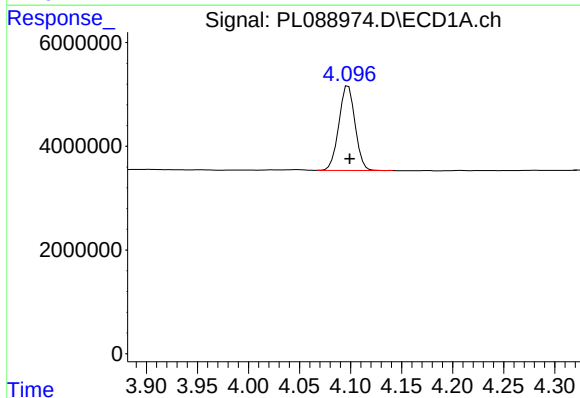


#2 alpha-BHC

R.T.: 4.098 min
Delta R.T.: -0.001 min
Response: 17999202
Conc: 4.61 ng/ml

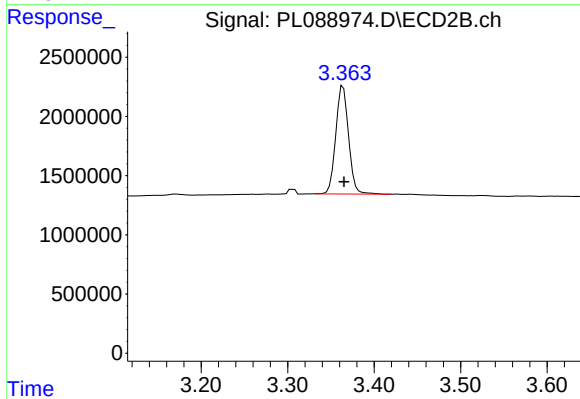

#2 alpha-BHC


R.T.: 3.364 min
Delta R.T.: 0.000 min
Response: 9337494
Conc: 4.49 ng/ml

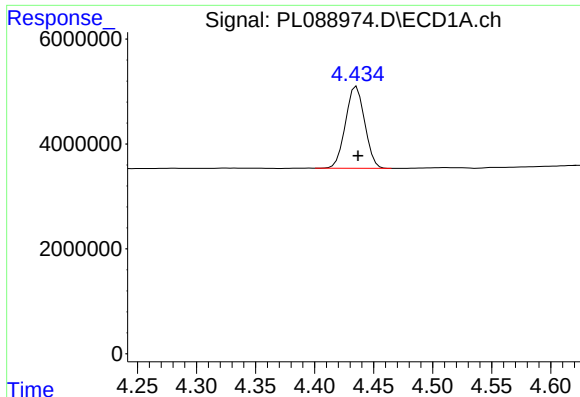

#3 gamma-BHC (Lindane)


R.T.: 4.436 min
Delta R.T.: -0.001 min
Response: 17670957
Conc: 4.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA1251

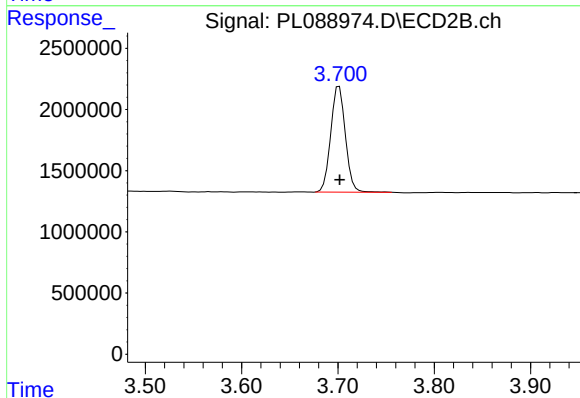


#3 gamma-BHC (Lindane)

R.T.: 3.701 min
Delta R.T.: 0.000 min
Response: 9164008
Conc: 4.59 ng/ml

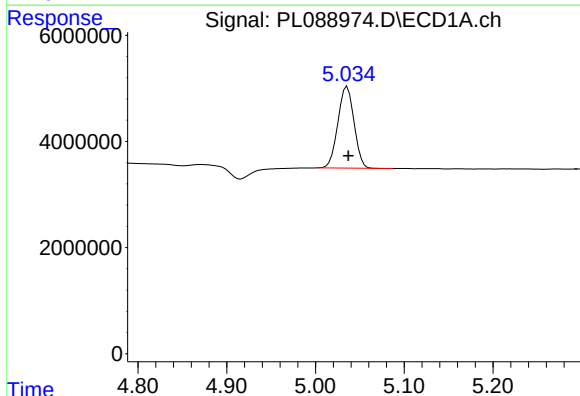


#4 Heptachlor

R.T.: 5.036 min
Delta R.T.: -0.001 min
Response: 19476342
Conc: 4.97 ng/ml

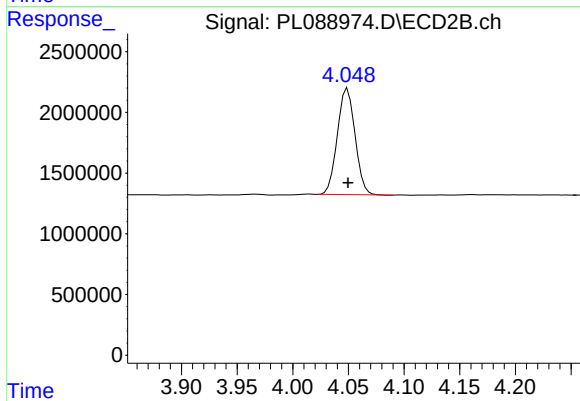

#4 Heptachlor


R.T.: 4.049 min
Delta R.T.: 0.000 min
Response: 9689541
Conc: 4.80 ng/ml

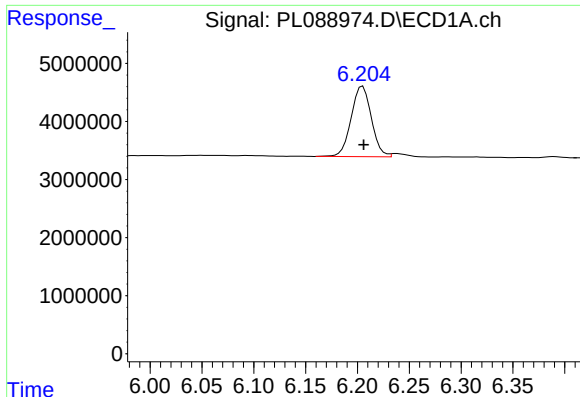

#9 Endosulfan I


R.T.: 6.205 min
Delta R.T.: 0.000 min
Response: 16473499
Conc: 5.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA1251

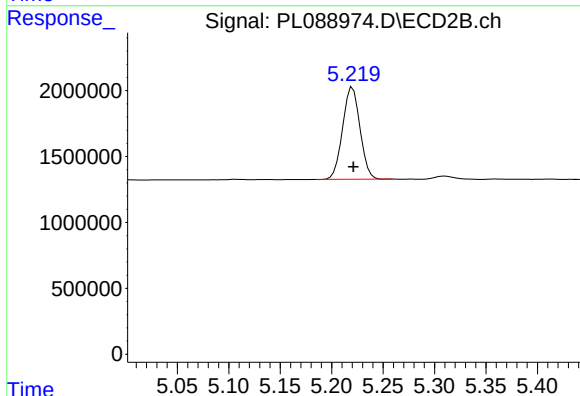


#9 Endosulfan I

R.T.: 5.220 min
Delta R.T.: 0.000 min
Response: 8232327
Conc: 4.86 ng/ml

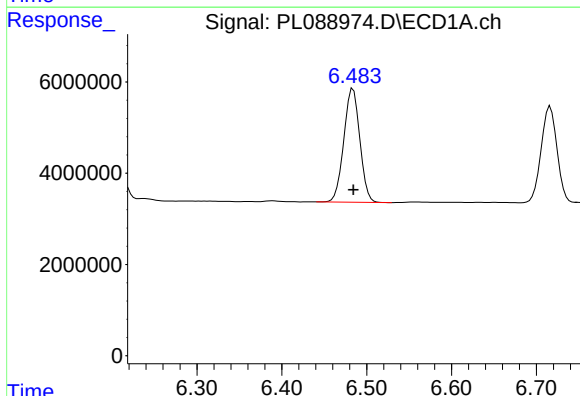


#13 Dieldrin

R.T.: 6.484 min
Delta R.T.: 0.000 min
Response: 32622638
Conc: 9.70 ng/ml

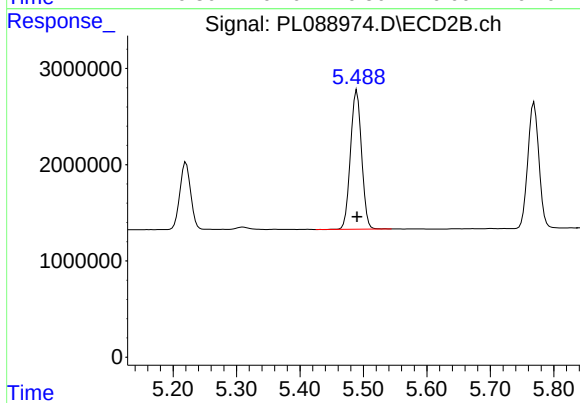

#13 Dieldrin


R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 17518142
Conc: 9.23 ng/ml

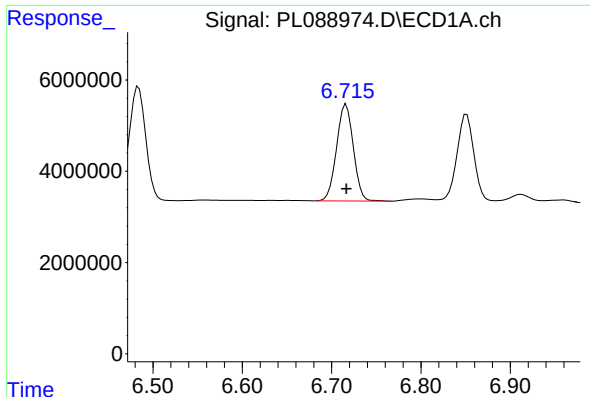

#14 Endrin


R.T.: 6.716 min
Delta R.T.: 0.000 min
Response: 27637772
Conc: 9.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA1251

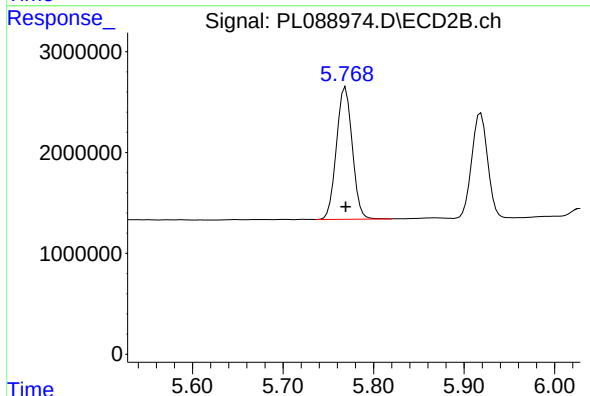


#14 Endrin

R.T.: 5.769 min
Delta R.T.: 0.000 min
Response: 15887048
Conc: 9.44 ng/ml

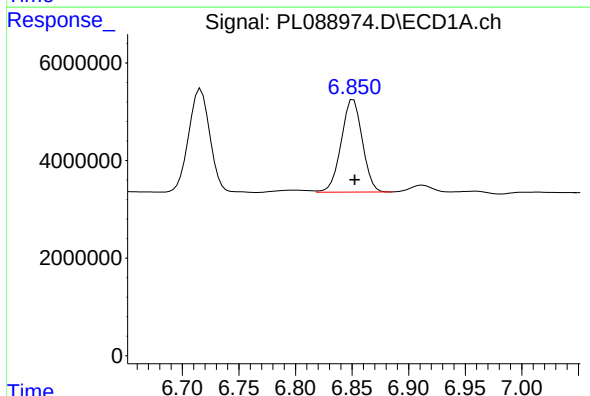


#16 4,4'-DDD

R.T.: 6.851 min
Delta R.T.: -0.001 min
Response: 24687205
Conc: 9.76 ng/ml

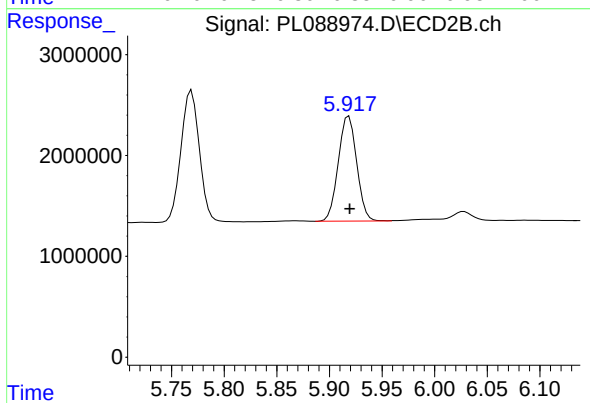

#16 4,4'-DDD


R.T.: 5.918 min
Delta R.T.: 0.000 min
Response: 12737127
Conc: 9.23 ng/ml

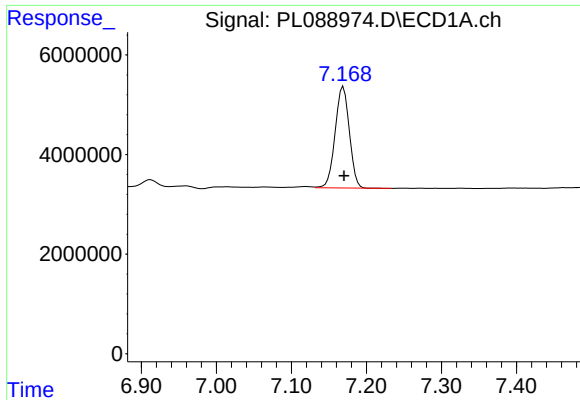

#17 4,4'-DDT


R.T.: 7.169 min
Delta R.T.: -0.001 min
Response: 26853711
Conc: 9.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA1251

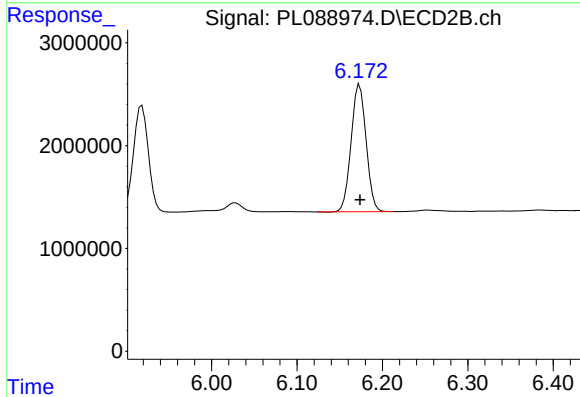


#17 4,4'-DDT

R.T.: 6.173 min
Delta R.T.: 0.000 min
Response: 15123796
Conc: 9.33 ng/ml

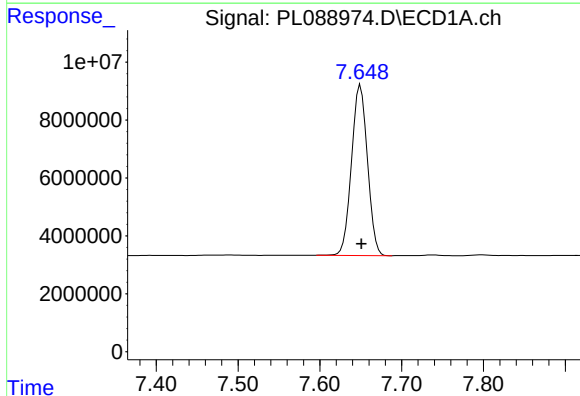


#20 Methoxychlor

R.T.: 7.650 min
Delta R.T.: -0.001 min
Response: 79570808
Conc: 52.15 ng/ml

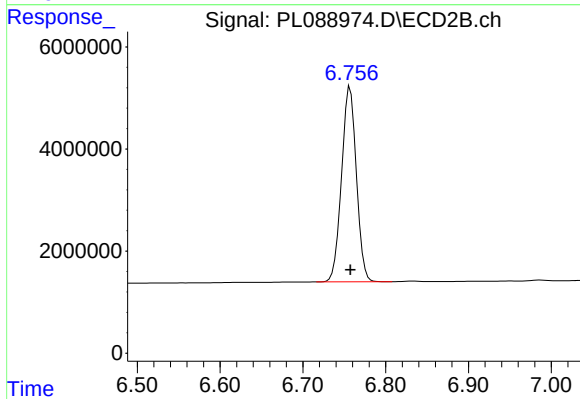

#20 Methoxychlor


R.T.: 6.757 min
Delta R.T.: 0.000 min
Response: 47498512
Conc: 52.41 ng/ml

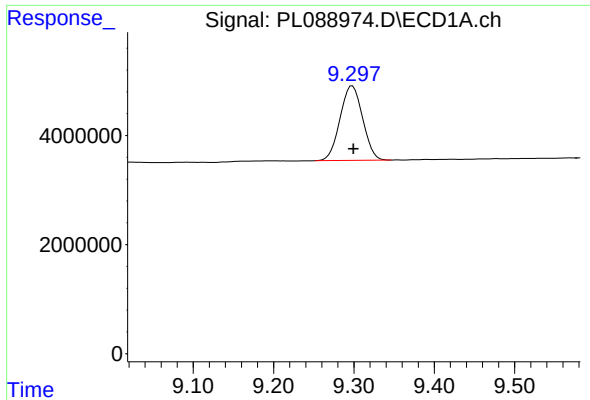

#27 Decachlorobiphenyl

R.T.: 9.298 min
Delta R.T.: -0.001 min
Response: 26686653
Conc: 10.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA1251

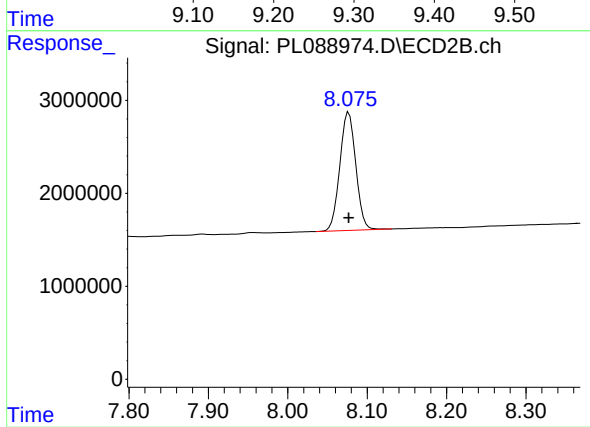

#27 Decachlorobiphenyl

R.T.: 8.077 min
Delta R.T.: 0.000 min
Response: 17839631
Conc: 10.88 ng/ml