

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041024\
 Data File : PL088980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2024 21:11
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA4257

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 05:00:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 04:57:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.852	108.2E6	58966131	40.391	39.738
27)	SA Decachlor...	9.300	8.077	194.4E6	125.8E6	76.933	76.703
Target Compounds							
2)	A alpha-BHC	4.099	3.366	167.4E6	90528816	42.845	43.564
3)	MA gamma-BHC...	4.437	3.702	157.6E6	85274397	42.181	42.708
4)	MA Heptachlor	5.037	4.050	161.2E6	84710382	41.147	41.960
9)	A Endosulfan I	6.206	5.222	129.4E6	69589702	40.038	41.059
13)	MA Dieldrin	6.485	5.490	281.4E6	160.2E6	83.648	84.373
14)	MA Endrin	6.717	5.770	233.1E6	141.0E6	83.296	83.789
16)	A 4,4'-DDD	6.853	5.919	211.7E6	116.0E6	83.709	84.059
17)	MA 4,4'-DDT	7.171	6.174	227.8E6	136.8E6	82.943	84.389
20)	A Methoxychlor	7.652	6.757	601.0E6	350.9E6	393.883	387.156


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041024\
Data File : PL088980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 21:11
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 05:00:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 04:57:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

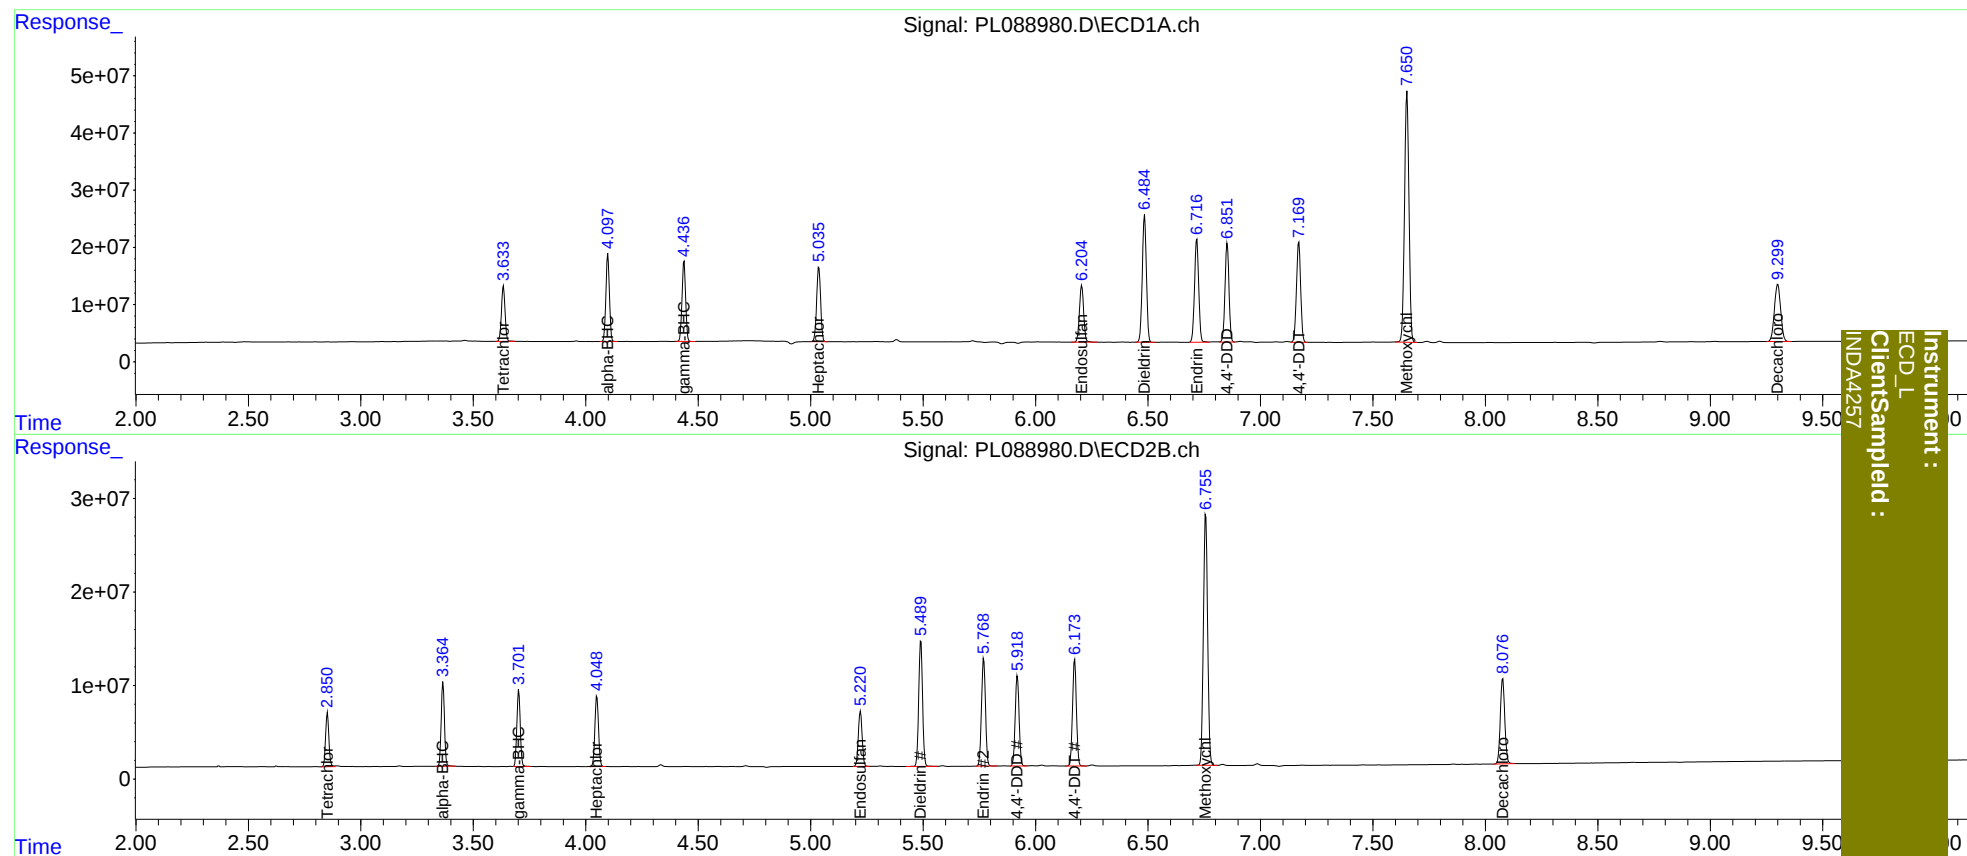


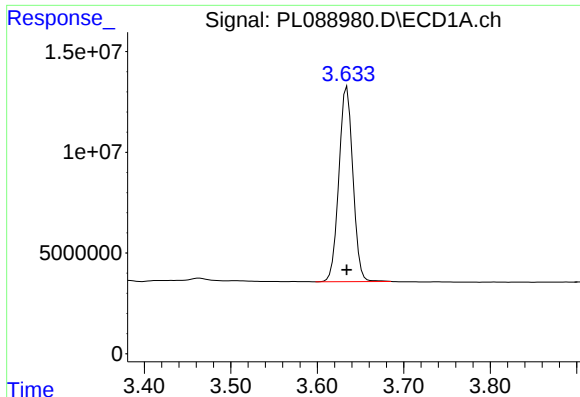

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 108232391
Conc: 40.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4257

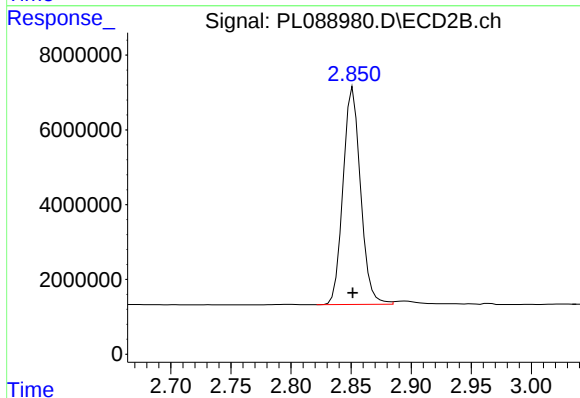


#1 Tetrachloro-m-xylene

R.T.: 2.852 min
Delta R.T.: 0.000 min
Response: 58966131
Conc: 39.74 ng/ml

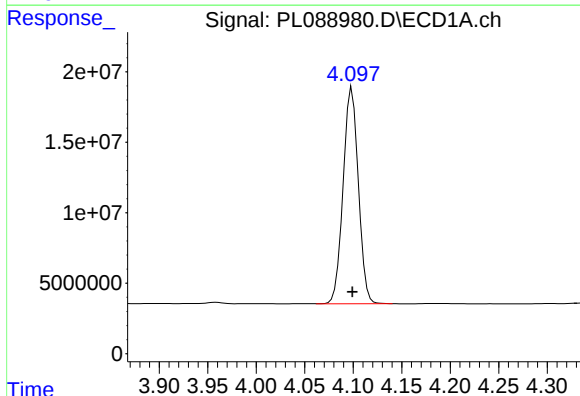


#2 alpha-BHC

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 167431617
Conc: 42.84 ng/ml

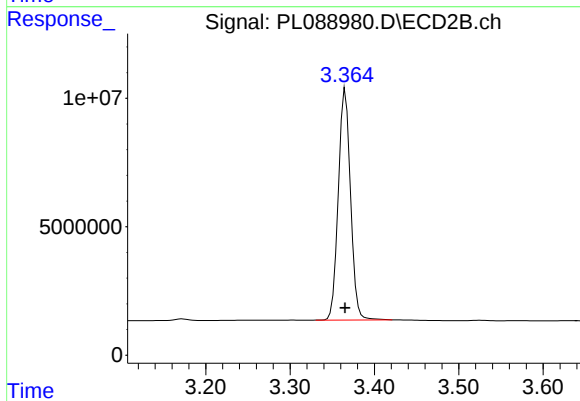

#2 alpha-BHC


R.T.: 3.366 min
Delta R.T.: 0.000 min
Response: 90528816
Conc: 43.56 ng/ml

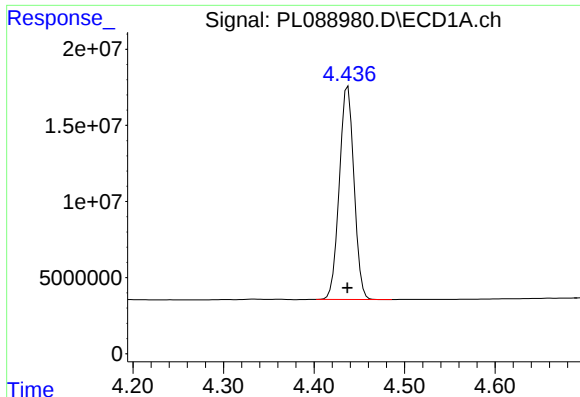

#3 gamma-BHC (Lindane)


R.T.: 4.437 min
Delta R.T.: 0.000 min
Response: 157633891
Conc: 42.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4257

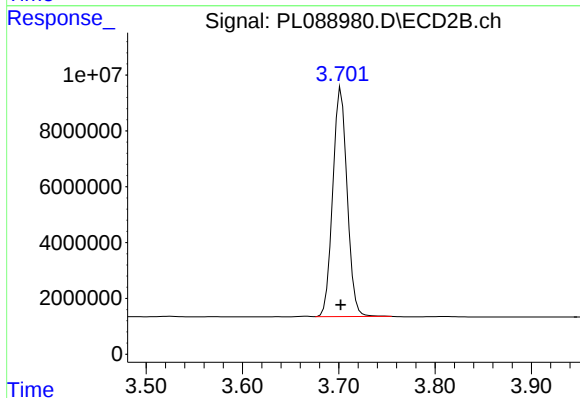


#3 gamma-BHC (Lindane)

R.T.: 3.702 min
Delta R.T.: 0.000 min
Response: 85274397
Conc: 42.71 ng/ml

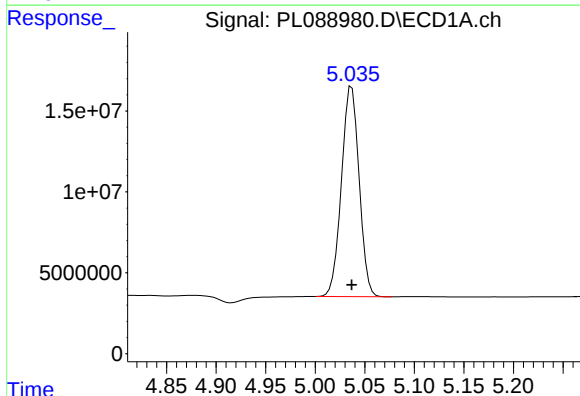


#4 Heptachlor

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 161203791
Conc: 41.15 ng/ml

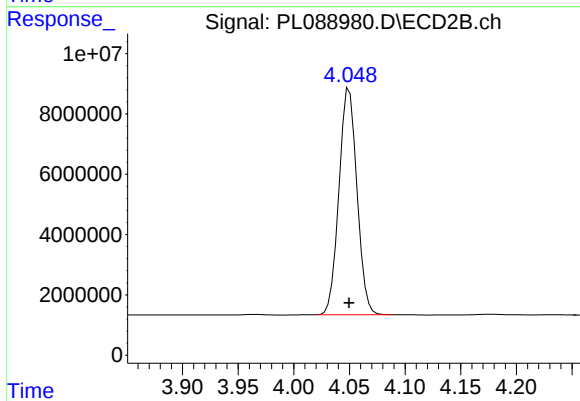

#4 Heptachlor


R.T.: 4.050 min
Delta R.T.: 0.000 min
Response: 84710382
Conc: 41.96 ng/ml

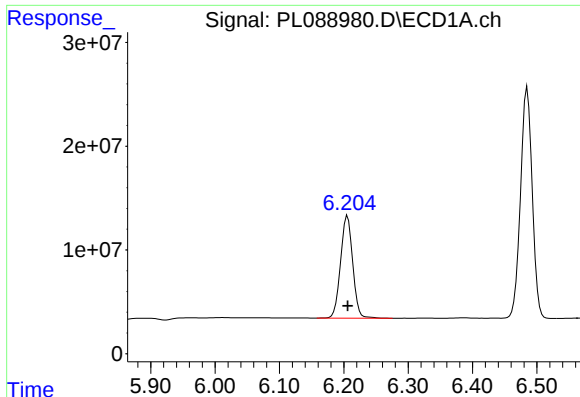

#9 Endosulfan I


R.T.: 6.206 min
Delta R.T.: 0.000 min
Response: 129359062
Conc: 40.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4257

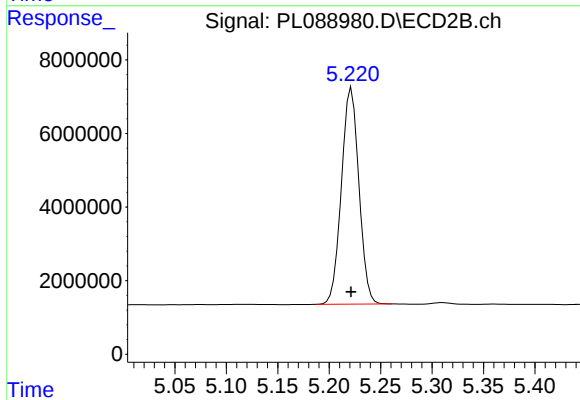


#9 Endosulfan I

R.T.: 5.222 min
Delta R.T.: 0.000 min
Response: 69589702
Conc: 41.06 ng/ml

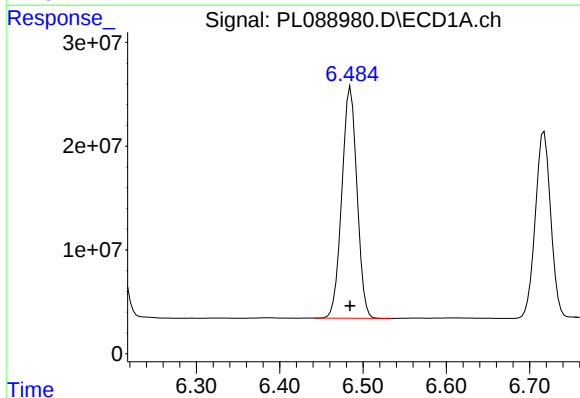


#13 Dieldrin

R.T.: 6.485 min
Delta R.T.: 0.000 min
Response: 281378063
Conc: 83.65 ng/ml

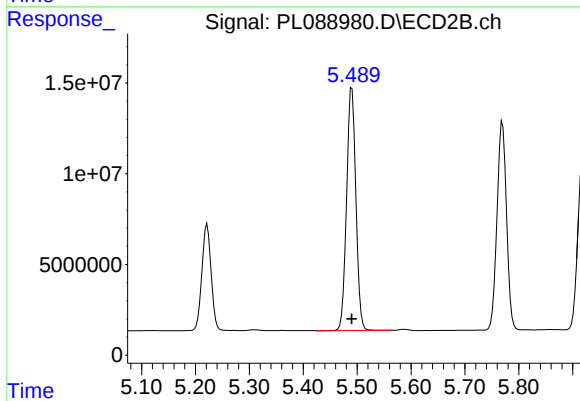

#13 Dieldrin


R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 160165086
Conc: 84.37 ng/ml

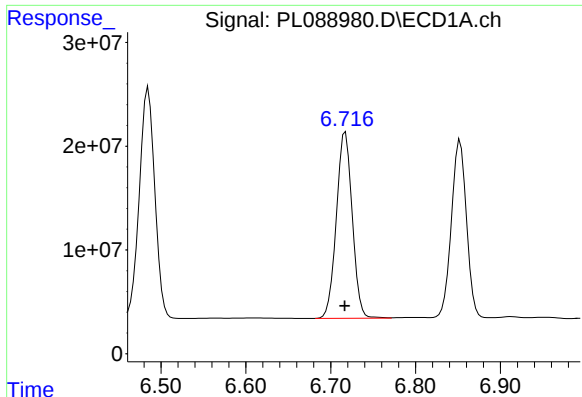

#14 Endrin


R.T.: 6.717 min
Delta R.T.: 0.000 min
Response: 233105771
Conc: 83.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4257

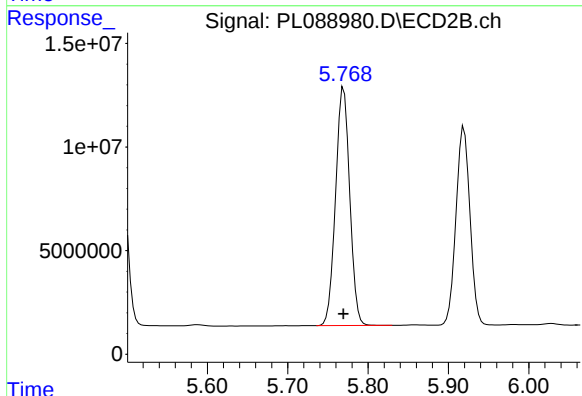


#14 Endrin

R.T.: 5.770 min
Delta R.T.: 0.000 min
Response: 140978335
Conc: 83.79 ng/ml

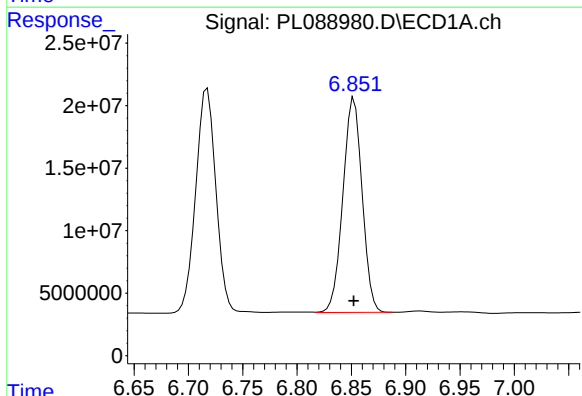


#16 4,4'-DDD

R.T.: 6.853 min
Delta R.T.: 0.000 min
Response: 211733496
Conc: 83.71 ng/ml

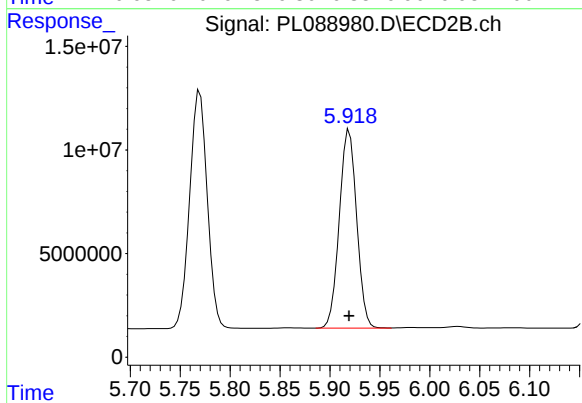

#16 4,4'-DDD


R.T.: 5.919 min
Delta R.T.: 0.000 min
Response: 115974962
Conc: 84.06 ng/ml

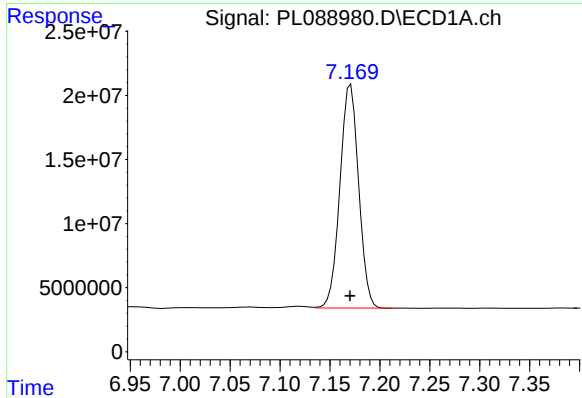

#17 4,4'-DDT


R.T.: 7.171 min
Delta R.T.: 0.000 min
Response: 227828792
Conc: 82.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4257

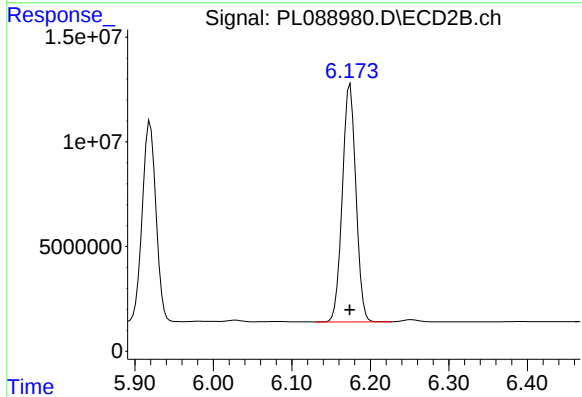


#17 4,4'-DDT

R.T.: 6.174 min
Delta R.T.: 0.000 min
Response: 136809344
Conc: 84.39 ng/ml

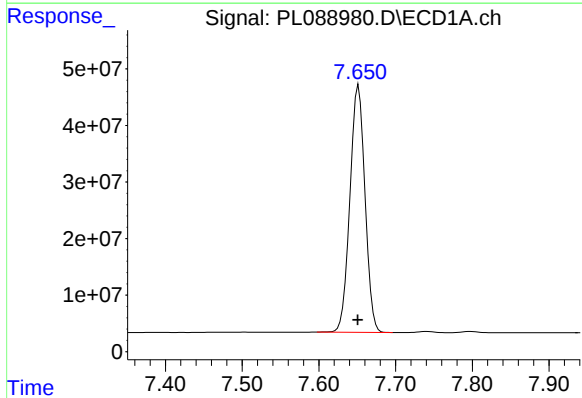


#20 Methoxychlor

R.T.: 7.652 min
Delta R.T.: 0.000 min
Response: 601033254
Conc: 393.88 ng/ml

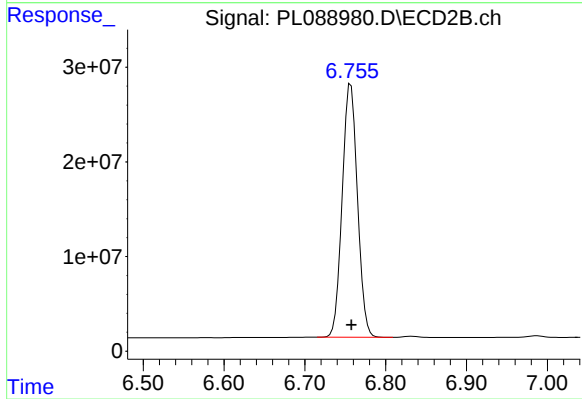

#20 Methoxychlor


R.T.: 6.757 min
Delta R.T.: 0.000 min
Response: 350893774
Conc: 387.16 ng/ml

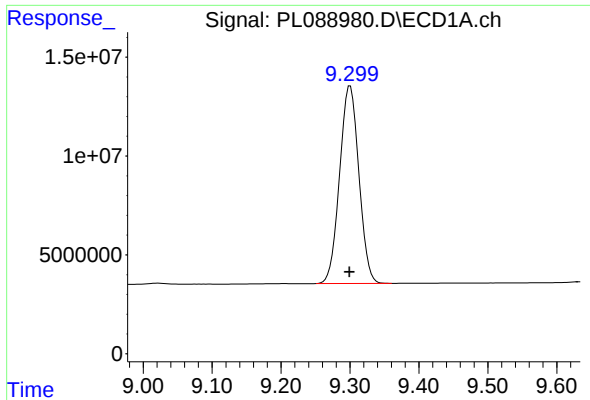

#27 Decachlorobiphenyl

R.T.: 9.300 min
Delta R.T.: 0.000 min
Response: 194435945
Conc: 76.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4257

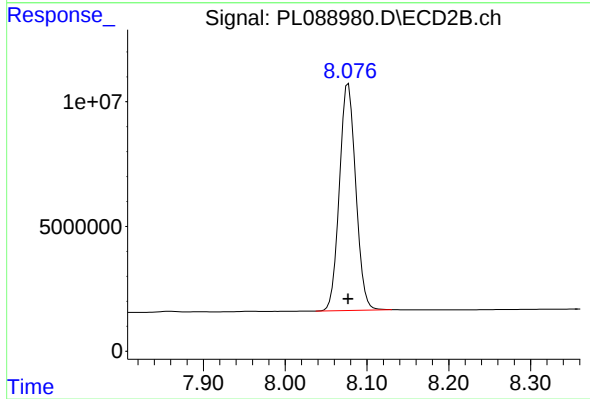

#27 Decachlorobiphenyl

R.T.: 8.077 min
Delta R.T.: 0.000 min
Response: 125791356
Conc: 76.70 ng/ml