

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041024\
 Data File : PL088982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2024 21:39
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA5259

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 05:00:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 04:57:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.852	229.0E6	128.0E6	85.467	86.248
27)	SA Decachlor...	9.300	8.077	387.3E6	252.7E6	153.237	154.109
Target Compounds							
2)	A alpha-BHC	4.099	3.366	372.1E6	202.9E6	95.222	97.623
3)	MA gamma-BHC...	4.437	3.702	346.1E6	188.2E6	92.624	94.263
4)	MA Heptachlor	5.037	4.050	342.4E6	183.2E6	87.397	90.769
9)	A Endosulfan I	6.206	5.221	269.5E6	148.0E6	83.404	87.299
13)	MA Dieldrin	6.485	5.490	597.4E6	343.3E6	177.589	180.830
14)	MA Endrin	6.717	5.770	493.8E6	301.1E6	176.462	178.962
16)	A 4,4'-DDD	6.852	5.919	450.2E6	247.3E6	177.995	179.253
17)	MA 4,4'-DDT	7.170	6.174	483.6E6	293.8E6	176.051	181.214
20)	A Methoxychlor	7.651	6.757	1195.4E6	684.3E6	783.378	755.026


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041024\
Data File : PL088982.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 21:39
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 05:00:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 04:57:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

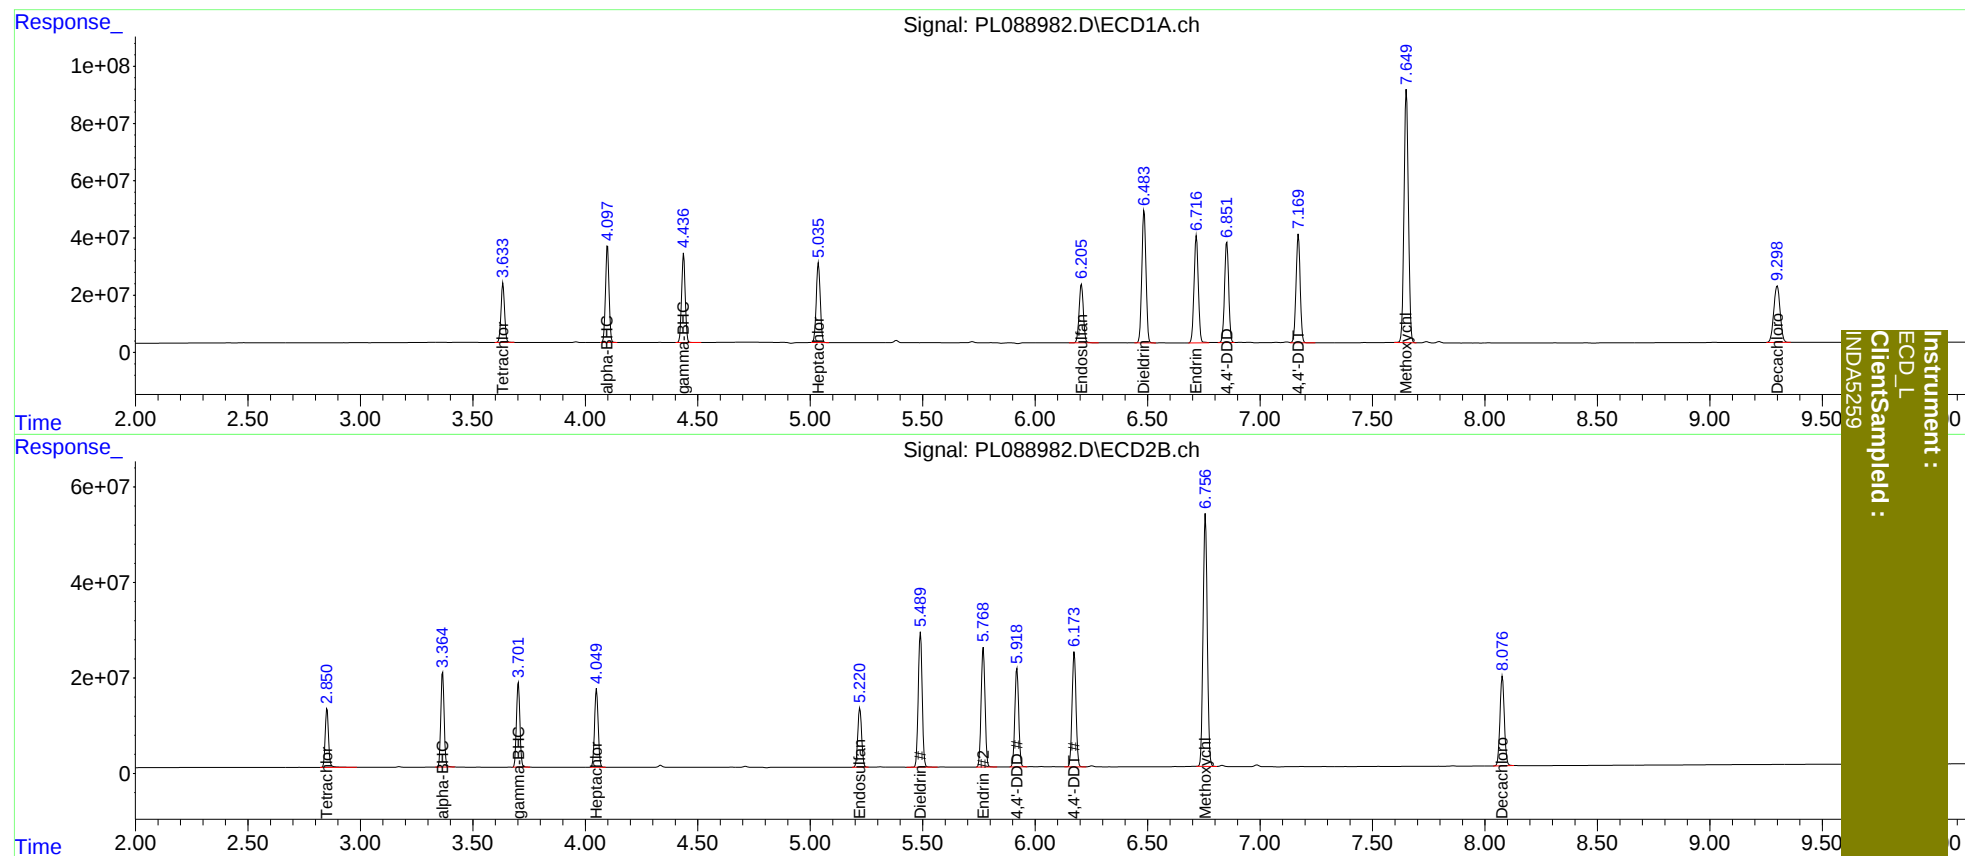


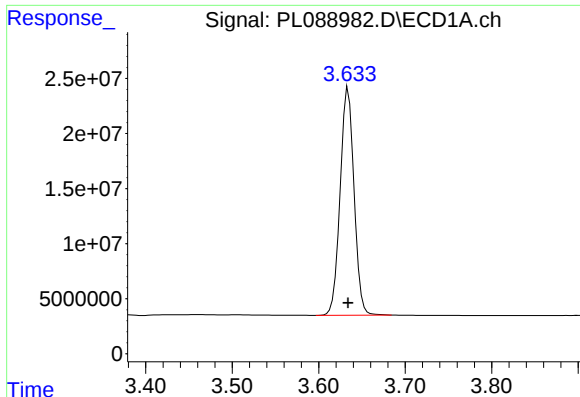

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 229018569
Conc: 85.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5259

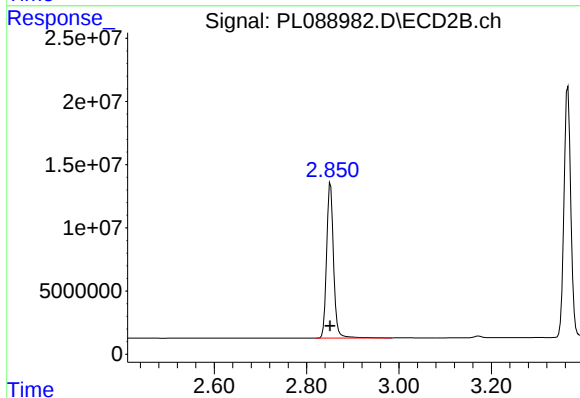


#1 Tetrachloro-m-xylene

R.T.: 2.852 min
Delta R.T.: 0.000 min
Response: 127980972
Conc: 86.25 ng/ml

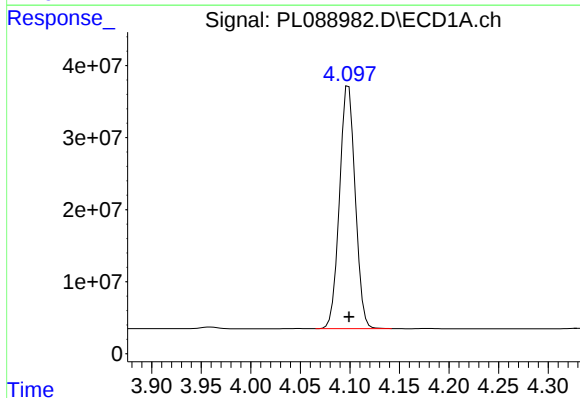


#2 alpha-BHC

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 372113410
Conc: 95.22 ng/ml

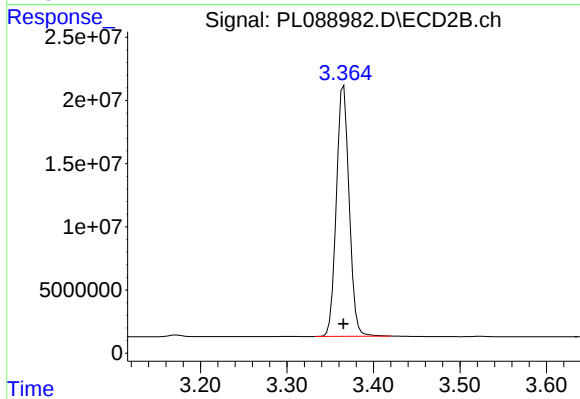

#2 alpha-BHC


R.T.: 3.366 min
Delta R.T.: 0.000 min
Response: 202864472
Conc: 97.62 ng/ml

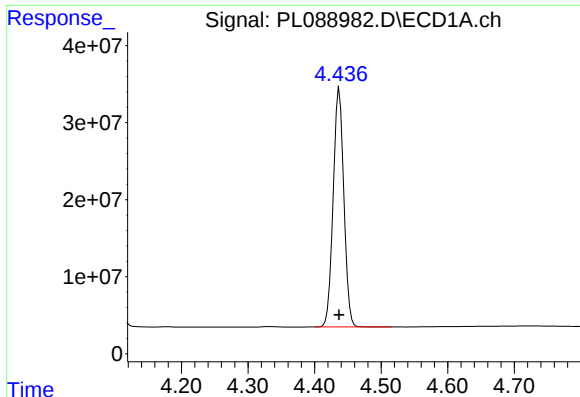

#3 gamma-BHC (Lindane)


R.T.: 4.437 min
Delta R.T.: 0.000 min
Response: 346145098
Conc: 92.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5259

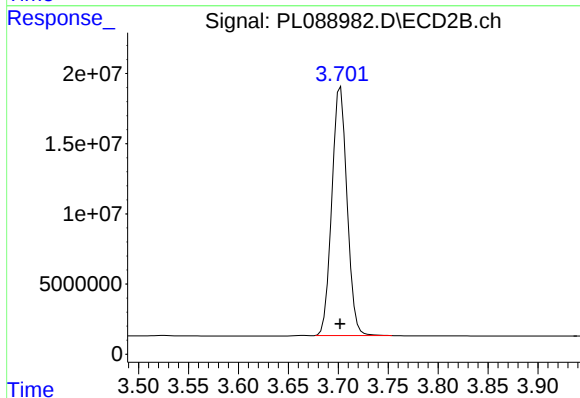


#3 gamma-BHC (Lindane)

R.T.: 3.702 min
Delta R.T.: 0.000 min
Response: 188212850
Conc: 94.26 ng/ml

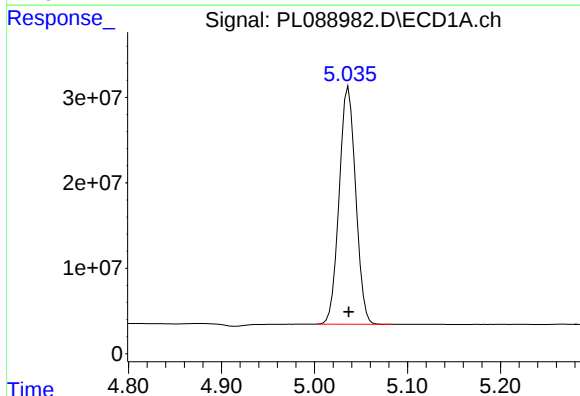


#4 Heptachlor

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 342399670
Conc: 87.40 ng/ml

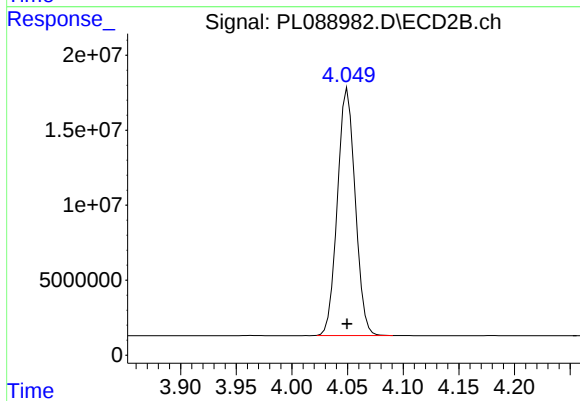

#4 Heptachlor


R.T.: 4.050 min
Delta R.T.: 0.000 min
Response: 183247785
Conc: 90.77 ng/ml

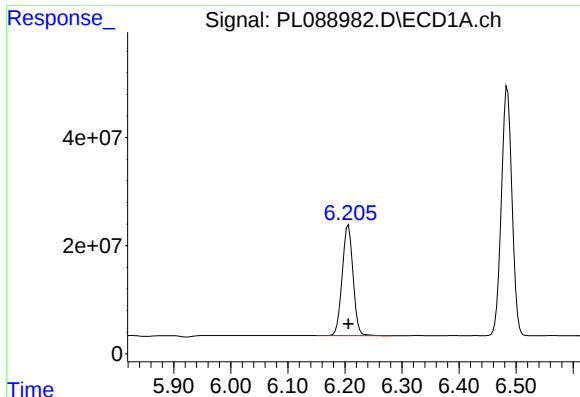

#9 Endosulfan I


R.T.: 6.206 min
Delta R.T.: 0.000 min
Response: 269472111
Conc: 83.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5259

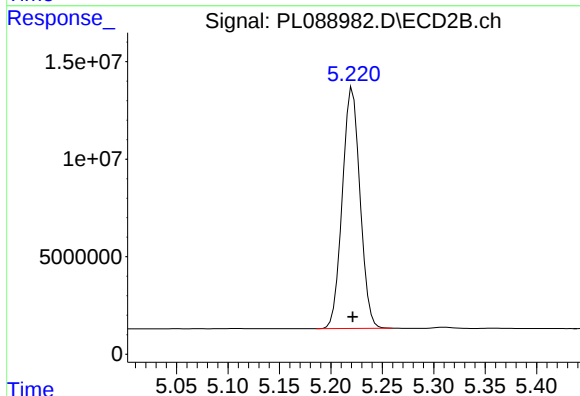


#9 Endosulfan I

R.T.: 5.221 min
Delta R.T.: 0.000 min
Response: 147959190
Conc: 87.30 ng/ml

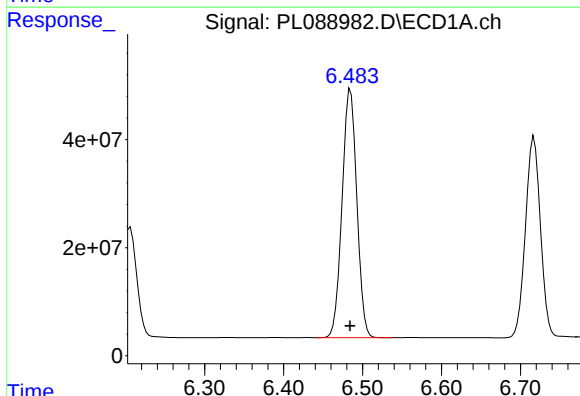


#13 Dieldrin

R.T.: 6.485 min
Delta R.T.: 0.000 min
Response: 597381459
Conc: 177.59 ng/ml

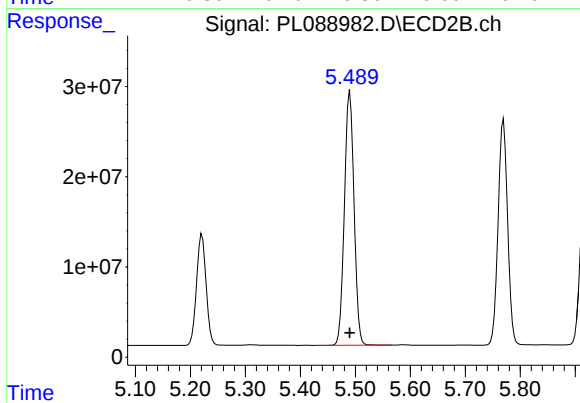

#13 Dieldrin


R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 343272035
Conc: 180.83 ng/ml

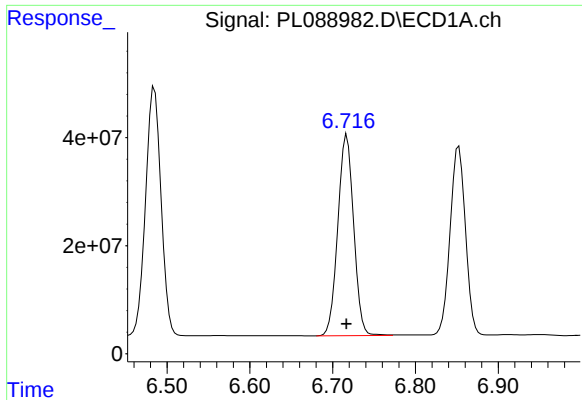

#14 Endrin


R.T.: 6.717 min
Delta R.T.: 0.000 min
Response: 493833105
Conc: 176.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5259

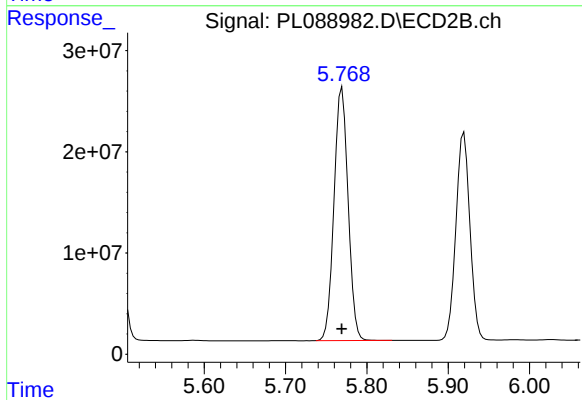


#14 Endrin

R.T.: 5.770 min
Delta R.T.: 0.000 min
Response: 301109338
Conc: 178.96 ng/ml

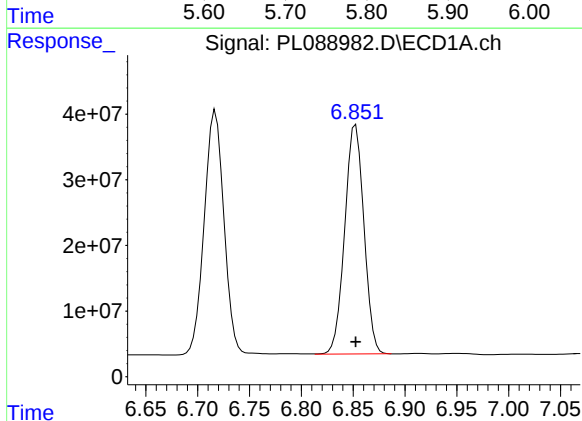


#16 4,4'-DDD

R.T.: 6.852 min
Delta R.T.: 0.000 min
Response: 450222657
Conc: 178.00 ng/ml

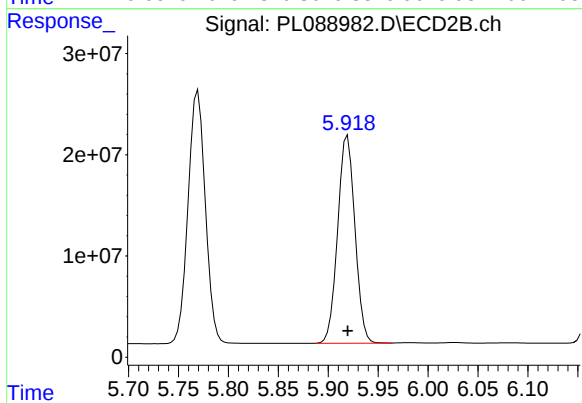

#16 4,4'-DDD


R.T.: 5.919 min
Delta R.T.: 0.000 min
Response: 247314520
Conc: 179.25 ng/ml

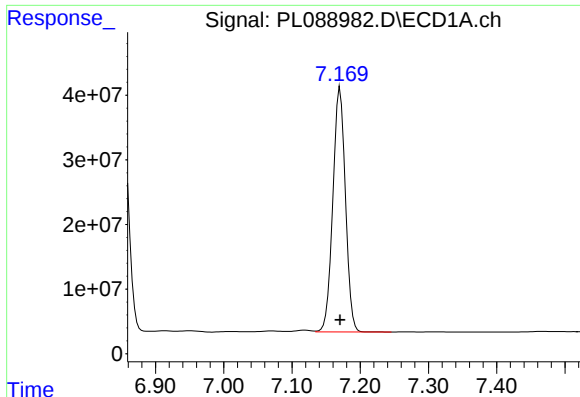

#17 4,4'-DDT


R.T.: 7.170 min
Delta R.T.: 0.000 min
Response: 483578042
Conc: 176.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5259

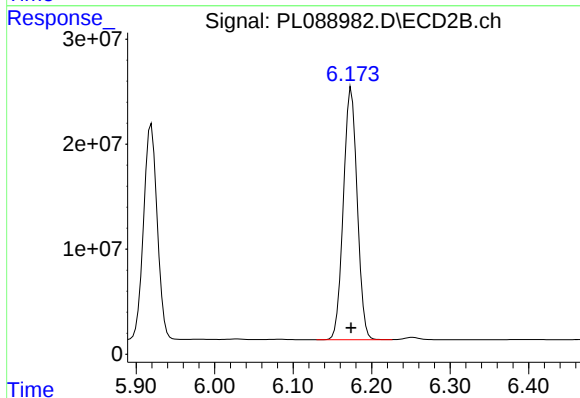


#17 4,4'-DDT

R.T.: 6.174 min
Delta R.T.: 0.000 min
Response: 293779597
Conc: 181.21 ng/ml

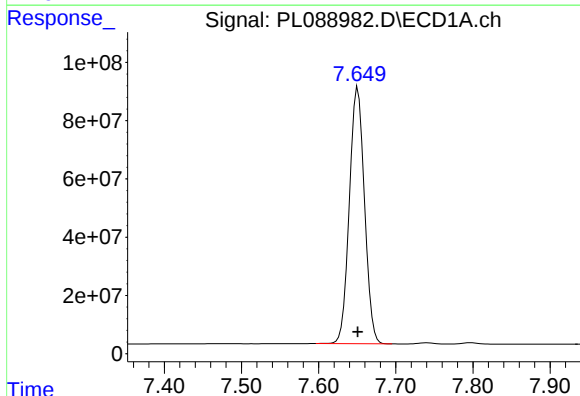


#20 Methoxychlor

R.T.: 7.651 min
Delta R.T.: 0.000 min
Response: 1195371876
Conc: 783.38 ng/ml

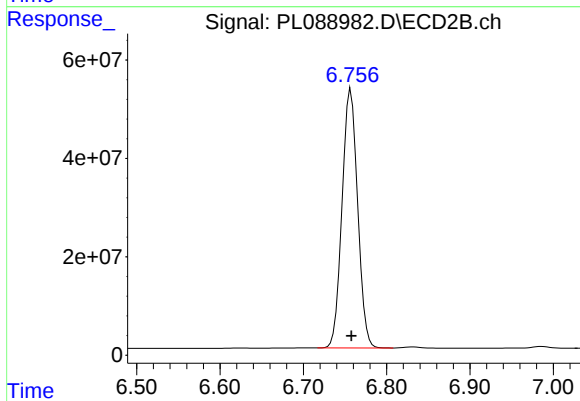

#20 Methoxychlor


R.T.: 6.757 min
Delta R.T.: 0.000 min
Response: 684309133
Conc: 755.03 ng/ml

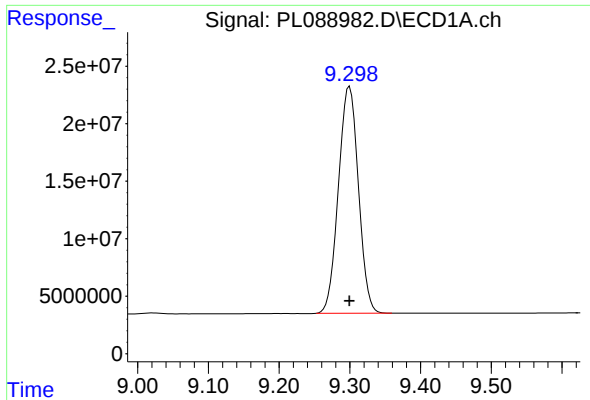

#27 Decachlorobiphenyl

R.T.: 9.300 min
Delta R.T.: 0.000 min
Response: 387283168
Conc: 153.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5259

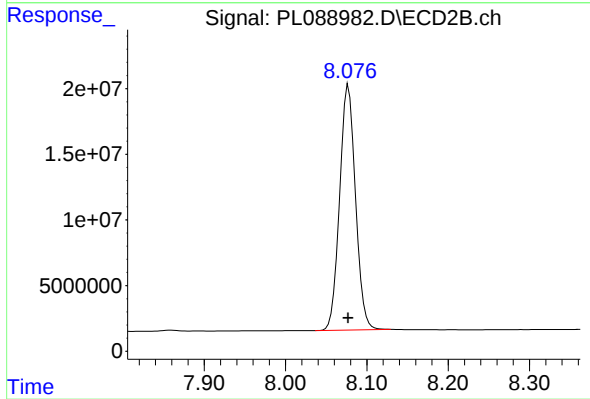

#27 Decachlorobiphenyl

R.T.: 8.077 min
Delta R.T.: 0.000 min
Response: 252736526
Conc: 154.11 ng/ml