

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041025\
 Data File : PL095165.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2025 12:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 20:35:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.768	55440089	73911073	19.586	20.708
28)	SA Decachlor...	9.045	7.898	45338564	84567241	21.513	20.936
Target Compounds							
13)	MA Dieldrin	0.000	5.370	0	3010788	N.D.	0.621 #
22)	Mirex	0.000	7.044f	0	32890486	N.D.	8.666 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041025\
Data File : PL095165.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2025 12:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 20:35:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

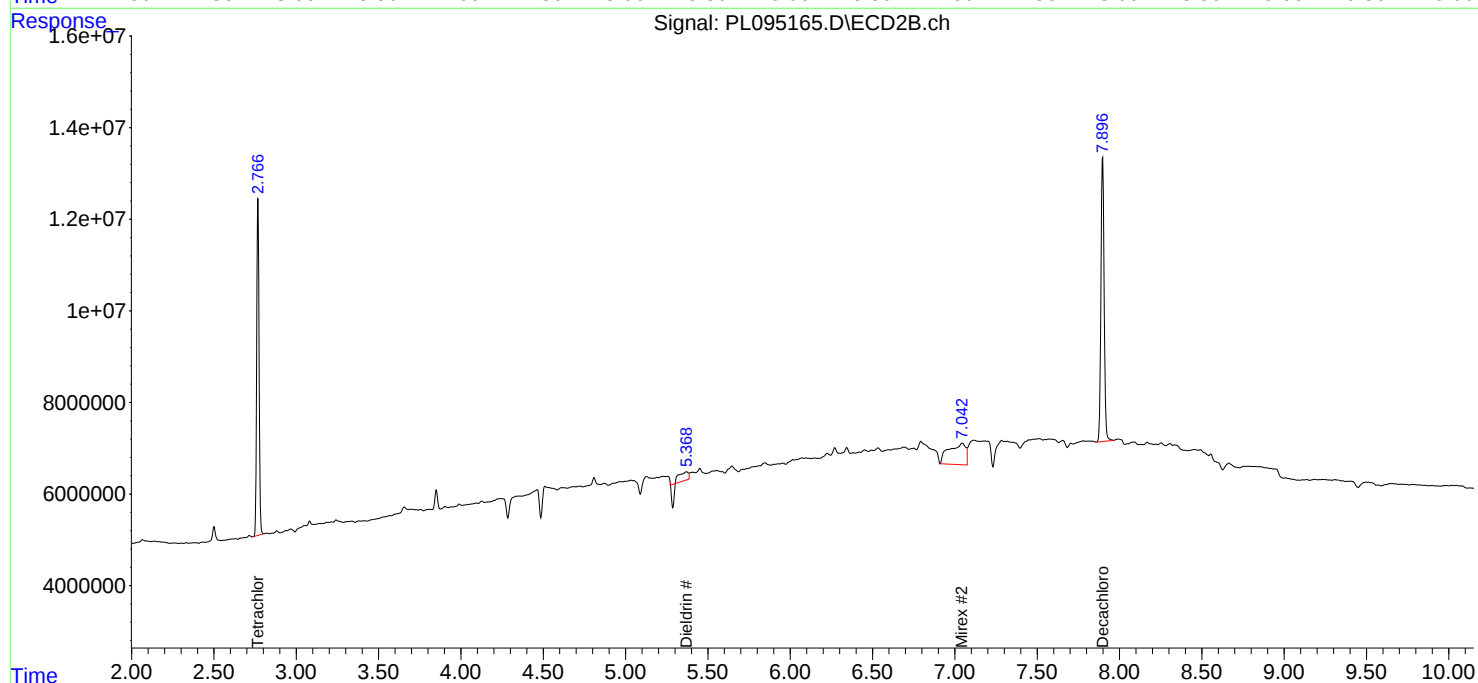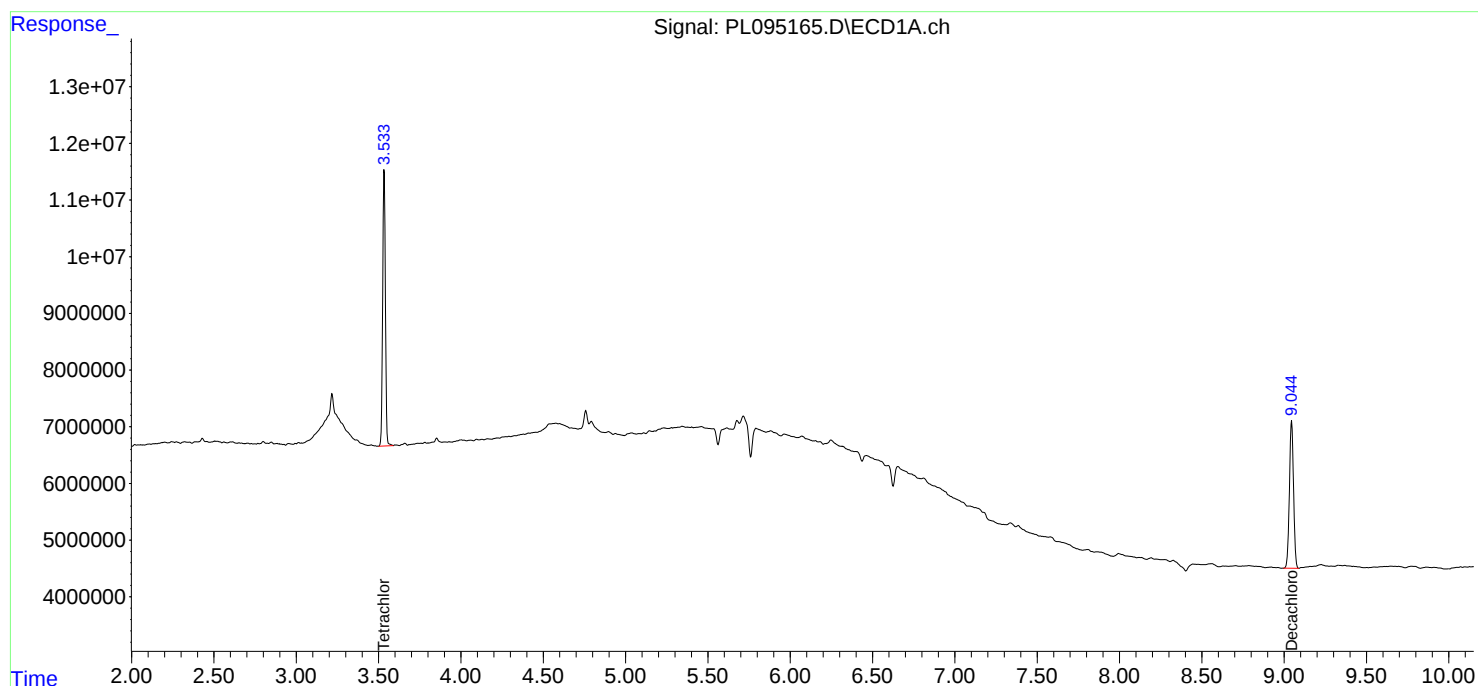


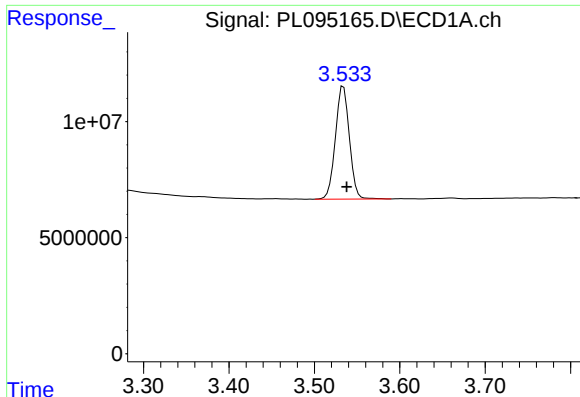

#1 Tetrachloro-m-xylene


R.T.: 3.534 min
Delta R.T.: -0.004 min
Response: 55440089
Conc: 19.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

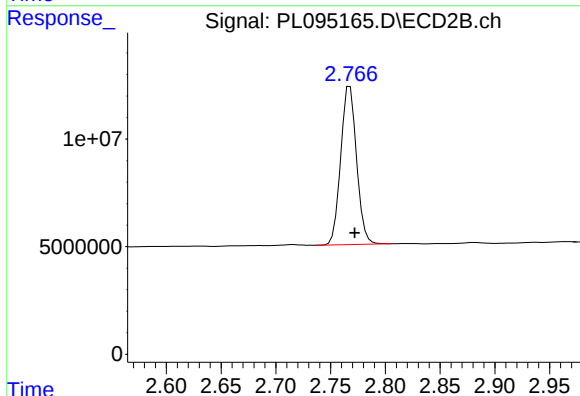


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: -0.004 min
Response: 73911073
Conc: 20.71 ng/ml

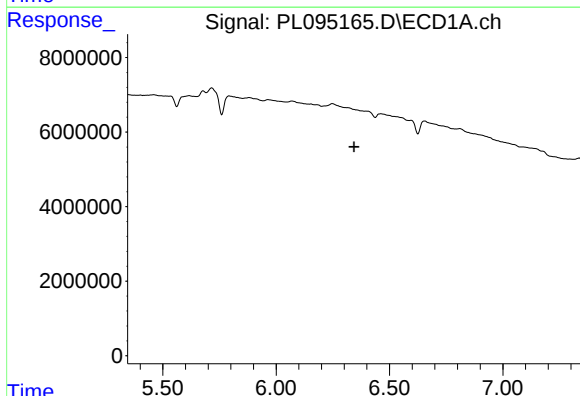


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.344 min
Response: 0
Conc: N.D.

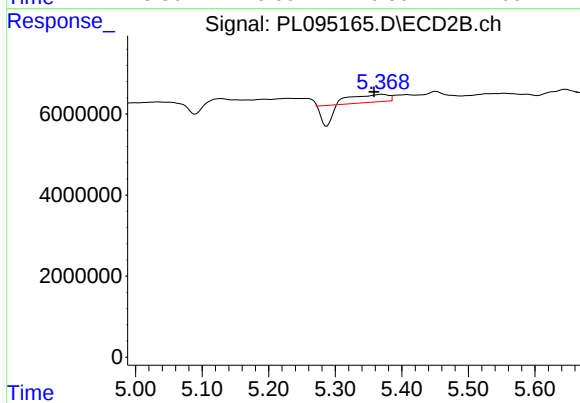

#13 Dieldrin


R.T.: 5.370 min
Delta R.T.: 0.012 min
Response: 3010788
Conc: 0.62 ng/ml

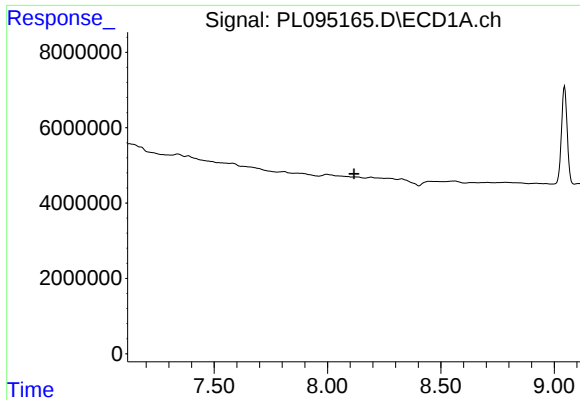

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.117 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

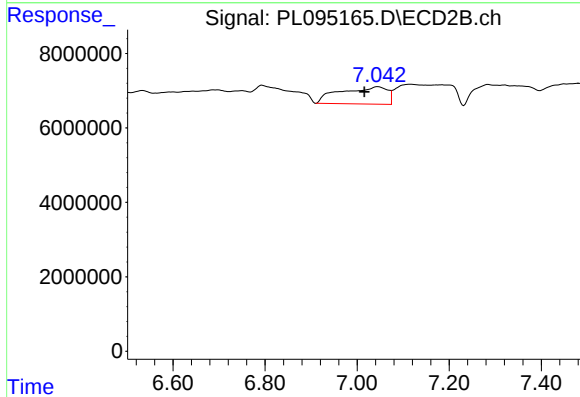


#22 Mirex

R.T.: 7.044 min
Delta R.T.: 0.029 min
Response: 32890486
Conc: 8.67 ng/ml

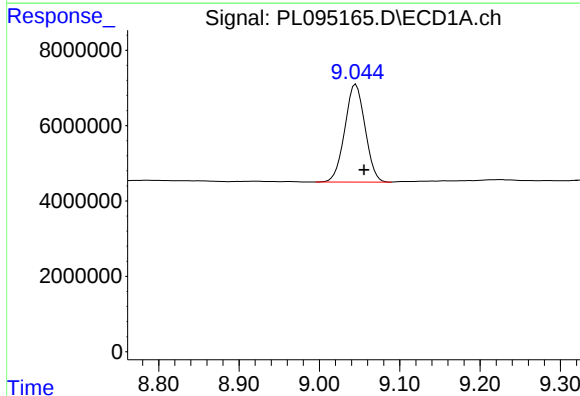

#28 Decachlorobiphenyl

R.T.: 9.045 min
Delta R.T.: -0.010 min
Response: 45338564
Conc: 21.51 ng/ml

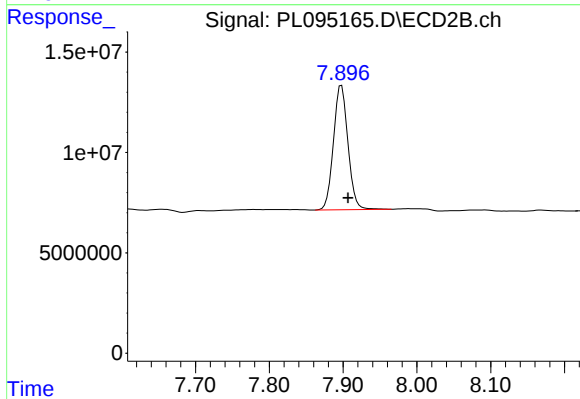

#28 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.009 min
Response: 84567241
Conc: 20.94 ng/ml