

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041119\
 Data File : PL047300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2019 21:47
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 01:19:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.356	3.975	140.2E6	44052809	19.266	19.240
28) SA Decachlor...	8.031	9.026	180.7E6	52677975	21.488	22.721
Target Compounds						
8) B Heptachlo...	0.000	5.837f	0	1970193	N.D.	0.747 #
14) MA Endrin	0.000	6.682	0	4144354	N.D.	1.734 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041119\
Data File : PL047300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2019 21:47
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 01:19:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

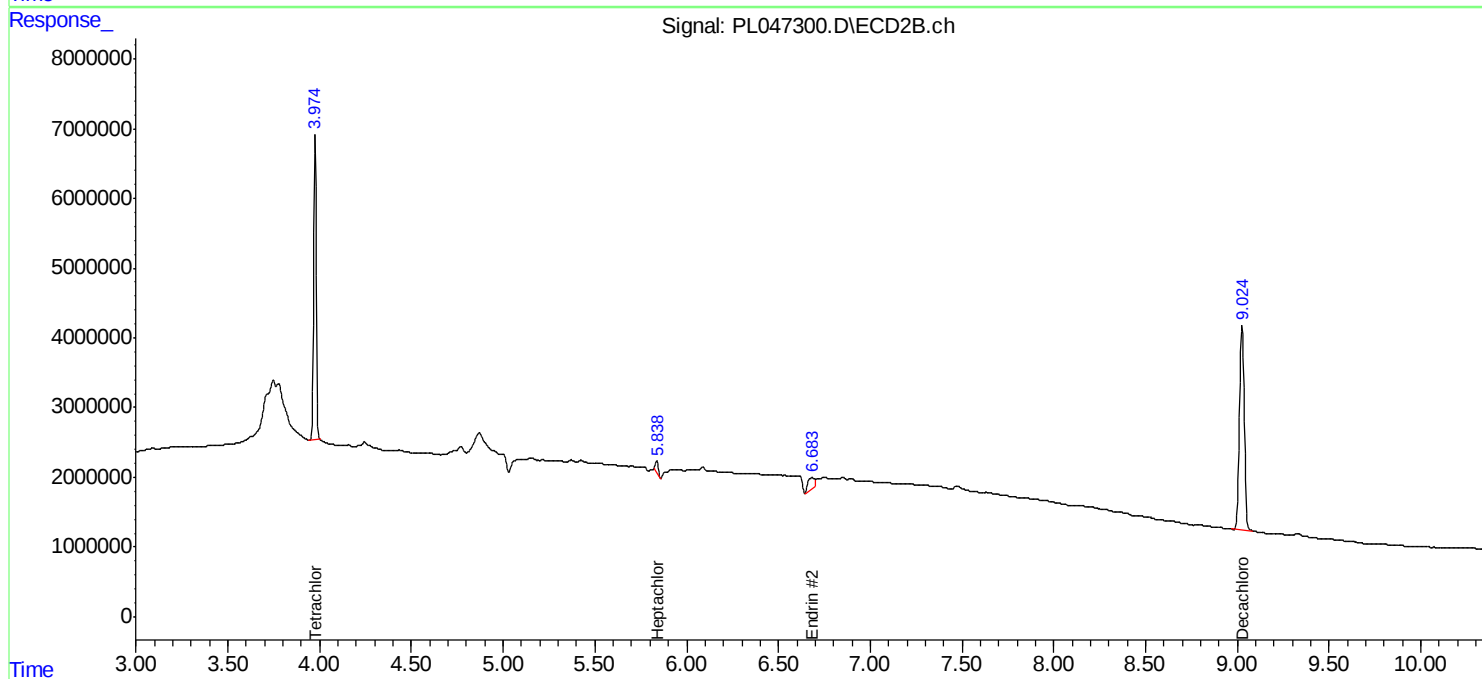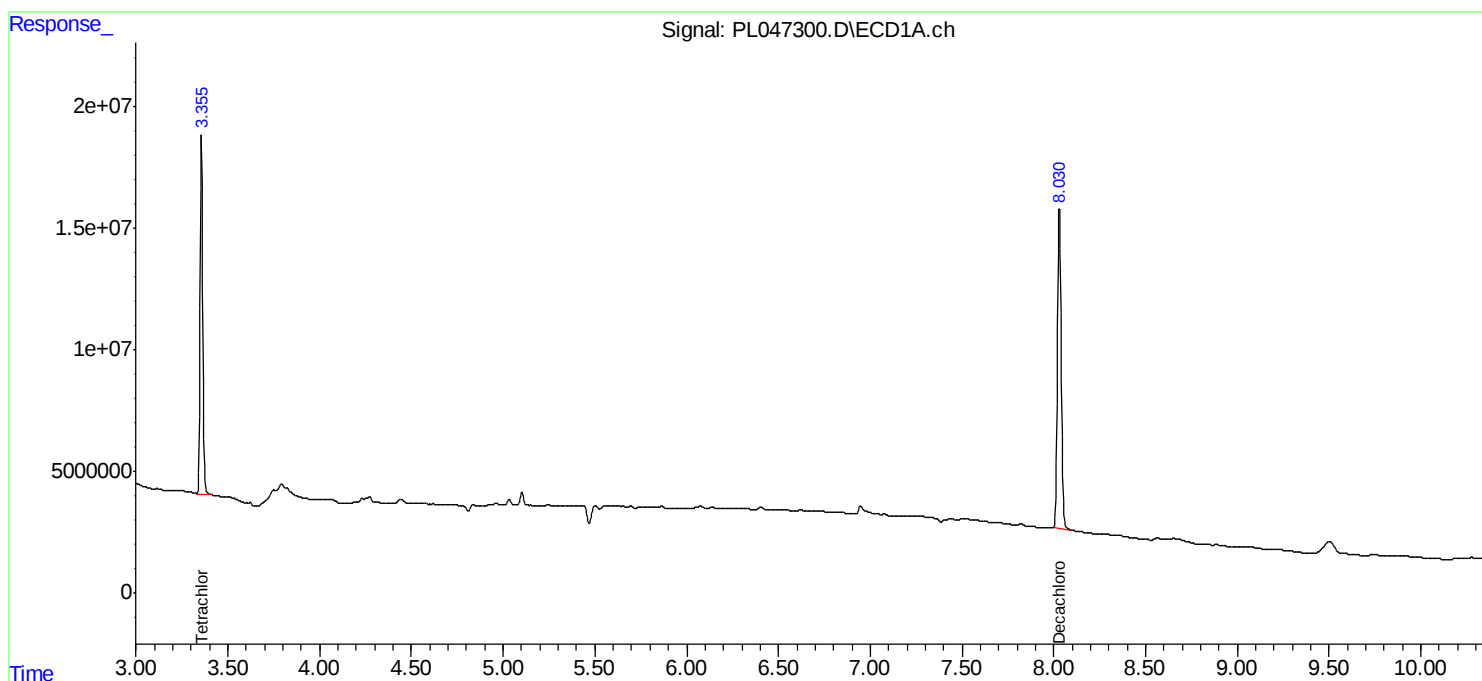


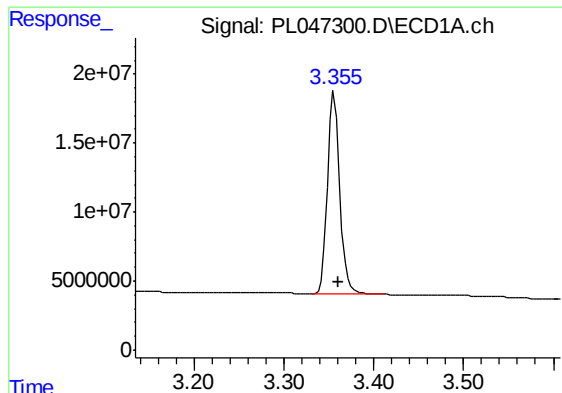

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 140155187
Conc: 19.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

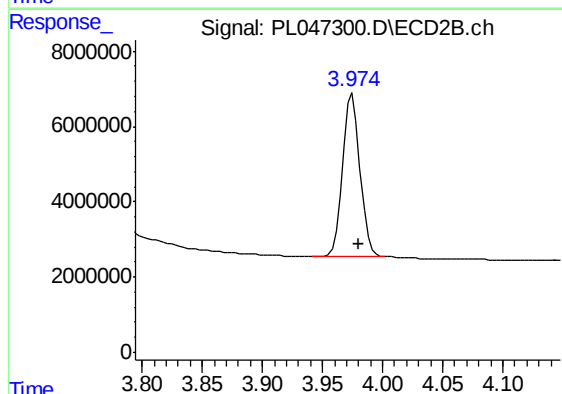


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.006 min
Response: 44052809
Conc: 19.24 ng/ml

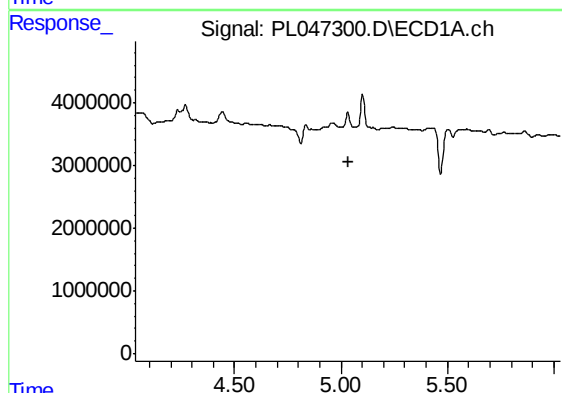


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.034 min
Response: 0
Conc: N.D.

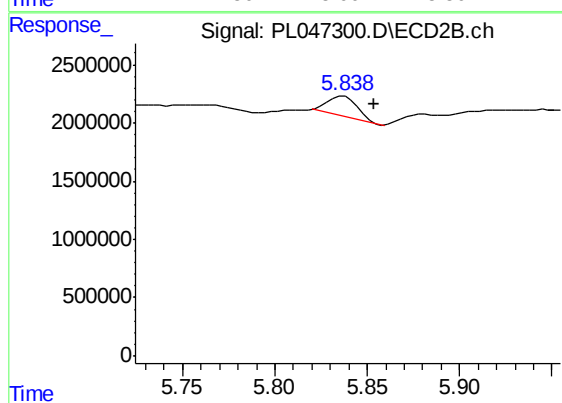

#8 Heptachlor epoxide


R.T.: 5.837 min
Delta R.T.: -0.016 min
Response: 1970193
Conc: 0.75 ng/ml

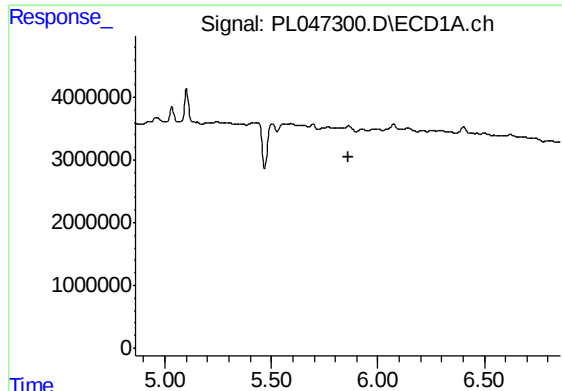

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.860 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

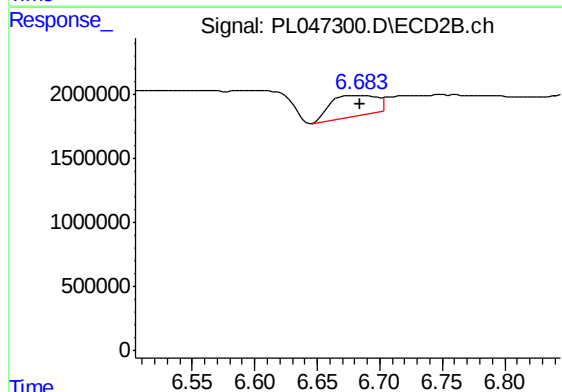


#14 Endrin

R.T.: 6.682 min
Delta R.T.: -0.002 min
Response: 4144354
Conc: 1.73 ng/ml

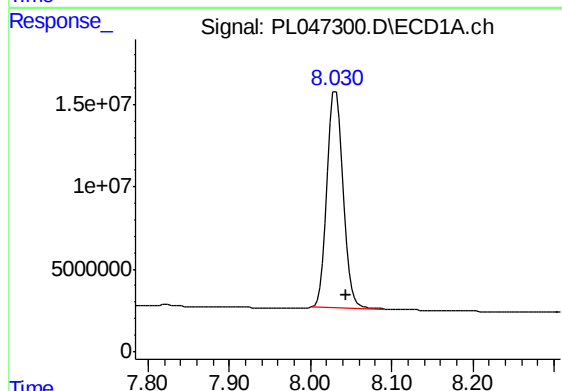

#28 Decachlorobiphenyl

R.T.: 8.031 min
Delta R.T.: -0.013 min
Response: 180732555
Conc: 21.49 ng/ml

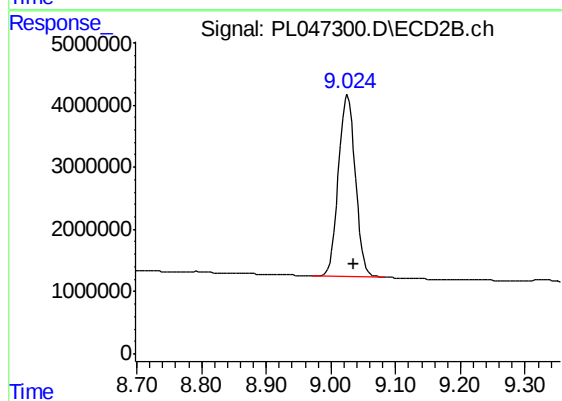

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.009 min
Response: 52677975
Conc: 22.72 ng/ml