

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041119\
Data File : PL047283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2019 17:42
Operator : AJ\SJ
Sample : K2311-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
0237-COMP-CS-2-ELTRT-DISS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 01:14:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.356	3.974	103.4E6	32586372	14.216	14.232
28)	SA Decachlor...	8.032	9.025	111.1E6	32853660	13.212	14.170

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041119\
Data File : PL047283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2019 17:42
Operator : AJ\SJ
Sample : K2311-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
0237-COMP-CS-2-ELTRT-DISS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 01:14:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

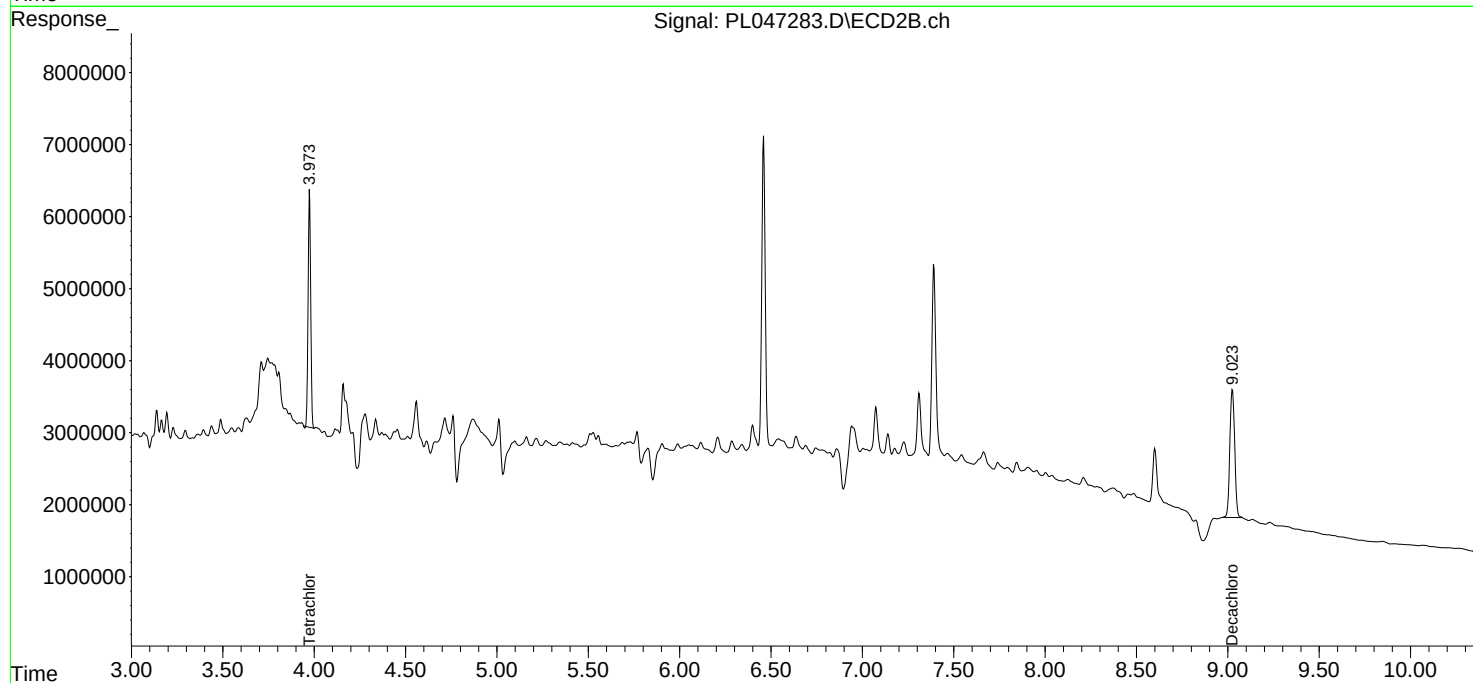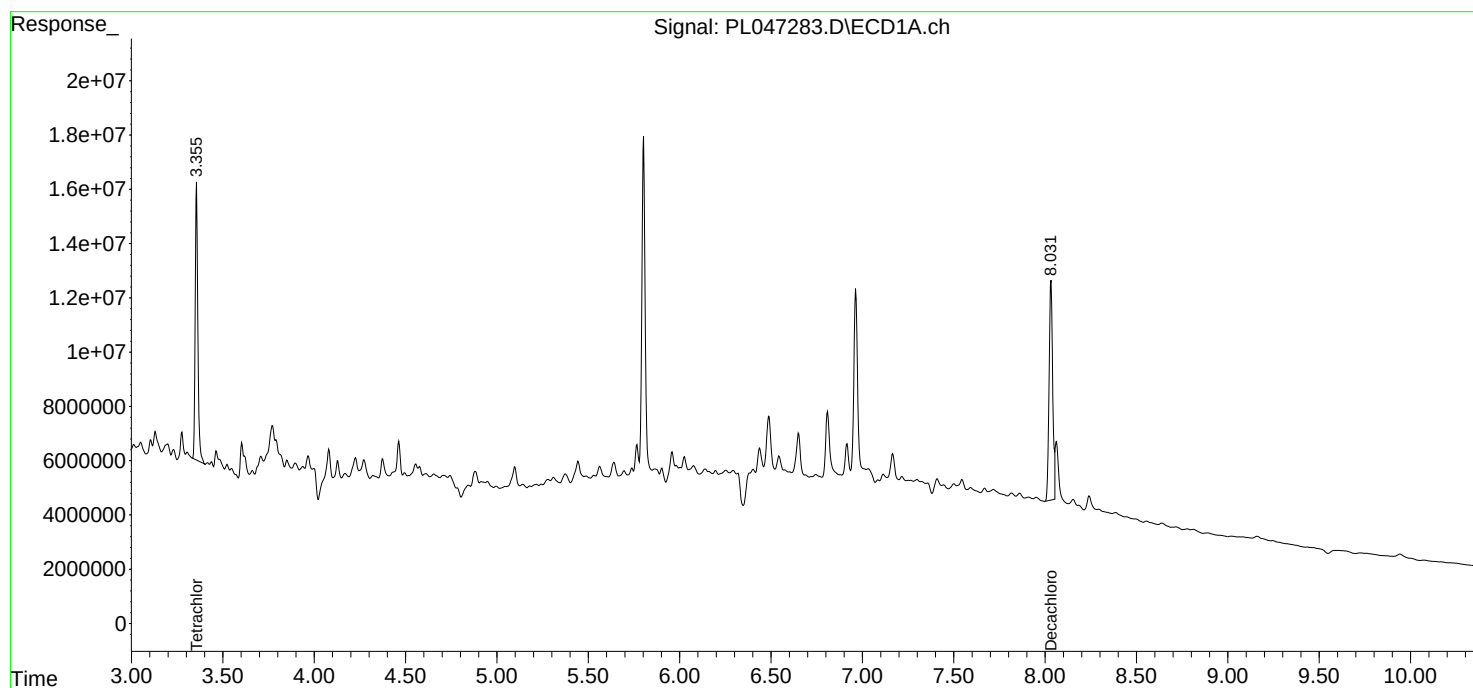


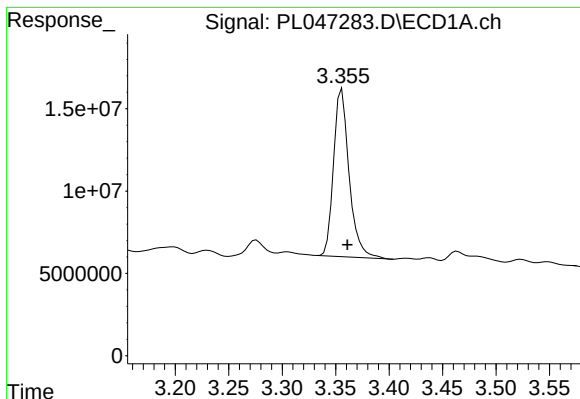

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 103419469
Conc: 14.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
0237-COMP-CS-2-ELTRT-DISS

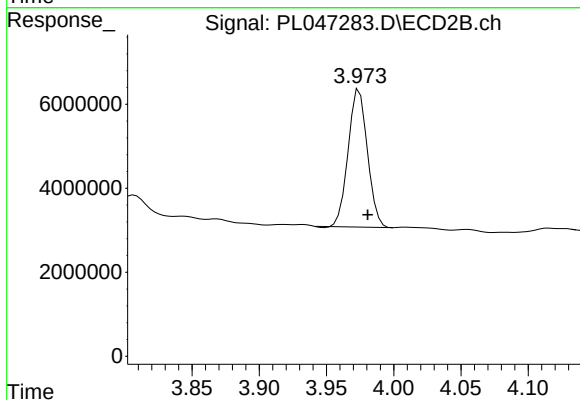


#1 Tetrachloro-m-xylene

R.T.: 3.974 min
Delta R.T.: -0.006 min
Response: 32586372
Conc: 14.23 ng/ml

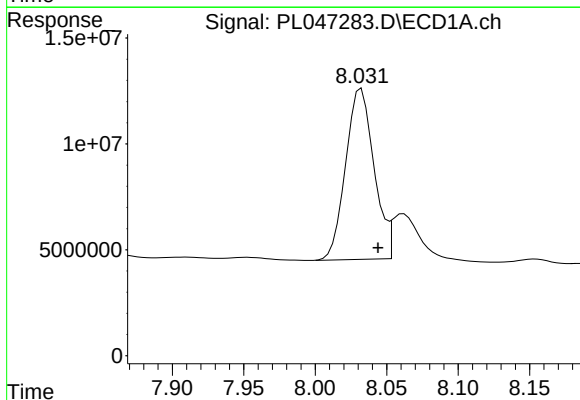

#28 Decachlorobiphenyl

R.T.: 8.032 min
Delta R.T.: -0.012 min
Response: 111129206
Conc: 13.21 ng/ml

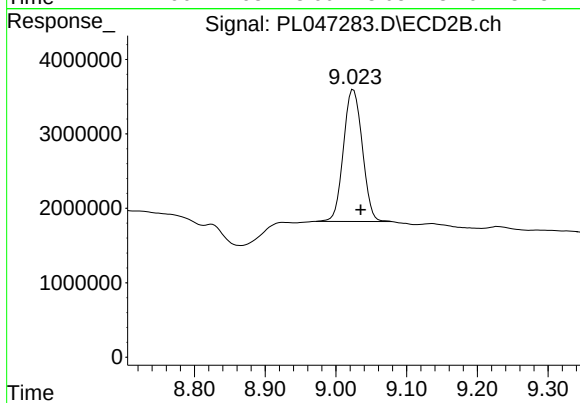

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: -0.010 min
Response: 32853660
Conc: 14.17 ng/ml