

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041122\
 Data File : PL073946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2022 16:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 02:07:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 08 15:48:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.638	5.490	7454615	40148271	23.071	22.518
28)	SA Decachlor...	10.411	11.332	11452187	39005636	22.022	22.083
Target Compounds							
4)	MA Heptachlor	0.000	7.114	0	24218	N.D.	0.009 #
5)	MB Aldrin	0.000	7.476	0	23542	N.D.	0.010 #
6)	B beta-BHC	0.000	6.673	0	637551	N.D.	0.566 #
7)	B delta-BHC	0.000	6.958	0	3147058	N.D.	1.289 #
10)	B gamma-Chl...	0.000	8.193	0	559488	N.D.	0.251 #
13)	MA Dieldrin	0.000	8.603	0	77941	N.D.	0.039 #
14)	MA Endrin	8.084f	0.000	63242	0	0.156	N.D. #
15)	B Endosulfa...	8.348f	9.055f	71281	210276	0.173	0.121 #
19)	B Endosulfa...	0.000	9.444	0	89322	N.D.	0.054 #
23)	Chlordane-1	0.000	6.855	0	922454	N.D.	11.559 #
24)	Chlordane-2	0.000	7.442	0	154607	N.D.	1.871 #
25)	Chlordane-3	0.000	8.193	0	559488	N.D.	1.654 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041122\
Data File : PL073946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2022 16:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 02:07:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Fri Apr 08 15:48:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

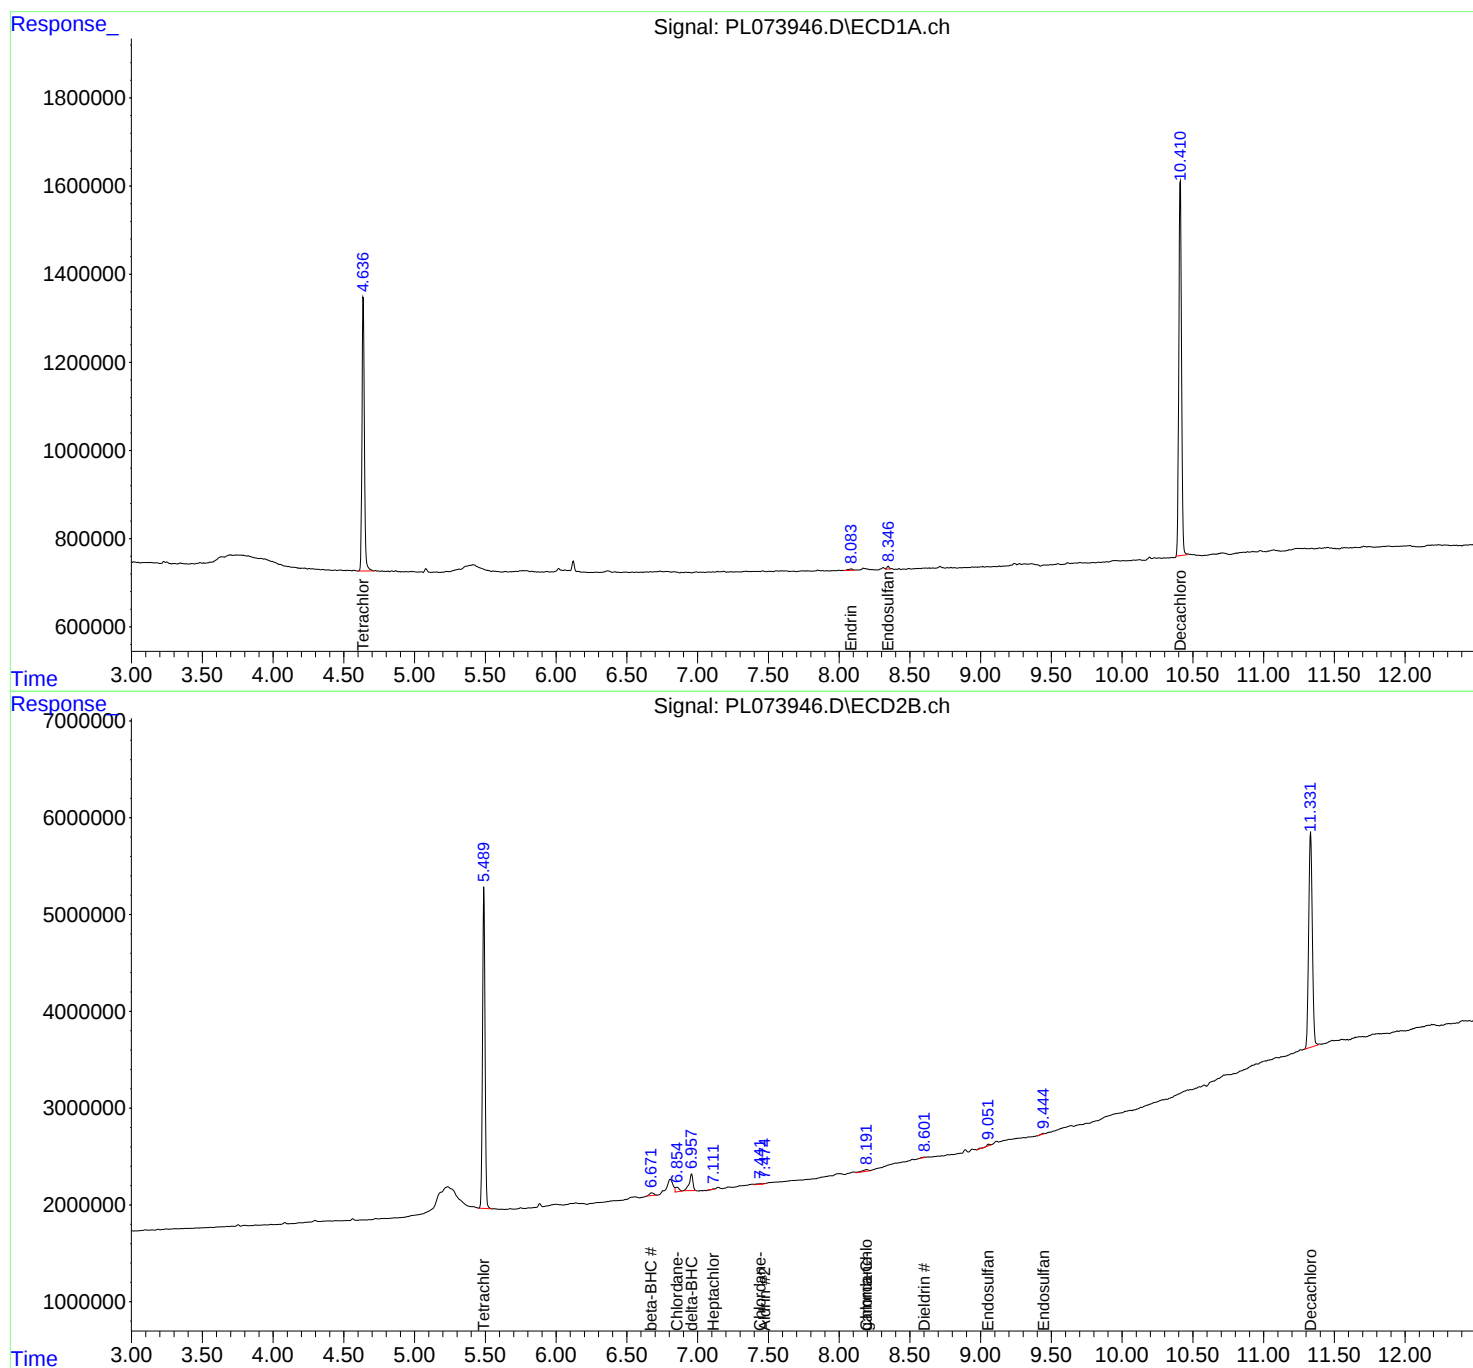


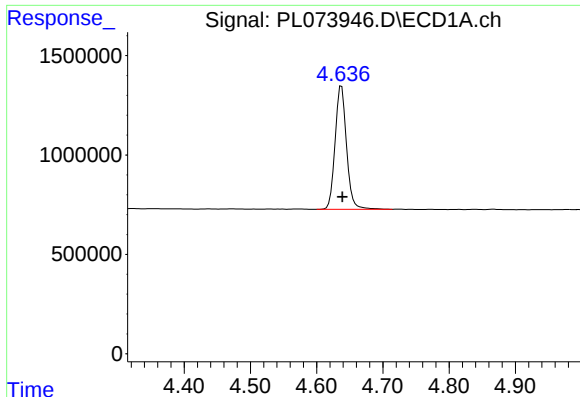

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: -0.001 min
Response: 7454615
Conc: 23.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

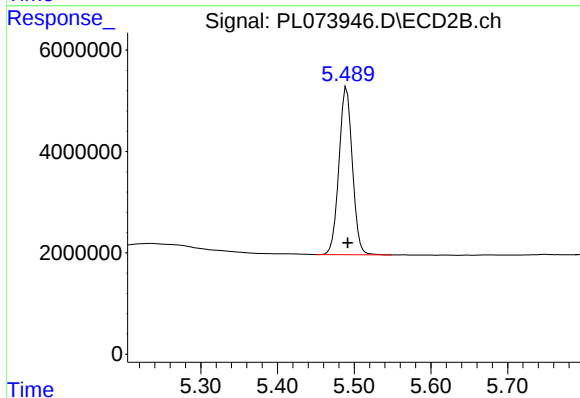


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.001 min
Response: 40148271
Conc: 22.52 ng/ml

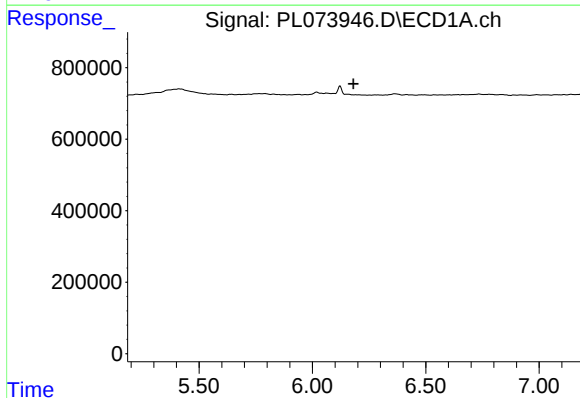


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.181 min
Response: 0
Conc: N.D.

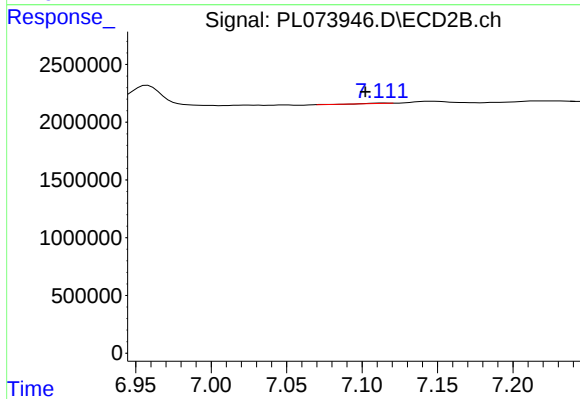

#4 Heptachlor


R.T.: 7.114 min
Delta R.T.: 0.011 min
Response: 24218
Conc: 0.01 ng/ml

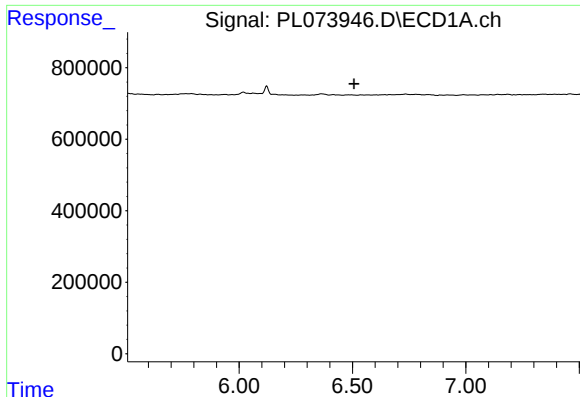

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

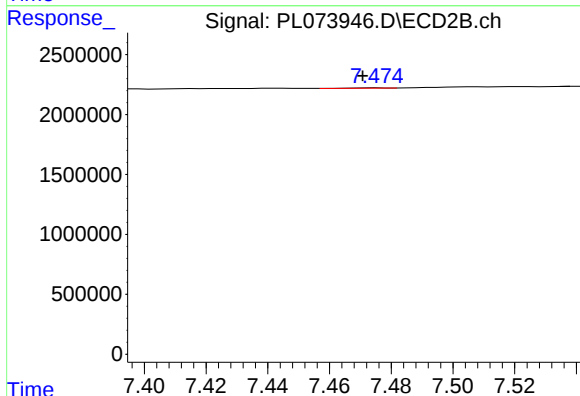


#5 Aldrin

R.T.: 7.476 min
Delta R.T.: 0.005 min
Response: 23542
Conc: 0.01 ng/ml

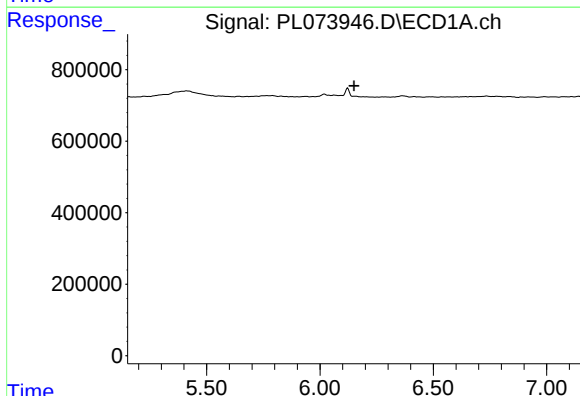


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

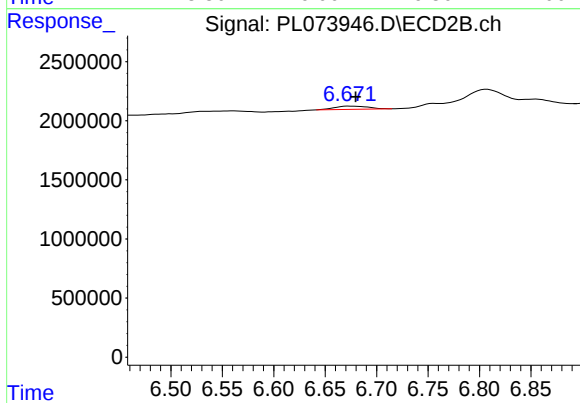

#6 beta-BHC


R.T.: 6.673 min
Delta R.T.: -0.007 min
Response: 637551
Conc: 0.57 ng/ml

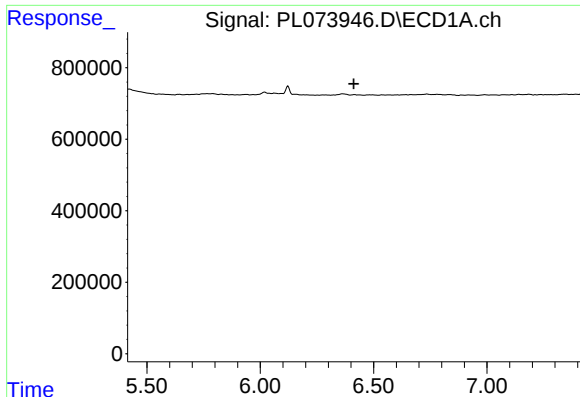

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

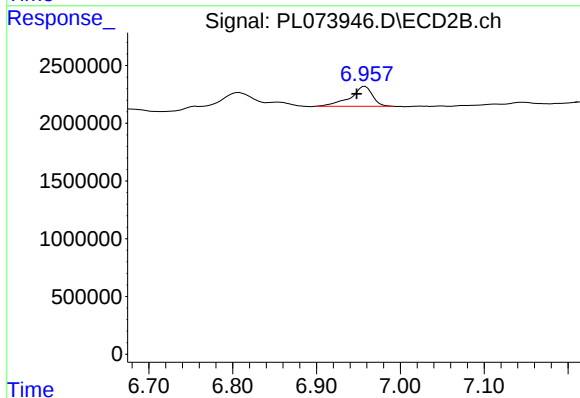


#7 delta-BHC

R.T.: 6.958 min
Delta R.T.: 0.010 min
Response: 3147058
Conc: 1.29 ng/ml

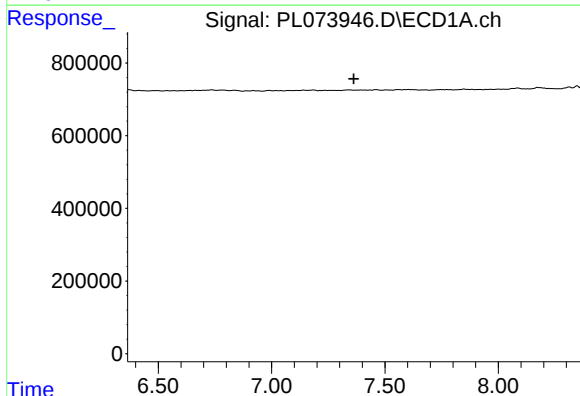


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

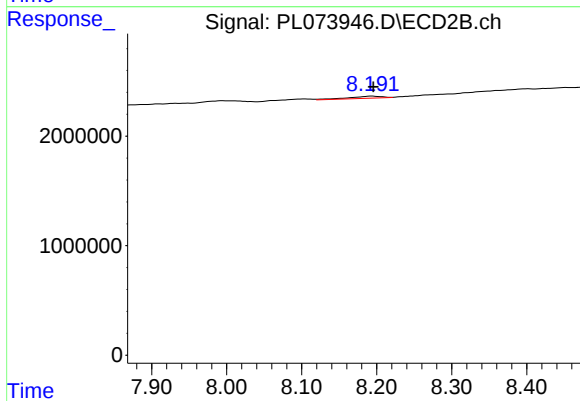

#10 gamma-Chlordane


R.T.: 8.193 min
Delta R.T.: -0.002 min
Response: 559488
Conc: 0.25 ng/ml

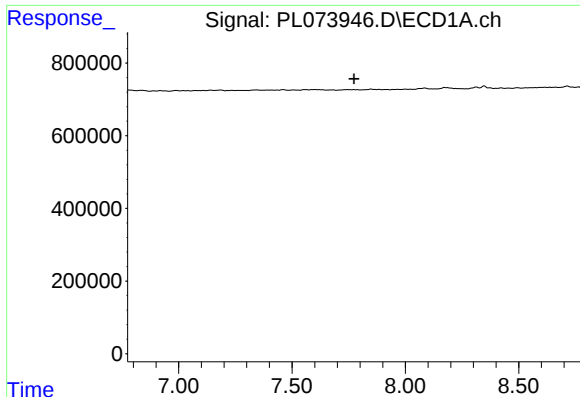

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

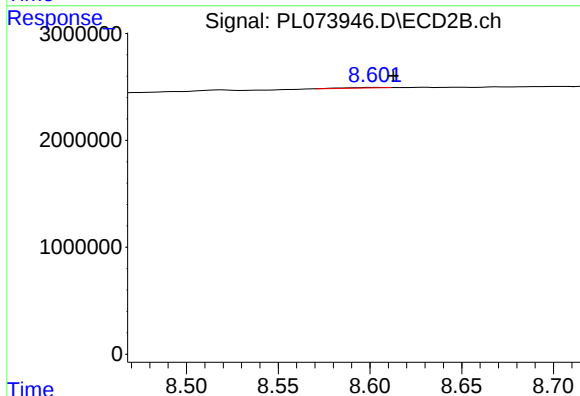


#13 Dieldrin

R.T.: 8.603 min
Delta R.T.: -0.010 min
Response: 77941
Conc: 0.04 ng/ml

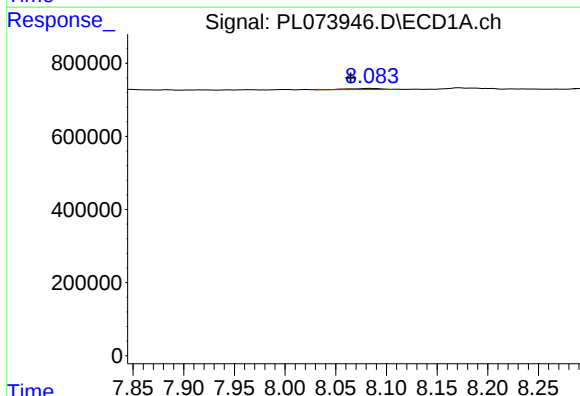


#14 Endrin

R.T.: 8.084 min
Delta R.T.: 0.020 min
Response: 63242
Conc: 0.16 ng/ml

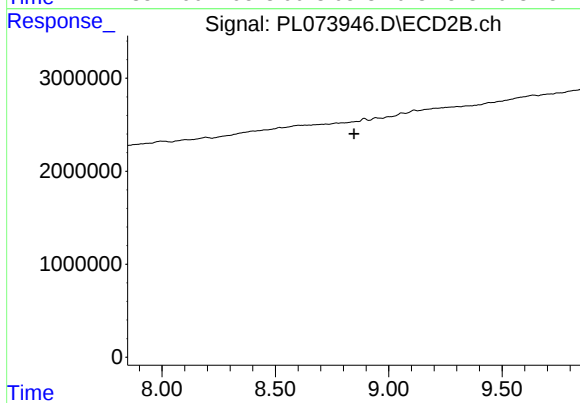

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.847 min
Response: 0
Conc: N.D.

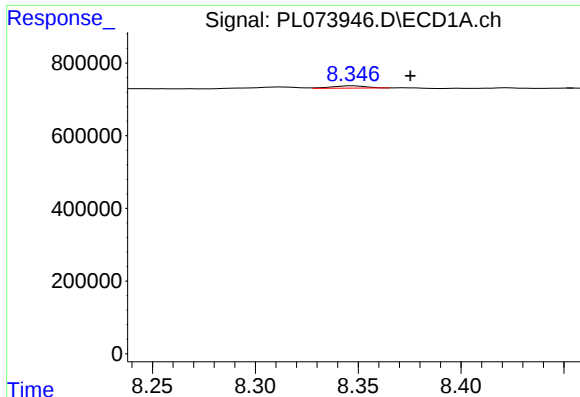

#15 Endosulfan II


R.T.: 8.348 min
Delta R.T.: -0.028 min
Response: 71281
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

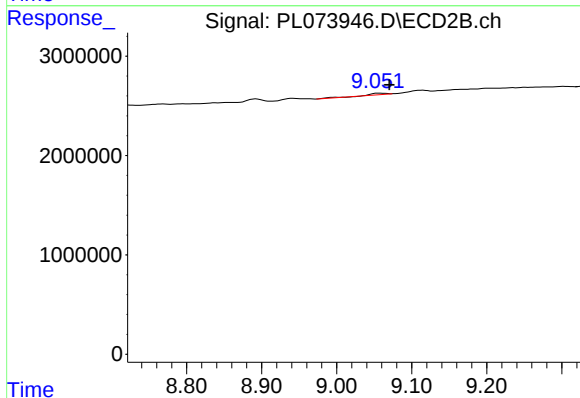


#15 Endosulfan II

R.T.: 9.055 min
Delta R.T.: -0.015 min
Response: 210276
Conc: 0.12 ng/ml

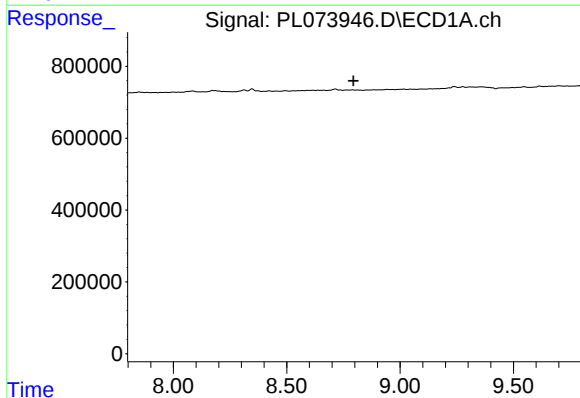


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 8.795 min
Response: 0
Conc: N.D.

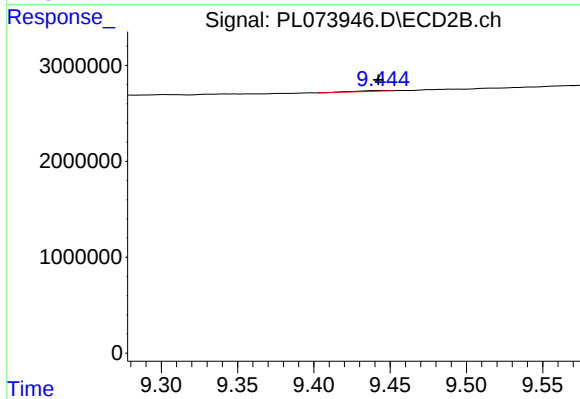

#19 Endosulfan Sulfate


R.T.: 9.444 min
Delta R.T.: 0.002 min
Response: 89322
Conc: 0.05 ng/ml

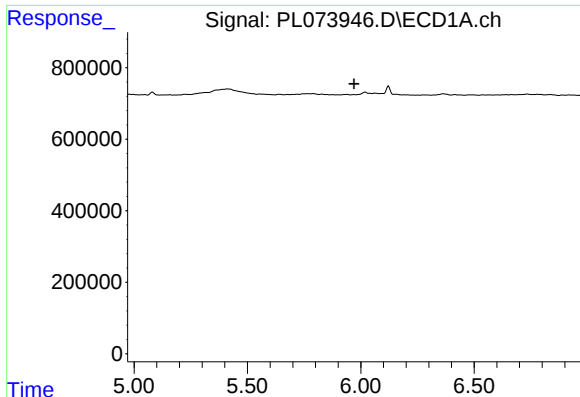

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

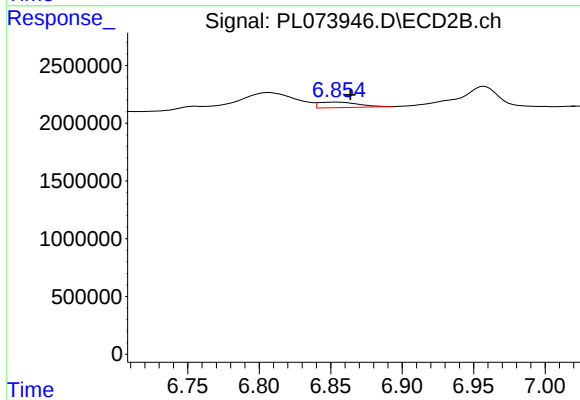


#23 Chlordane-1

R.T.: 6.855 min
Delta R.T.: -0.009 min
Response: 922454
Conc: 11.56 ng/ml

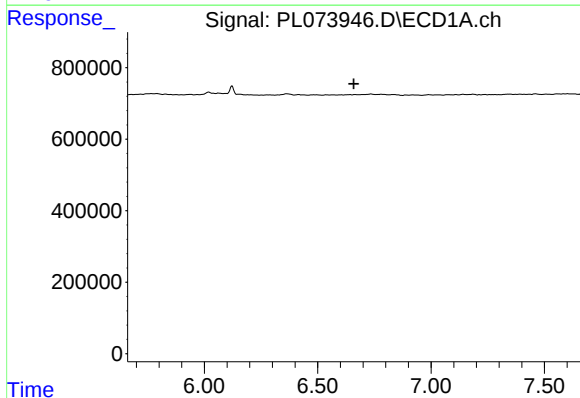


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 6.659 min
Response: 0
Conc: N.D.

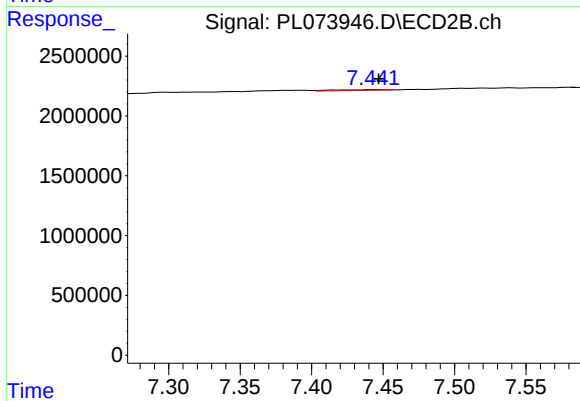

#24 Chlordane-2


R.T.: 7.442 min
Delta R.T.: -0.005 min
Response: 154607
Conc: 1.87 ng/ml

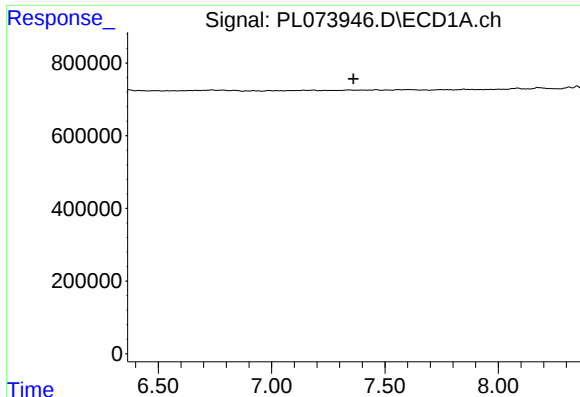

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

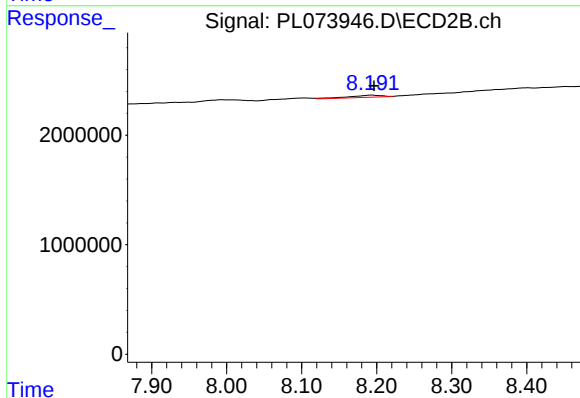


#25 Chlordane-3

R.T.: 8.193 min
Delta R.T.: -0.004 min
Response: 559488
Conc: 1.65 ng/ml

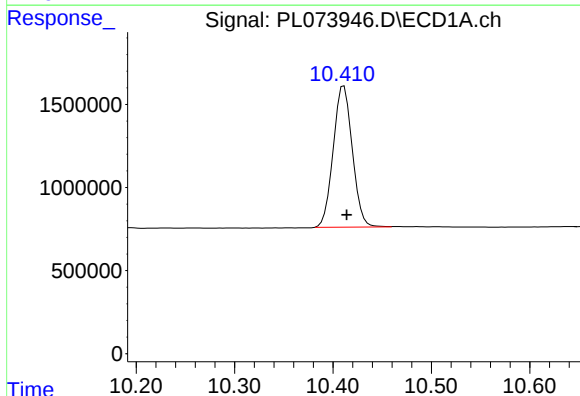

#28 Decachlorobiphenyl

R.T.: 10.411 min
Delta R.T.: -0.003 min
Response: 11452187
Conc: 22.02 ng/ml

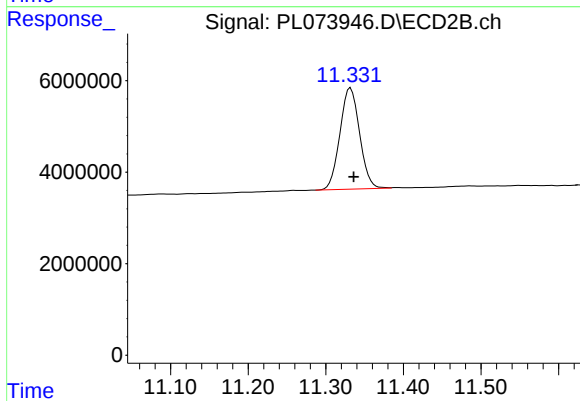

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: -0.004 min
Response: 39005636
Conc: 22.08 ng/ml