

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041122\
 Data File : PL073964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2022 22:34
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 02:12:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 08 15:48:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.638	5.490	7344099	39428915	22.729	22.114
28)	SA Decachlor...	10.411	11.333	10921601	34792674	21.002	19.698
Target Compounds							
6)	B beta-BHC	0.000	6.677	0	770975	N.D.	0.684 #
7)	B delta-BHC	0.000	6.959	0	3156319	N.D.	1.292 #
9)	A Endosulfan I	7.470f	8.325	13840	172425	0.034	0.088 #
10)	B gamma-Chl...	7.339f	8.200	27062	899583	0.062	0.403 #
14)	MA Endrin	8.087f	0.000	93570	0	0.230	N.D. #
15)	B Endosulfa...	8.347f	9.054f	75019	633124	0.182	0.364 #
16)	A 4,4'-DDD	0.000	9.004	0	605408	N.D.	0.393 #
17)	MA 4,4'-DDT	0.000	9.329f	0	330896	N.D.	0.187 #
18)	B Endrin al...	0.000	9.207	0	69836	N.D.	0.054 #
20)	A Methoxychlor	9.073	0.000	75201	0	0.303	N.D. #
23)	Chlordane-1	0.000	6.855	0	808792	N.D.	10.135 #
25)	Chlordane-3	7.339f	8.200	27062	899583	0.626	2.659 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041122\
Data File : PL073964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2022 22:34
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 02:12:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Fri Apr 08 15:48:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

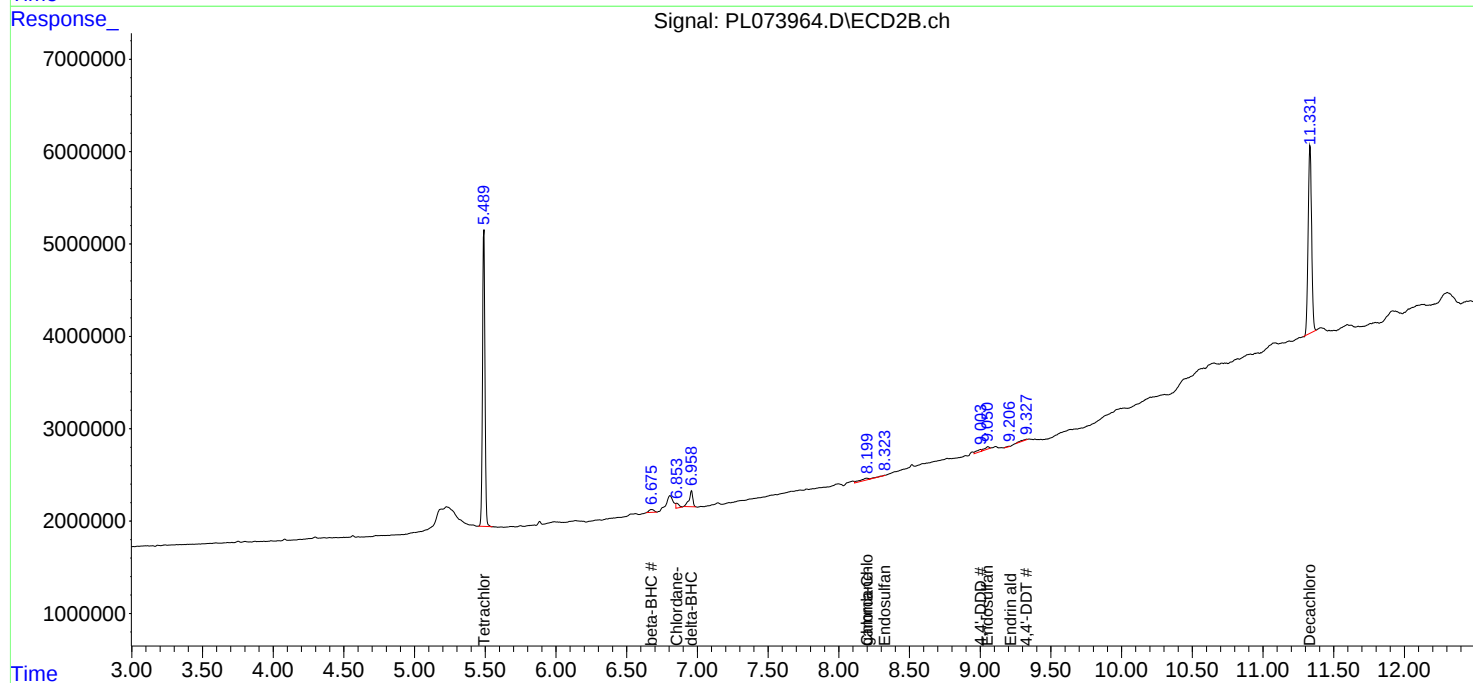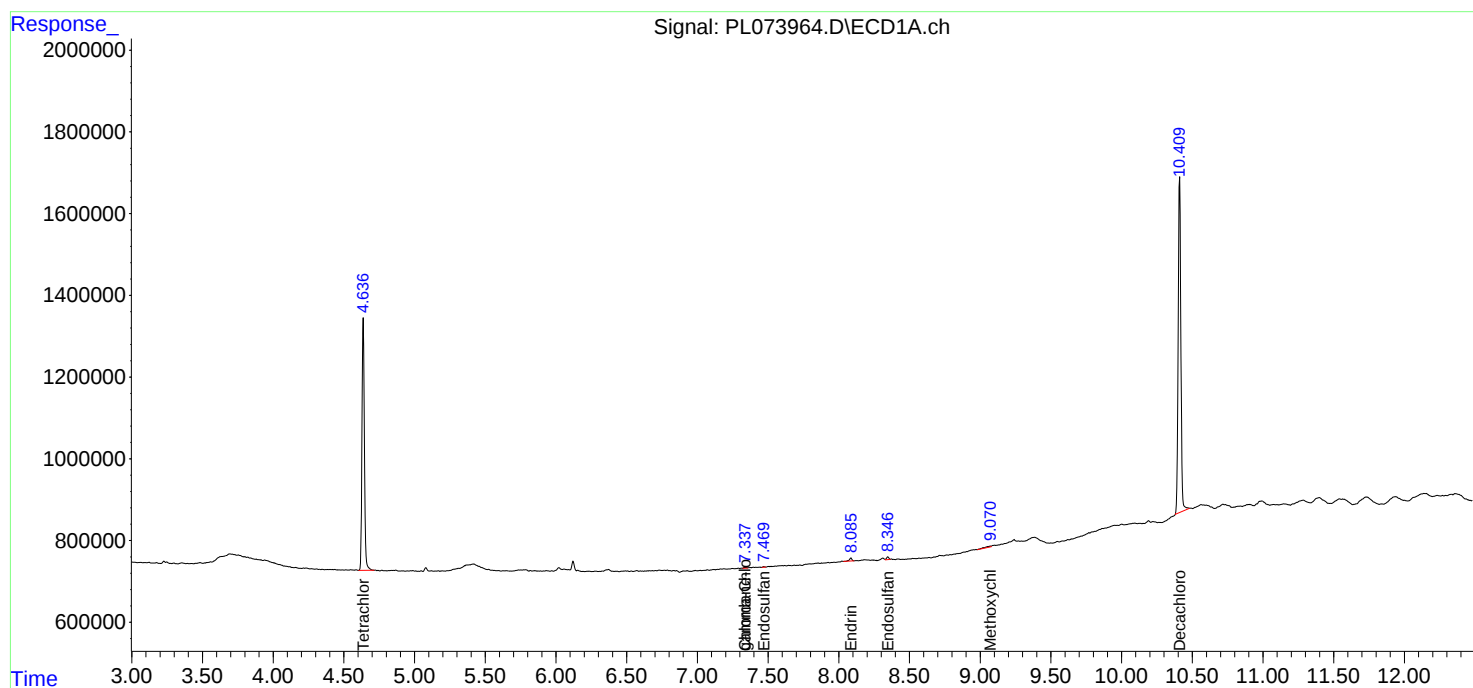


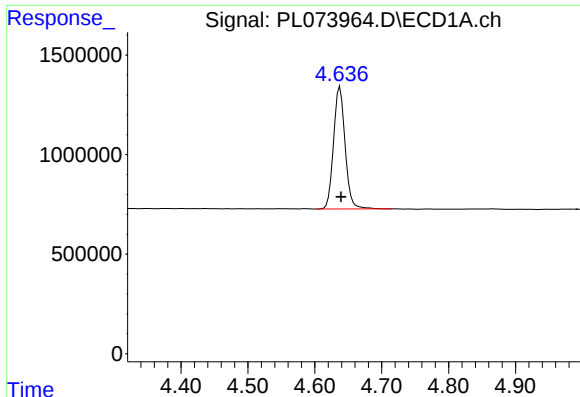

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: -0.001 min
Response: 7344099
Conc: 22.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

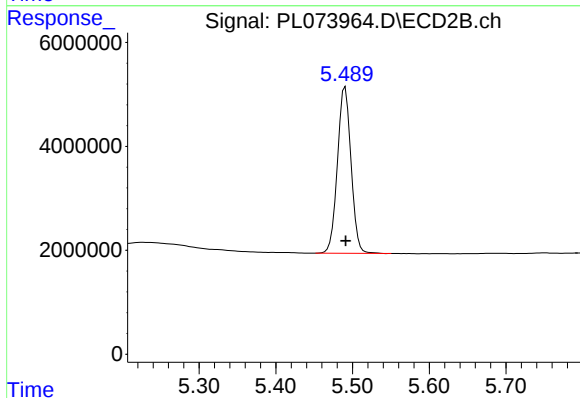


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.001 min
Response: 39428915
Conc: 22.11 ng/ml

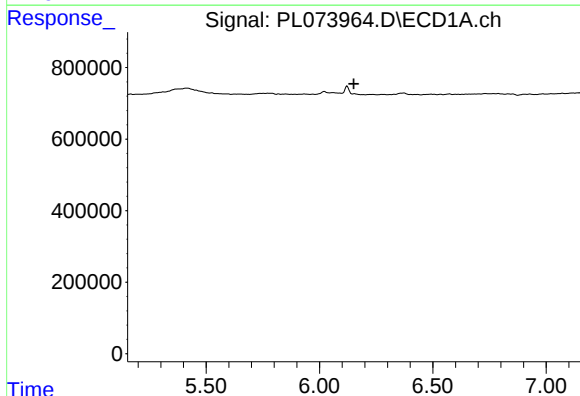


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.151 min
Response: 0
Conc: N.D.

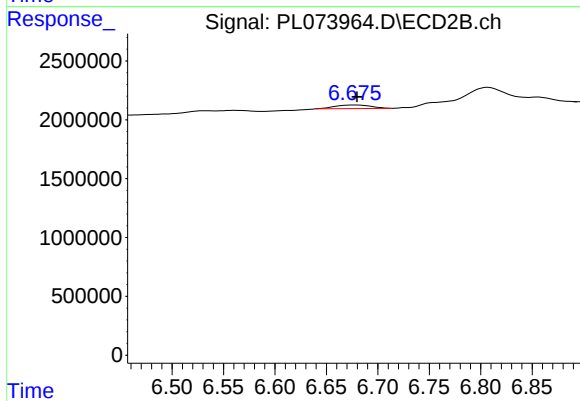

#6 beta-BHC


R.T.: 6.677 min
Delta R.T.: -0.003 min
Response: 770975
Conc: 0.68 ng/ml

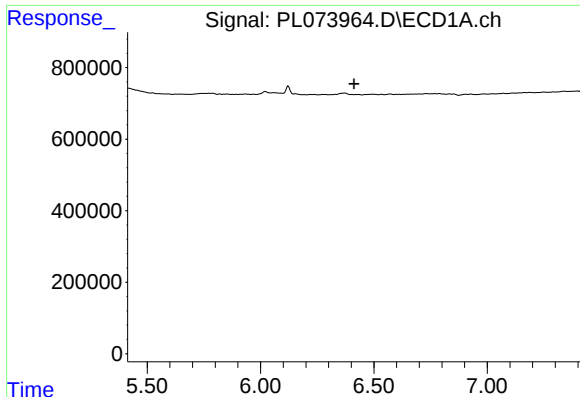

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

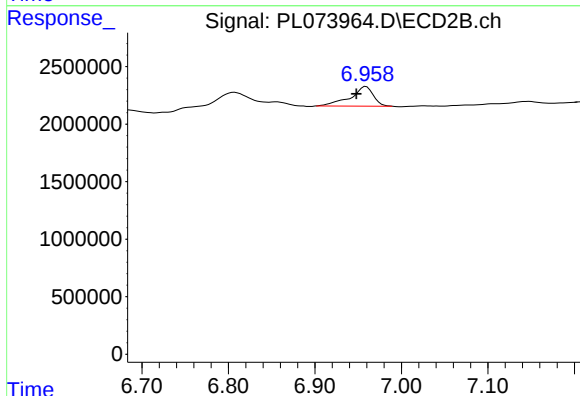


#7 delta-BHC

R.T.: 6.959 min
Delta R.T.: 0.011 min
Response: 3156319
Conc: 1.29 ng/ml

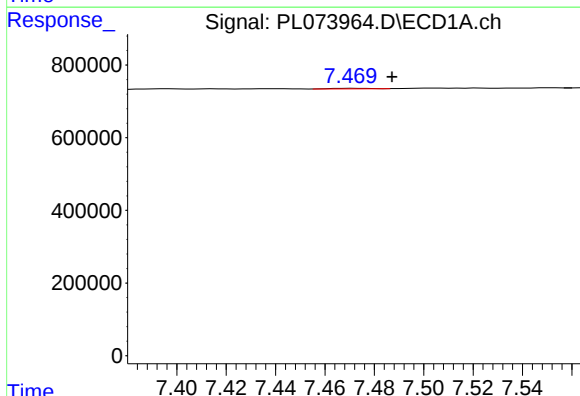


#9 Endosulfan I

R.T.: 7.470 min
Delta R.T.: -0.017 min
Response: 13840
Conc: 0.03 ng/ml

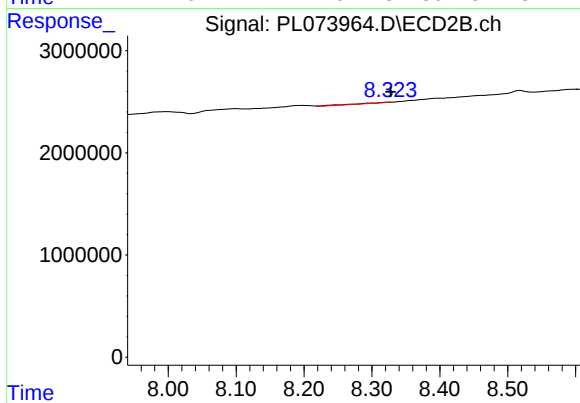

#9 Endosulfan I


R.T.: 8.325 min
Delta R.T.: -0.003 min
Response: 172425
Conc: 0.09 ng/ml

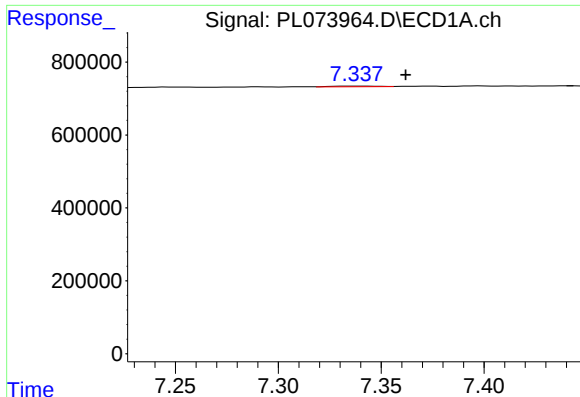

#10 gamma-Chlordane


R.T.: 7.339 min
Delta R.T.: -0.023 min
Response: 27062
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

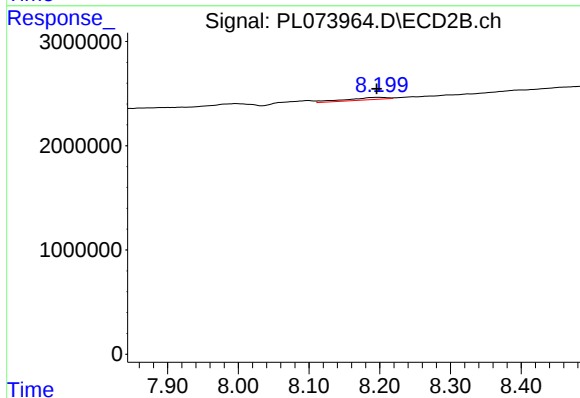


#10 gamma-Chlordane

R.T.: 8.200 min
Delta R.T.: 0.005 min
Response: 899583
Conc: 0.40 ng/ml

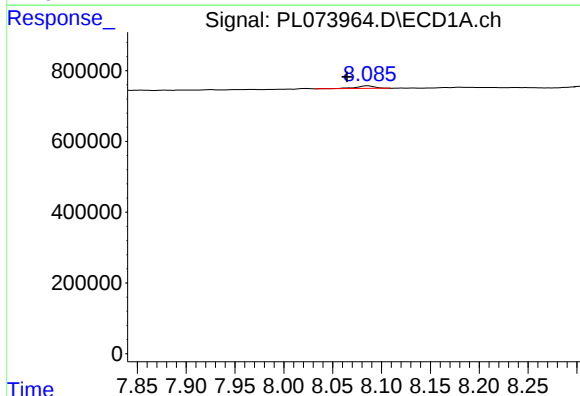


#14 Endrin

R.T.: 8.087 min
Delta R.T.: 0.022 min
Response: 93570
Conc: 0.23 ng/ml

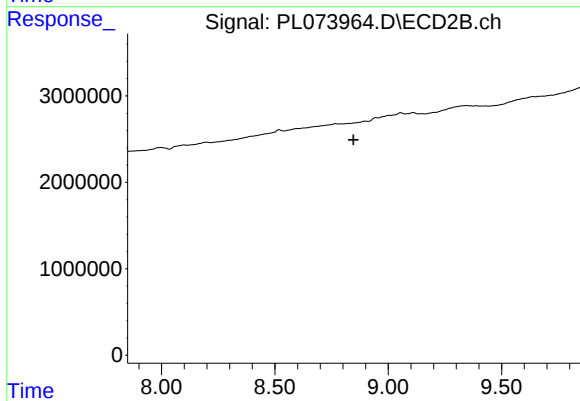

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.847 min
Response: 0
Conc: N.D.

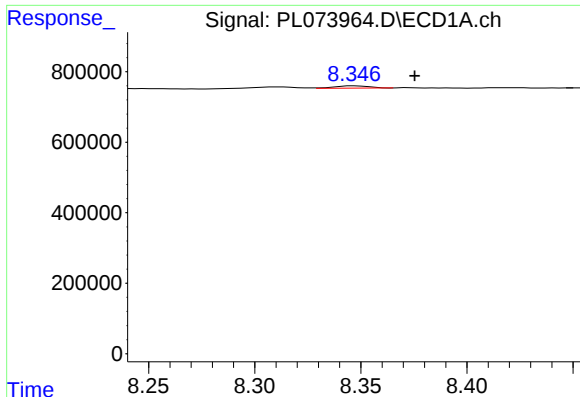

#15 Endosulfan II


R.T.: 8.347 min
Delta R.T.: -0.028 min
Response: 75019
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

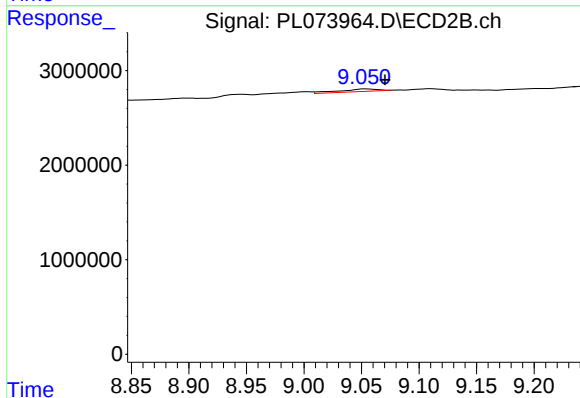


#15 Endosulfan II

R.T.: 9.054 min
Delta R.T.: -0.016 min
Response: 633124
Conc: 0.36 ng/ml

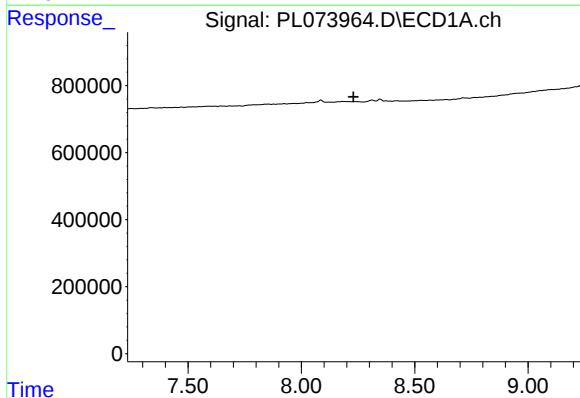


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.231 min
Response: 0
Conc: N.D.

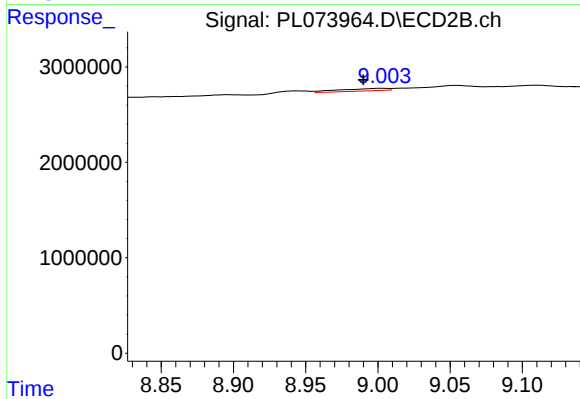

#16 4,4'-DDD

R.T.: 9.004 min
Delta R.T.: 0.014 min
Response: 605408
Conc: 0.39 ng/ml

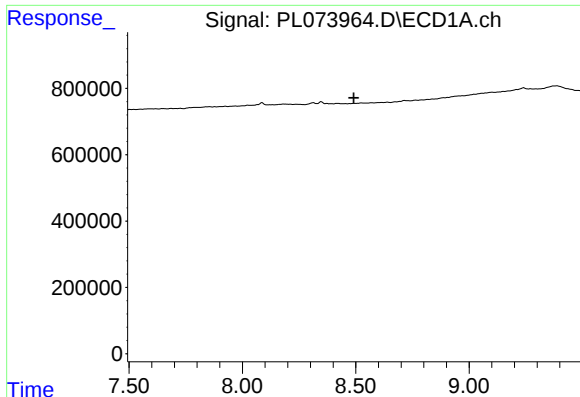

#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#17 4,4'-DDT


R.T.: 9.329 min
Delta R.T.: 0.021 min
Response: 330896
Conc: 0.19 ng/ml

#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

#18 Endrin aldehyde


R.T.: 9.207 min
Delta R.T.: 0.003 min
Response: 69836
Conc: 0.05 ng/ml

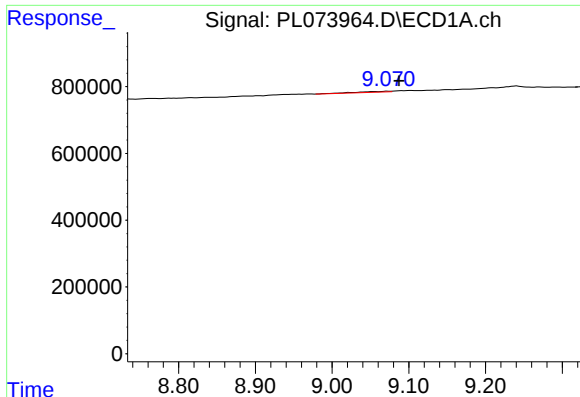

#20 Methoxychlor


R.T.: 9.073 min
Delta R.T.: -0.015 min
Response: 75201
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

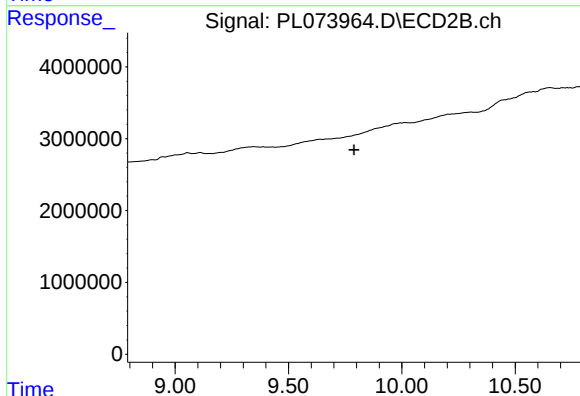


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.789 min
Response: 0
Conc: N.D.

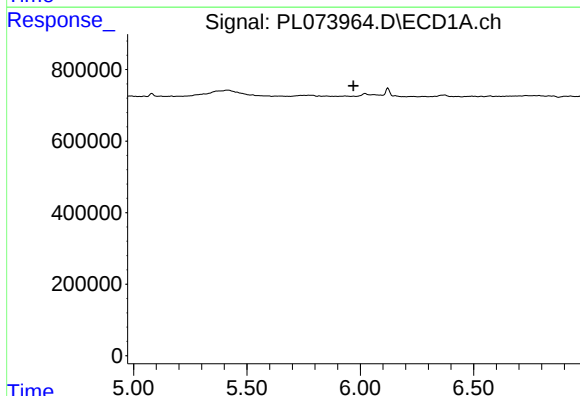


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.970 min
Response: 0
Conc: N.D.

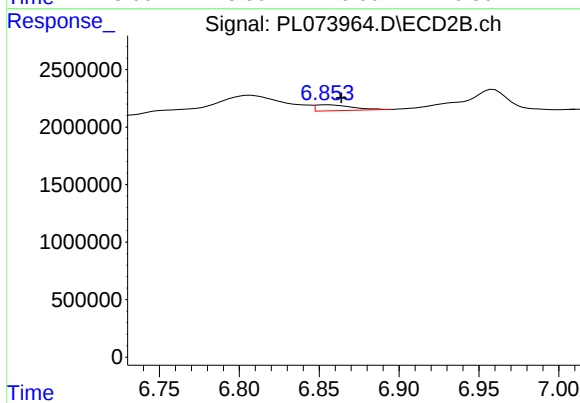

#23 Chlordane-1


R.T.: 6.855 min
Delta R.T.: -0.009 min
Response: 808792
Conc: 10.14 ng/ml

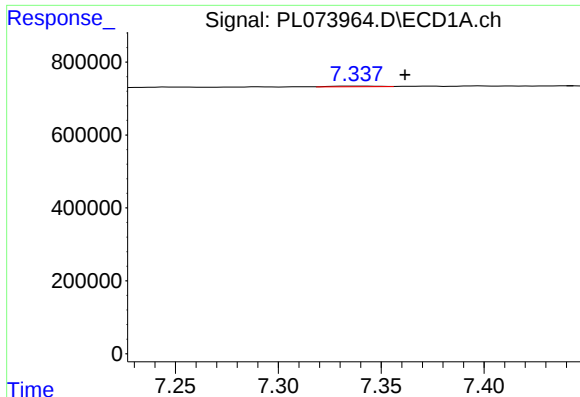

#25 Chlordane-3


R.T.: 7.339 min
Delta R.T.: -0.023 min
Response: 27062
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

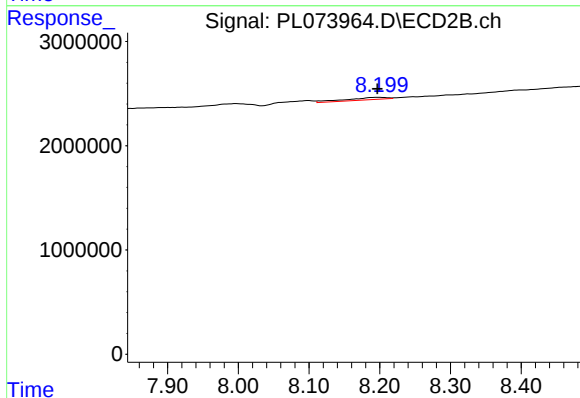


#25 Chlordane-3

R.T.: 8.200 min
Delta R.T.: 0.004 min
Response: 899583
Conc: 2.66 ng/ml

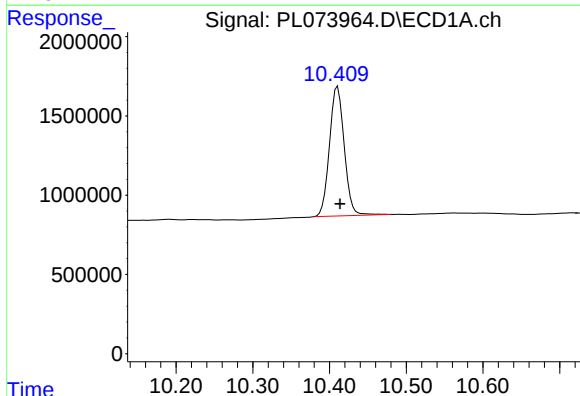

#28 Decachlorobiphenyl

R.T.: 10.411 min
Delta R.T.: -0.003 min
Response: 10921601
Conc: 21.00 ng/ml

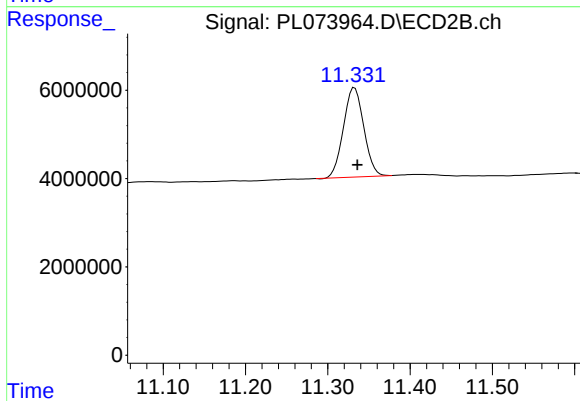

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: -0.003 min
Response: 34792674
Conc: 19.70 ng/ml