

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041123\
 Data File : PL081998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2023 17:33
 Operator : AR\AJ
 Sample : 02269-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-20424

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 22:21:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 23 01:07:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.327	2.656	14826756	20880871	6.375	10.461 #
28) SA Decachlor...	8.746	7.768	43910174	46204767	24.536	23.298
Target Compounds						
10) B gamma-Chl...	5.703	4.842	127.0E6	127.5E6	48.380	52.471
11) B alpha-Chl...	5.782	4.904	181.8E6	151.0E6	70.230	62.163



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041123\
Data File : PL081998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2023 17:33
Operator : AR\AJ
Sample : 02269-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CHRT-20424

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 22:21:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 23 01:07:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

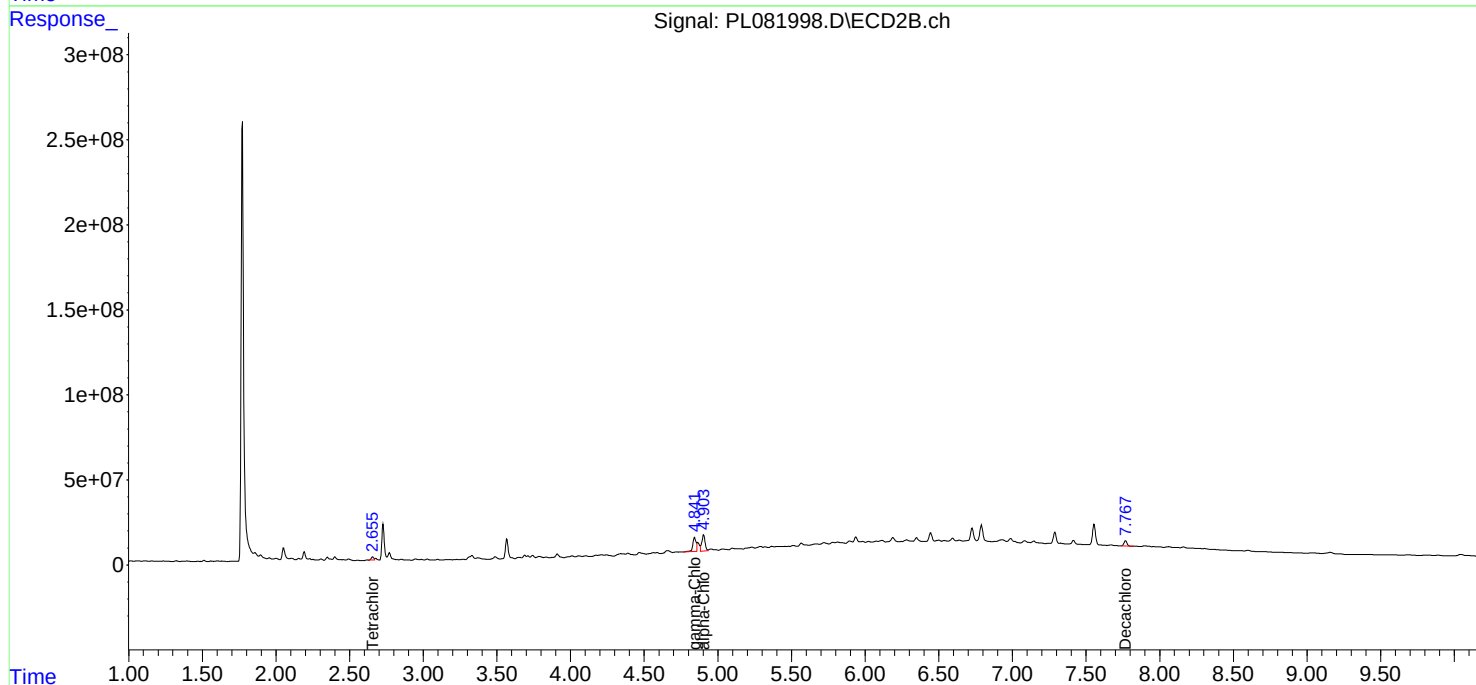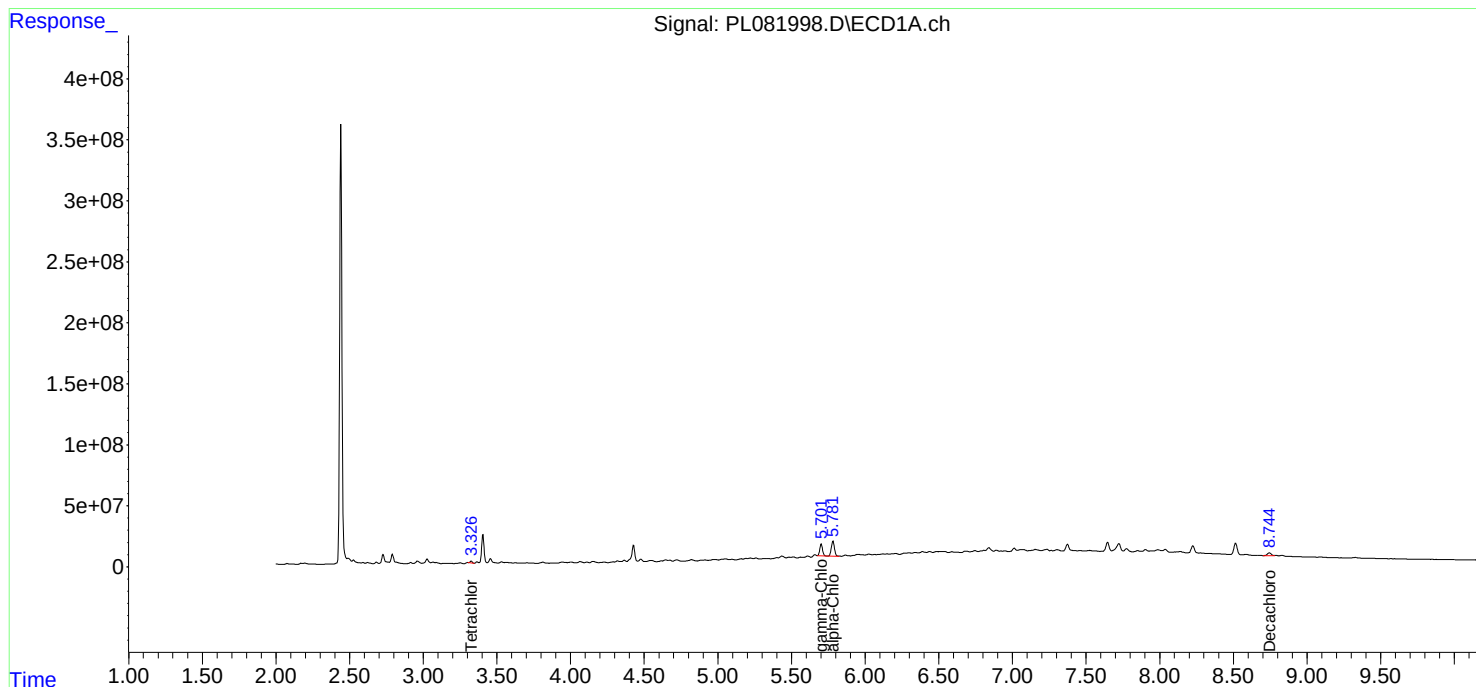


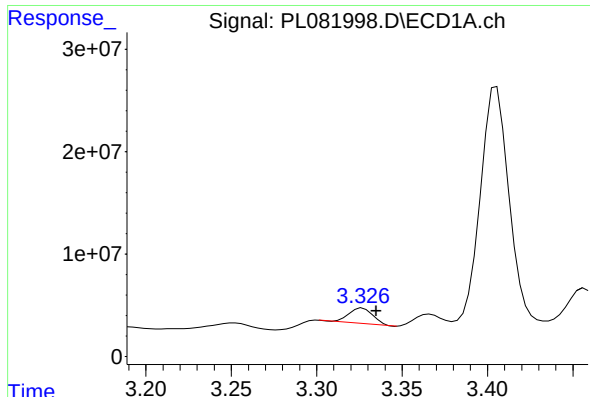

#1 Tetrachloro-m-xylene


R.T.: 3.327 min
Delta R.T.: -0.008 min
Response: 14826756
Conc: 6.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-20424

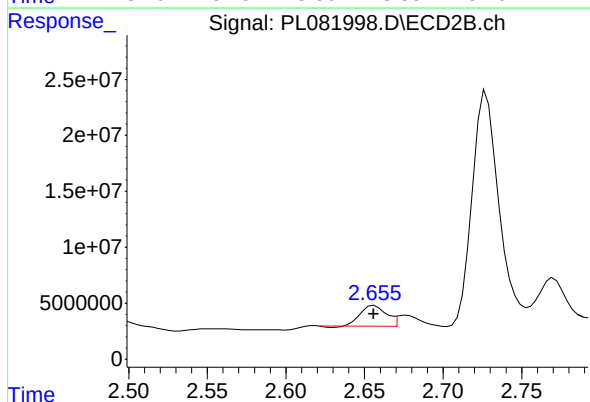


#1 Tetrachloro-m-xylene

R.T.: 2.656 min
Delta R.T.: 0.000 min
Response: 20880871
Conc: 10.46 ng/ml

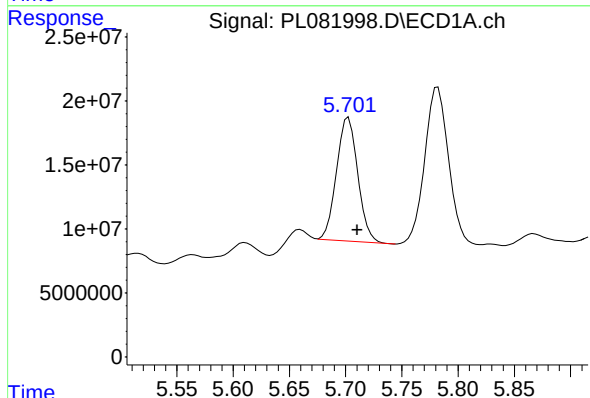


#10 gamma-Chlordane

R.T.: 5.703 min
Delta R.T.: -0.008 min
Response: 127009421
Conc: 48.38 ng/ml

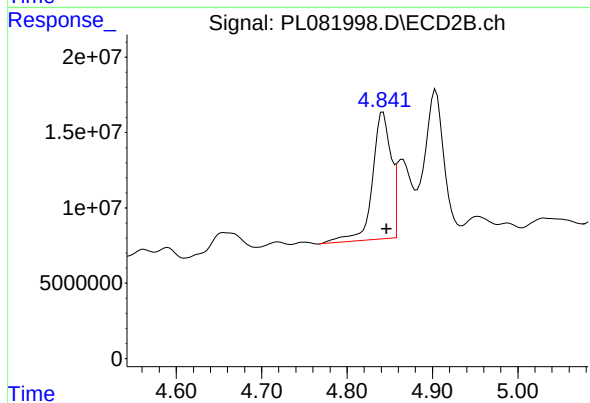

#10 gamma-Chlordane


R.T.: 4.842 min
Delta R.T.: -0.004 min
Response: 127524824
Conc: 52.47 ng/ml

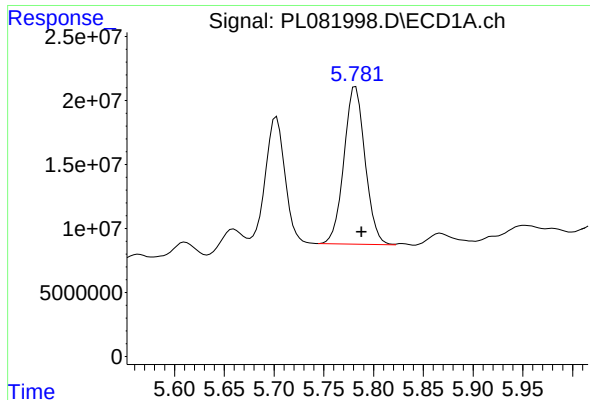

#11 alpha-Chlordane


R.T.: 5.782 min
Delta R.T.: -0.006 min
Response: 181785111
Conc: 70.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-20424

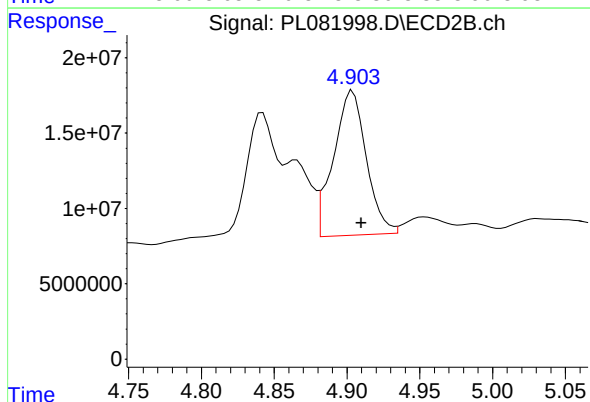


#11 alpha-Chlordane

R.T.: 4.904 min
Delta R.T.: -0.006 min
Response: 150990384
Conc: 62.16 ng/ml

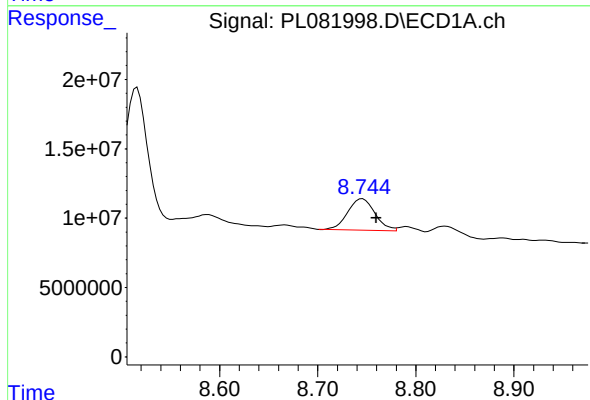

#28 Decachlorobiphenyl

R.T.: 8.746 min
Delta R.T.: -0.014 min
Response: 43910174
Conc: 24.54 ng/ml

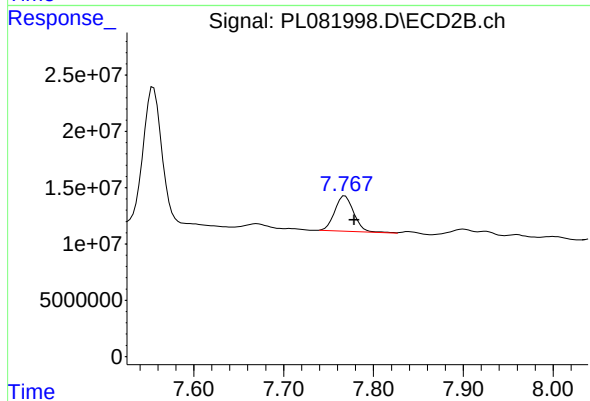

#28 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: -0.010 min
Response: 46204767
Conc: 23.30 ng/ml