

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041219\
 Data File : PL047327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2019 15:57
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 23:26:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.356	3.975	148.1E6	46428252	20.355	20.278
28) SA Decachlor...	8.032	9.027	191.7E6	54923048	22.796	23.689
Target Compounds						
2) A alpha-BHC	3.790	0.000	10055818	0	0.862	N.D. #
8) B Heptachlo...	0.000	5.839	0	1898281	N.D.	0.720 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041219\
Data File : PL047327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2019 15:57
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 23:26:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

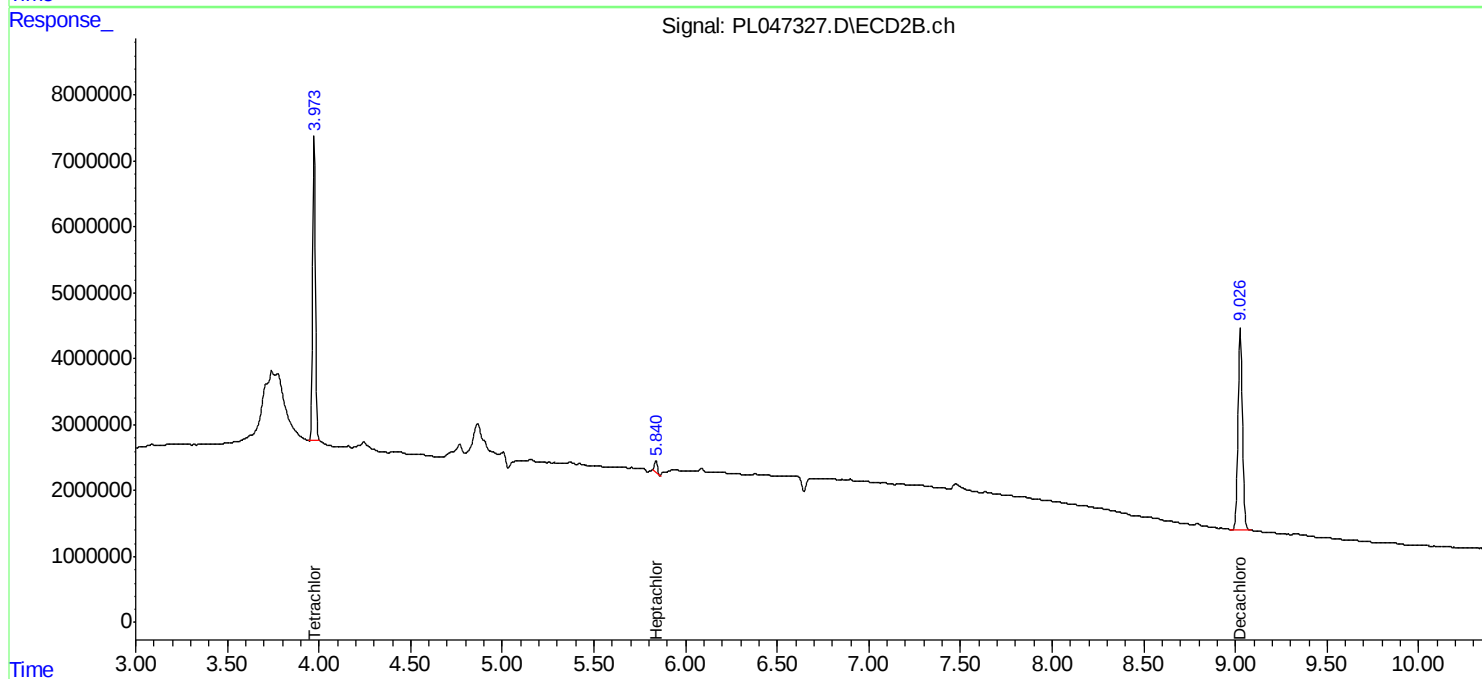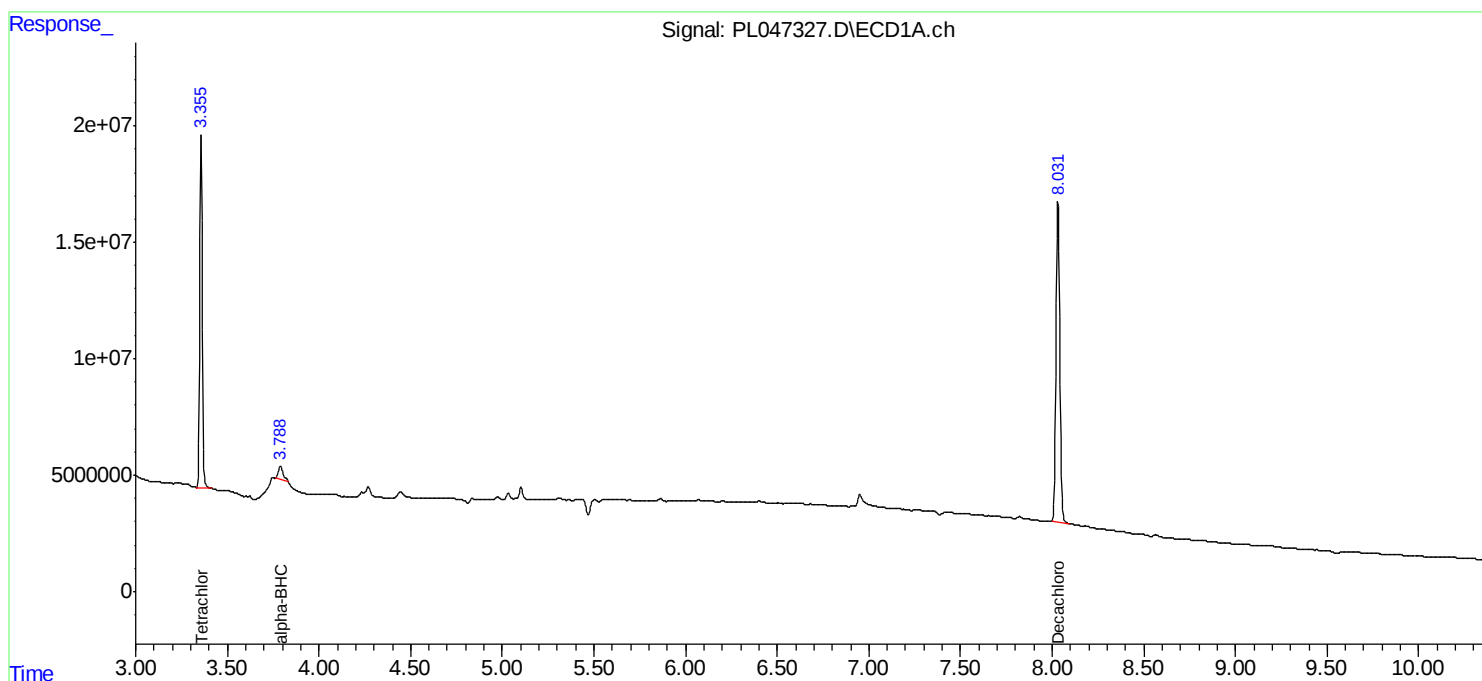


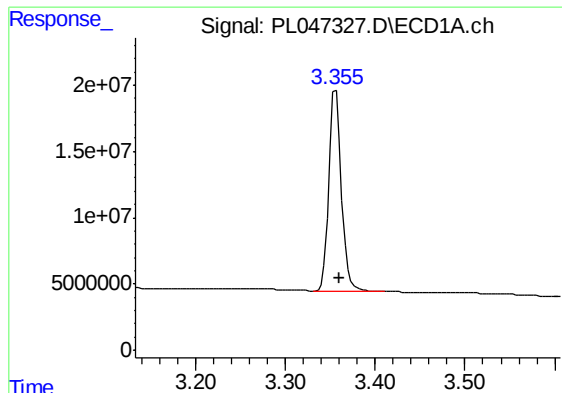

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 148076575
Conc: 20.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

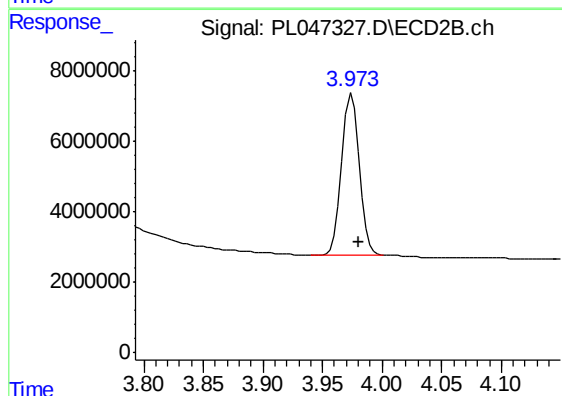


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.006 min
Response: 46428252
Conc: 20.28 ng/ml

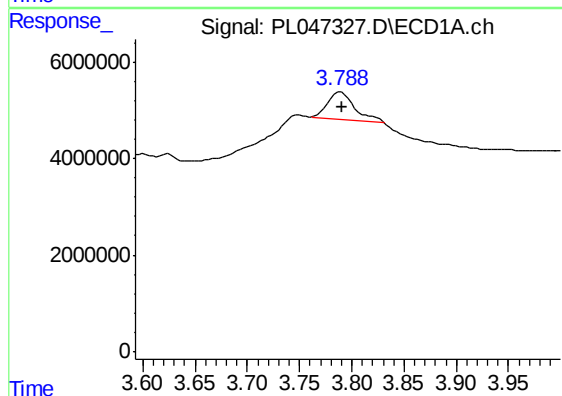


#2 alpha-BHC

R.T.: 3.790 min
Delta R.T.: 0.000 min
Response: 10055818
Conc: 0.86 ng/ml

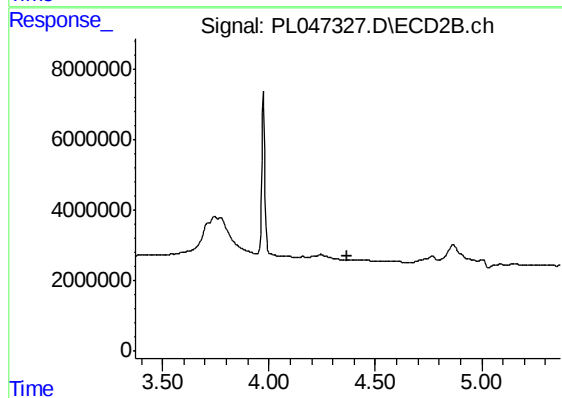

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

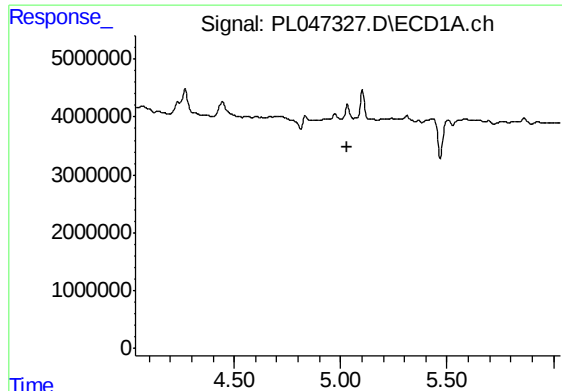

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.034 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

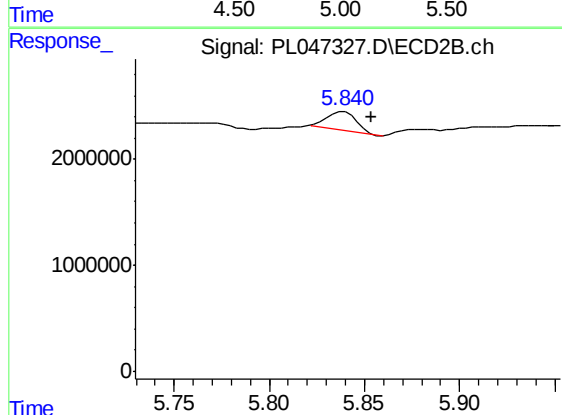


#8 Heptachlor epoxide

R.T.: 5.839 min
Delta R.T.: -0.014 min
Response: 1898281
Conc: 0.72 ng/ml

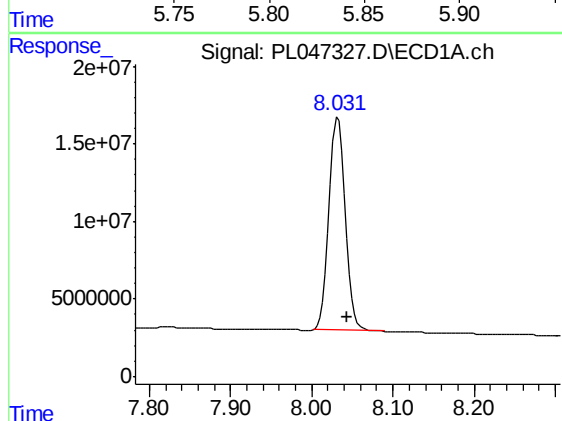

#28 Decachlorobiphenyl

R.T.: 8.032 min
Delta R.T.: -0.012 min
Response: 191734220
Conc: 22.80 ng/ml

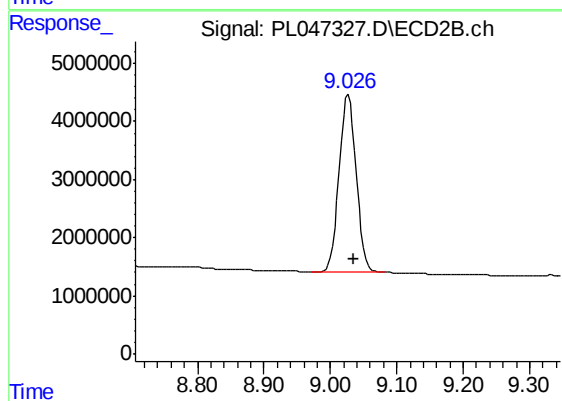

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.008 min
Response: 54923048
Conc: 23.69 ng/ml