

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041219\
 Data File : PL047338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2019 18:37
 Operator : AJ\SJ
 Sample : K2358-16
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-7-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 23:29:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.356	3.975	155.4E6	48925245	21.364	21.368
28) SA Decachlor...	8.030	9.025	195.8E6	57775714	23.276	24.920
Target Compounds						
2) A alpha-BHC	3.789	0.000	14063858	0	1.206	N.D. #
6) B beta-BHC	0.000	4.826	0	239550	N.D.	0.181 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041219\
Data File : PL047338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2019 18:37
Operator : AJ\SJ
Sample : K2358-16
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-7-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 23:29:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

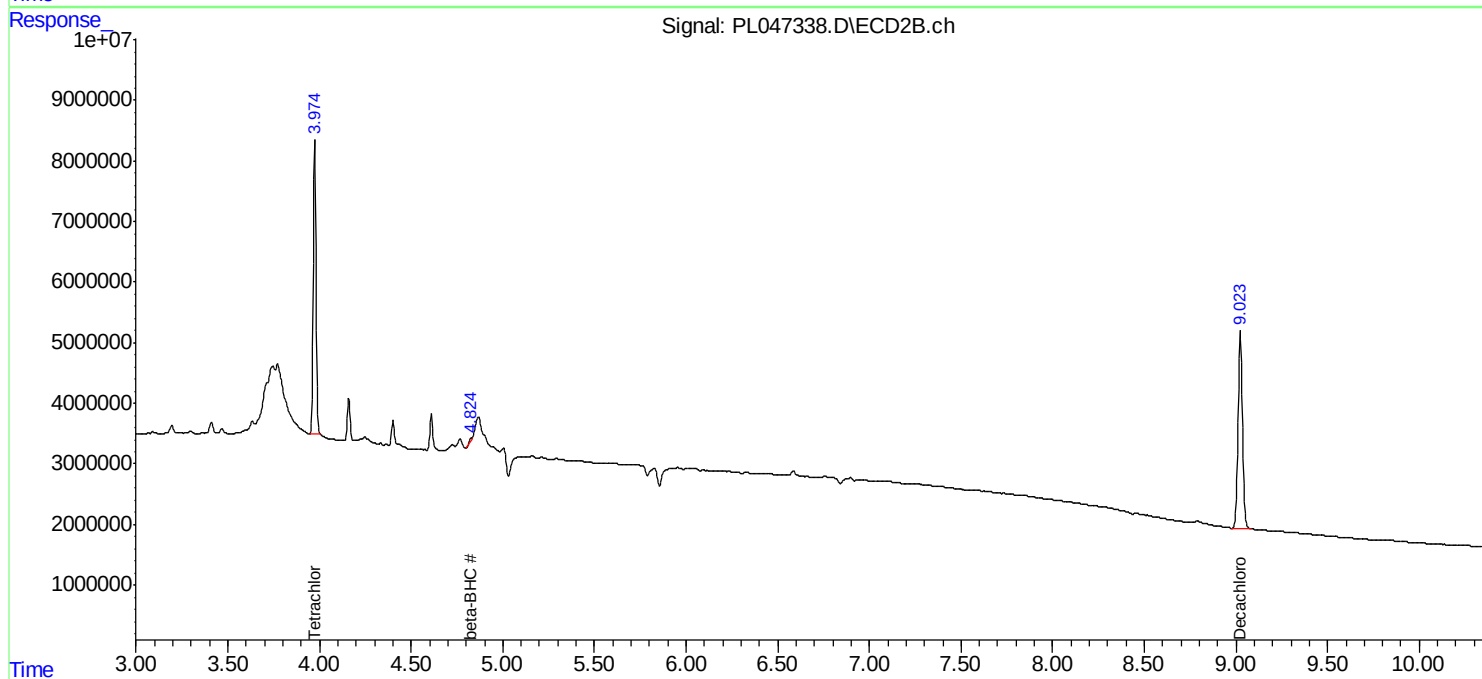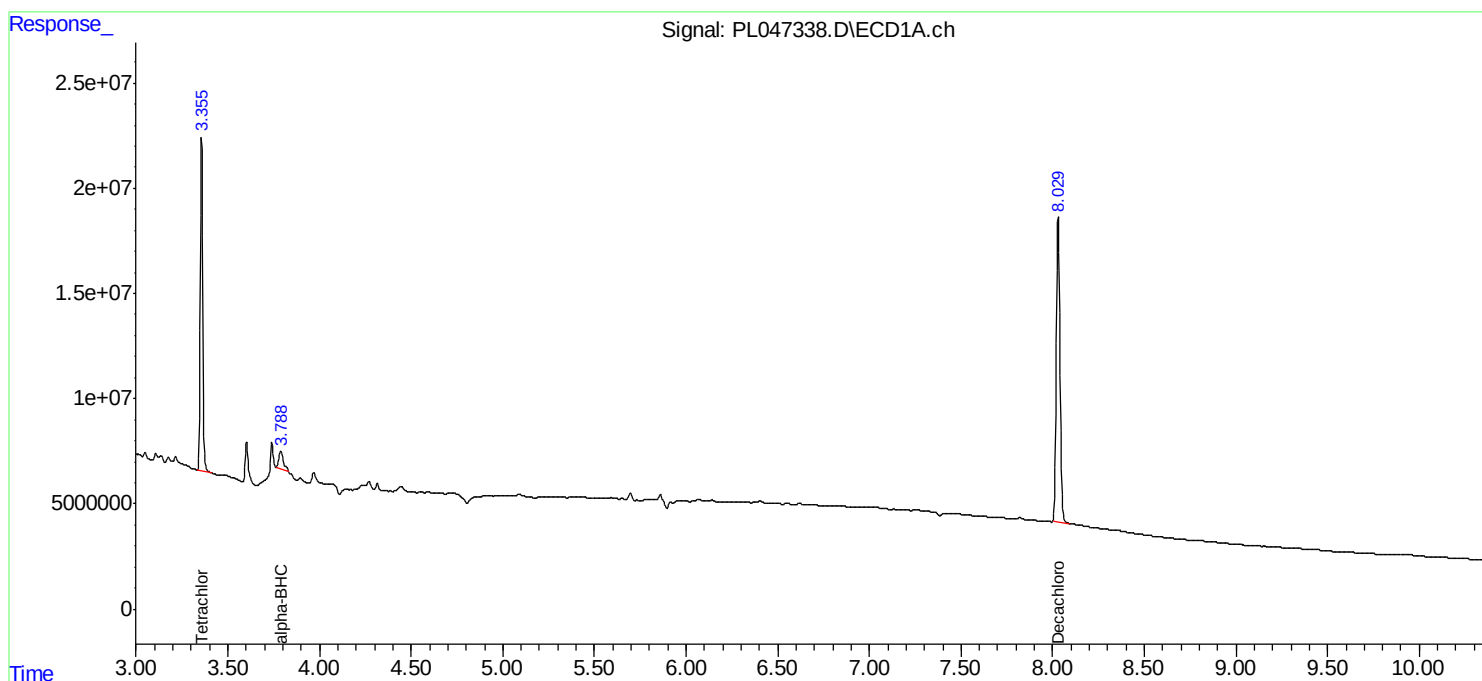


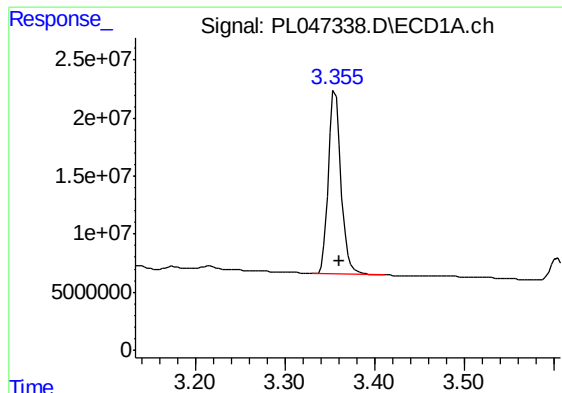

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 155418896
Conc: 21.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-D

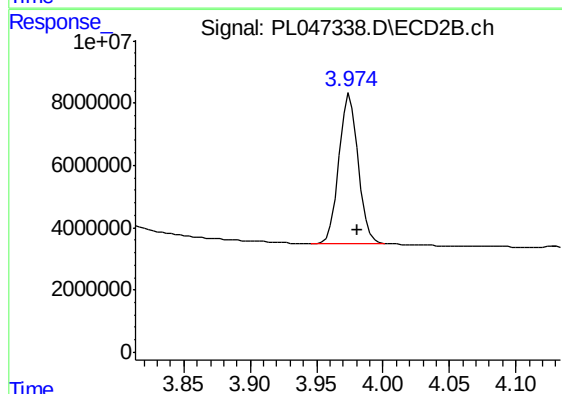


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.006 min
Response: 48925245
Conc: 21.37 ng/ml

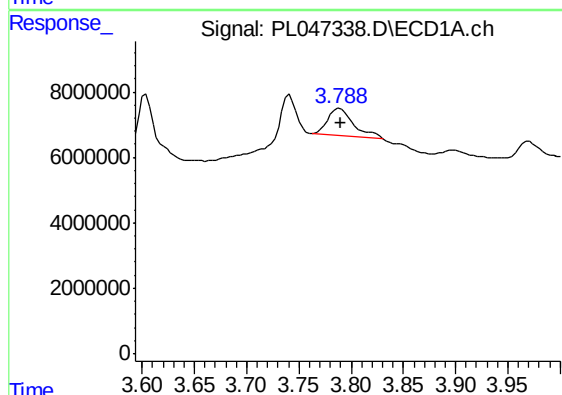


#2 alpha-BHC

R.T.: 3.789 min
Delta R.T.: -0.002 min
Response: 14063858
Conc: 1.21 ng/ml

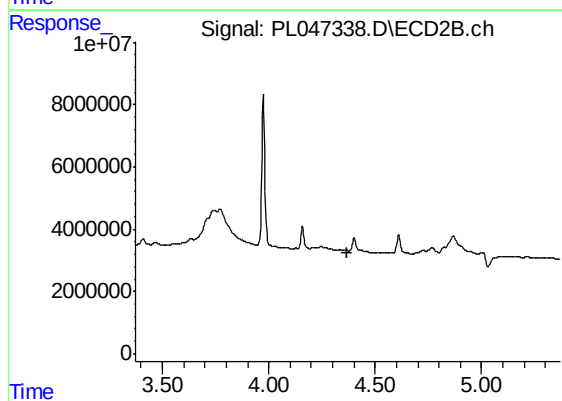

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

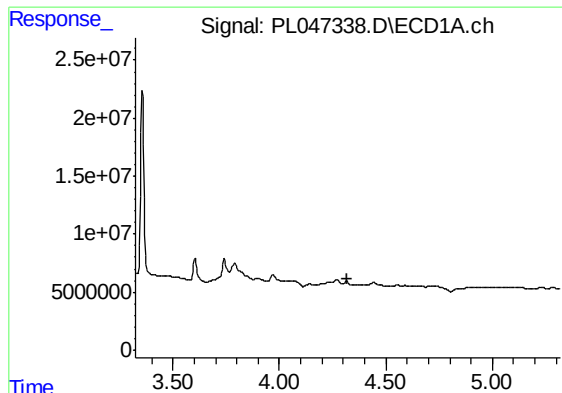

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.321 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-7-D

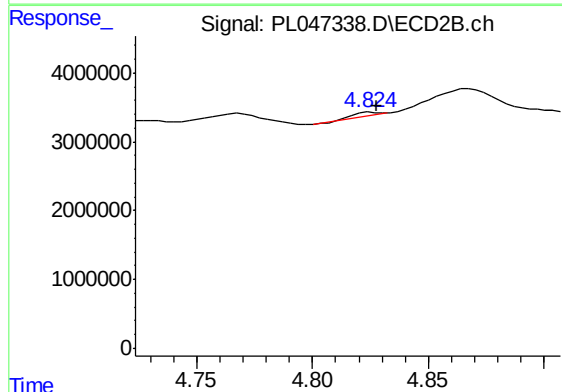


#6 beta-BHC

R.T.: 4.826 min
Delta R.T.: -0.002 min
Response: 239550
Conc: 0.18 ng/ml

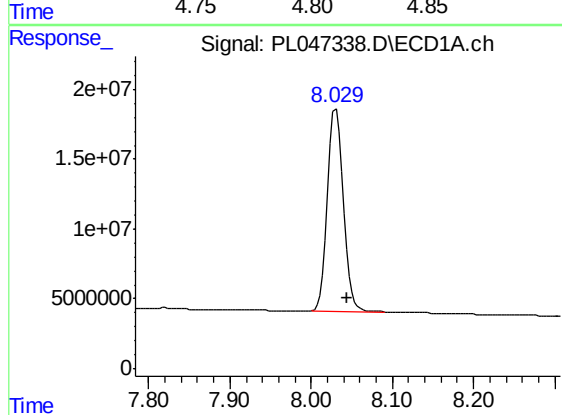

#28 Decachlorobiphenyl

R.T.: 8.030 min
Delta R.T.: -0.014 min
Response: 195777073
Conc: 23.28 ng/ml

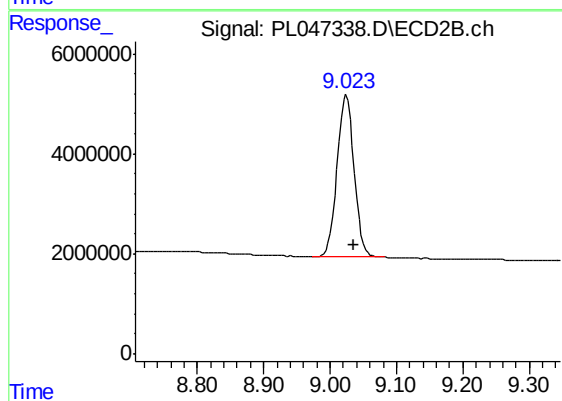

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: -0.010 min
Response: 57775714
Conc: 24.92 ng/ml