

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041219\
 Data File : PL047343.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2019 19:49
 Operator : AJ\SJ
 Sample : K2376-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 23:30:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.357	3.975	139.9E6	43886779	19.235	19.168
28) SA Decachlor...	8.031	9.025	164.9E6	47615979	19.602	20.538
Target Compounds						
2) A alpha-BHC	3.786	4.364	25609944	2435669	2.196	0.758 #
6) B beta-BHC	4.316	4.822	96387657	26929646	21.408	20.314



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041219\
Data File : PL047343.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2019 19:49
Operator : AJ\SJ
Sample : K2376-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-4-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 23:30:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

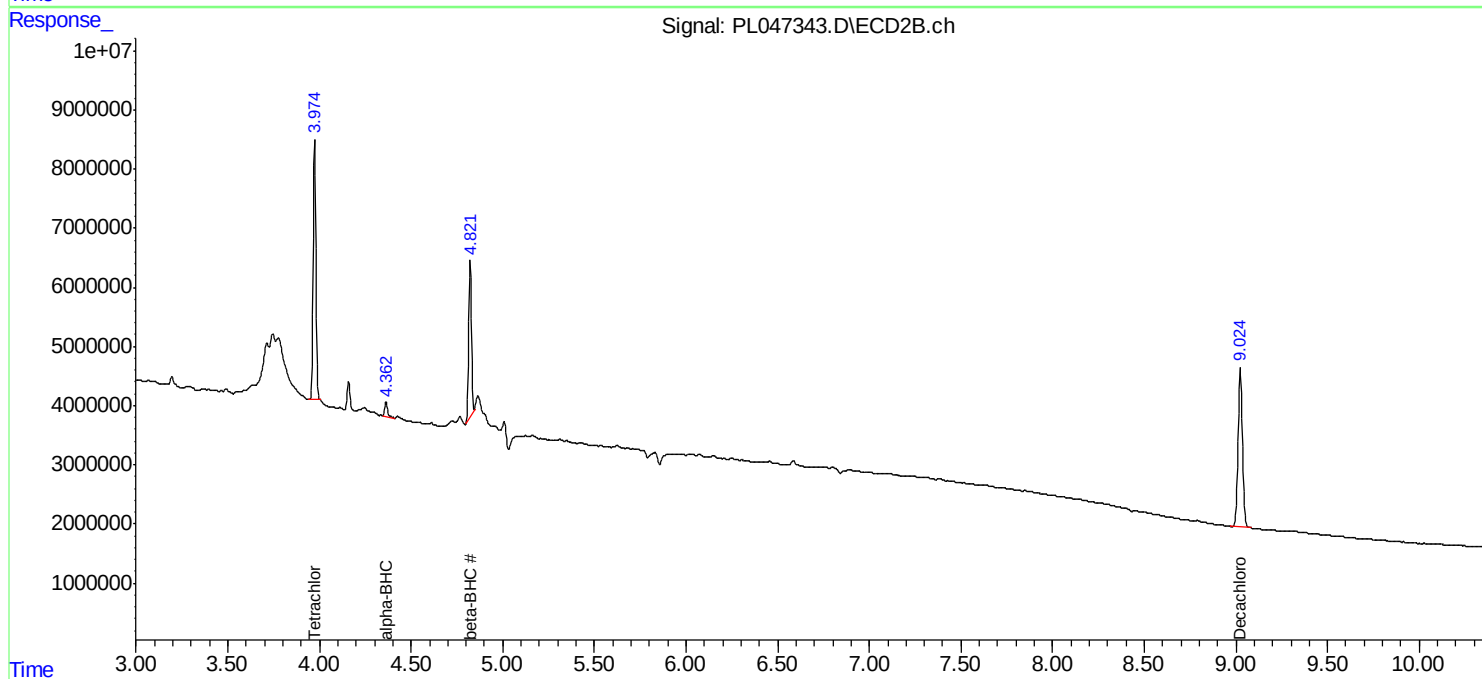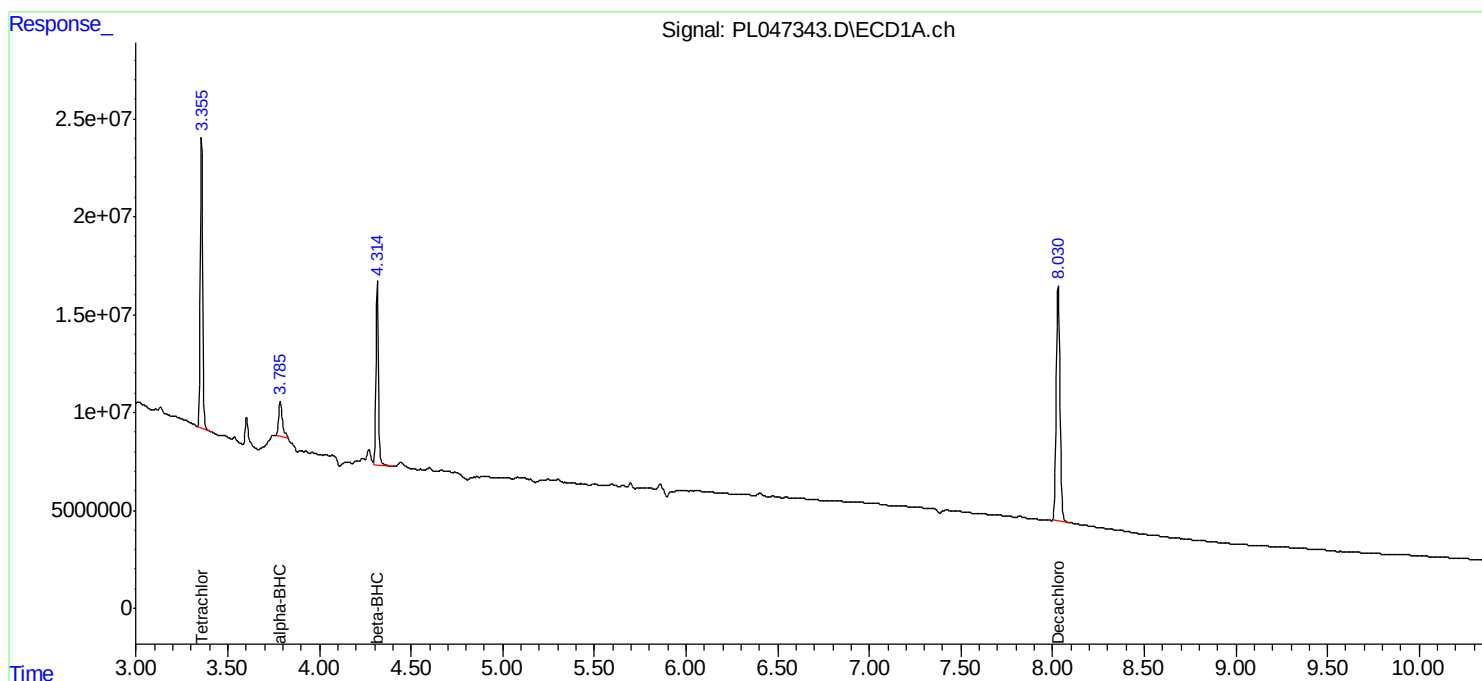


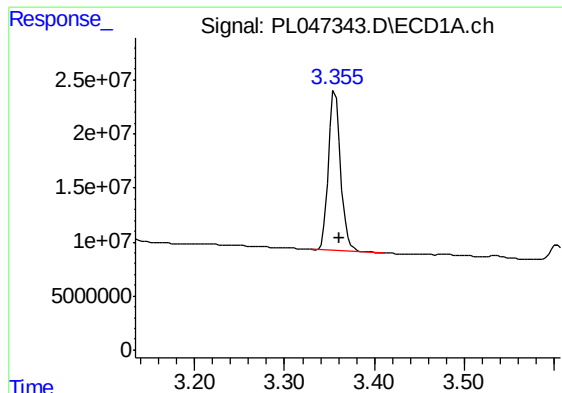

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: -0.004 min
Response: 139928352
Conc: 19.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-S

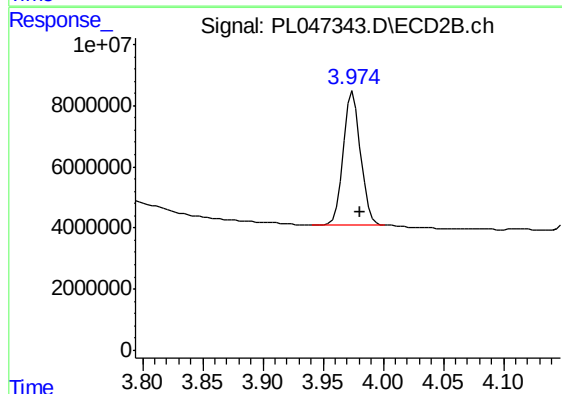


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.006 min
Response: 43886779
Conc: 19.17 ng/ml

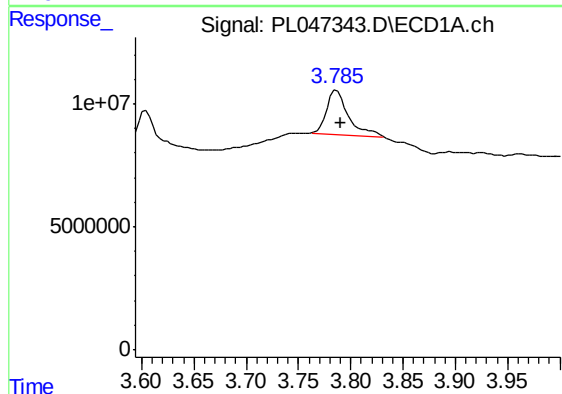


#2 alpha-BHC

R.T.: 3.786 min
Delta R.T.: -0.004 min
Response: 25609944
Conc: 2.20 ng/ml

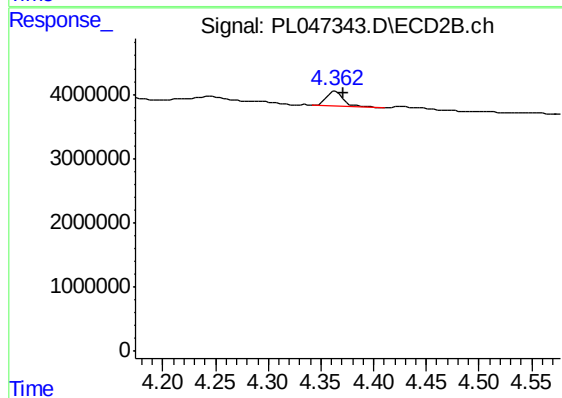

#2 alpha-BHC


R.T.: 4.364 min
Delta R.T.: -0.007 min
Response: 2435669
Conc: 0.76 ng/ml

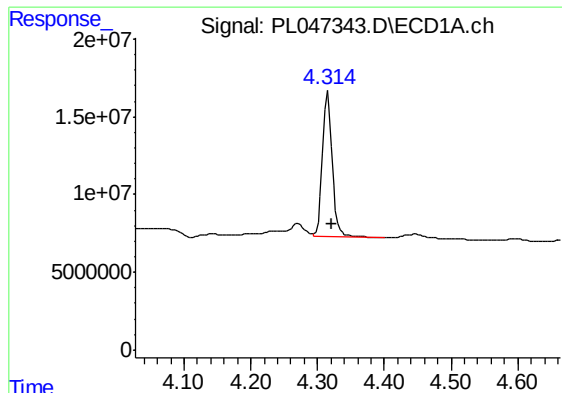

#6 beta-BHC


R.T.: 4.316 min
Delta R.T.: -0.005 min
Response: 96387657
Conc: 21.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-S

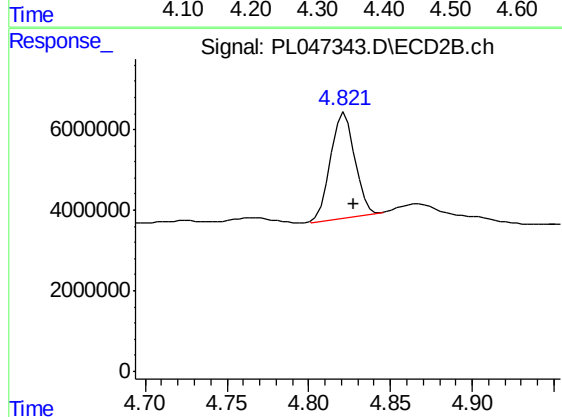


#6 beta-BHC

R.T.: 4.822 min
Delta R.T.: -0.006 min
Response: 26929646
Conc: 20.31 ng/ml

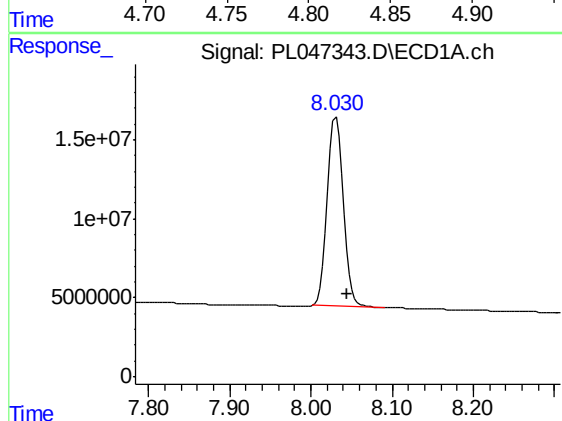

#28 Decachlorobiphenyl

R.T.: 8.031 min
Delta R.T.: -0.013 min
Response: 164874965
Conc: 19.60 ng/ml

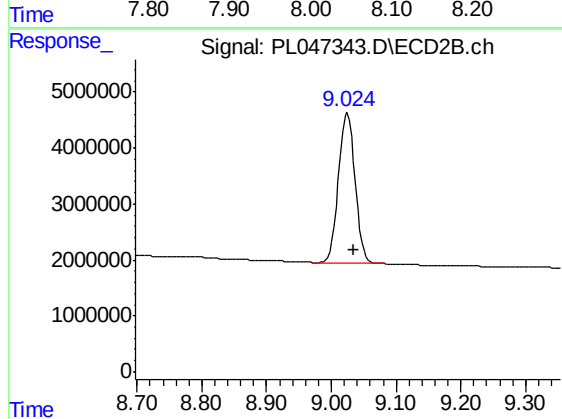

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: -0.010 min
Response: 47615979
Conc: 20.54 ng/ml