

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041219\
 Data File : PL047344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2019 20:04
 Operator : AJ\SJ
 Sample : K2377-04
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-13-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 23:31:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.356	3.974	145.0E6	46083197	19.931	20.127
28)	SA Decachlor...	8.030	9.024	144.3E6	42123411	17.150	18.169
Target Compounds							
2)	A alpha-BHC	3.790	0.000	13868600	0	1.189	N.D. #
23)	Chlordane-1	4.232f	0.000	18560589	0	55.191	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041219\
Data File : PL047344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2019 20:04
Operator : AJ\SJ
Sample : K2377-04
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-13-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 23:31:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

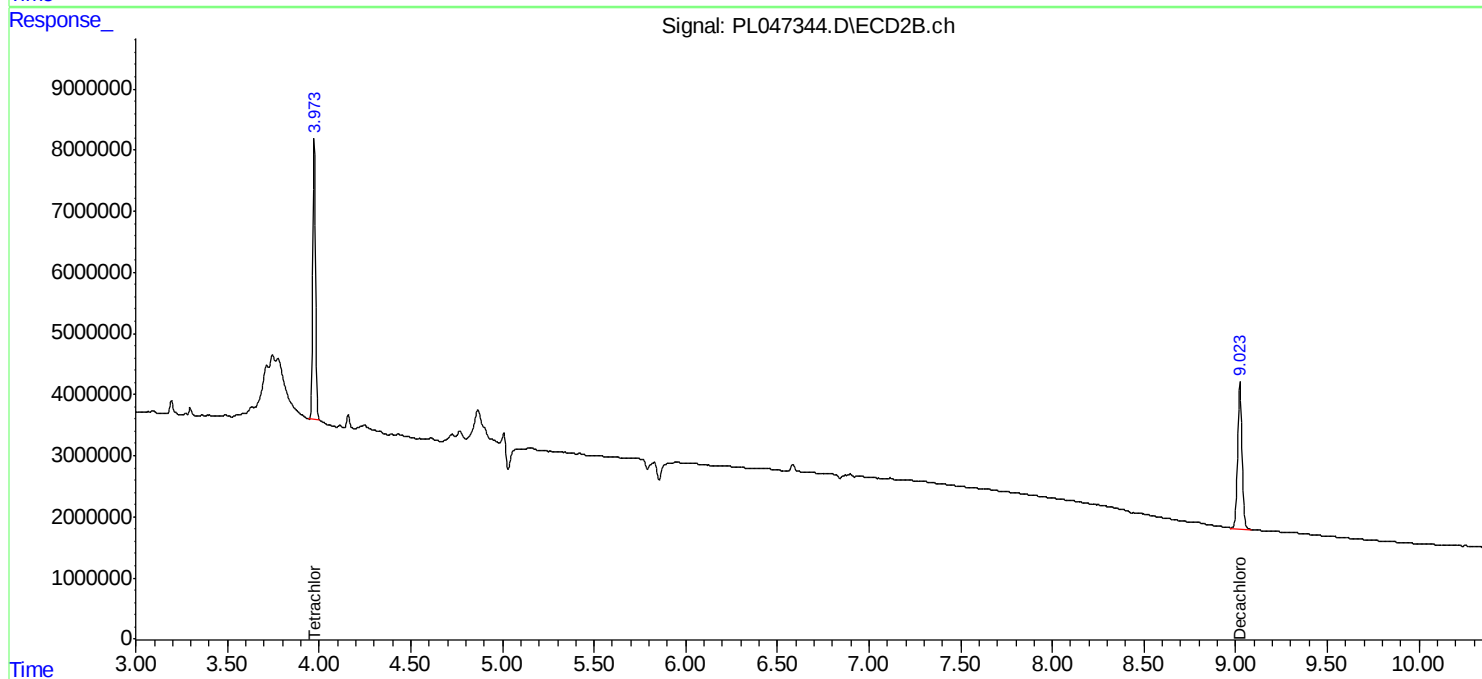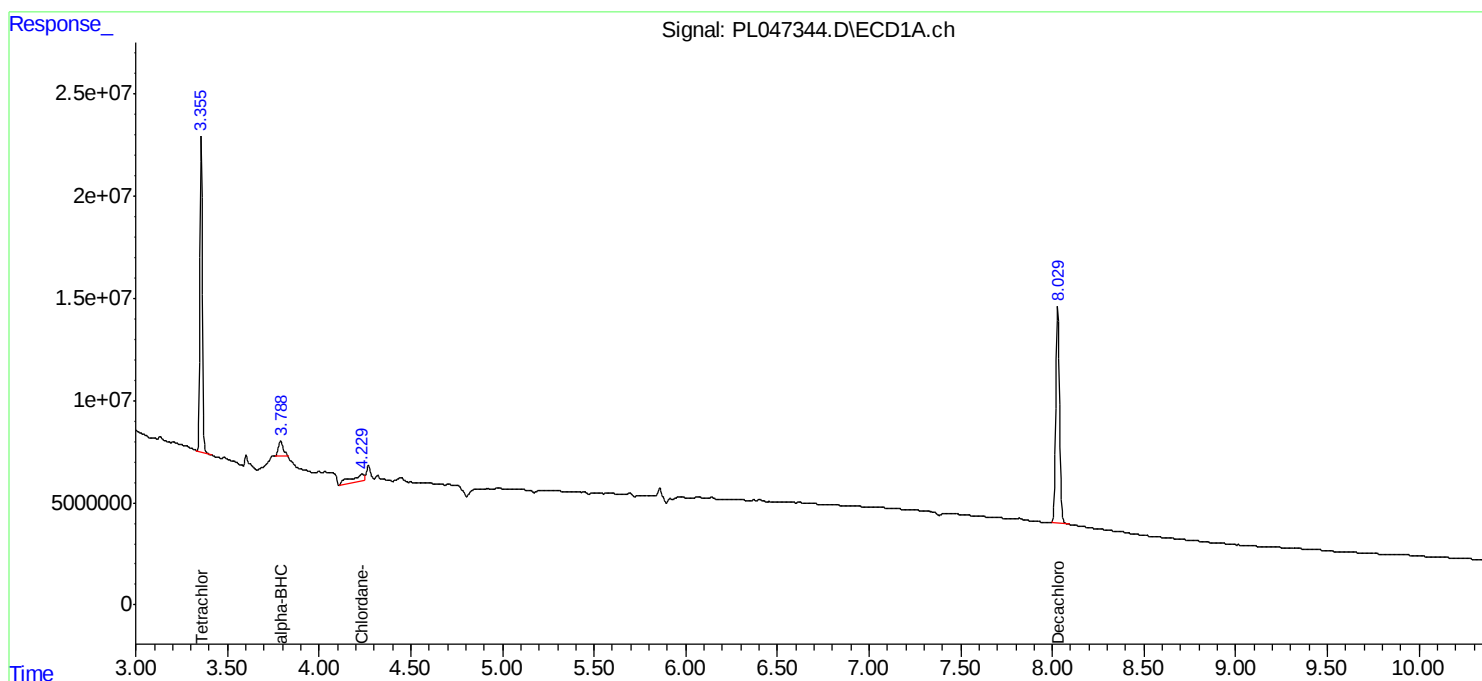


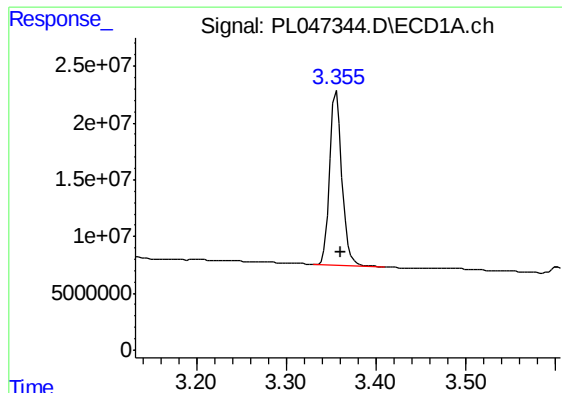

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 144993258
Conc: 19.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13-S

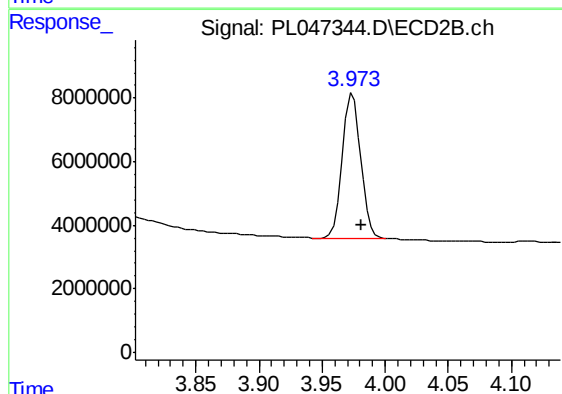


#1 Tetrachloro-m-xylene

R.T.: 3.974 min
Delta R.T.: -0.006 min
Response: 46083197
Conc: 20.13 ng/ml

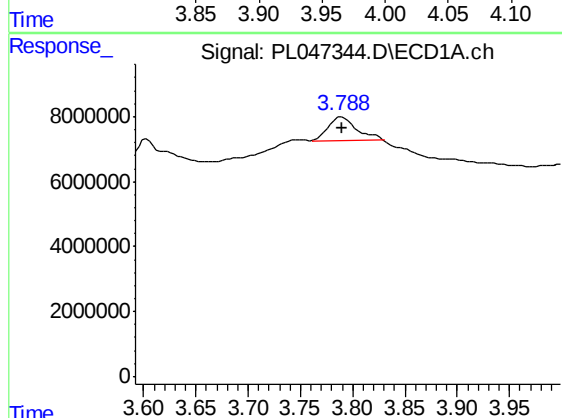


#2 alpha-BHC

R.T.: 3.790 min
Delta R.T.: 0.000 min
Response: 13868600
Conc: 1.19 ng/ml

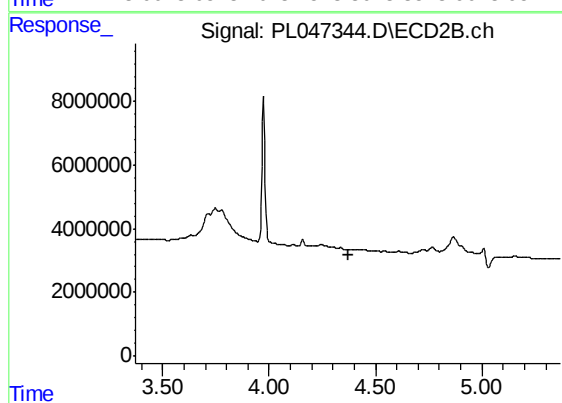

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

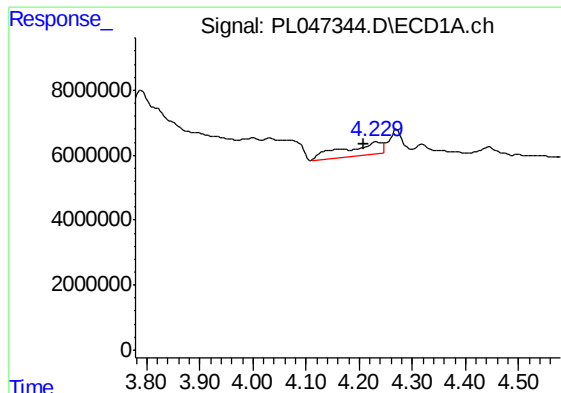

#23 Chlordane-1


R.T.: 4.232 min
Delta R.T.: 0.024 min
Response: 18560589
Conc: 55.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13-S

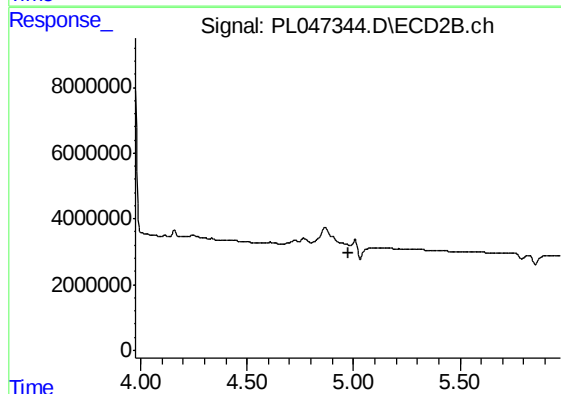


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

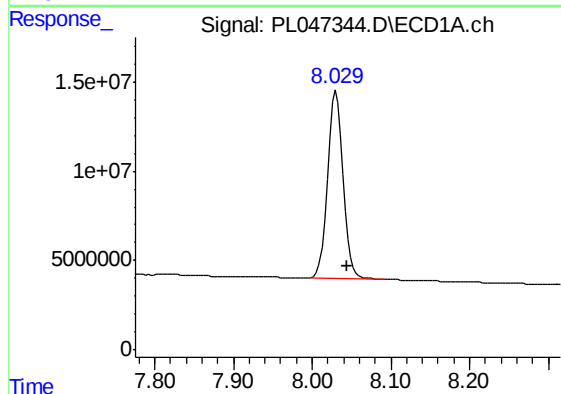

#28 Decachlorobiphenyl

R.T.: 8.030 min
Delta R.T.: -0.014 min
Response: 144252177
Conc: 17.15 ng/ml

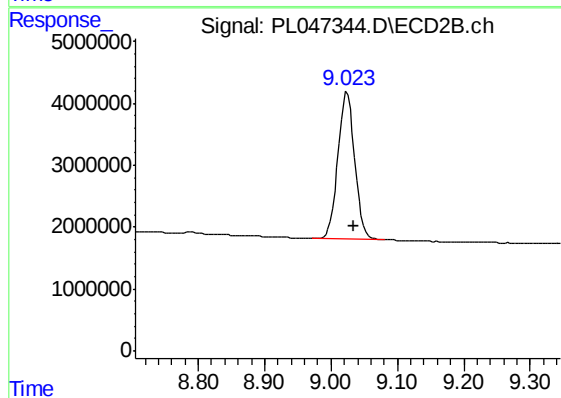

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: -0.011 min
Response: 42123411
Conc: 18.17 ng/ml