

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041219\
 Data File : PL047361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2019 00:09
 Operator : AJ\SJ
 Sample : K2196-03 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-02-041119

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 05:42:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.356	3.974	9722918	2774094	1.337	1.212
28)	SA Decachlor...	8.031	9.024	13418159	4053626	1.595	1.748
Target Compounds							
2)	A alpha-BHC	3.791	0.000	8327033	0	0.714	N.D. #
10)	B gamma-Chl...	0.000	6.078	0	2398435	N.D.	0.845 #
23)	Chlordane-1	4.207	0.000	6130858	0	18.231	N.D. #
25)	Chlordane-3	0.000	6.078	0	2398435	N.D.	6.291 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041219\
Data File : PL047361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2019 00:09
Operator : AJ\SJ
Sample : K2196-03 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HD-02-041119

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 05:42:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

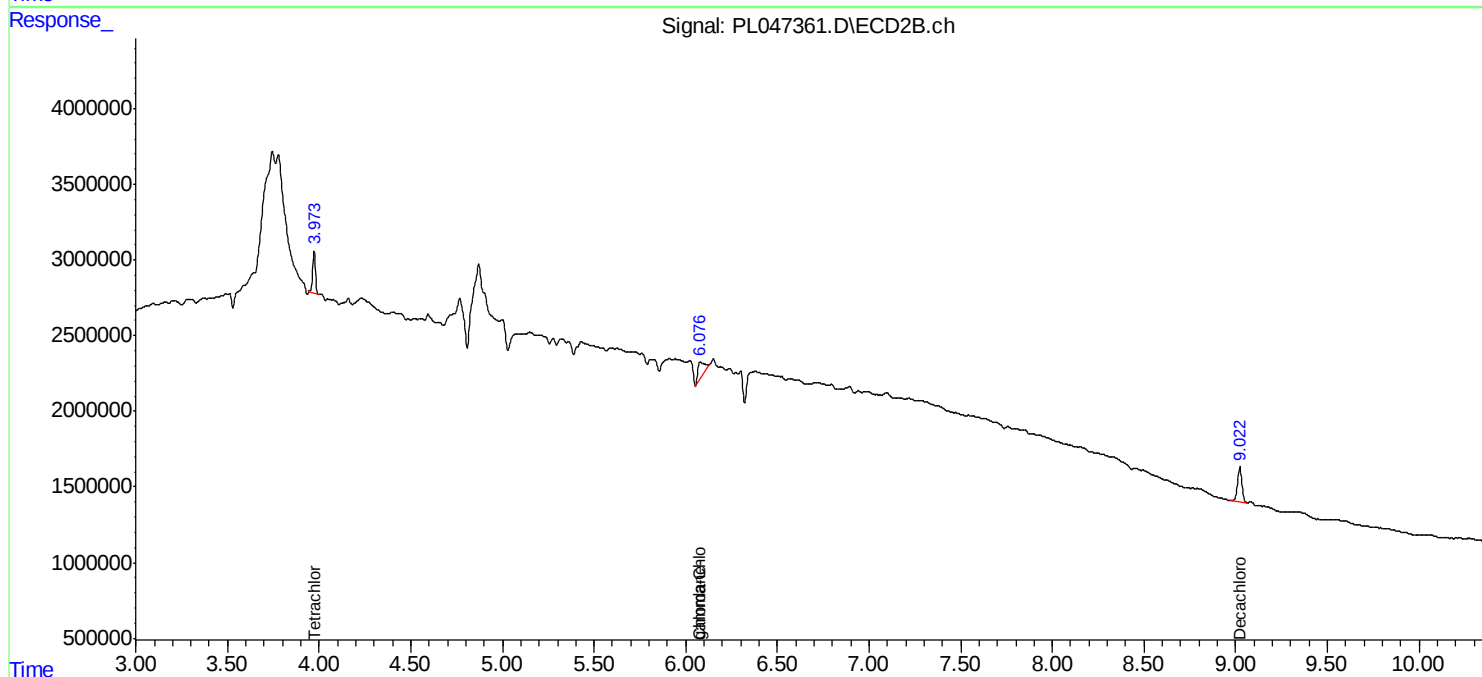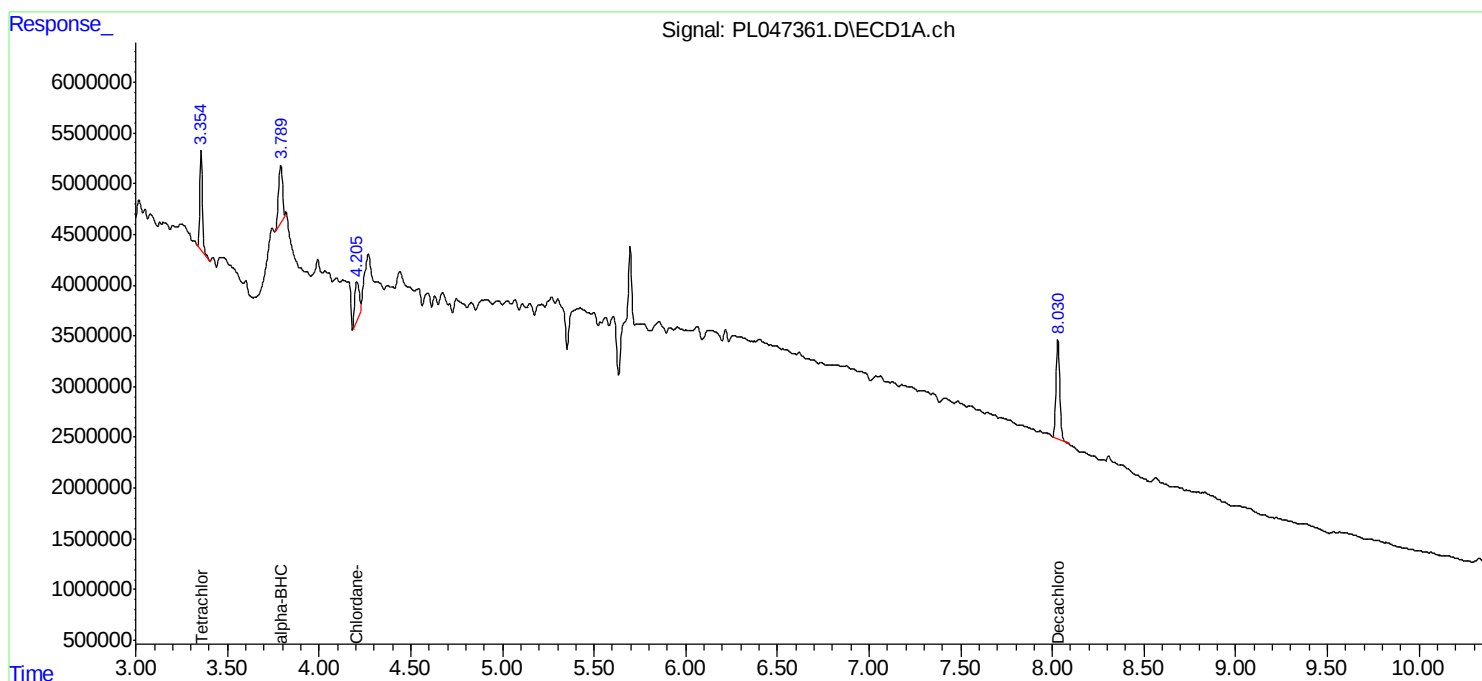


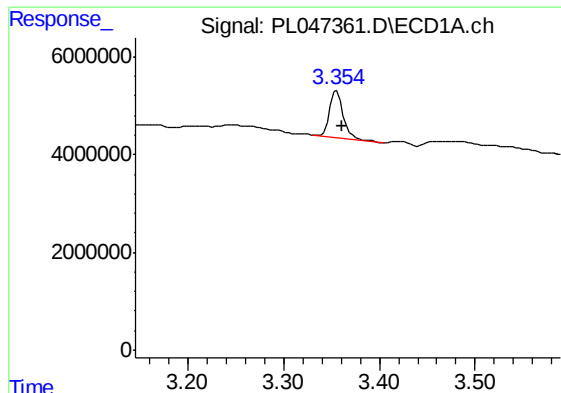

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 9722918
Conc: 1.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-041119

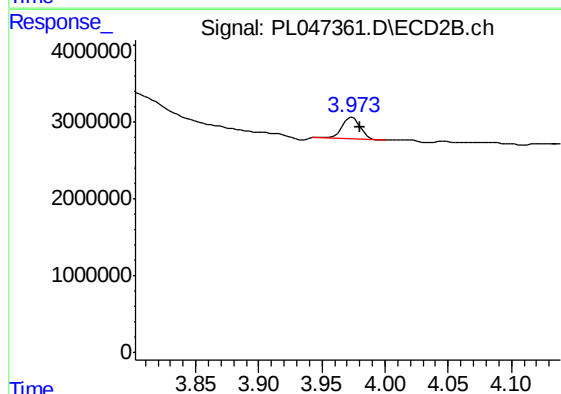


#1 Tetrachloro-m-xylene

R.T.: 3.974 min
Delta R.T.: -0.006 min
Response: 2774094
Conc: 1.21 ng/ml

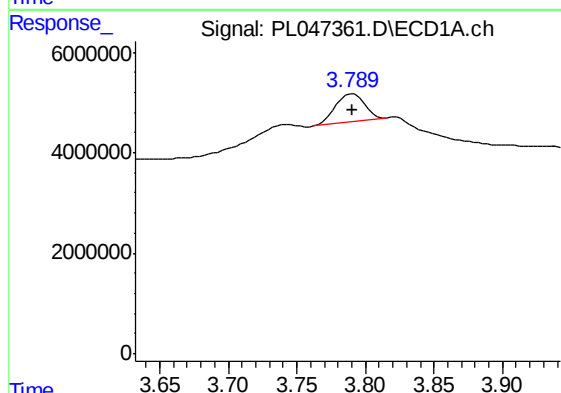


#2 alpha-BHC

R.T.: 3.791 min
Delta R.T.: 0.000 min
Response: 8327033
Conc: 0.71 ng/ml

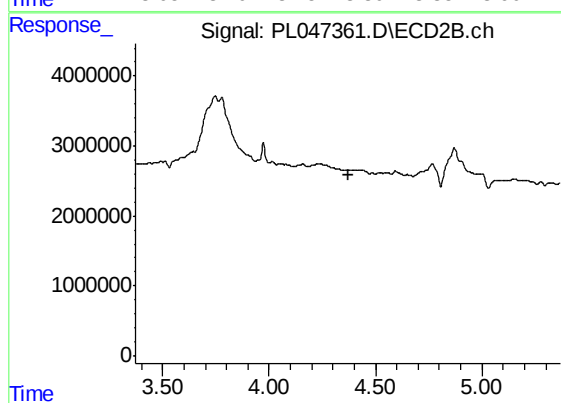

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

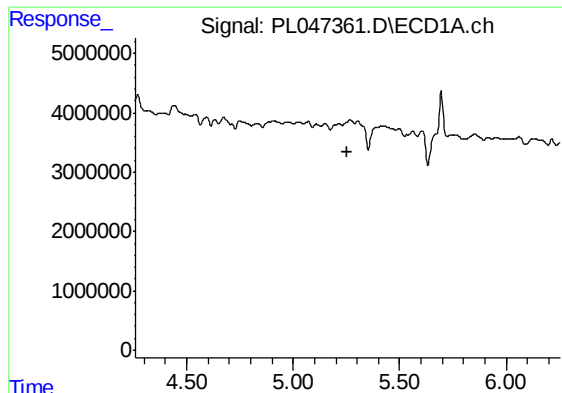

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HD-02-041119

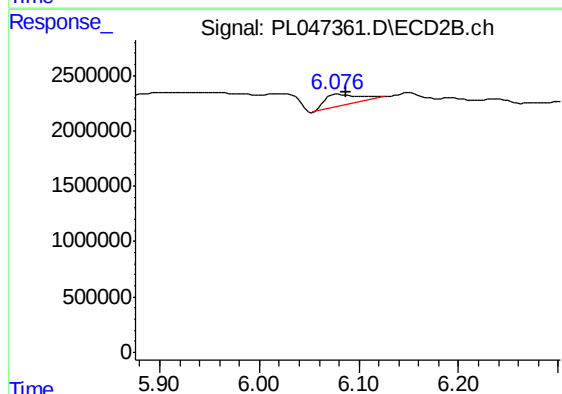


#10 gamma-Chlordane

R.T.: 6.078 min
Delta R.T.: -0.009 min
Response: 2398435
Conc: 0.85 ng/ml

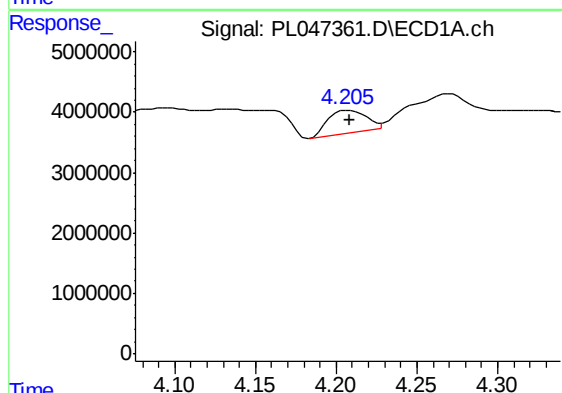


#23 Chlordane-1

R.T.: 4.207 min
Delta R.T.: -0.002 min
Response: 6130858
Conc: 18.23 ng/ml

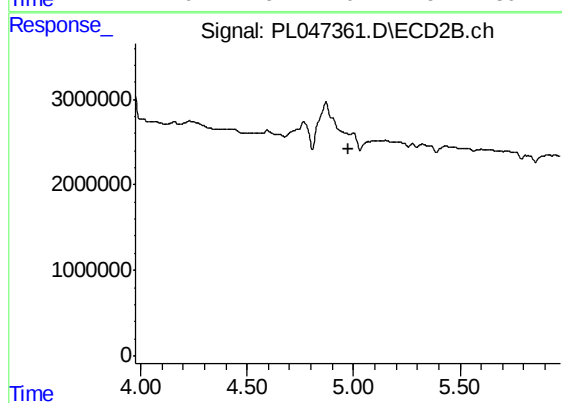

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

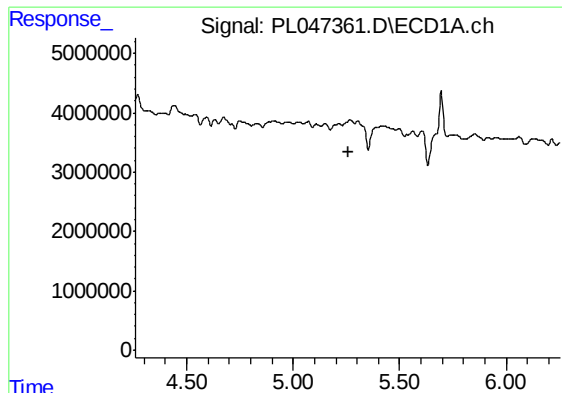

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HD-02-041119

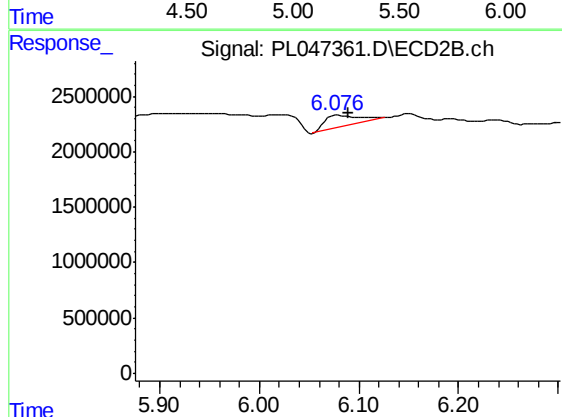


#25 Chlordane-3

R.T.: 6.078 min
Delta R.T.: -0.011 min
Response: 2398435
Conc: 6.29 ng/ml

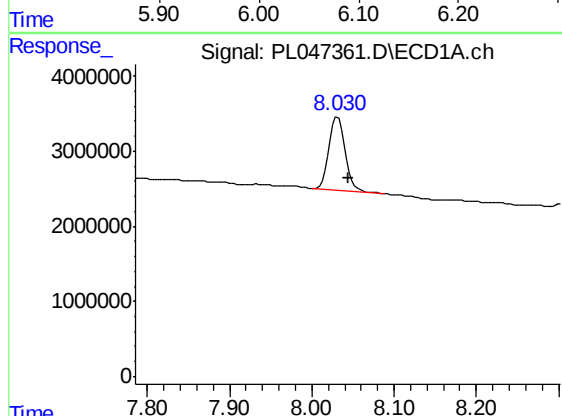

#28 Decachlorobiphenyl

R.T.: 8.031 min
Delta R.T.: -0.013 min
Response: 13418159
Conc: 1.60 ng/ml

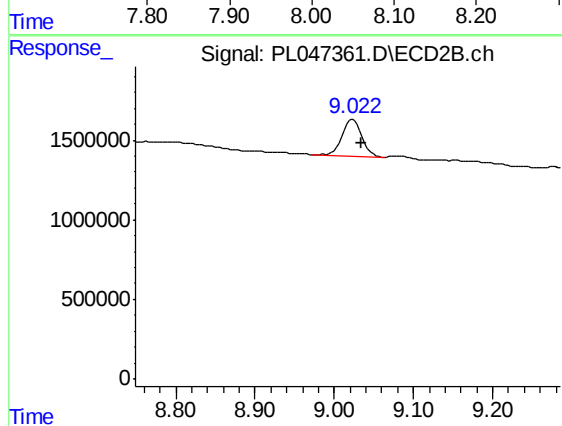

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: -0.011 min
Response: 4053626
Conc: 1.75 ng/ml