

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
 Data File : PL066014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2021 11:50
 Operator : AR\AJ
 Sample : PB135629BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 01:29:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.156	44436573	55395391	18.298	20.097
28)	SA Decachlor...	8.175	9.356	38674715	40563155	17.928	21.400
Target Compounds							
2)	A alpha-BHC	3.871	0.000	2719990	0	0.712	N.D. #
4)	MA Heptachlor	0.000	5.357	0	827188	N.D.	0.240 #
6)	B beta-BHC	0.000	5.038	0	7956965	N.D.	1.730 #
12)	B 4,4'-DDE	0.000	6.563f	0	399046	N.D.	0.160 #
15)	B Endosulfa...	0.000	7.127	0	1936908	N.D.	0.909 #
16)	A 4,4'-DDD	0.000	7.009f	0	1345368	N.D.	0.645 #
21)	B Endrin ke...	0.000	7.977	0	1364924	N.D.	0.604 #
27)	Chlordane-5	0.000	7.204	0	317158	N.D.	3.883 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
Data File : PL066014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2021 11:50
Operator : AR\AJ
Sample : PB135629BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 01:29:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

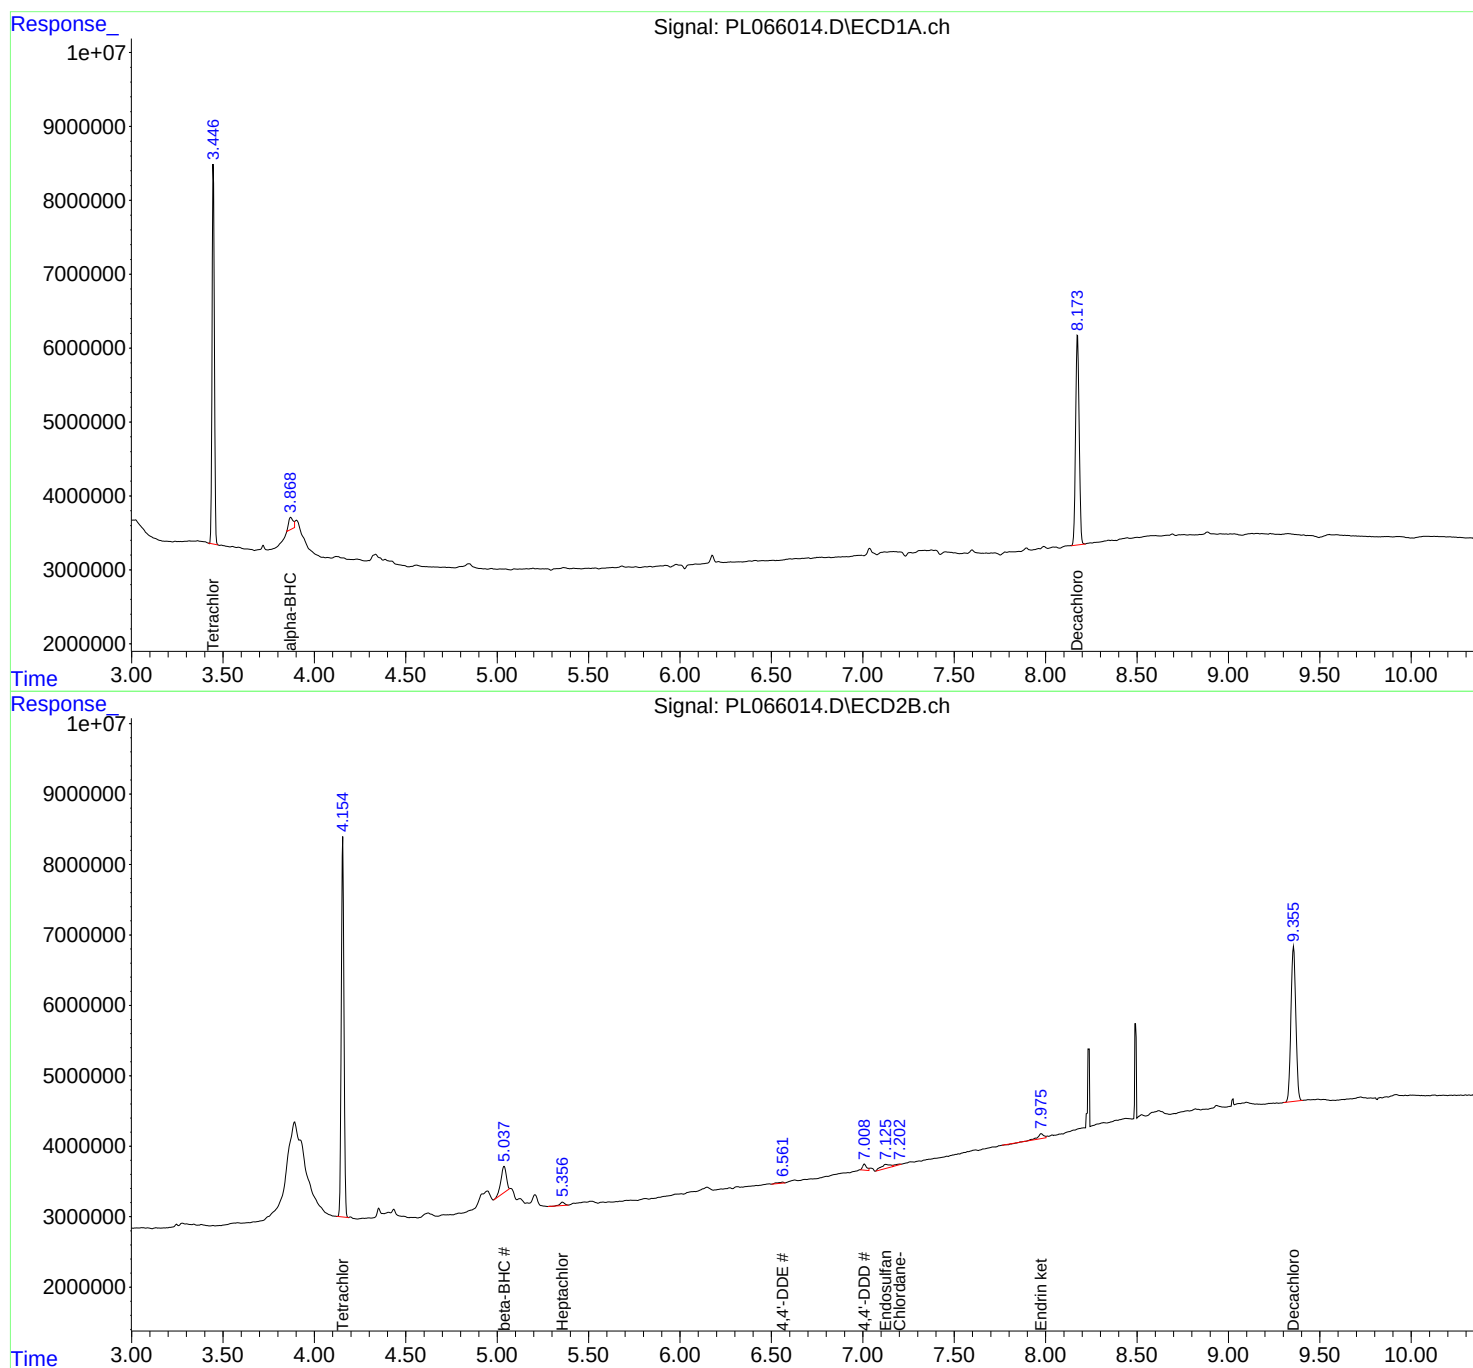


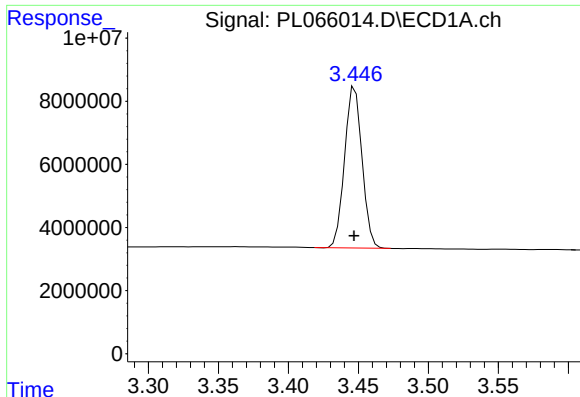

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 44436573
Conc: 18.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

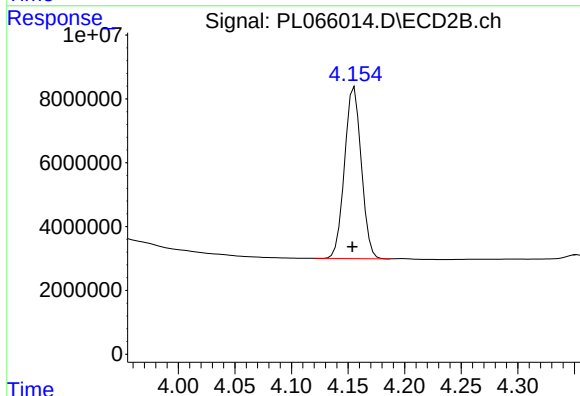


#1 Tetrachloro-m-xylene

R.T.: 4.156 min
Delta R.T.: 0.002 min
Response: 55395391
Conc: 20.10 ng/ml

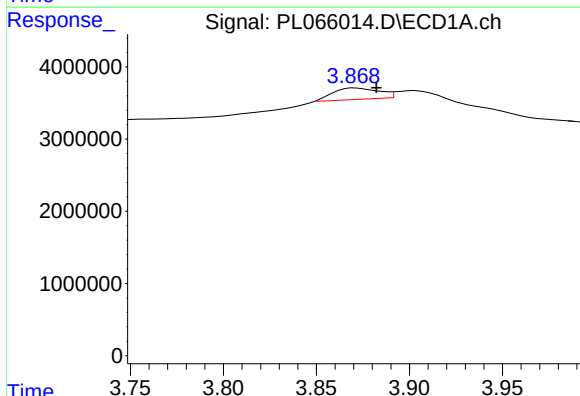


#2 alpha-BHC

R.T.: 3.871 min
Delta R.T.: -0.012 min
Response: 2719990
Conc: 0.71 ng/ml

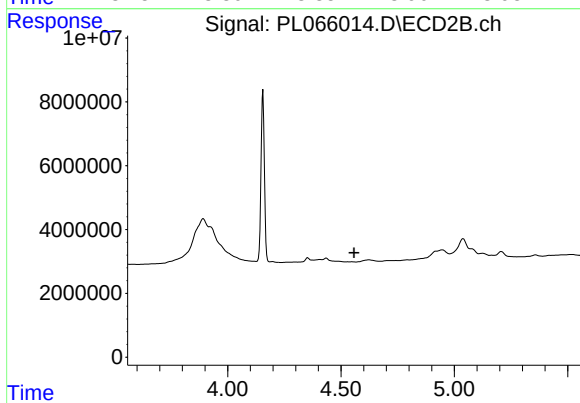

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.558 min
Response: 0
Conc: N.D.

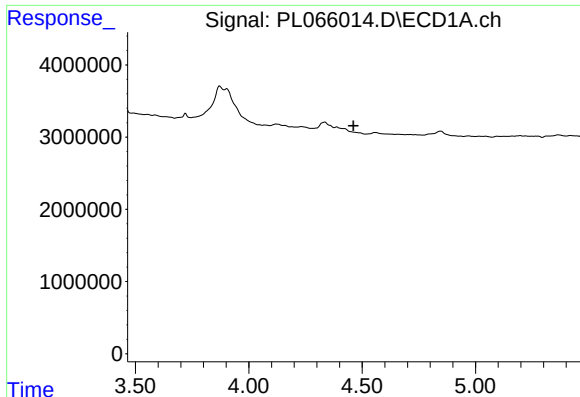

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.462 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

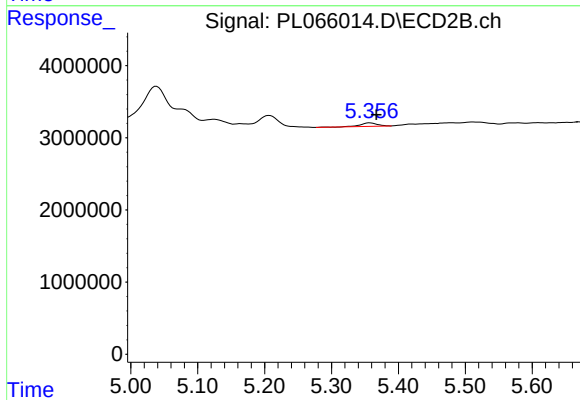


#4 Heptachlor

R.T.: 5.357 min
Delta R.T.: -0.010 min
Response: 827188
Conc: 0.24 ng/ml

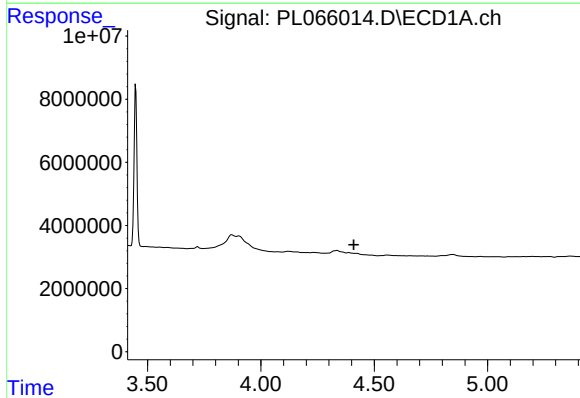


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.410 min
Response: 0
Conc: N.D.

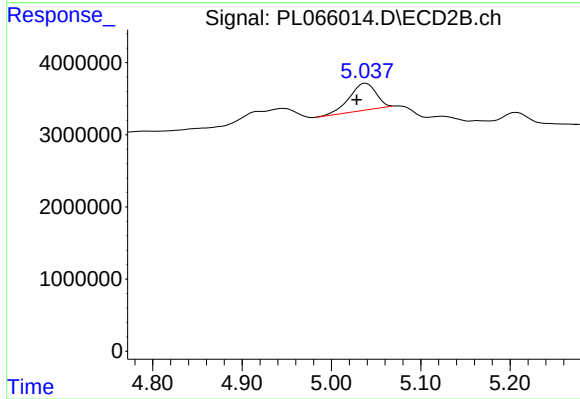

#6 beta-BHC


R.T.: 5.038 min
Delta R.T.: 0.010 min
Response: 7956965
Conc: 1.73 ng/ml

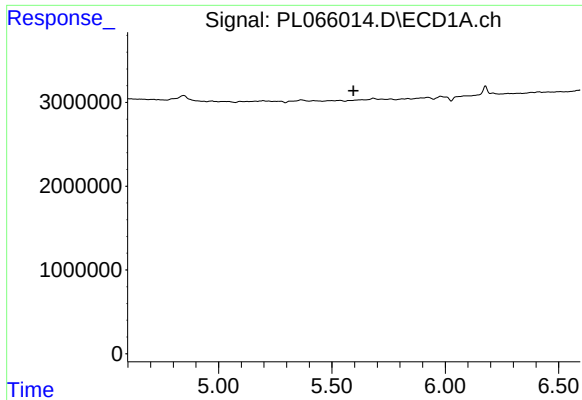

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

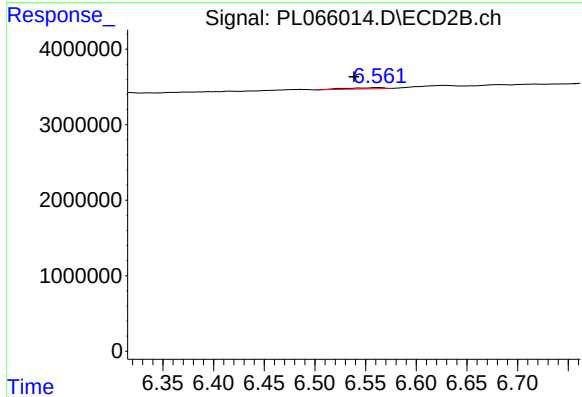


#12 4,4'-DDE

R.T.: 6.563 min
Delta R.T.: 0.024 min
Response: 399046
Conc: 0.16 ng/ml

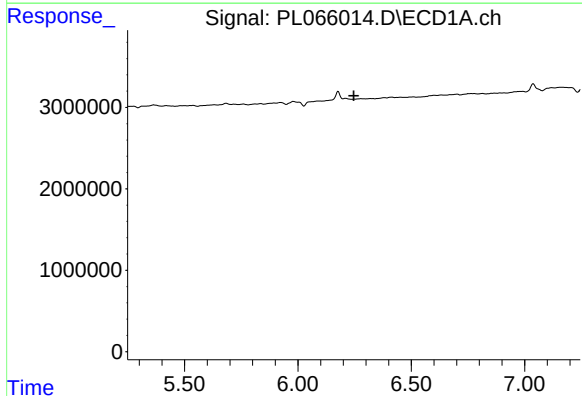


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

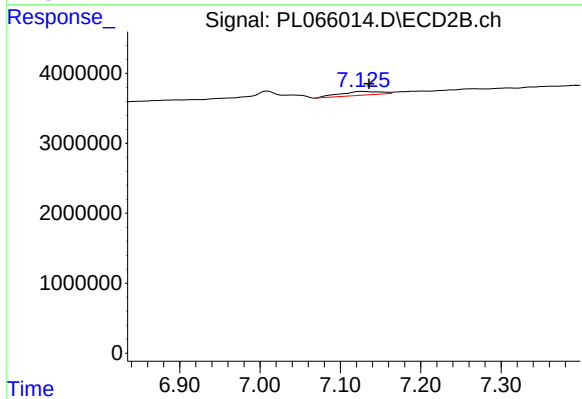

#15 Endosulfan II


R.T.: 7.127 min
Delta R.T.: -0.009 min
Response: 1936908
Conc: 0.91 ng/ml

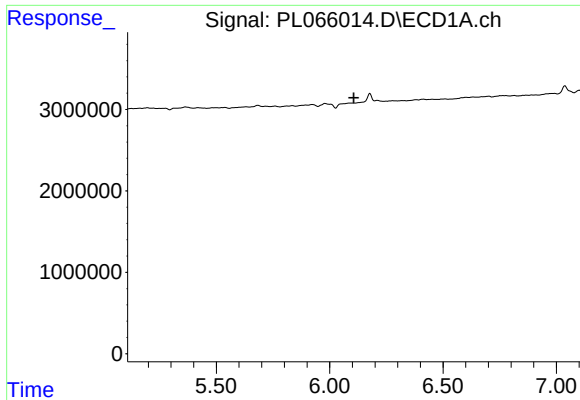

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.106 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

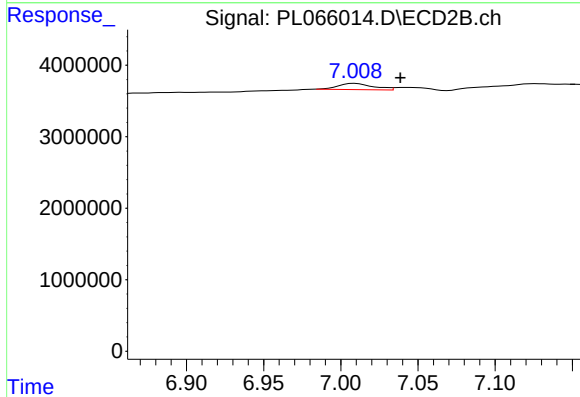


#16 4,4'-DDD

R.T.: 7.009 min
Delta R.T.: -0.030 min
Response: 1345368
Conc: 0.65 ng/ml

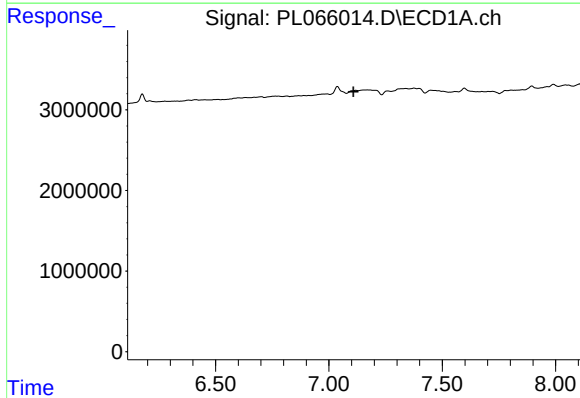


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.109 min
Response: 0
Conc: N.D.

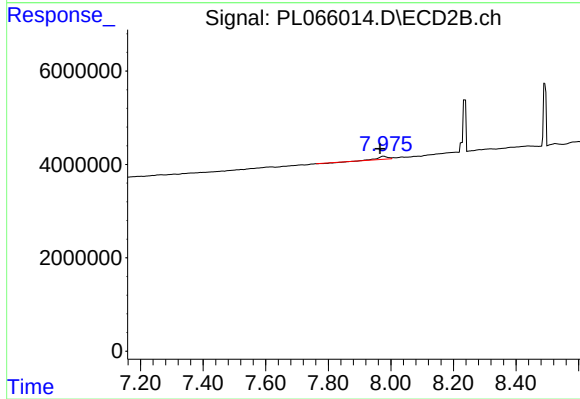

#21 Endrin ketone


R.T.: 7.977 min
Delta R.T.: 0.011 min
Response: 1364924
Conc: 0.60 ng/ml

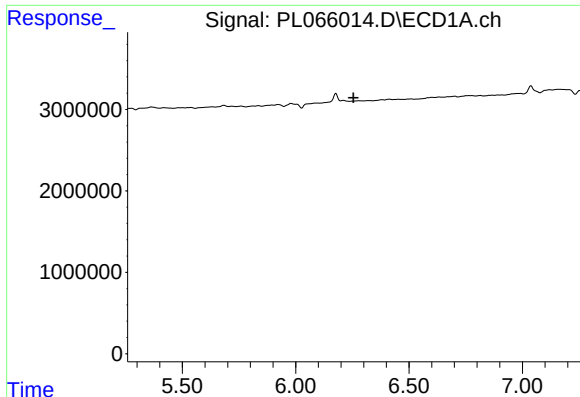

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.255 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

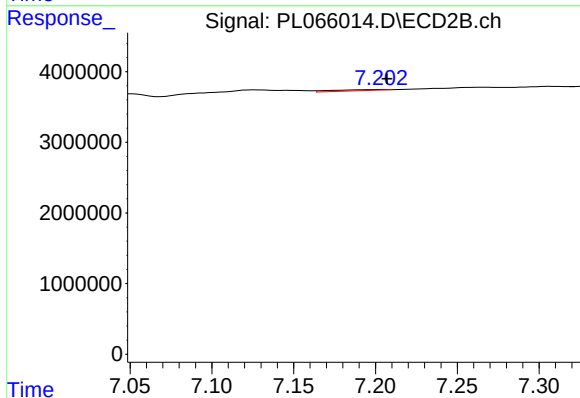


#27 Chlordane-5

R.T.: 7.204 min
Delta R.T.: -0.003 min
Response: 317158
Conc: 3.88 ng/ml

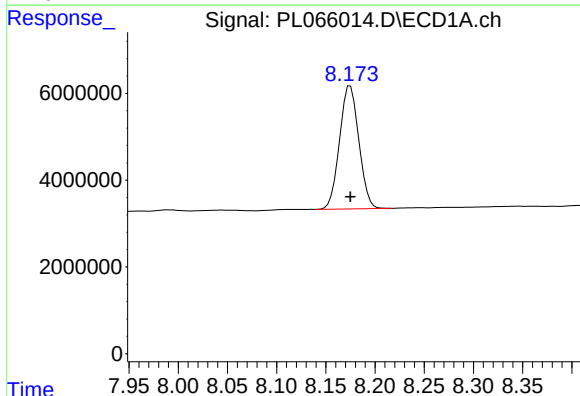

#28 Decachlorobiphenyl

R.T.: 8.175 min
Delta R.T.: 0.000 min
Response: 38674715
Conc: 17.93 ng/ml

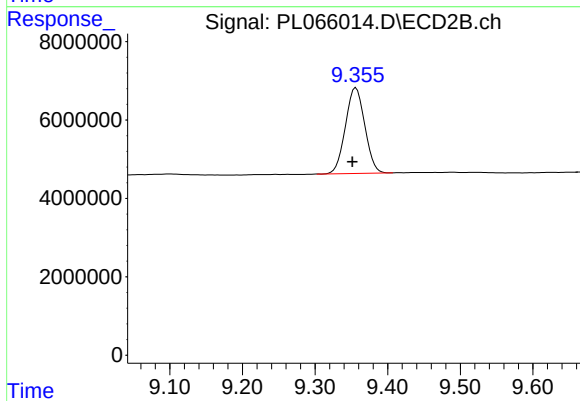

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.005 min
Response: 40563155
Conc: 21.40 ng/ml