

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
 Data File : PL066047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2021 21:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 01:37:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.155	47133949	62074070	19.409	22.520
28)	SA Decachlor...	8.172	9.354	44509739	49183779	20.633	25.947 #
Target Compounds							
2)	A alpha-BHC	3.870	0.000	1464478	0	0.383	N.D. #
4)	MA Heptachlor	0.000	5.353	0	1688966	N.D.	0.490 #
6)	B beta-BHC	0.000	5.034	0	6174598	N.D.	0.661 #
8)	B Heptachlo...	0.000	6.068	0	6273958	N.D.	2.208 #
12)	B 4,4'-DDE	0.000	6.553	0	147789	N.D.	0.059 #
14)	MA Endrin	5.977	0.000	1946518	0	0.660	N.D. #
21)	B Endrin ke...	0.000	7.975	0	1148204	N.D.	0.509 #
23)	Chlordane-1	4.330f	0.000	3088065	0	29.505	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
Data File : PL066047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2021 21:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 01:37:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

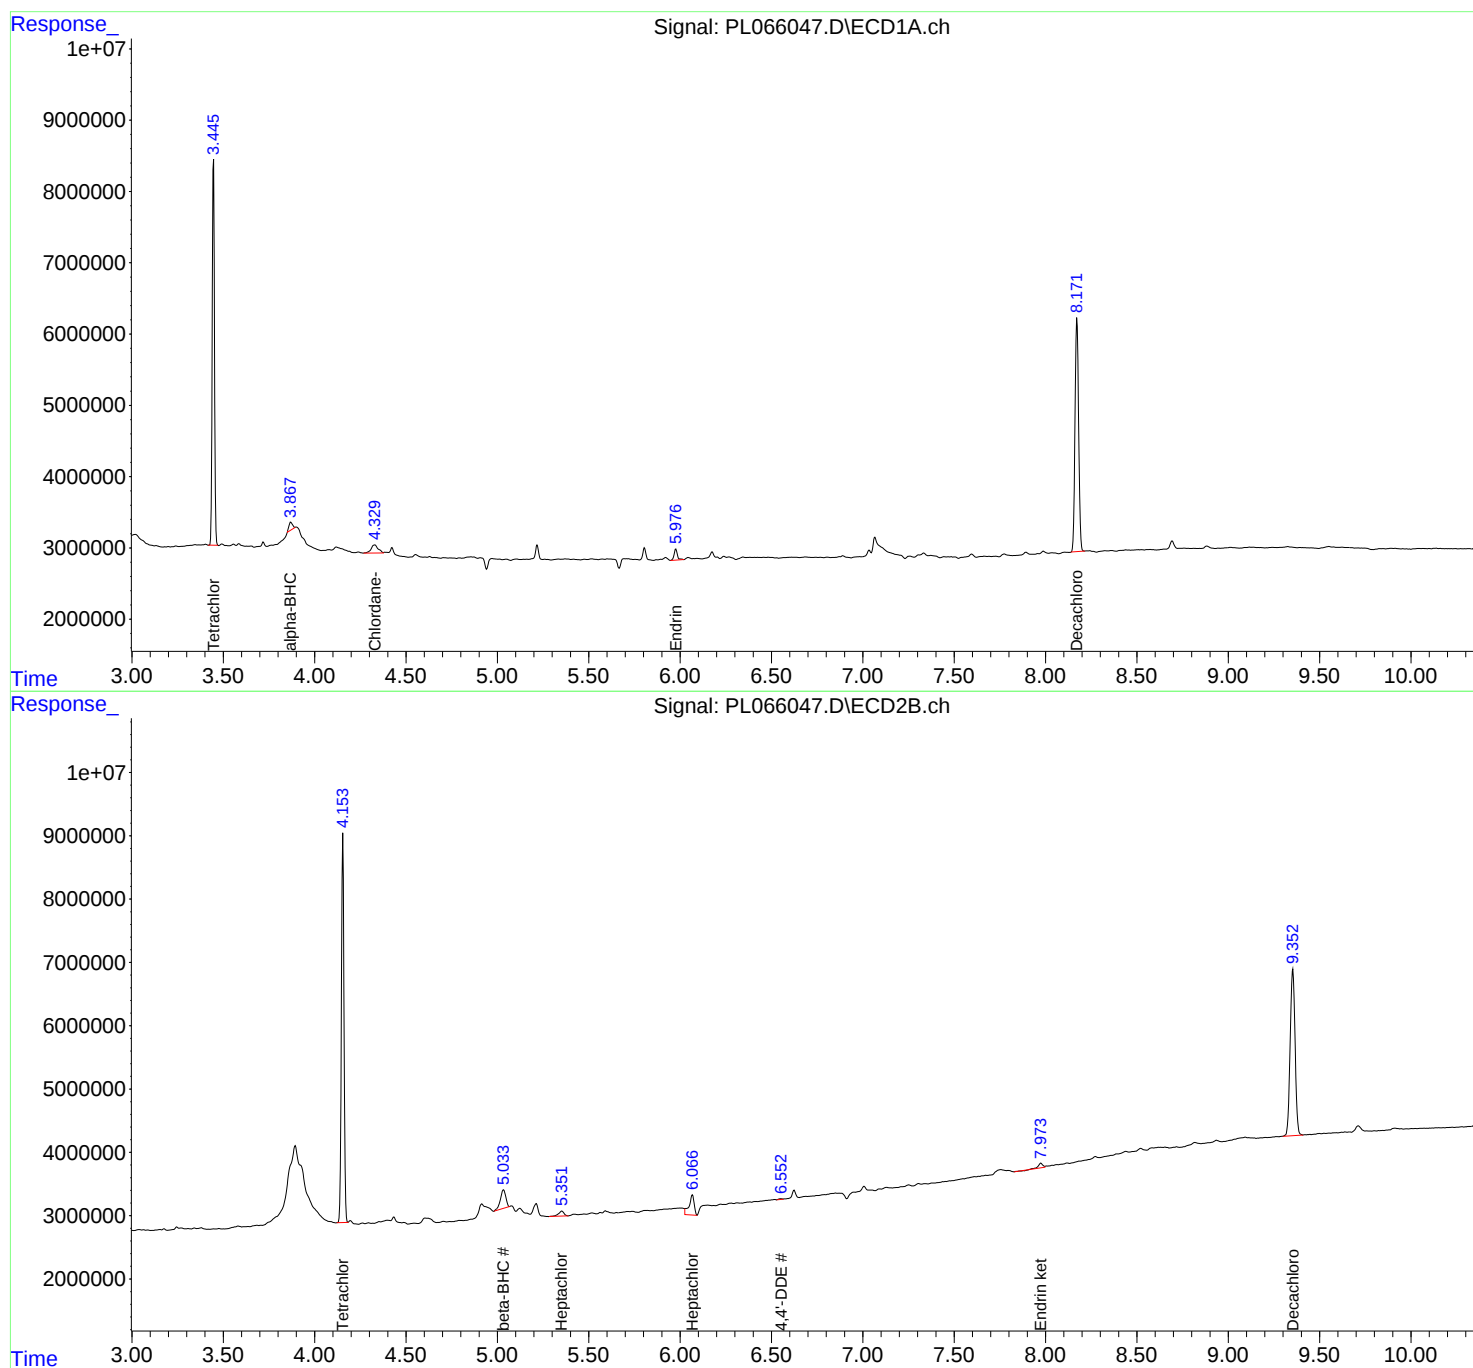


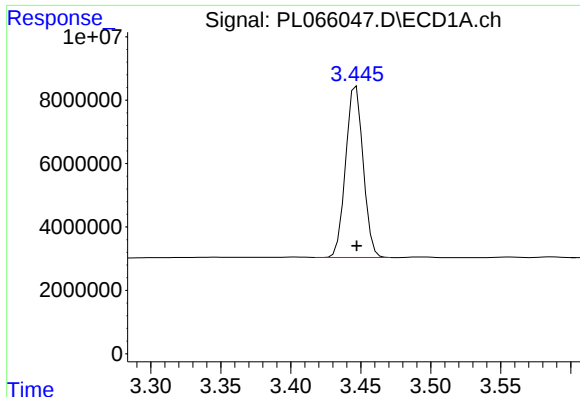

#1 Tetrachloro-m-xylene


R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 47133949
Conc: 19.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

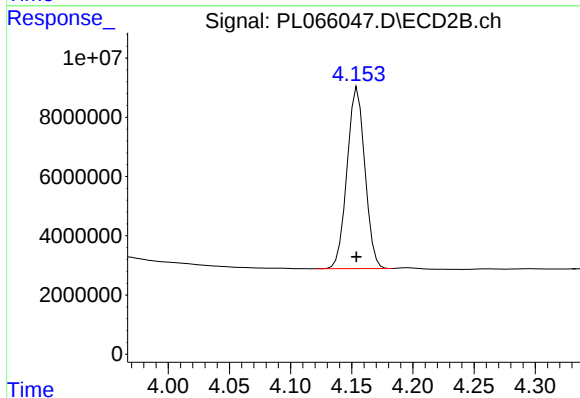


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.001 min
Response: 62074070
Conc: 22.52 ng/ml

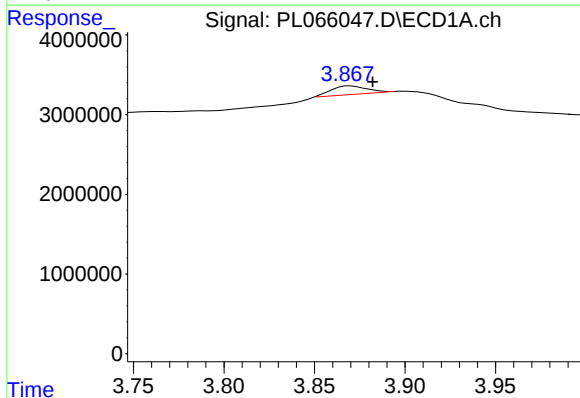


#2 alpha-BHC

R.T.: 3.870 min
Delta R.T.: -0.012 min
Response: 1464478
Conc: 0.38 ng/ml

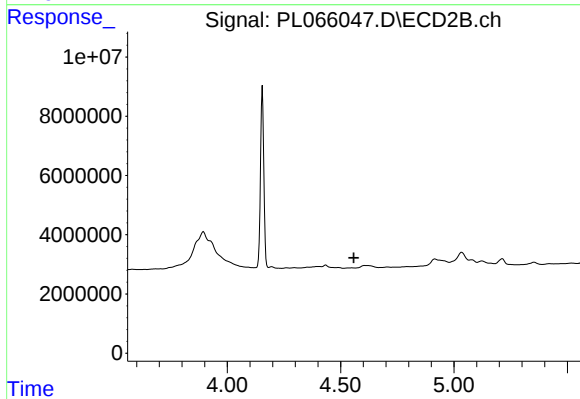

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.558 min
Response: 0
Conc: N.D.

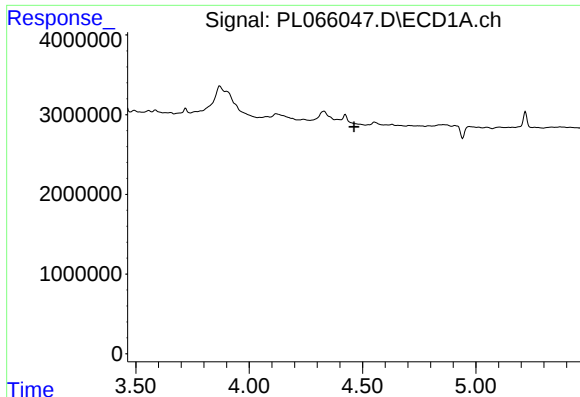

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.462 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

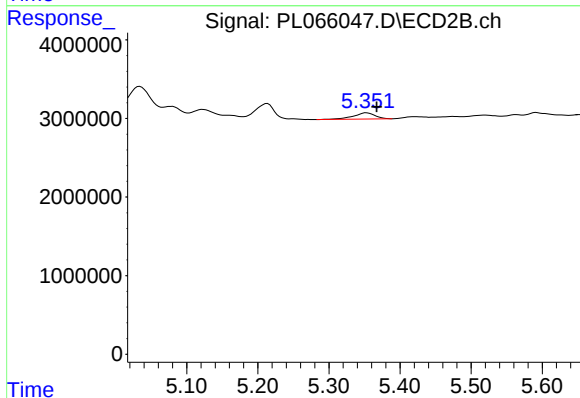


#4 Heptachlor

R.T.: 5.353 min
Delta R.T.: -0.015 min
Response: 1688966
Conc: 0.49 ng/ml

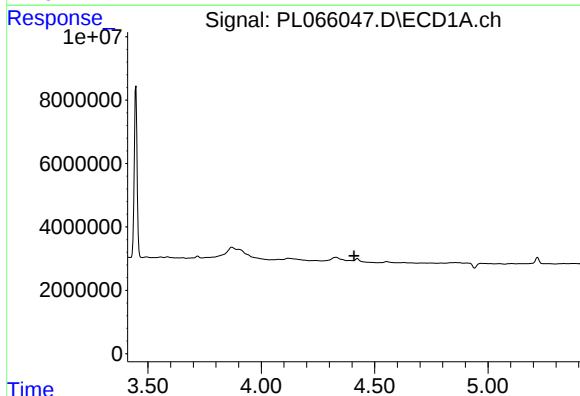


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.410 min
Response: 0
Conc: N.D.

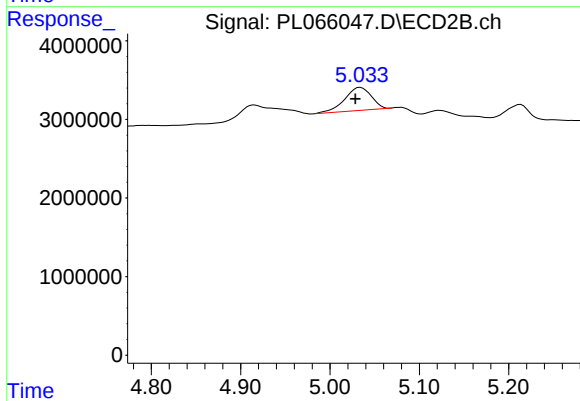

#6 beta-BHC


R.T.: 5.034 min
Delta R.T.: 0.006 min
Response: 6174598
Conc: 0.66 ng/ml

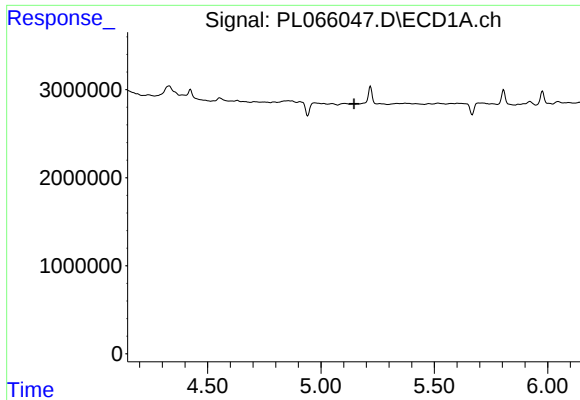

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.146 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

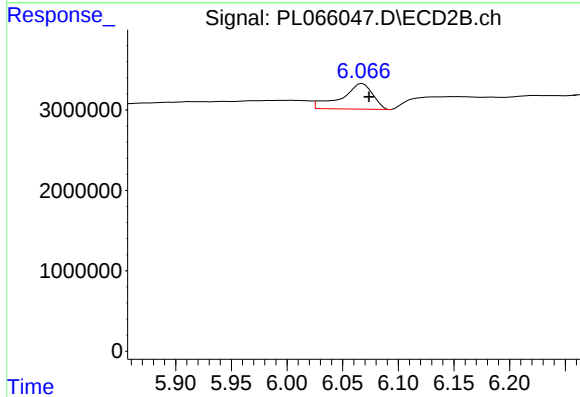


#8 Heptachlor epoxide

R.T.: 6.068 min
Delta R.T.: -0.006 min
Response: 6273958
Conc: 2.21 ng/ml

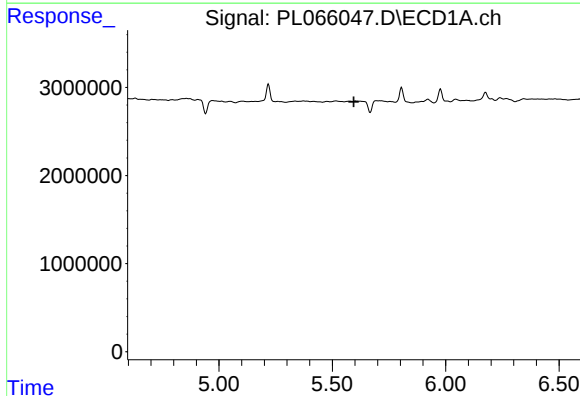


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.595 min
Response: 0
Conc: N.D.

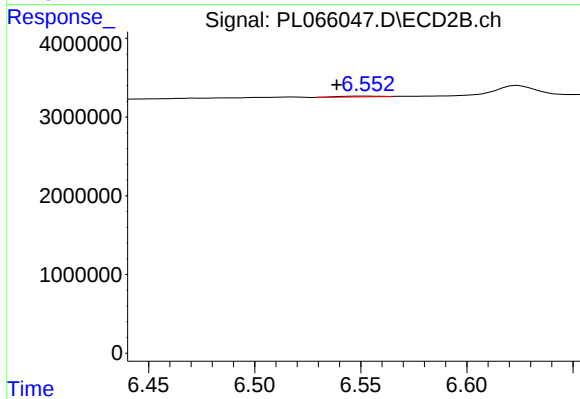

#12 4,4'-DDE


R.T.: 6.553 min
Delta R.T.: 0.014 min
Response: 147789
Conc: 0.06 ng/ml

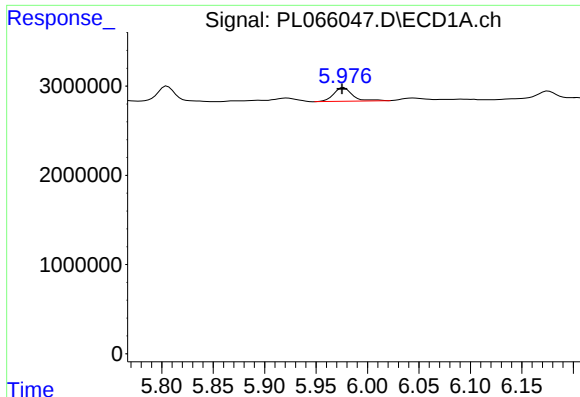

#14 Endrin


R.T.: 5.977 min
Delta R.T.: 0.002 min
Response: 1946518
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

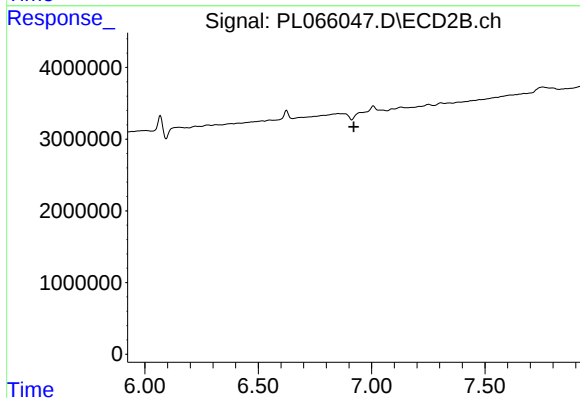


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

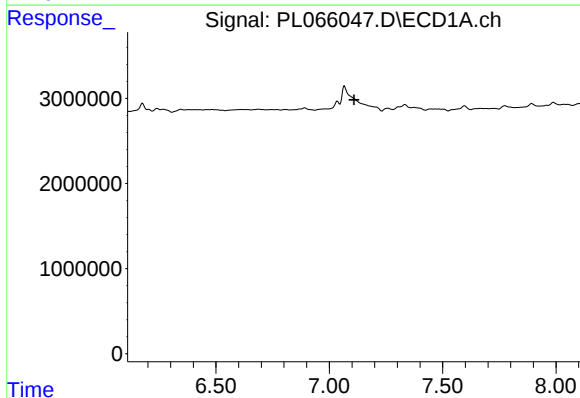


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.109 min
Response: 0
Conc: N.D.

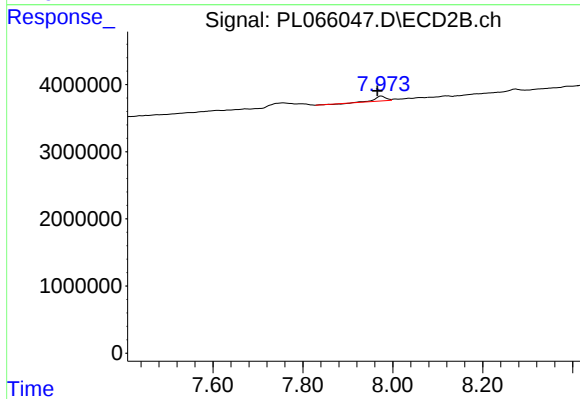

#21 Endrin ketone


R.T.: 7.975 min
Delta R.T.: 0.009 min
Response: 1148204
Conc: 0.51 ng/ml

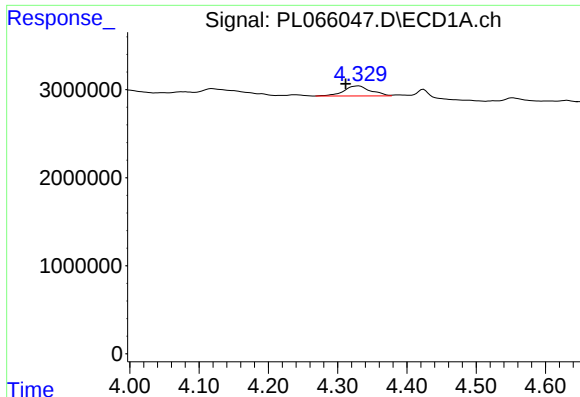

#23 Chlordane-1


R.T.: 4.330 min
Delta R.T.: 0.019 min
Response: 3088065
Conc: 29.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

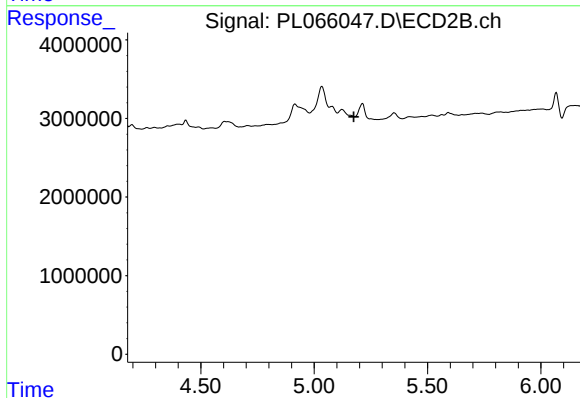


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

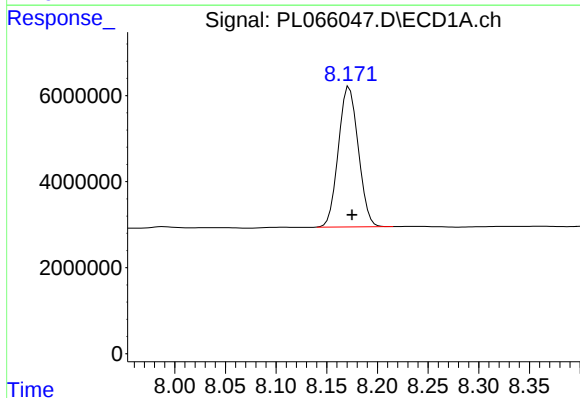

#28 Decachlorobiphenyl

R.T.: 8.172 min
Delta R.T.: -0.003 min
Response: 44509739
Conc: 20.63 ng/ml

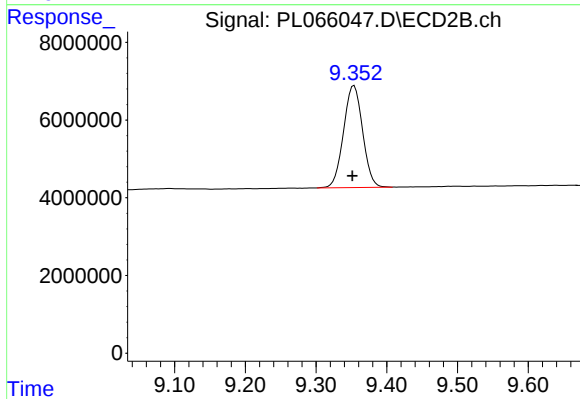

#28 Decachlorobiphenyl

R.T.: 9.354 min
Delta R.T.: 0.002 min
Response: 49183779
Conc: 25.95 ng/ml