

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
 Data File : PL066011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2021 11:07
 Operator : AR\AJ
 Sample : M1946-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FS-SB9

Manual Integrations
 APPROVED

Ankita
 4/13/2021 3:30:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 01:28:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.155	47497763	61397451	19.559	22.275
28)	SA Decachlor...	8.176	9.357	45050261	47119562	20.883	24.858
Target Compounds							
10)	B gamma-Chl...	5.370	6.312	1843540	4742315	0.561m	1.710m#
13)	MA Dieldrin	5.718	6.702	5556560	4803802	1.665m	1.875

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
Data File : PL066011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2021 11:07
Operator : AR\AJ
Sample : M1946-03
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
FS-SB9


Manual Integrations
APPROVED

Ankita
4/13/2021 3:30:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 01:28:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

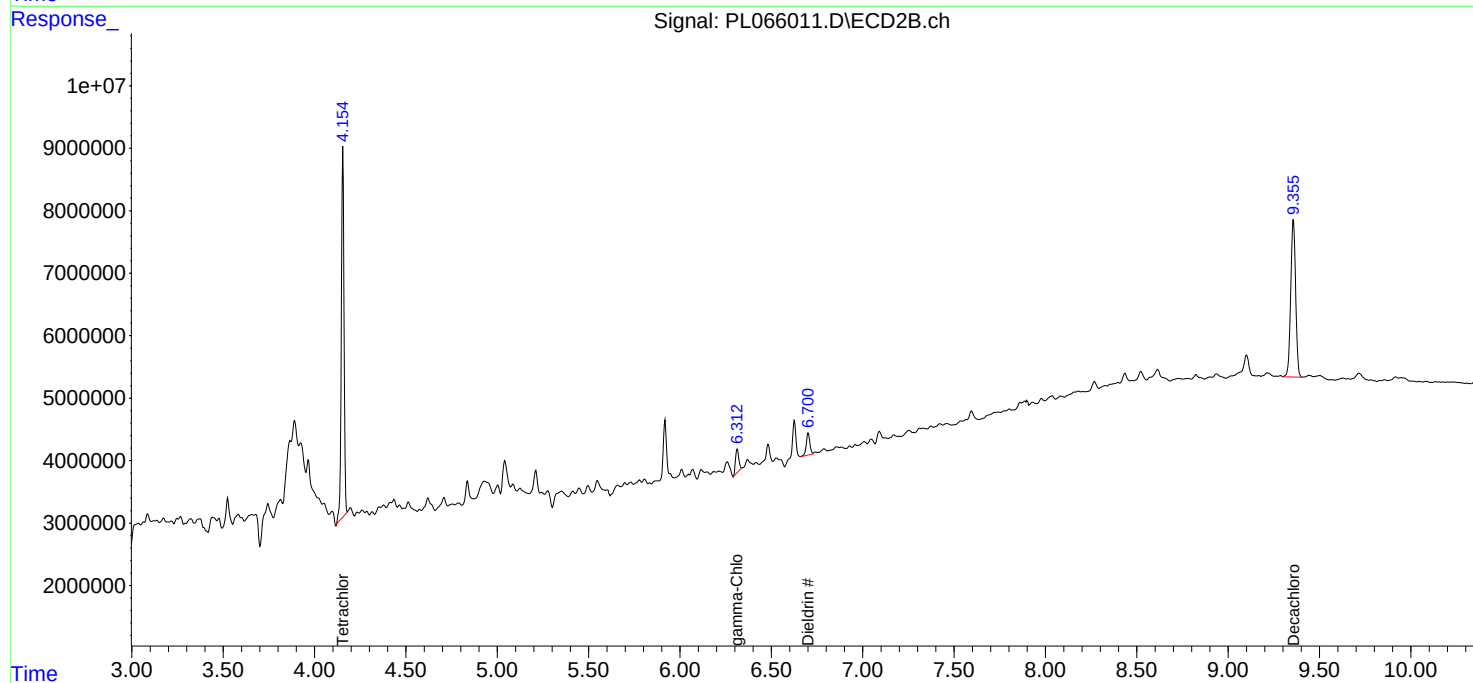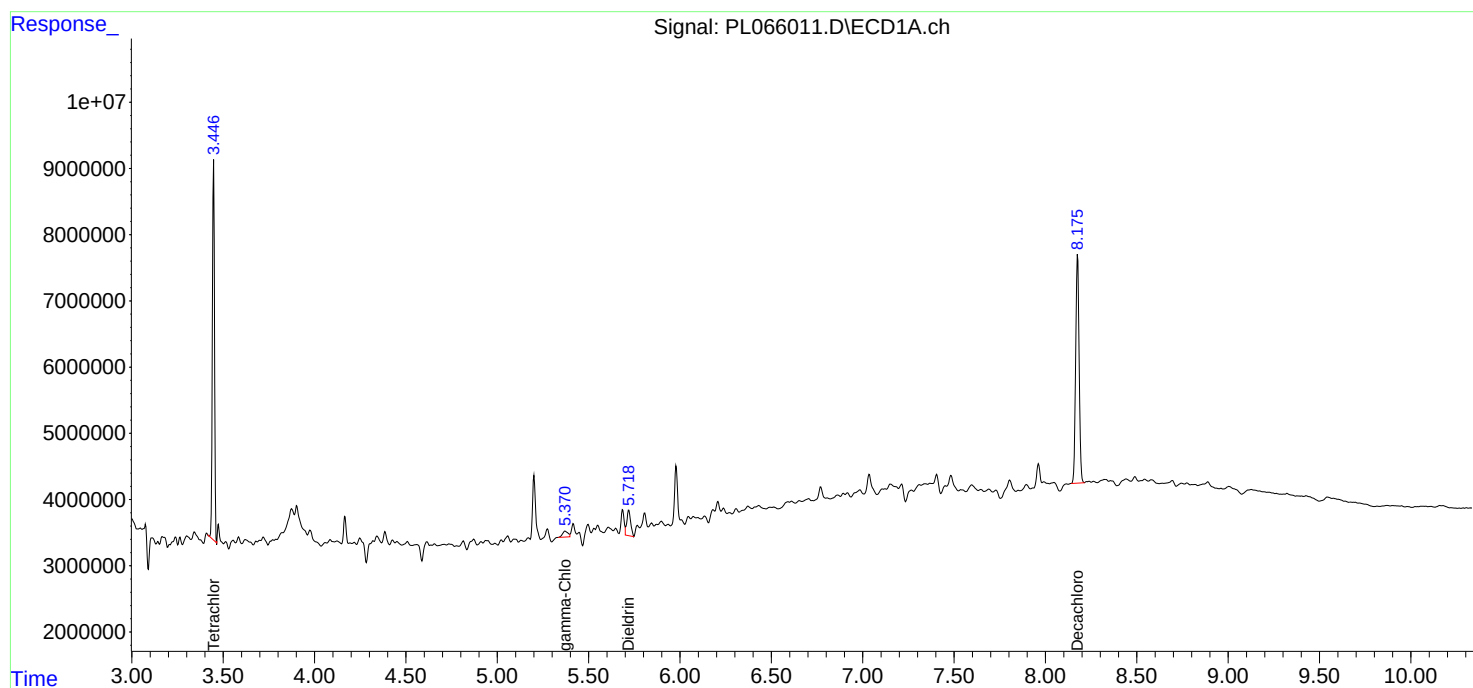

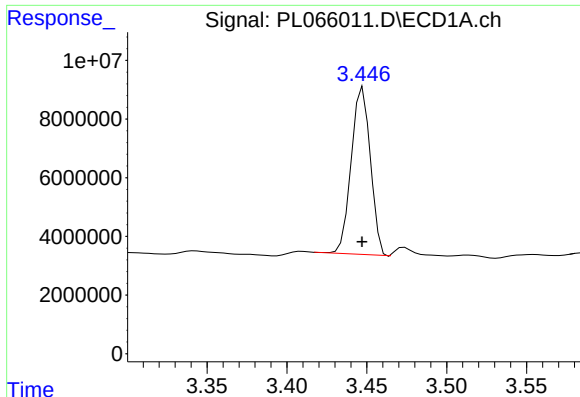


#1 Tetrachloro-m-xylene

R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 47497763
Conc: 19.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-SB9


Manual Integrations
APPROVED

Ankita
4/13/2021 3:30:48 PM

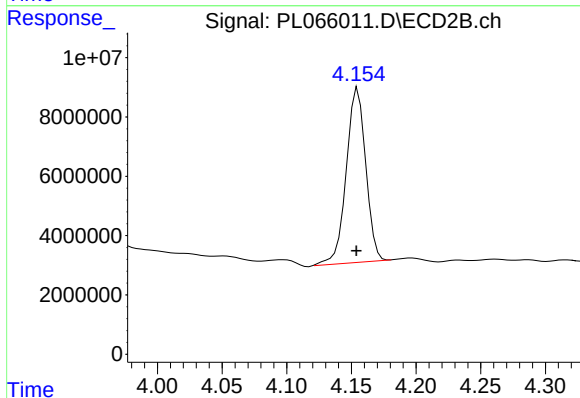


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.001 min
Response: 61397451
Conc: 22.27 ng/ml

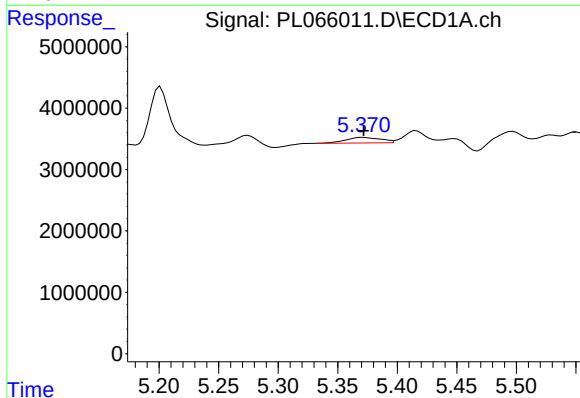


#10 gamma-Chlordane

R.T.: 5.370 min
Delta R.T.: -0.002 min
Response: 1843540
Conc: 0.56 ng/ml m

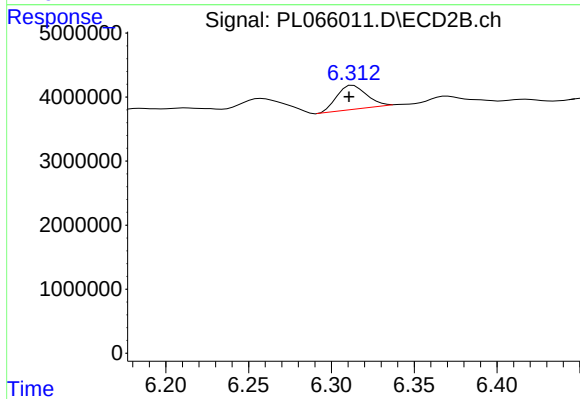

#10 gamma-Chlordane

R.T.: 6.312 min
Delta R.T.: 0.001 min
Response: 4742315
Conc: 1.71 ng/ml m

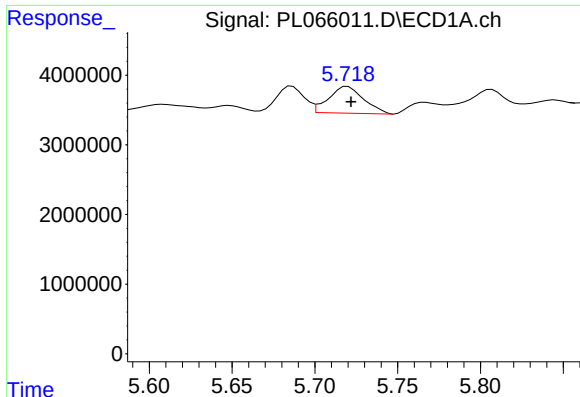


#13 Dieldrin

R.T.: 5.718 min
Delta R.T.: -0.003 min
Response: 5556560
Conc: 1.67 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FS-SB9


Manual Integrations
APPROVED

Ankita
4/13/2021 3:30:48 PM

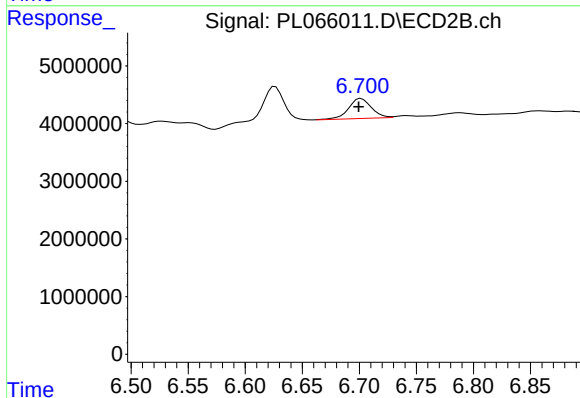


#13 Dieldrin

R.T.: 6.702 min
Delta R.T.: 0.002 min
Response: 4803802
Conc: 1.87 ng/ml

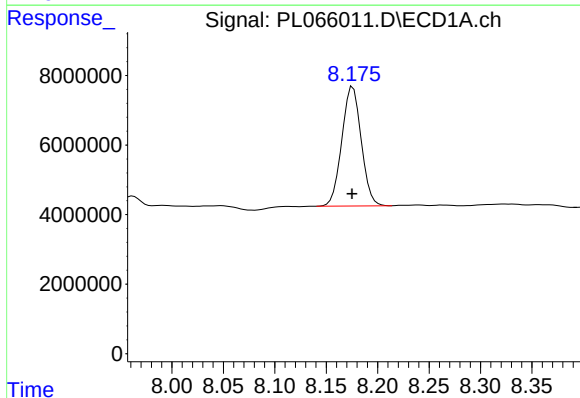

#28 Decachlorobiphenyl

R.T.: 8.176 min
Delta R.T.: 0.000 min
Response: 45050261
Conc: 20.88 ng/ml

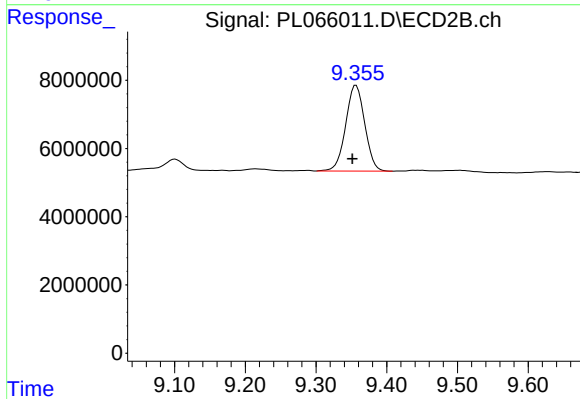

#28 Decachlorobiphenyl

R.T.: 9.357 min
Delta R.T.: 0.005 min
Response: 47119562
Conc: 24.86 ng/ml