

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
 Data File : PL066038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2021 19:36
 Operator : AR\AJ
 Sample : M1961-02
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR1-A-D-COMP

Manual Integrations
 APPROVED

Ankita
 4/13/2021 3:31:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 01:35:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.155	46189868	61870415	19.020m	22.446
28)	SA Decachlor...	8.174	9.356	40754039	44996512	18.892	23.738 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
Data File : PL066038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2021 19:36
Operator : AR\AJ
Sample : M1961-02
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR1-A-D-COMP


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 01:35:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

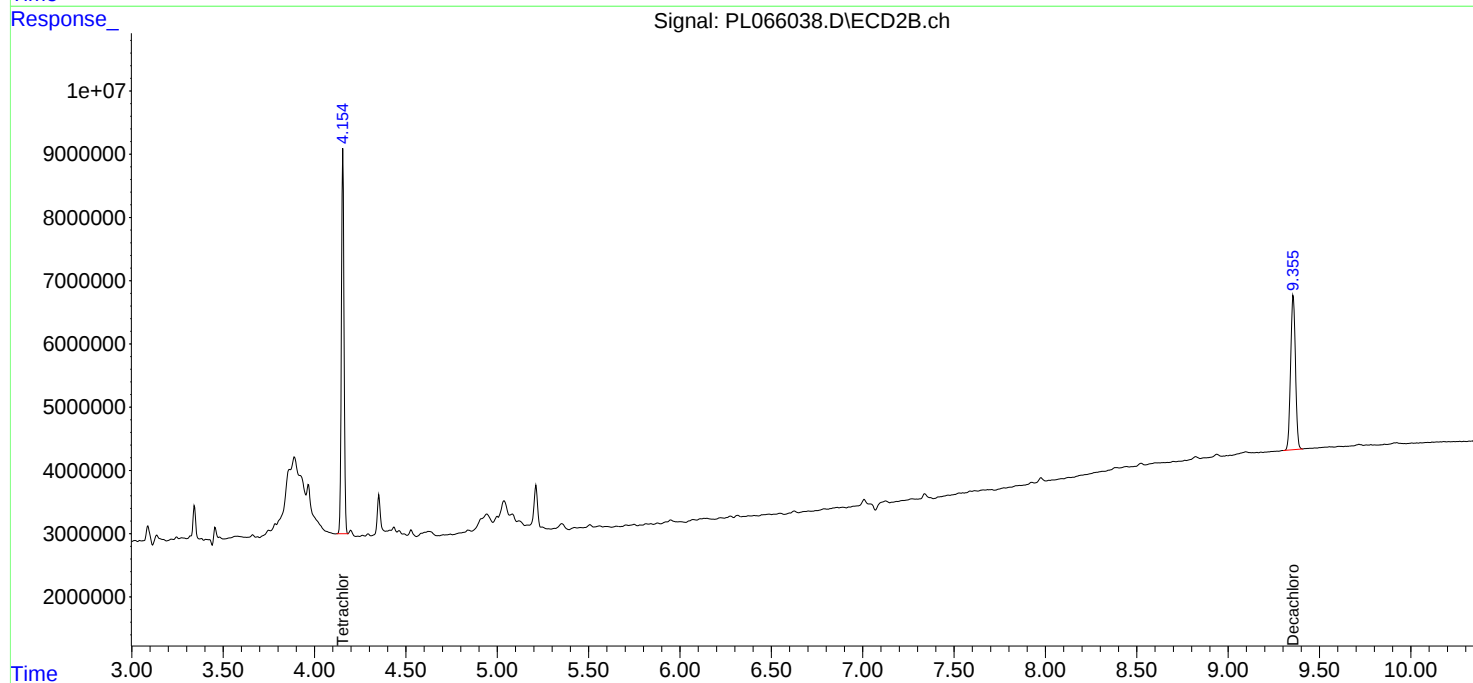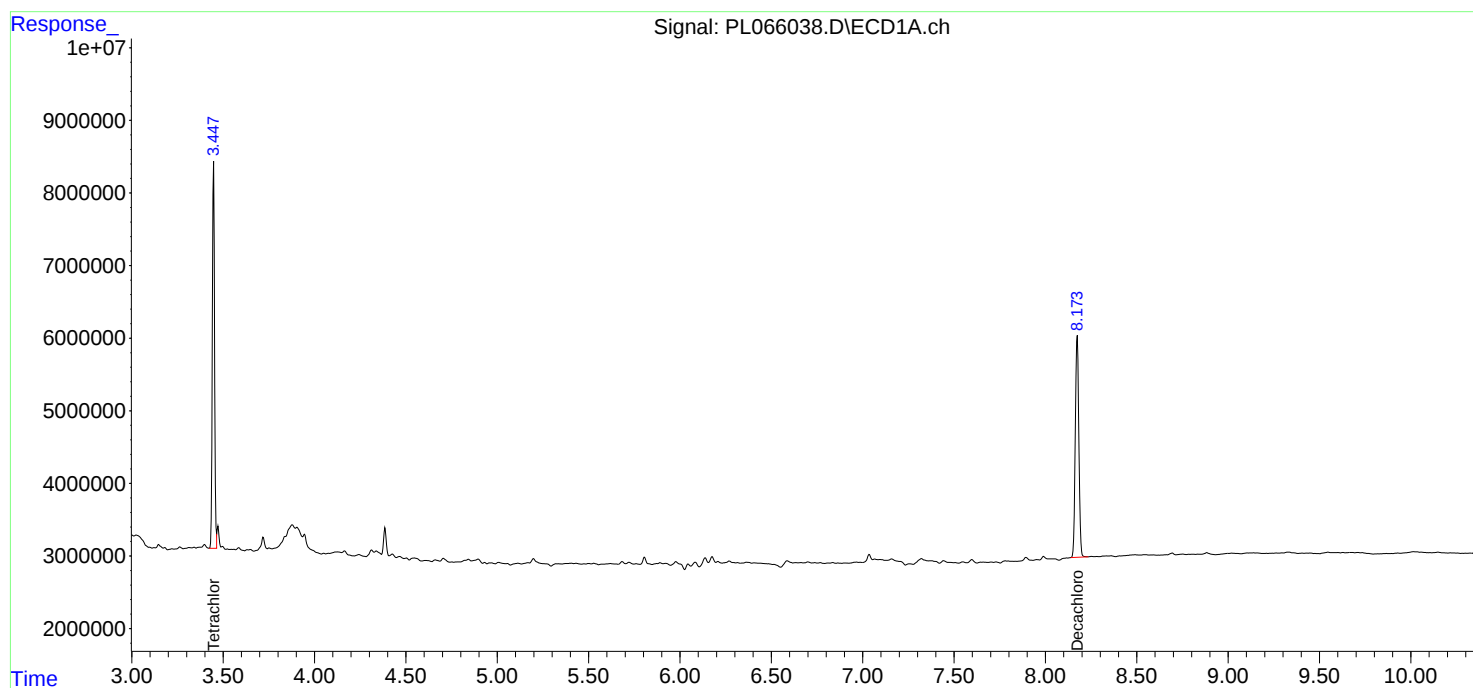

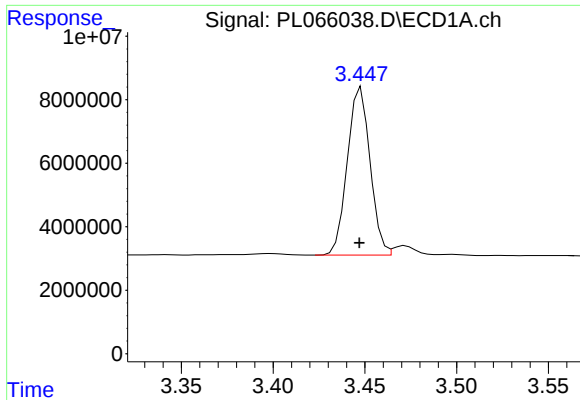


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 46189868
Conc: 19.02 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TR1-A-D-COMP


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:28 PM

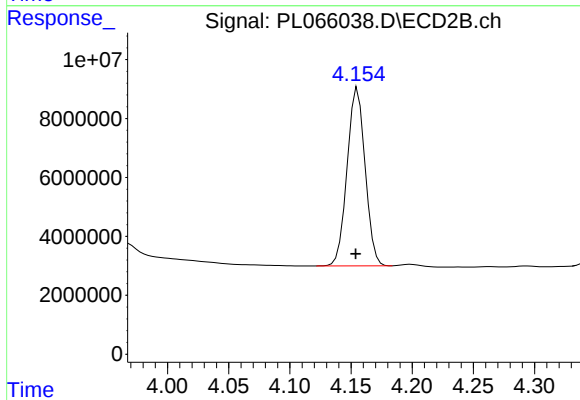


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 61870415
Conc: 22.45 ng/ml

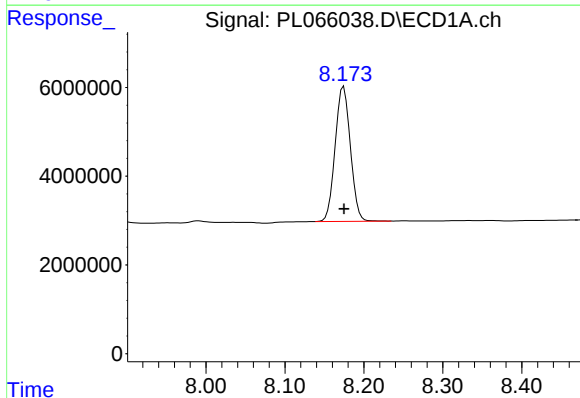

#28 Decachlorobiphenyl

R.T.: 8.174 min
Delta R.T.: 0.000 min
Response: 40754039
Conc: 18.89 ng/ml

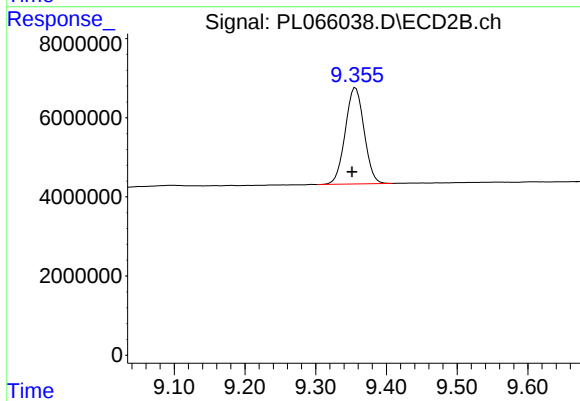

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.005 min
Response: 44996512
Conc: 23.74 ng/ml