

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
 Data File : PL066050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2021 22:43
 Operator : AR\AJ
 Sample : M1992-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-05-040921

Manual Integrations
 APPROVED

Ankita
 4/13/2021 3:31:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 01:37:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.447	4.155	31118783	41826207	12.814	15.174
28) SA Decachlor...	8.173	9.355	31388639	34542713	14.550	18.223 #
Target Compounds						
12) B 4,4'-DDE	5.593	6.540	4914060	6678848	1.609m	2.681 #
17) MA 4,4'-DDT	6.344	7.340	2456398	1843577	0.871	0.973m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
Data File : PL066050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2021 22:43
Operator : AR\AJ
Sample : M1992-01
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
AU-05-040921


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 01:37:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

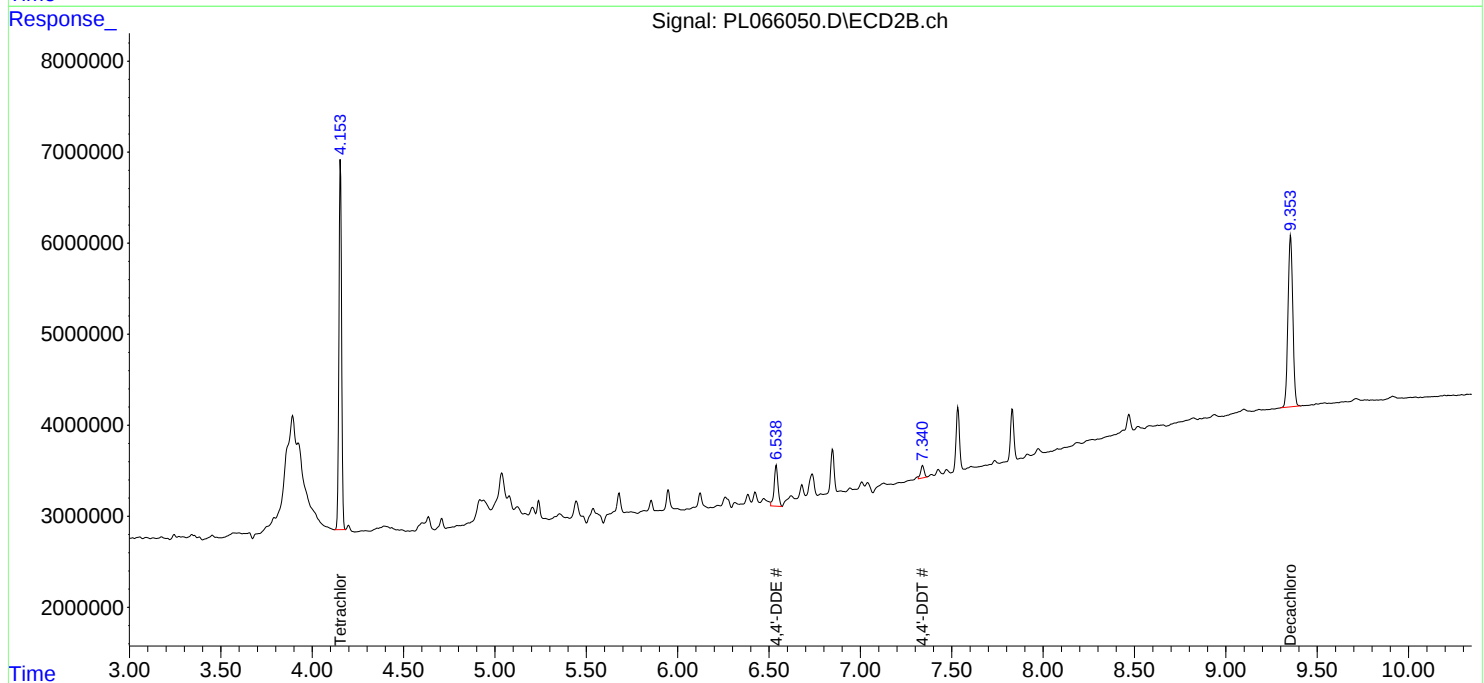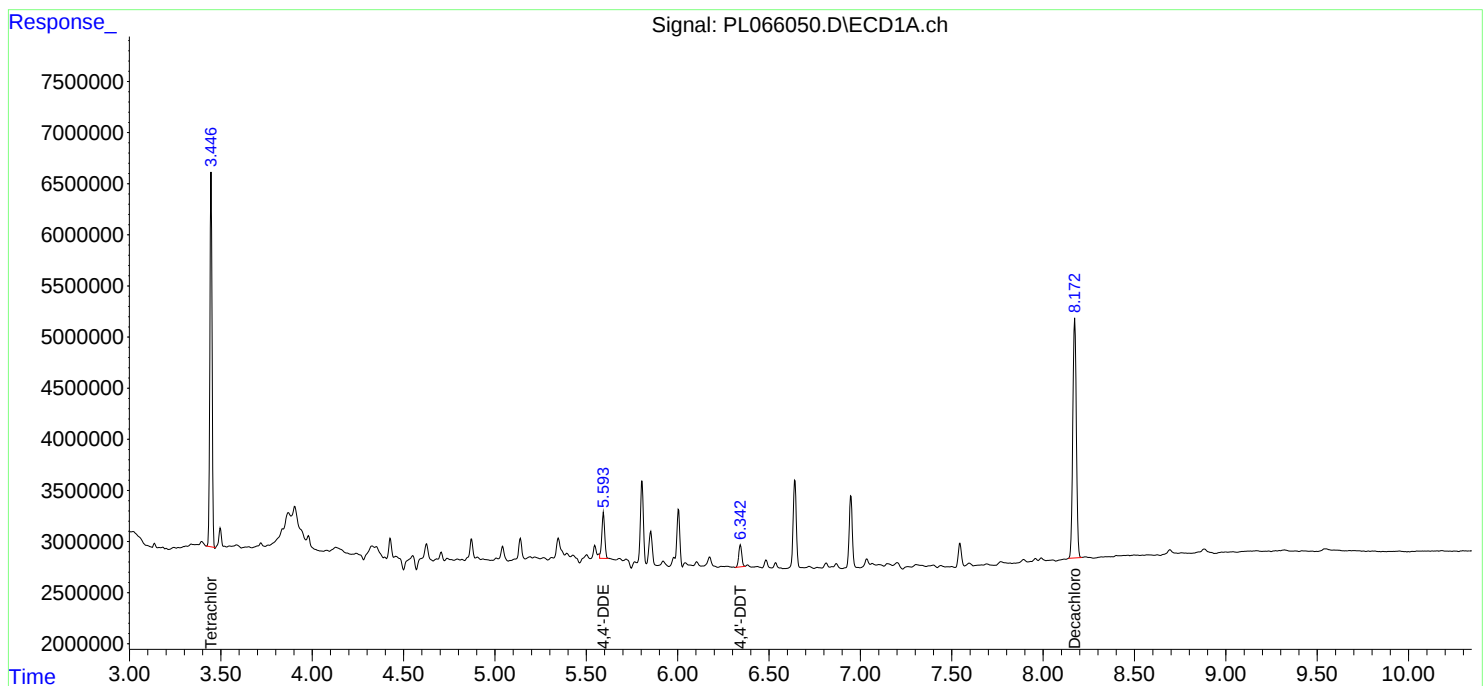

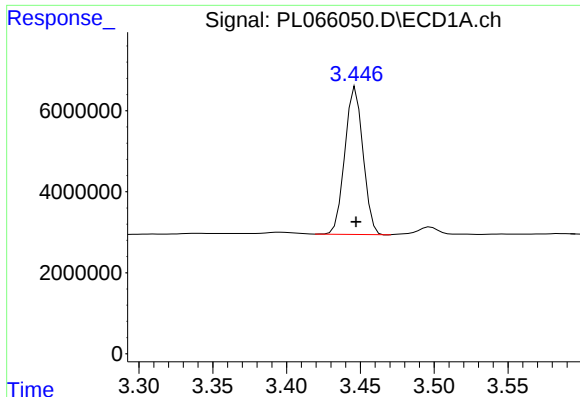


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 31118783
Conc: 12.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-040921


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:40 PM

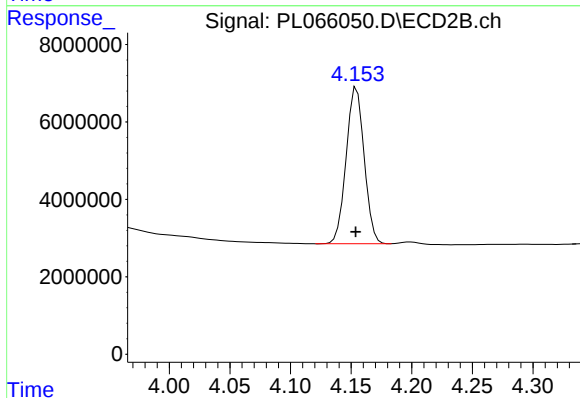


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.000 min
Response: 41826207
Conc: 15.17 ng/ml

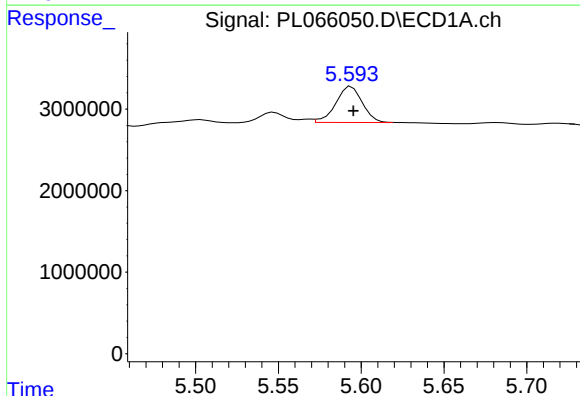


#12 4,4'-DDE

R.T.: 5.593 min
Delta R.T.: -0.003 min
Response: 4914060
Conc: 1.61 ng/ml m

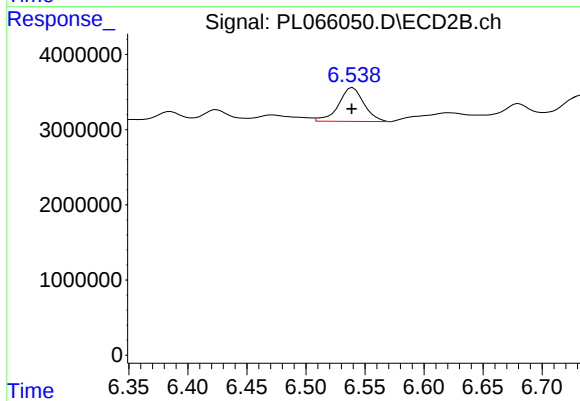

#12 4,4'-DDE

R.T.: 6.540 min
Delta R.T.: 0.001 min
Response: 6678848
Conc: 2.68 ng/ml

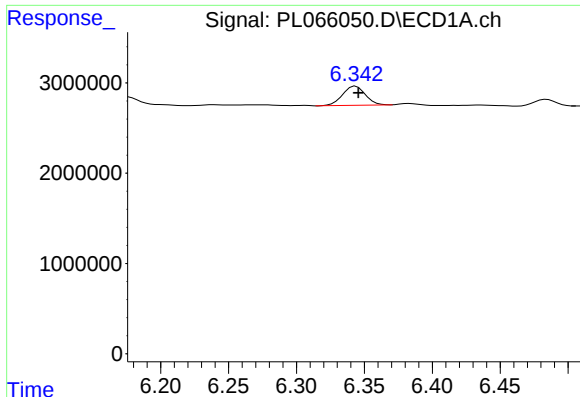


#17 4,4'-DDT

R.T.: 6.344 min
Delta R.T.: -0.002 min
Response: 2456398
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-040921


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:40 PM

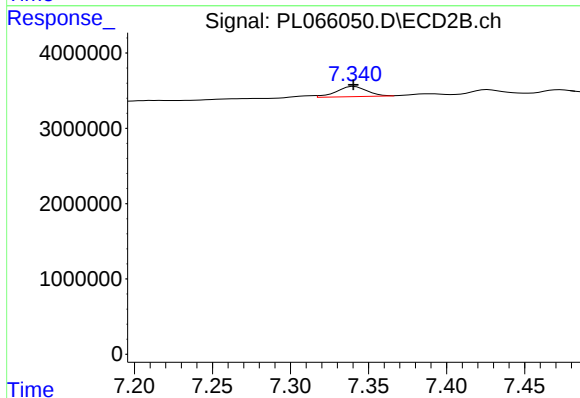


#17 4,4'-DDT

R.T.: 7.340 min
Delta R.T.: 0.000 min
Response: 1843577
Conc: 0.97 ng/ml m

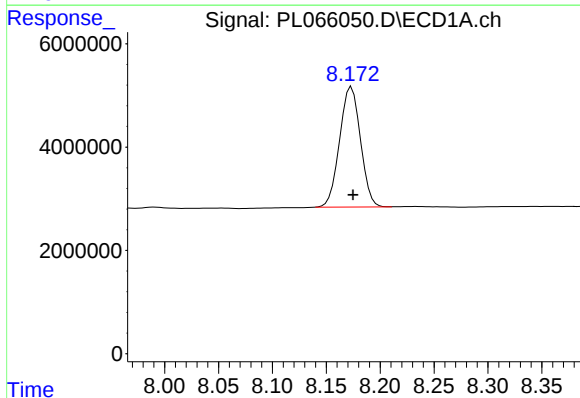

#28 Decachlorobiphenyl

R.T.: 8.173 min
Delta R.T.: -0.002 min
Response: 31388639
Conc: 14.55 ng/ml

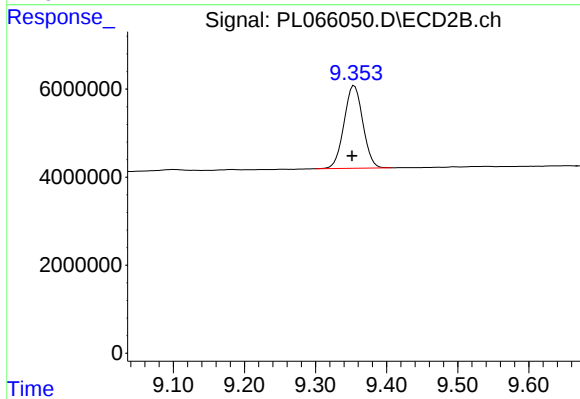

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.003 min
Response: 34542713
Conc: 18.22 ng/ml