

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
 Data File : PL066053.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2021 23:26
 Operator : AR\AJ
 Sample : M1997-04
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 801-675

Manual Integrations
 APPROVED

Ankita
 4/13/2021 3:31:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 01:38:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.154	25529290	35065605	10.513	12.722
28)	SA Decachlor...	8.173	9.354	27504290	30162517	12.750	15.913
Target Compounds							
11)	B alpha-Chl...	5.428	6.383	1540033	2628530	0.474m	0.959m#
12)	B 4,4'-DDE	5.595	6.540	4476842	6791644	1.466	2.726 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
Data File : PL066053.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2021 23:26
Operator : AR\AJ
Sample : M1997-04
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
801-675


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 01:38:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

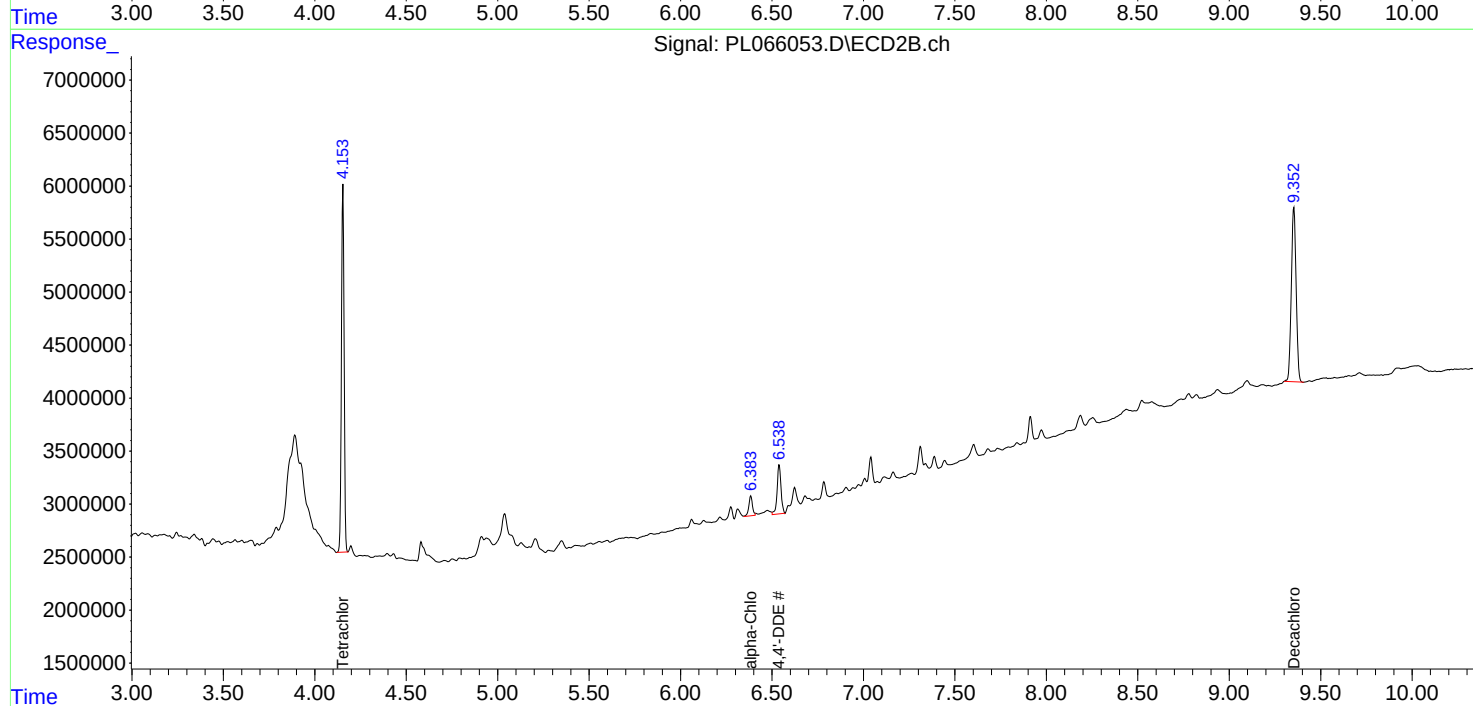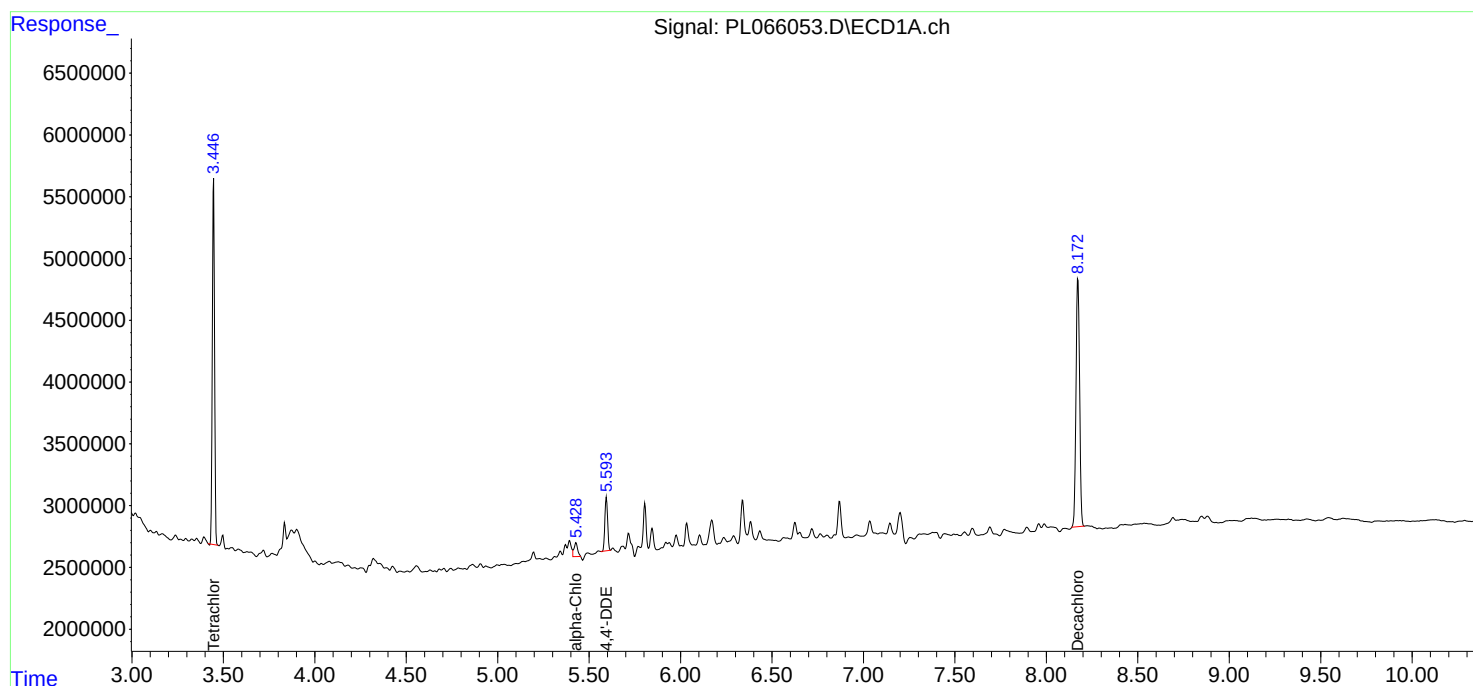

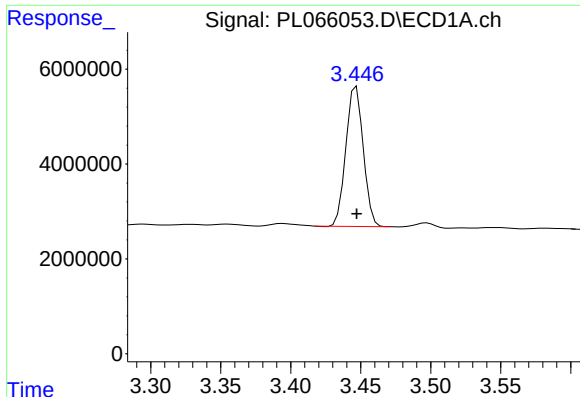


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 25529290
Conc: 10.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
801-675


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:48 PM

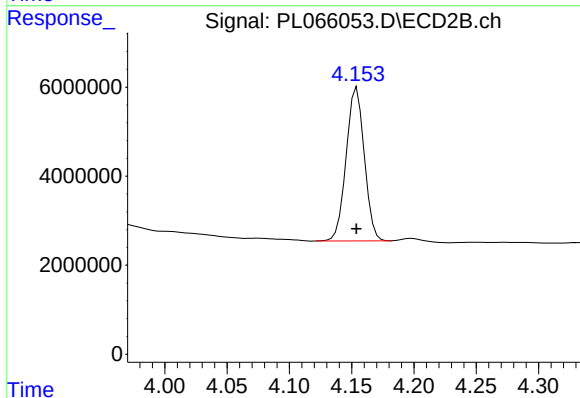


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 35065605
Conc: 12.72 ng/ml

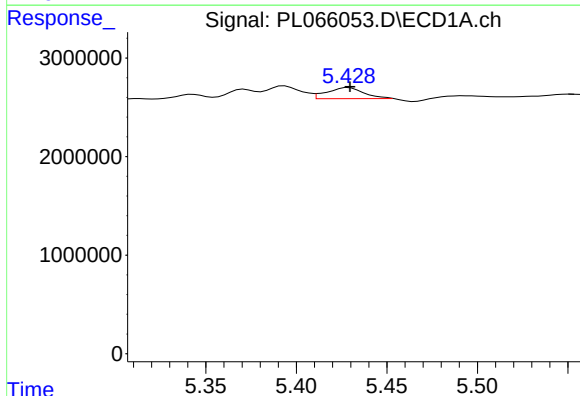


#11 alpha-Chlordane

R.T.: 5.428 min
Delta R.T.: -0.002 min
Response: 1540033
Conc: 0.47 ng/ml m

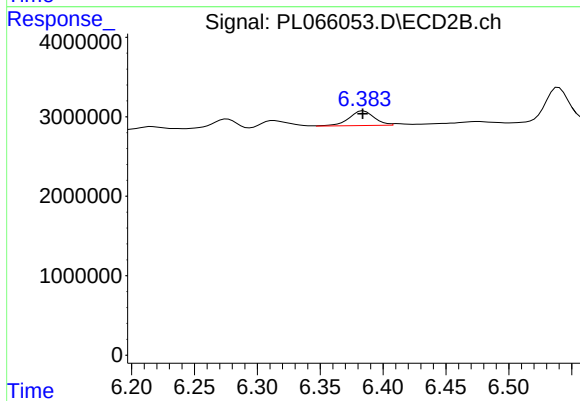

#11 alpha-Chlordane

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 2628530
Conc: 0.96 ng/ml m

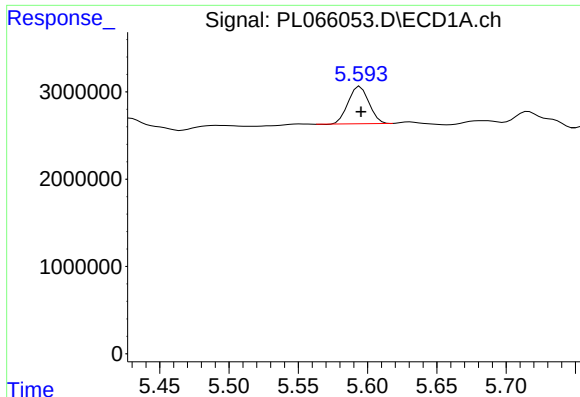


#12 4,4'-DDE

R.T.: 5.595 min
Delta R.T.: 0.000 min
Response: 4476842
Conc: 1.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
801-675


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:48 PM

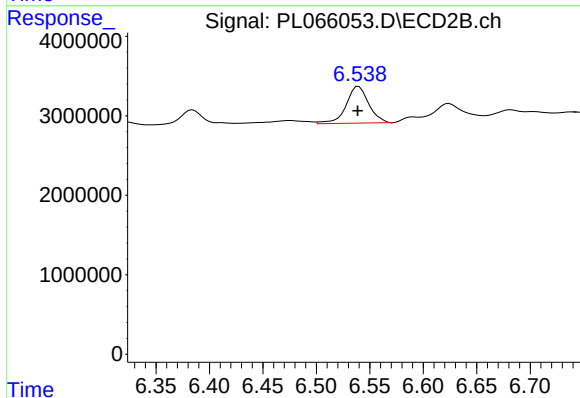


#12 4,4'-DDE

R.T.: 6.540 min
Delta R.T.: 0.001 min
Response: 6791644
Conc: 2.73 ng/ml

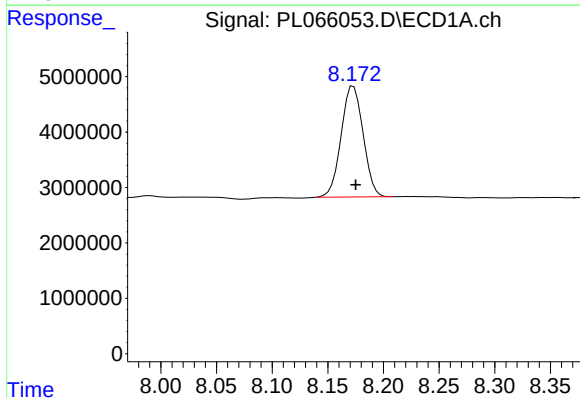

#28 Decachlorobiphenyl

R.T.: 8.173 min
Delta R.T.: -0.002 min
Response: 27504290
Conc: 12.75 ng/ml

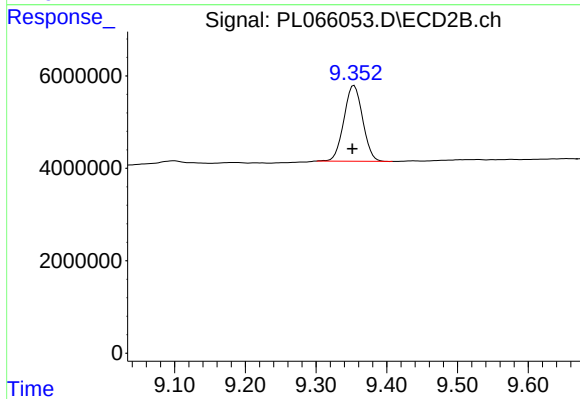

#28 Decachlorobiphenyl

R.T.: 9.354 min
Delta R.T.: 0.002 min
Response: 30162517
Conc: 15.91 ng/ml