

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
 Data File : PL066057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2021 00:23
 Operator : AR\AJ
 Sample : M1998-04
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-3D

Manual Integrations
 APPROVED

Ankita
 4/13/2021 3:31:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 01:39:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.155	27945750	37051333	11.508	13.442
28)	SA Decachlor...	8.173	9.354	30083454	35682806	13.945	18.825 #
Target Compounds							
12)	B 4,4'-DDE	5.593	6.541	156.5E6	188.4E6	51.234m	75.622 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
Data File : PL066057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2021 00:23
Operator : AR\AJ
Sample : M1998-04
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-3D


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 01:39:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

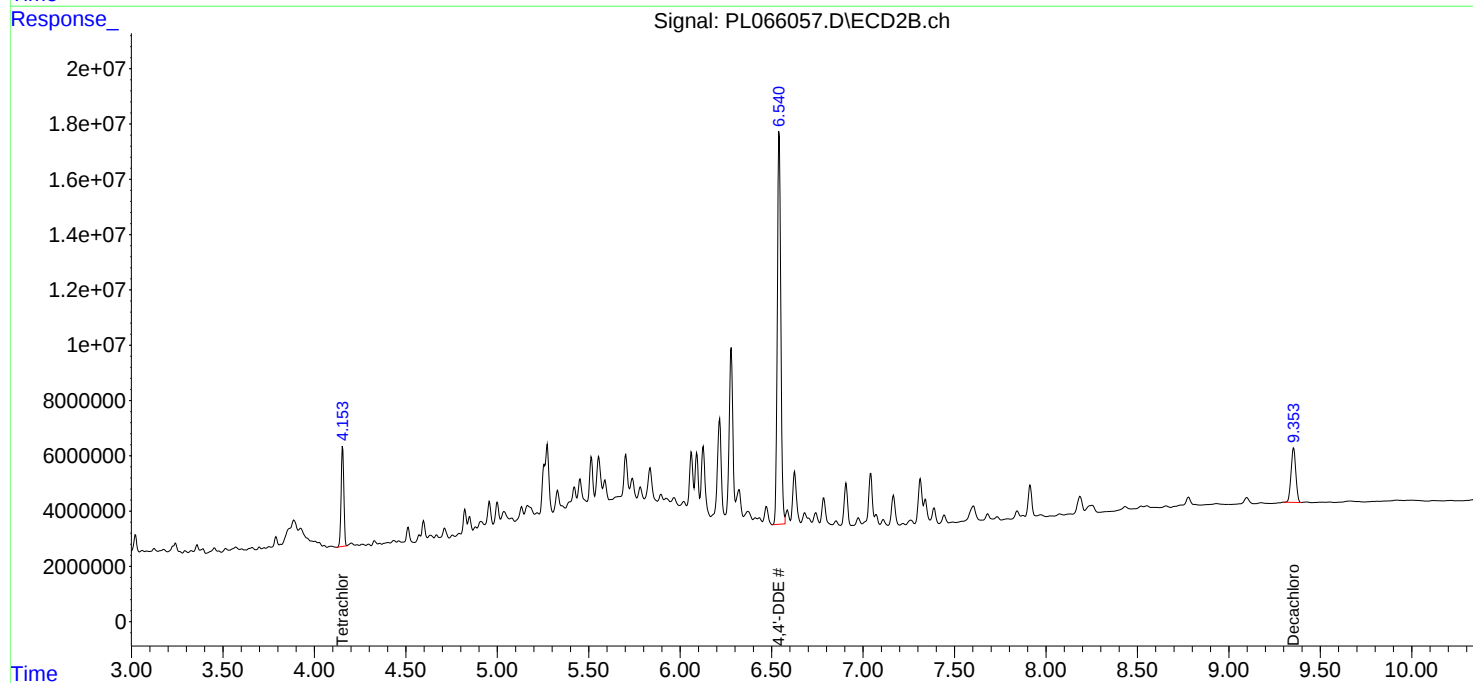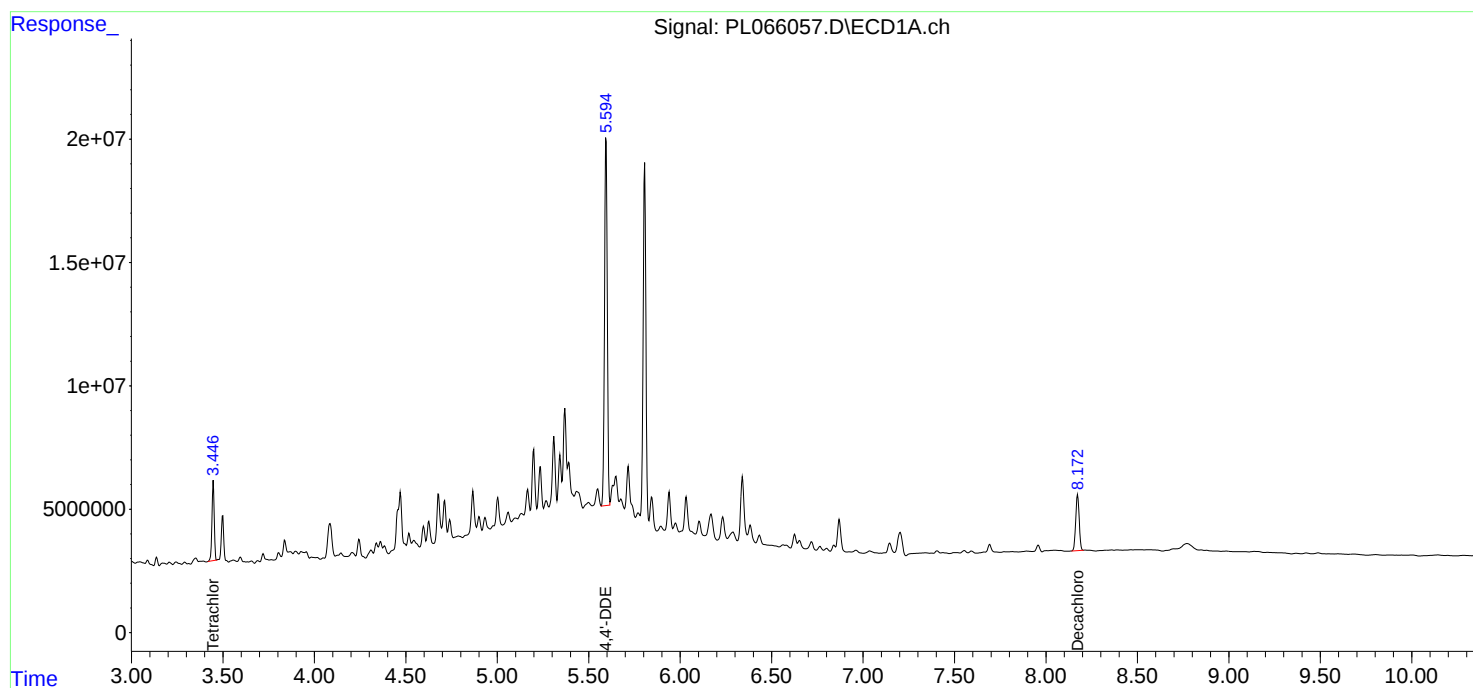

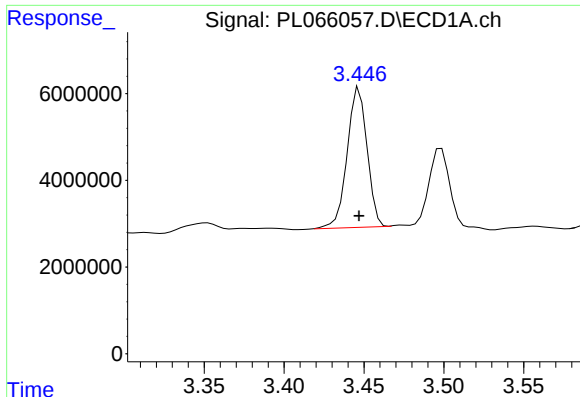


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 27945750
Conc: 11.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-3D


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:52 PM

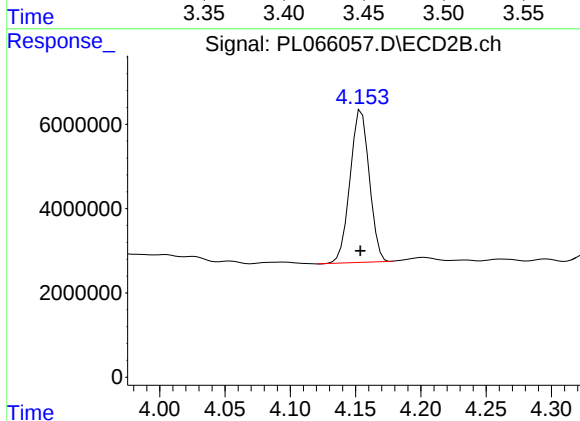


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.000 min
Response: 37051333
Conc: 13.44 ng/ml

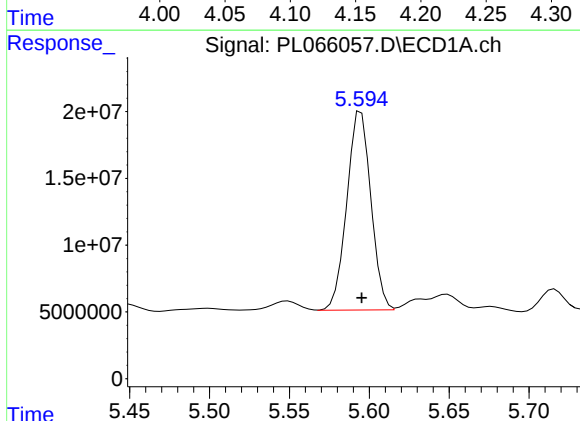


#12 4,4'-DDE

R.T.: 5.593 min
Delta R.T.: -0.002 min
Response: 156452444
Conc: 51.23 ng/ml m

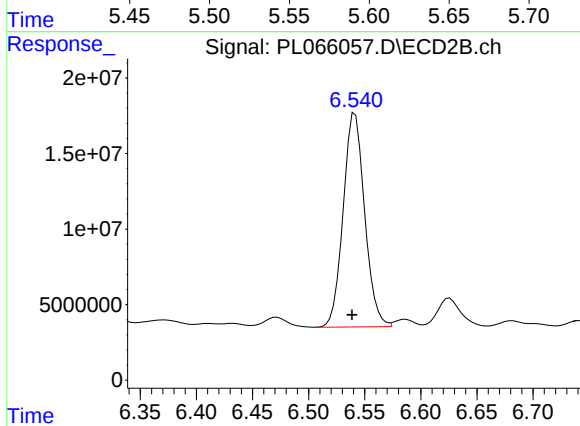

#12 4,4'-DDE

R.T.: 6.541 min
Delta R.T.: 0.003 min
Response: 188385078
Conc: 75.62 ng/ml

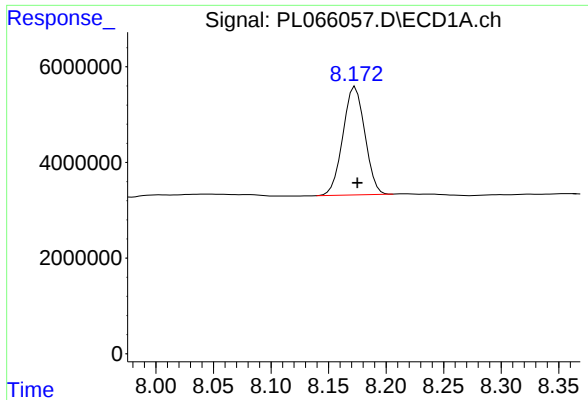


#28 Decachlorobiphenyl

R.T.: 8.173 min
Delta R.T.: -0.002 min
Response: 30083454
Conc: 13.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-3D

Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:52 PM

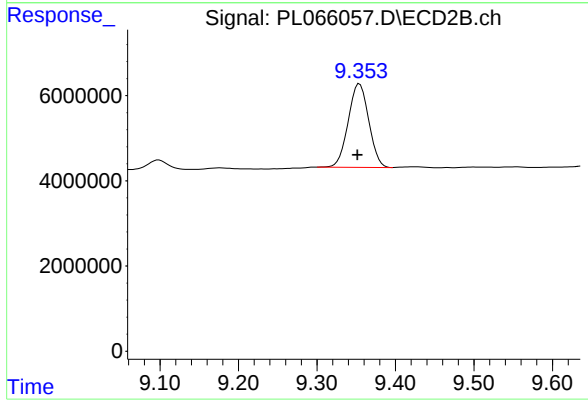

#28 Decachlorobiphenyl

R.T.: 9.354 min
Delta R.T.: 0.003 min
Response: 35682806
Conc: 18.82 ng/ml