

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
 Data File : PL066058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2021 00:38
 Operator : AR\AJ
 Sample : M1998-05
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-4A

Manual Integrations
 APPROVED

Ankita
 4/13/2021 3:31:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 01:39:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.155	31079950	40777828	12.798	14.794
28)	SA Decachlor...	8.173	9.355	26876445	29648600	12.459	15.641 #
Target Compounds							
12)	B 4,4'-DDE	5.593	6.541	11947470	14751009	3.912m	5.921 #
17)	MA 4,4'-DDT	6.341	7.341	12989891	5800713	4.607	3.061 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
Data File : PL066058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2021 00:38
Operator : AR\AJ
Sample : M1998-05
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-4A


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 01:39:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

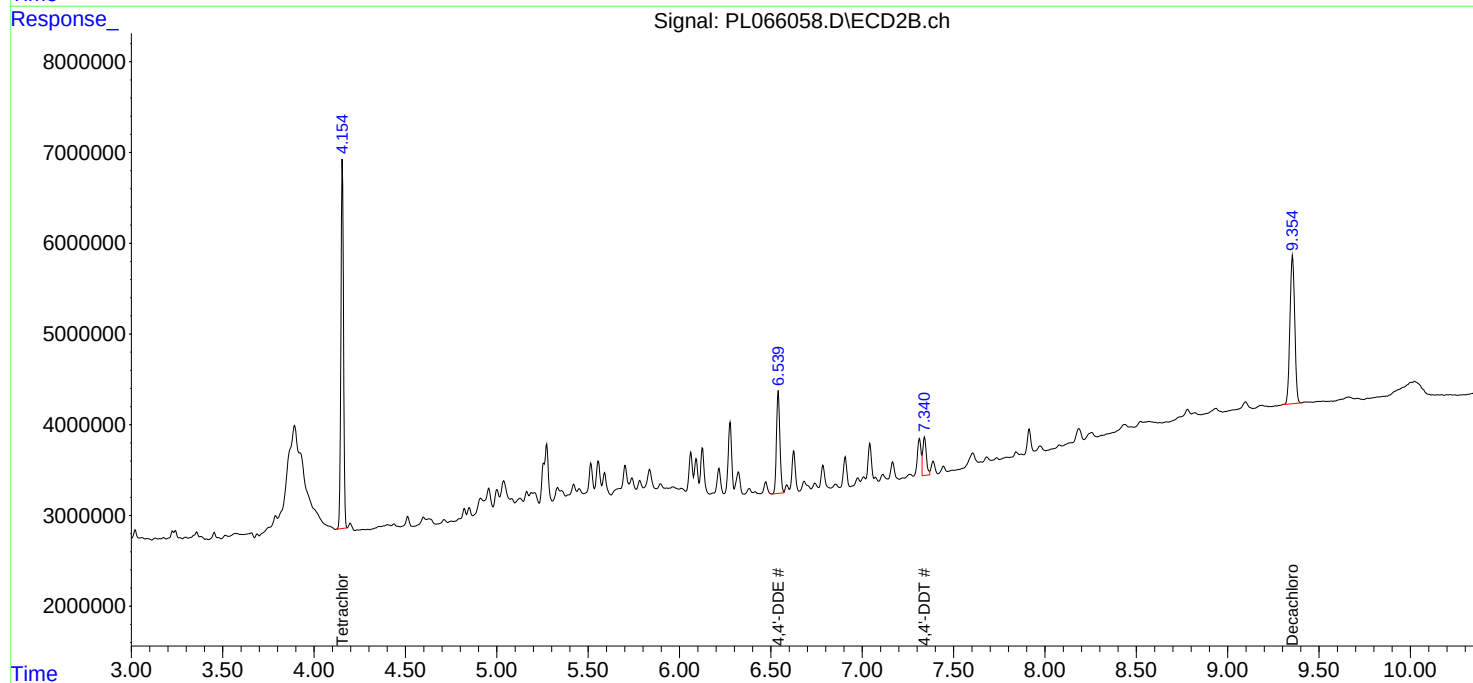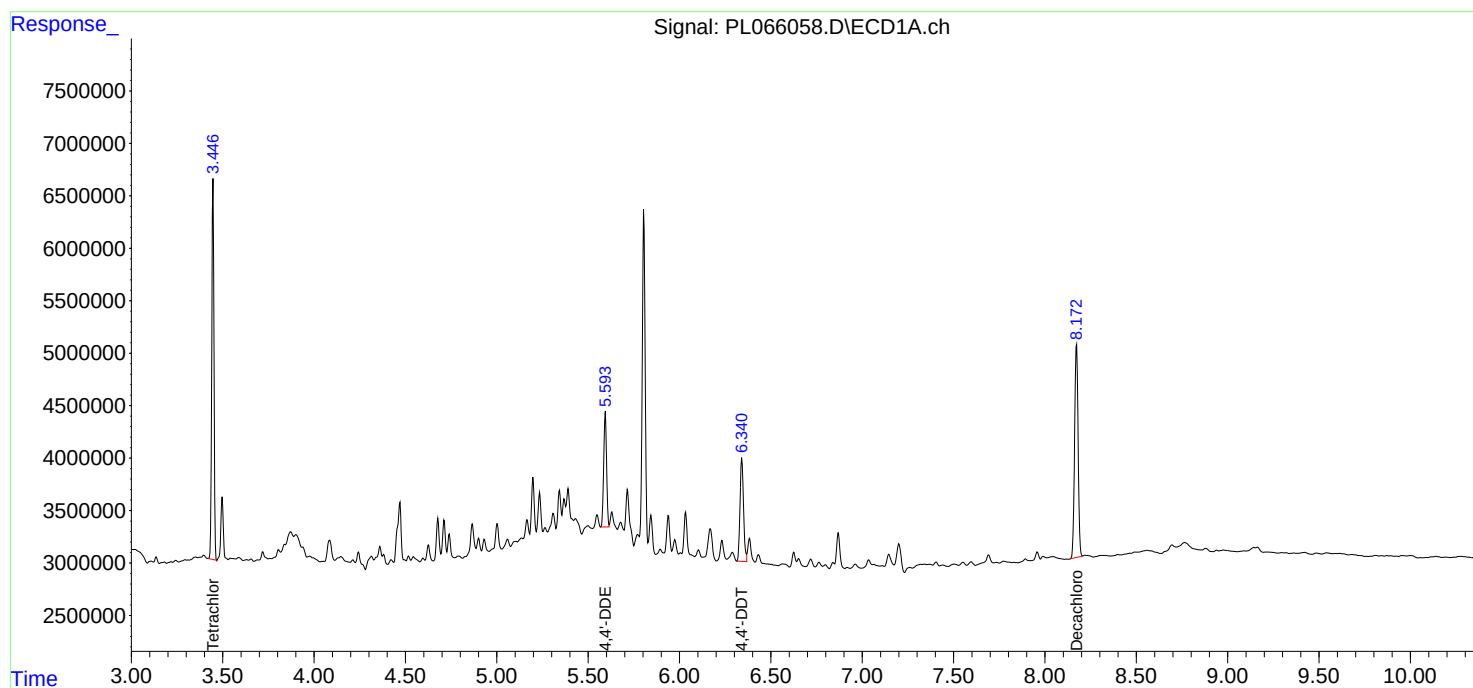

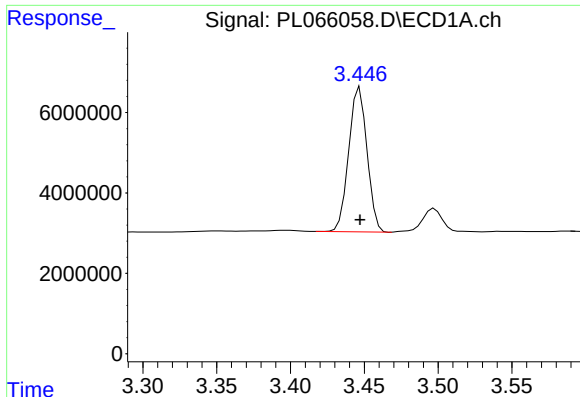


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 31079950
Conc: 12.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-4A


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:54 PM

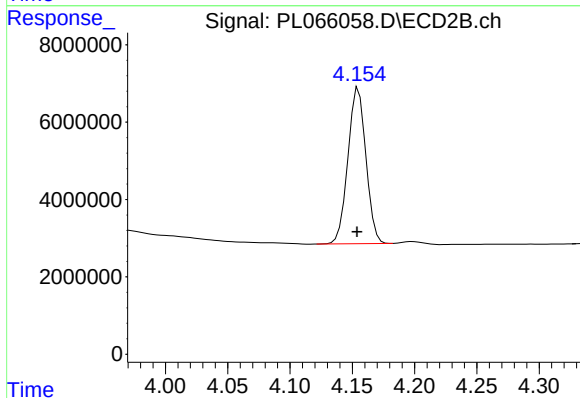


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.001 min
Response: 40777828
Conc: 14.79 ng/ml

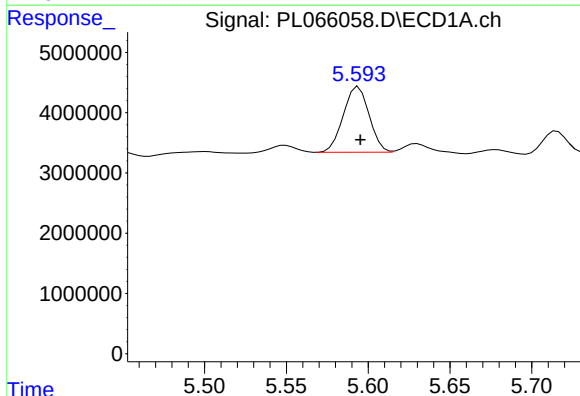


#12 4,4'-DDE

R.T.: 5.593 min
Delta R.T.: -0.003 min
Response: 11947470
Conc: 3.91 ng/ml m

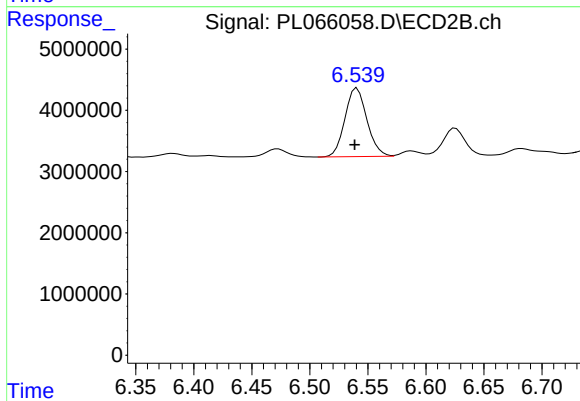

#12 4,4'-DDE

R.T.: 6.541 min
Delta R.T.: 0.002 min
Response: 14751009
Conc: 5.92 ng/ml

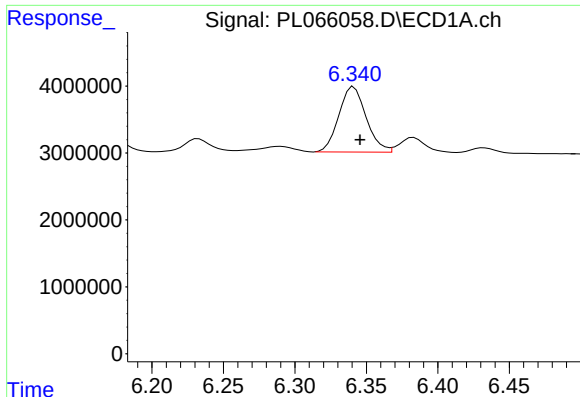


#17 4,4'-DDT

R.T.: 6.341 min
Delta R.T.: -0.004 min
Response: 12989891
Conc: 4.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-4A


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:54 PM

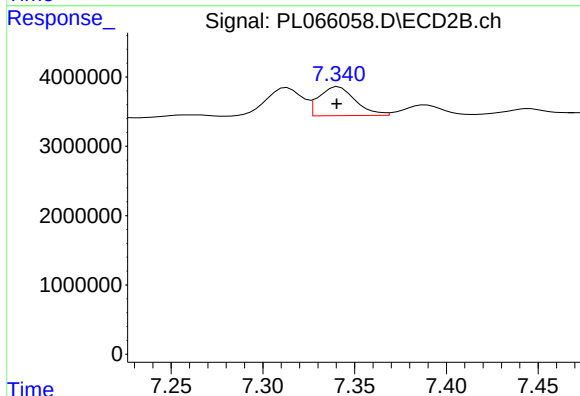


#17 4,4'-DDT

R.T.: 7.341 min
Delta R.T.: 0.001 min
Response: 5800713
Conc: 3.06 ng/ml

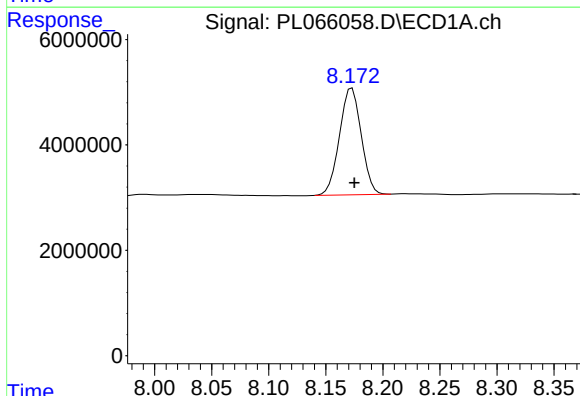

#28 Decachlorobiphenyl

R.T.: 8.173 min
Delta R.T.: -0.002 min
Response: 26876445
Conc: 12.46 ng/ml

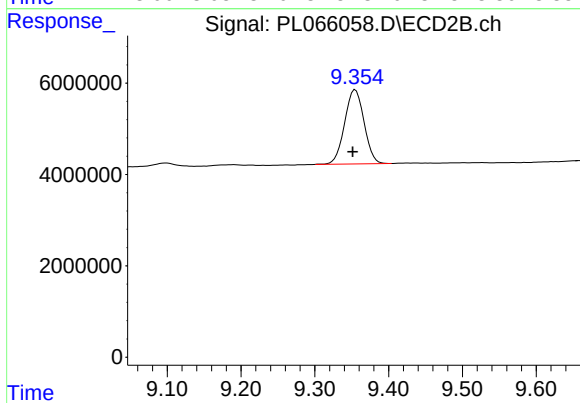

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.003 min
Response: 29648600
Conc: 15.64 ng/ml