

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
 Data File : PL066061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2021 01:21
 Operator : AR\AJ
 Sample : M1998-11
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-5B

Manual Integrations
 APPROVED

Ankita
 4/13/2021 3:31:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 04:47:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.447	4.155	20715576	28173227	8.530	10.221
28) SA Decachlor...	8.173	9.355	19591715	23330060	9.082	12.308 #
Target Compounds						
12) B 4,4'-DDE	5.593	6.541	186.5E6	213.0E6	61.064m	85.484 #
17) MA 4,4'-DDT	6.341	7.341	44437887	15583671	15.762	8.223 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041221\
Data File : PL066061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2021 01:21
Operator : AR\AJ
Sample : M1998-11
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-5B


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 04:47:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

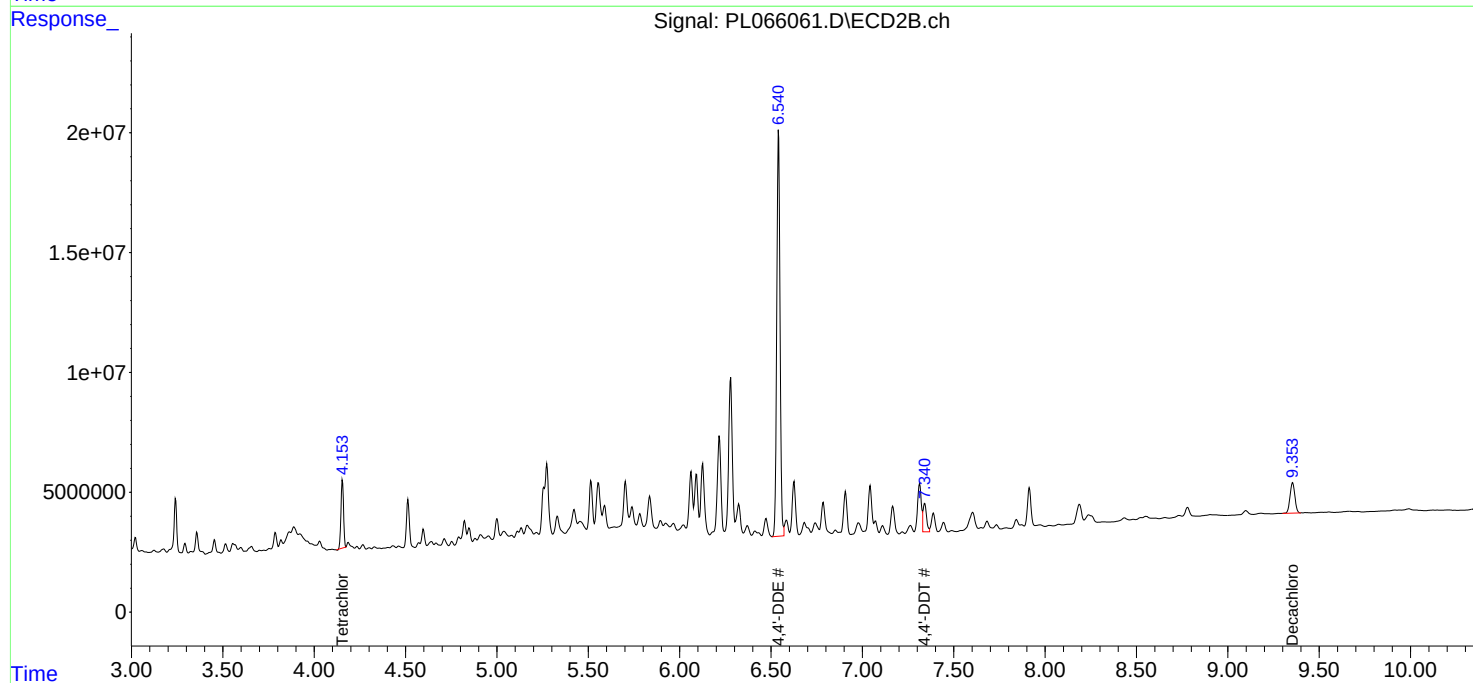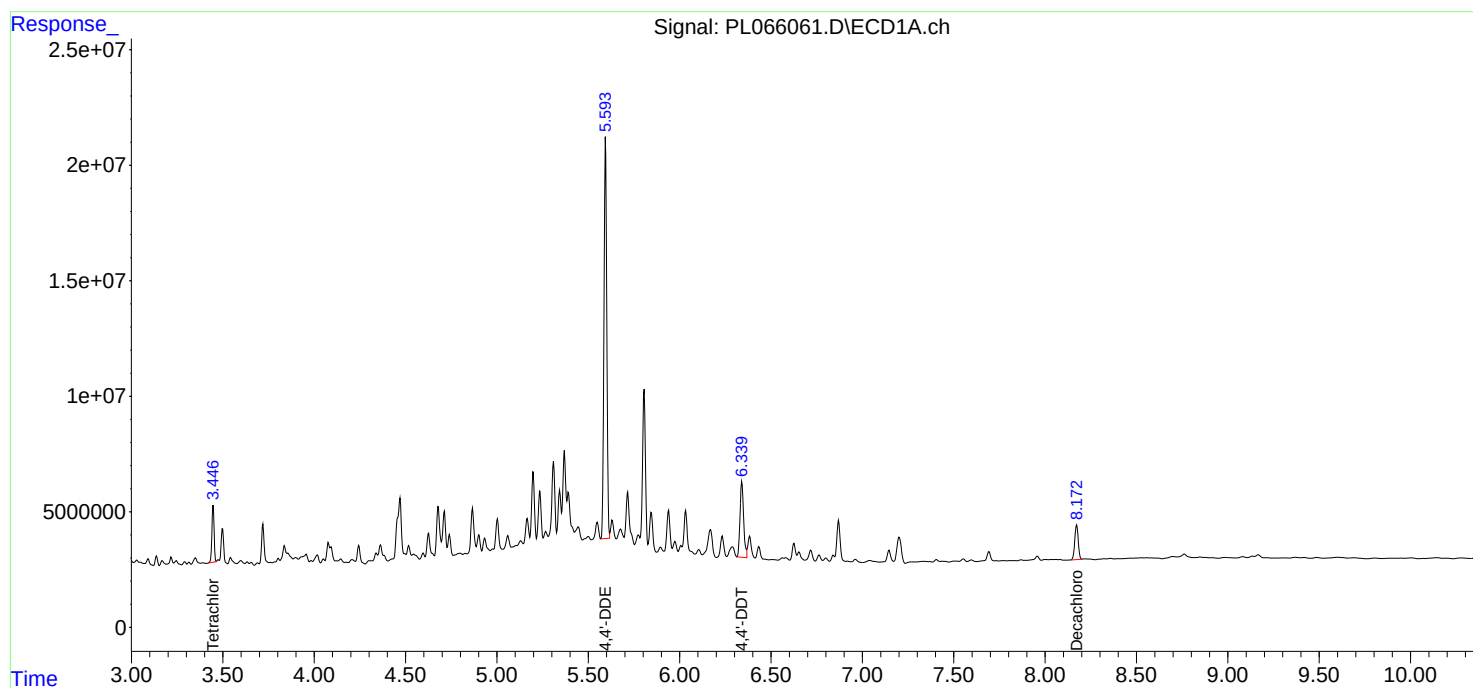

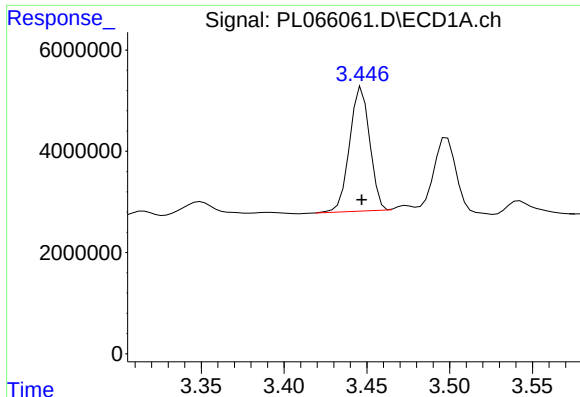


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 20715576
Conc: 8.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-5B


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:59 PM

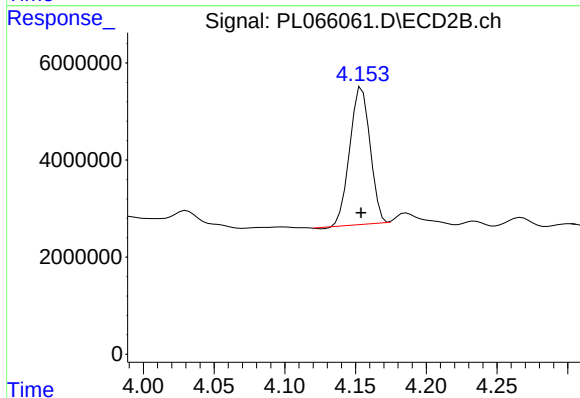


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.000 min
Response: 28173227
Conc: 10.22 ng/ml

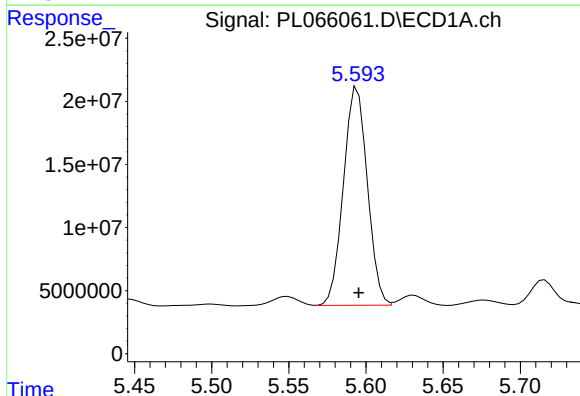


#12 4,4'-DDE

R.T.: 5.593 min
Delta R.T.: -0.002 min
Response: 186471220
Conc: 61.06 ng/ml m

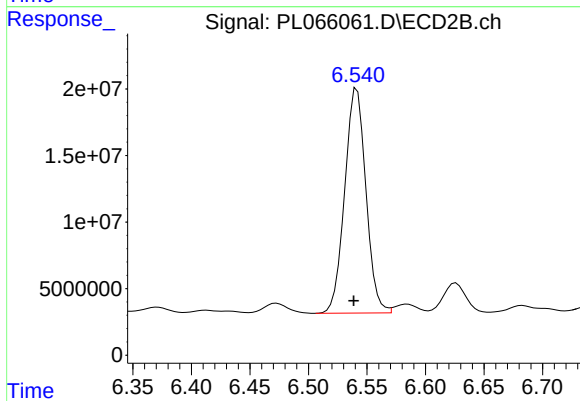

#12 4,4'-DDE

R.T.: 6.541 min
Delta R.T.: 0.003 min
Response: 212951771
Conc: 85.48 ng/ml

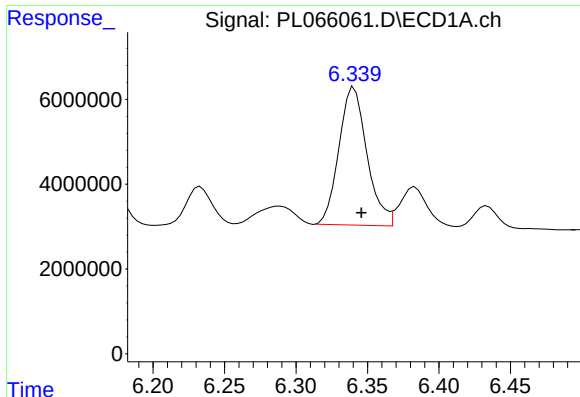


#17 4,4'-DDT

R.T.: 6.341 min
Delta R.T.: -0.005 min
Response: 44437887
Conc: 15.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-5B


Manual Integrations
APPROVED

Ankita
4/13/2021 3:31:59 PM

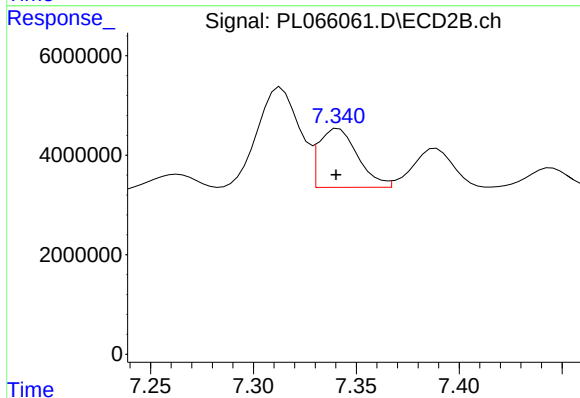


#17 4,4'-DDT

R.T.: 7.341 min
Delta R.T.: 0.001 min
Response: 15583671
Conc: 8.22 ng/ml

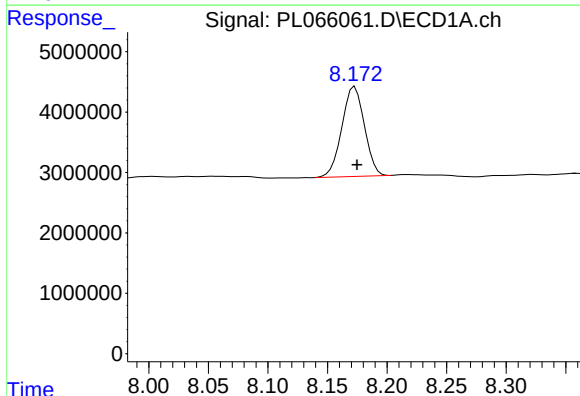

#28 Decachlorobiphenyl

R.T.: 8.173 min
Delta R.T.: -0.002 min
Response: 19591715
Conc: 9.08 ng/ml

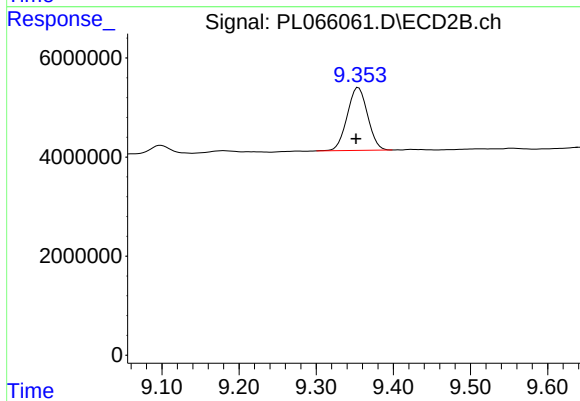

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.003 min
Response: 23330060
Conc: 12.31 ng/ml