

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041222\
 Data File : PL073983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2022 16:29
 Operator : AR\AJ
 Sample : PB144061BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 19:05:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 08 15:48:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.647	5.487	6677128	36777891	20.665	20.627
28)	SA Decachlor...	10.416	11.333	10509699	35130985	20.210	19.890
Target Compounds							
5)	MB Aldrin	0.000	7.470	0	117522	N.D.	0.050 #
6)	B beta-BHC	6.131f	6.686	37978	2306041	0.186	2.046 #
7)	B delta-BHC	0.000	6.957	0	709988	N.D.	0.291 #
10)	B gamma-Chl...	7.334f	8.192	6514	939849	0.015	0.421 #
14)	MA Endrin	8.093f	8.848	182107	27752	0.448	0.016 #
15)	B Endosulfa...	0.000	9.056	0	1281815	N.D.	0.738 #
19)	B Endosulfa...	8.806	0.000	43667	0	0.102	N.D. #
24)	Chlordane-2	0.000	7.470f	0	117522	N.D.	1.422 #
25)	Chlordane-3	7.334f	8.192	6514	939849	0.151	2.778 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041222\
Data File : PL073983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2022 16:29
Operator : AR\AJ
Sample : PB144061BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 19:05:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Fri Apr 08 15:48:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

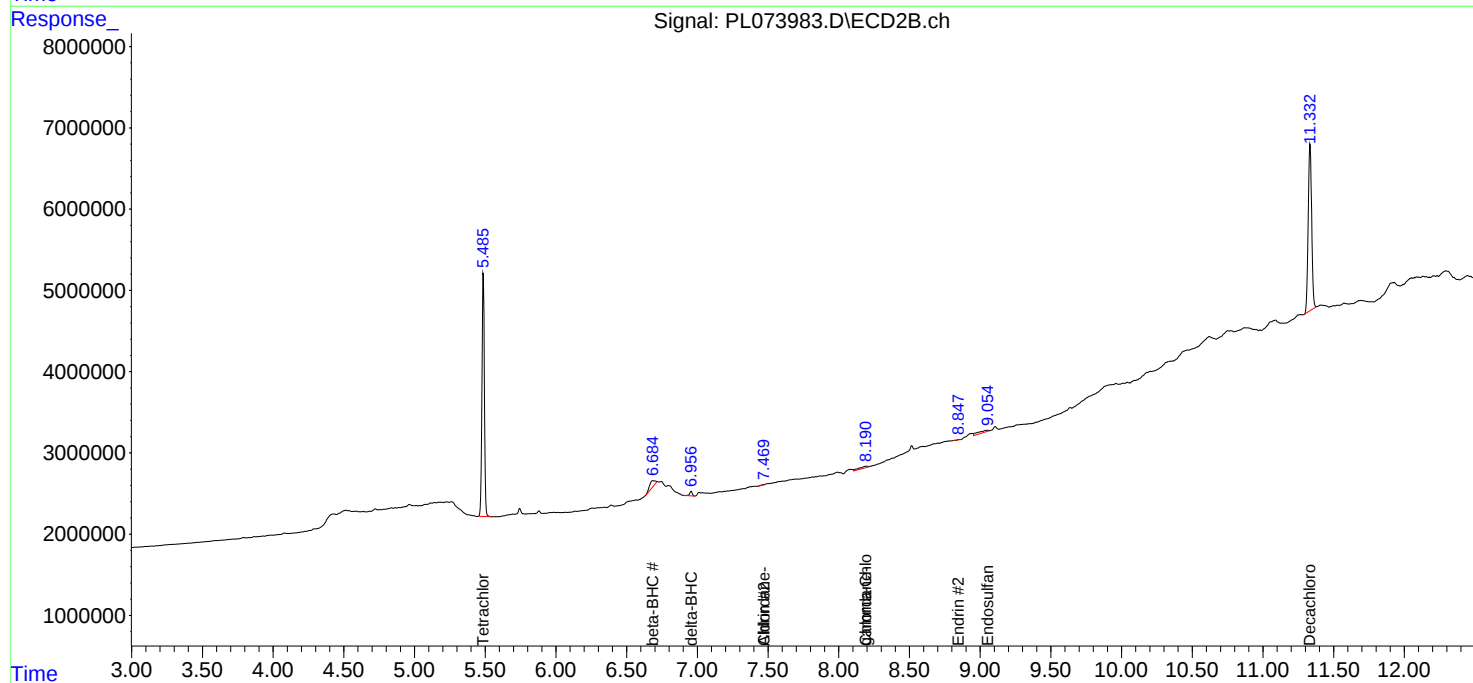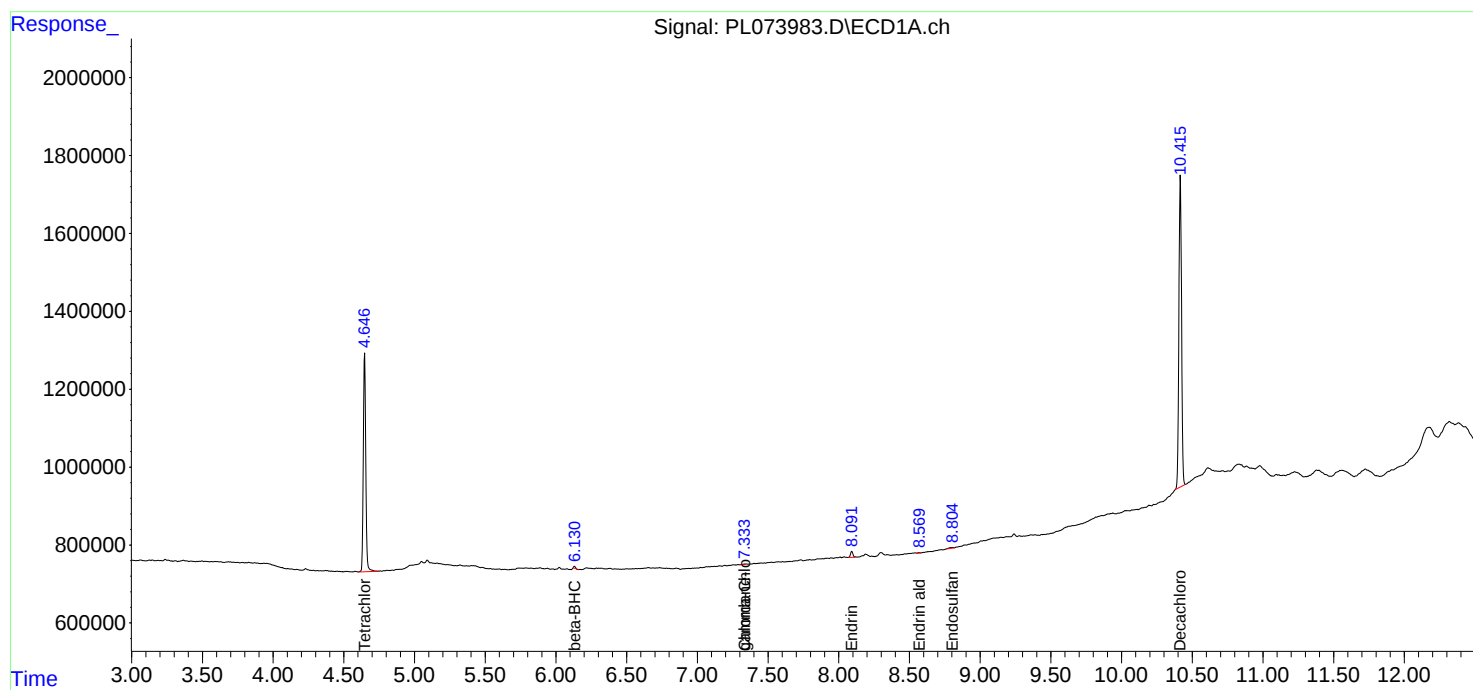


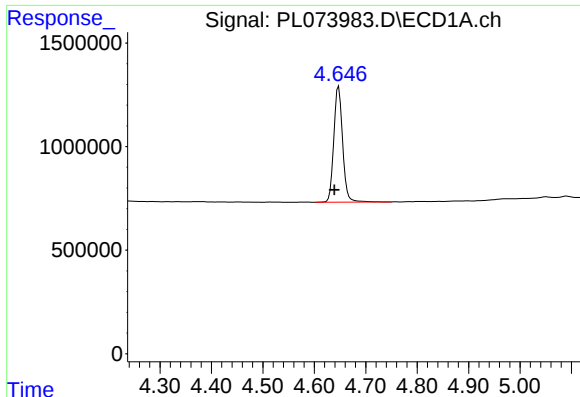

#1 Tetrachloro-m-xylene


R.T.: 4.647 min
Delta R.T.: 0.008 min
Response: 6677128
Conc: 20.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

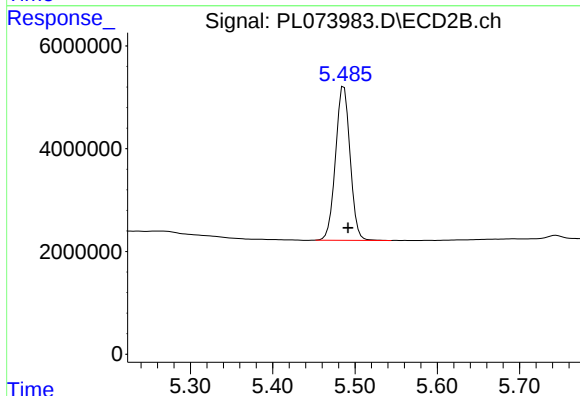


#1 Tetrachloro-m-xylene

R.T.: 5.487 min
Delta R.T.: -0.005 min
Response: 36777891
Conc: 20.63 ng/ml

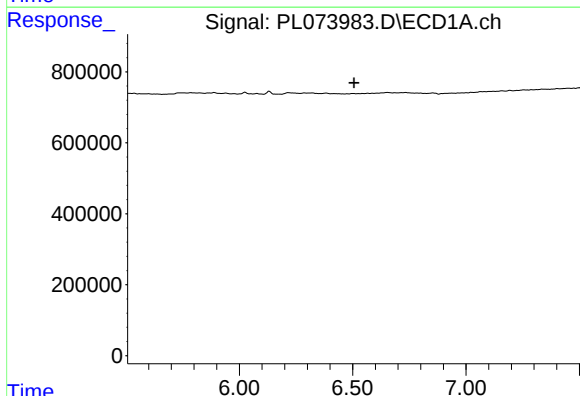


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.507 min
Response: 0
Conc: N.D.

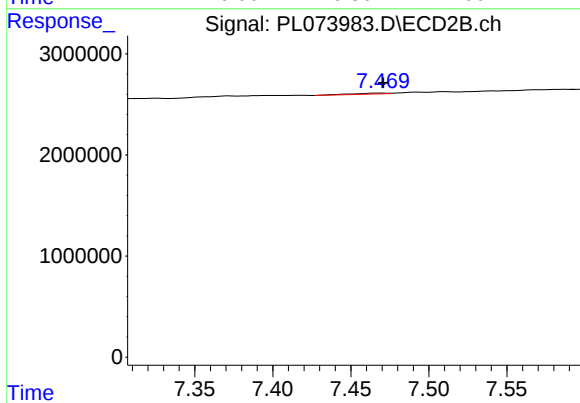

#5 Aldrin


R.T.: 7.470 min
Delta R.T.: -0.001 min
Response: 117522
Conc: 0.05 ng/ml

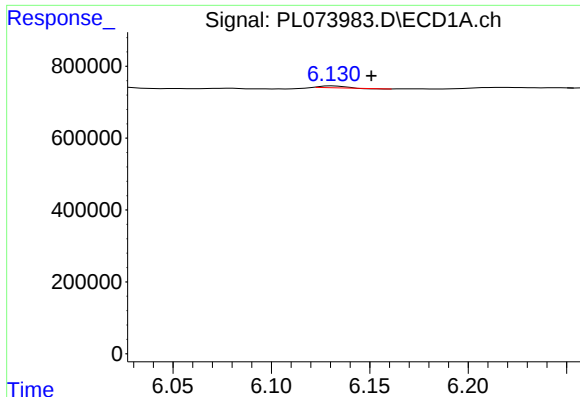

#6 beta-BHC


R.T.: 6.131 min
Delta R.T.: -0.020 min
Response: 37978
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

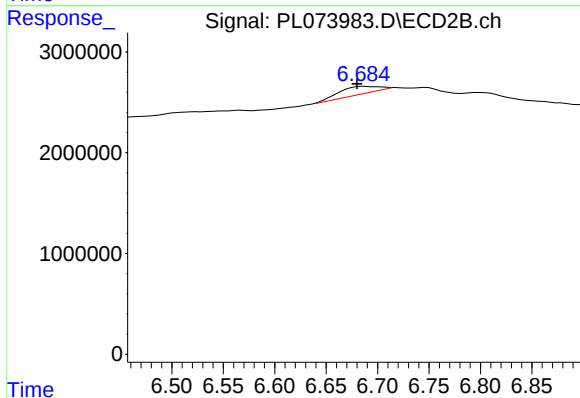


#6 beta-BHC

R.T.: 6.686 min
Delta R.T.: 0.006 min
Response: 2306041
Conc: 2.05 ng/ml

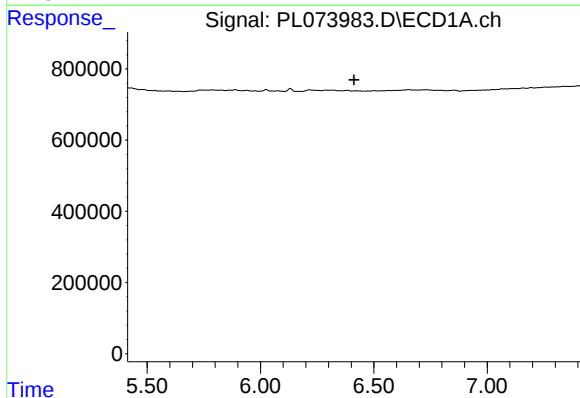


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.412 min
Response: 0
Conc: N.D.

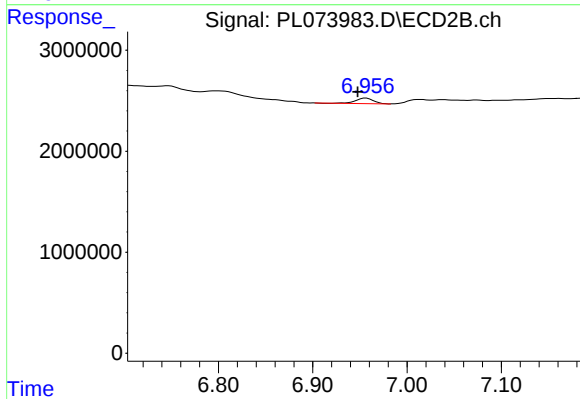

#7 delta-BHC


R.T.: 6.957 min
Delta R.T.: 0.009 min
Response: 709988
Conc: 0.29 ng/ml

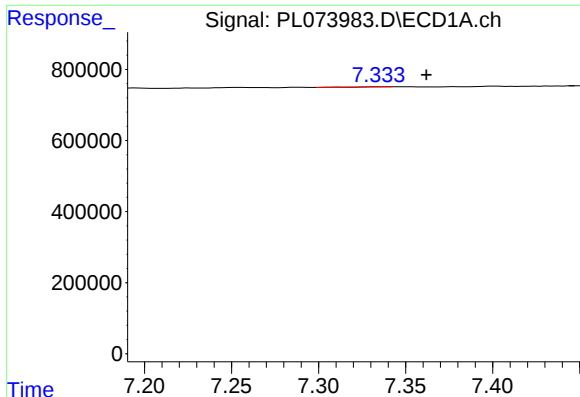

#10 gamma-Chlordane


R.T.: 7.334 min
Delta R.T.: -0.028 min
Response: 6514
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

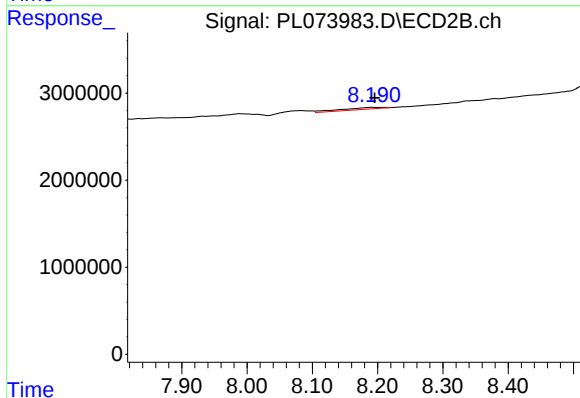


#10 gamma-Chlordane

R.T.: 8.192 min
Delta R.T.: -0.004 min
Response: 939849
Conc: 0.42 ng/ml

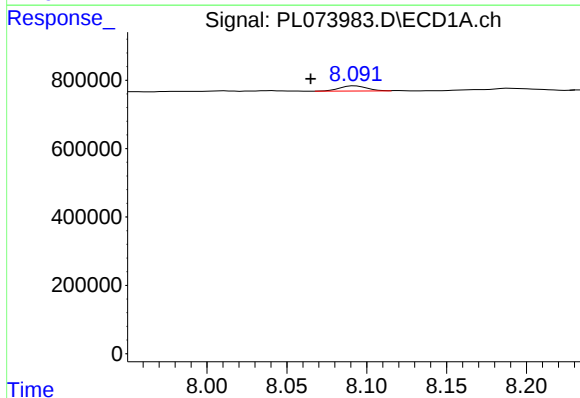


#14 Endrin

R.T.: 8.093 min
Delta R.T.: 0.028 min
Response: 182107
Conc: 0.45 ng/ml

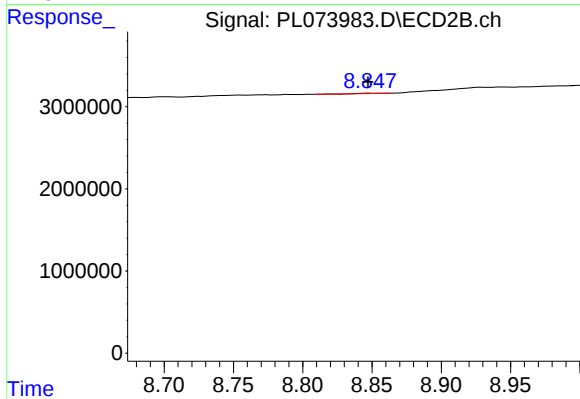

#14 Endrin


R.T.: 8.848 min
Delta R.T.: 0.000 min
Response: 27752
Conc: 0.02 ng/ml

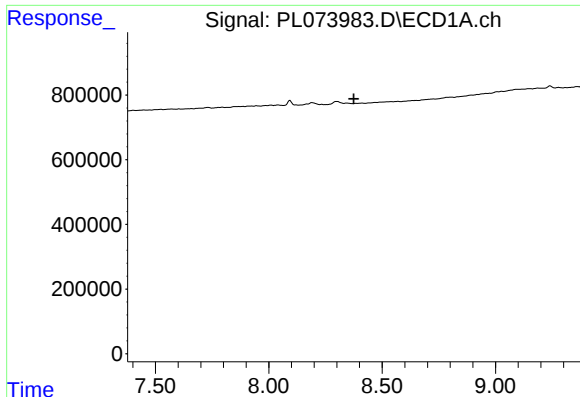

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

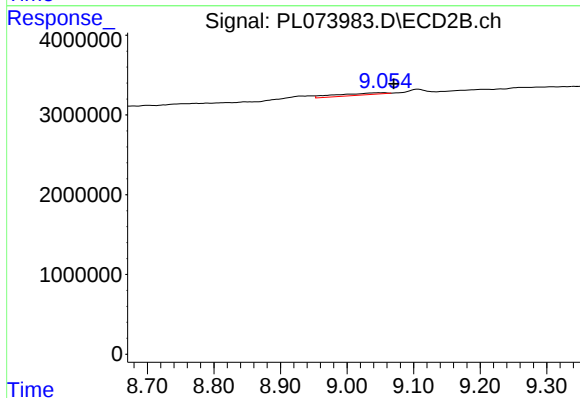


#15 Endosulfan II

R.T.: 9.056 min
Delta R.T.: -0.015 min
Response: 1281815
Conc: 0.74 ng/ml

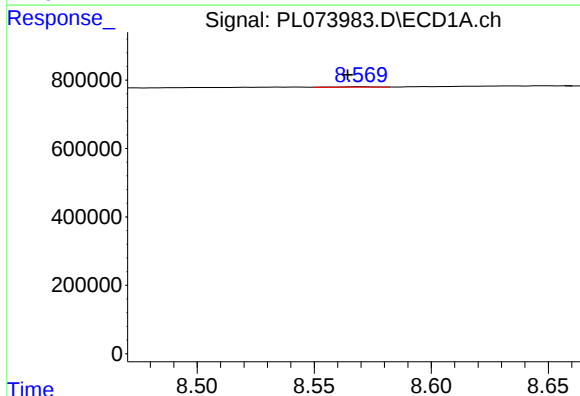


#18 Endrin aldehyde

R.T.: 8.570 min
Delta R.T.: 0.006 min
Response: 15680
Conc: 0.05 ng/ml

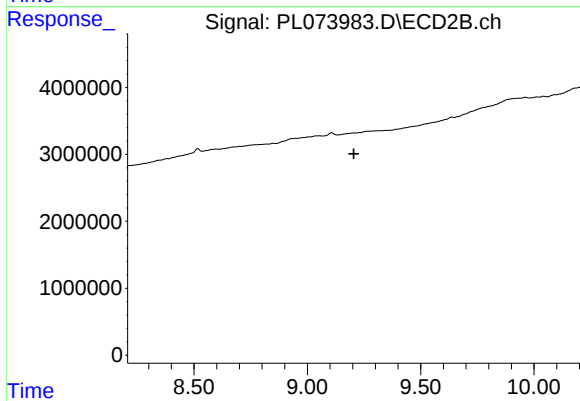

#18 Endrin aldehyde


R.T.: 9.212 min
Delta R.T.: 0.008 min
Response: -315126
Conc: N.D.

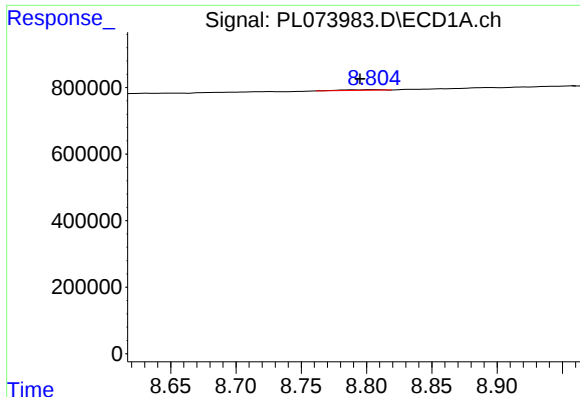

#19 Endosulfan Sulfate


R.T.: 8.806 min
Delta R.T.: 0.011 min
Response: 43667
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

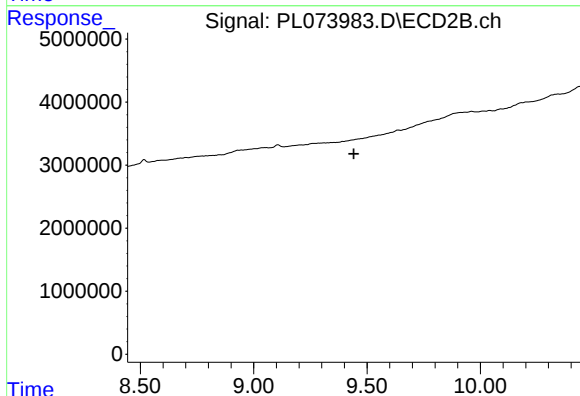


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.442 min
Response: 0
Conc: N.D.

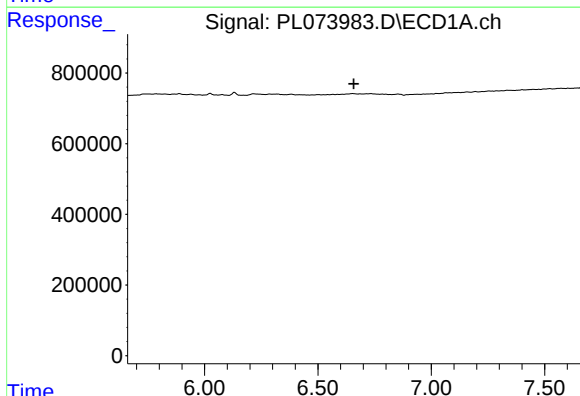


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.659 min
Response: 0
Conc: N.D.

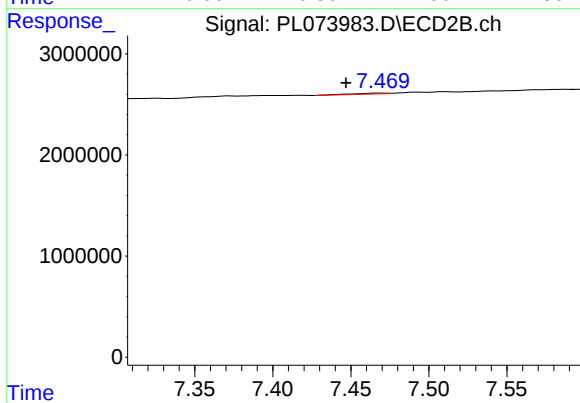

#24 Chlordane-2


R.T.: 7.470 min
Delta R.T.: 0.023 min
Response: 117522
Conc: 1.42 ng/ml

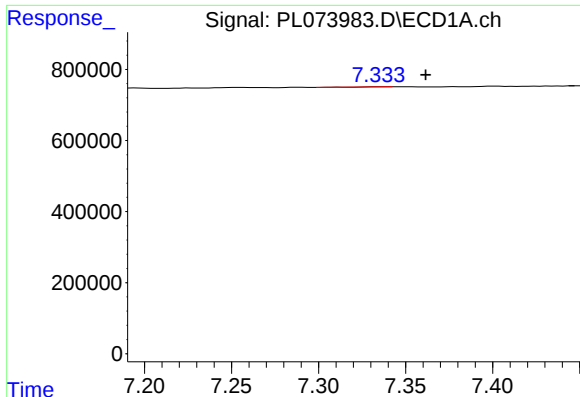

#25 Chlordane-3


R.T.: 7.334 min
Delta R.T.: -0.027 min
Response: 6514
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

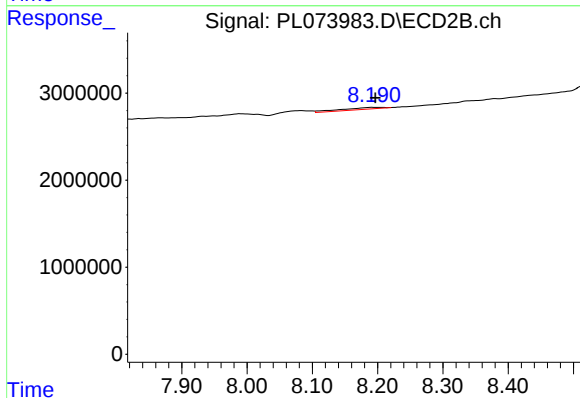


#25 Chlordane-3

R.T.: 8.192 min
Delta R.T.: -0.005 min
Response: 939849
Conc: 2.78 ng/ml

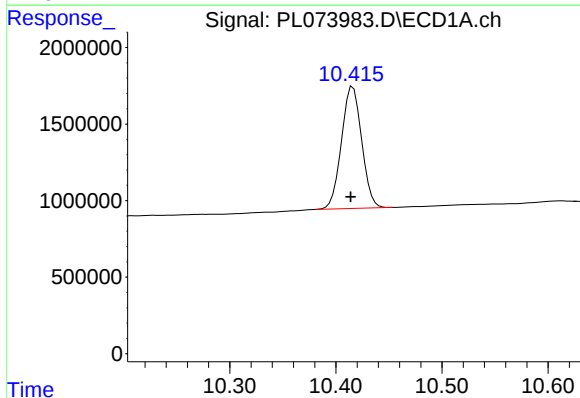

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: 0.002 min
Response: 10509699
Conc: 20.21 ng/ml

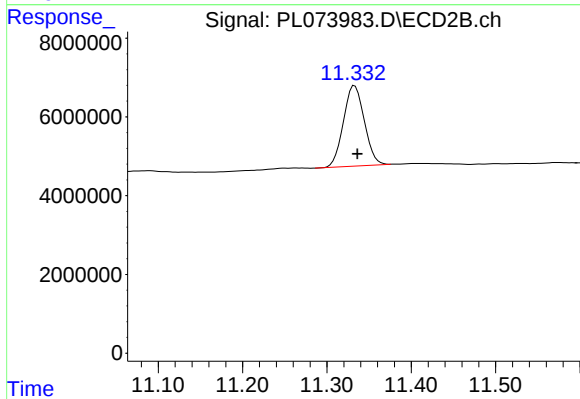

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: -0.003 min
Response: 35130985
Conc: 19.89 ng/ml