

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041224\
 Data File : PL089004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2024 15:21
 Operator : AR\AJ
 Sample : P2019-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB205-WATER

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/11/2024
 Supervised By : Ankita Jodhani 04/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 15:31:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.639	2.852	51195142	28012219	19.319m	21.019m
2) SA Decachlor...	9.307	8.080	32279074	20419814	13.058	15.060

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041224\
Data File : PL089004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2024 15:21
Operator : AR\AJ
Sample : P2019-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NB205-WATER


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/11/2024
Supervised By : Ankita Jodhani 04/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 15:31:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

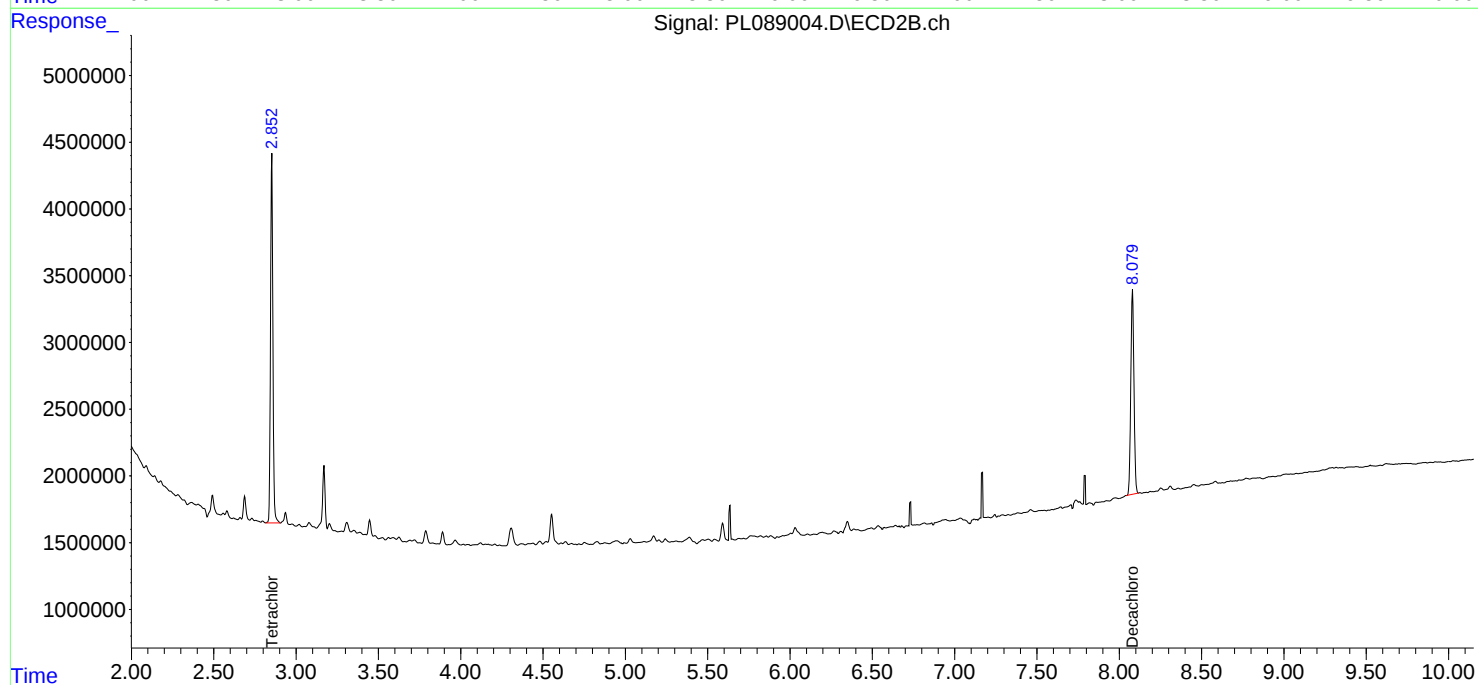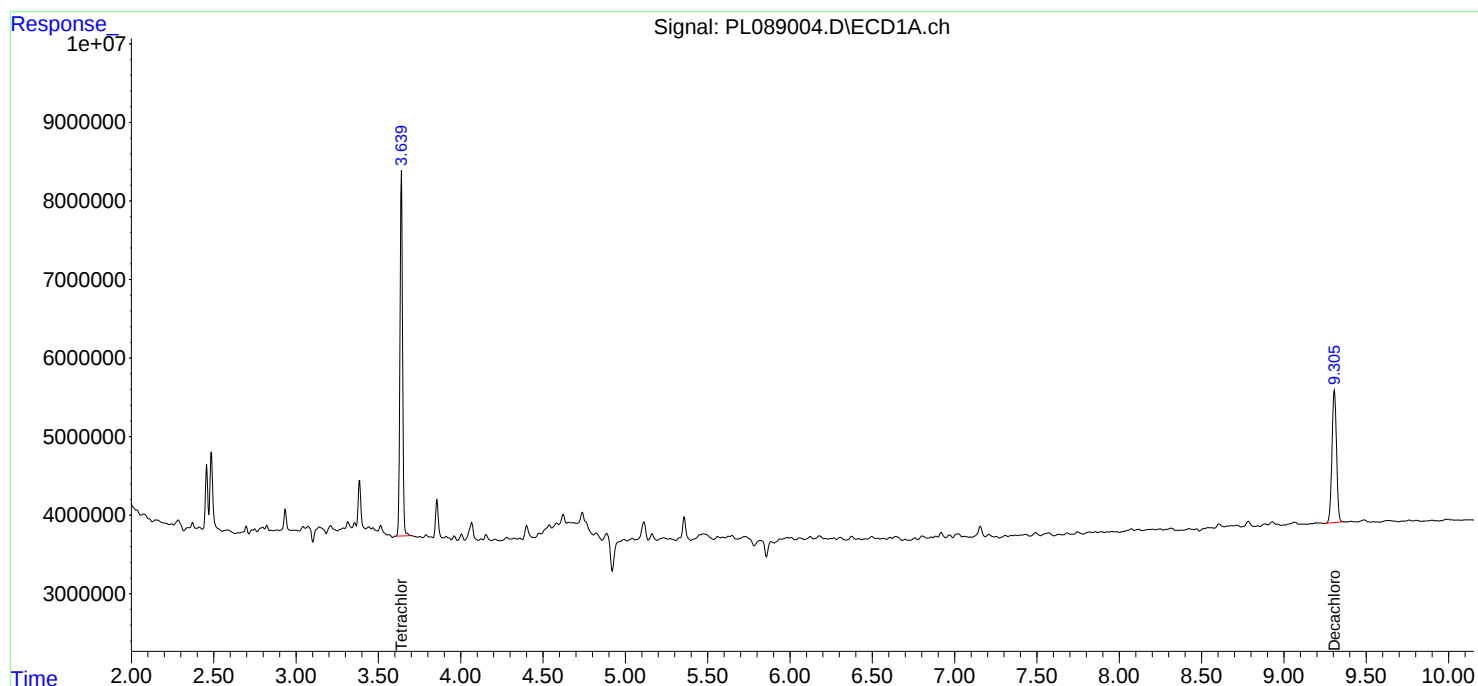

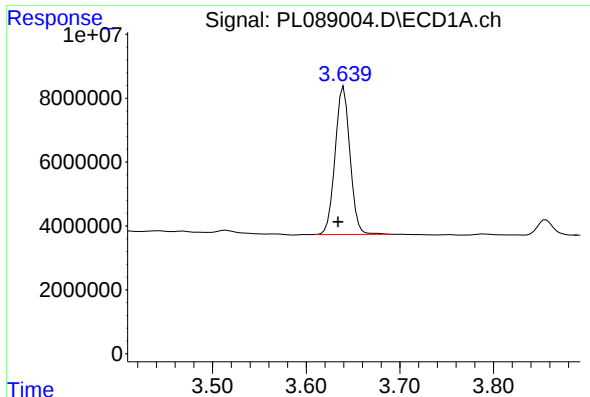


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: 0.005 min
Response: 51195142
Conc: 19.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB205-WATER


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/11/2024
Supervised By :Ankita Jodhani 04/11/2024

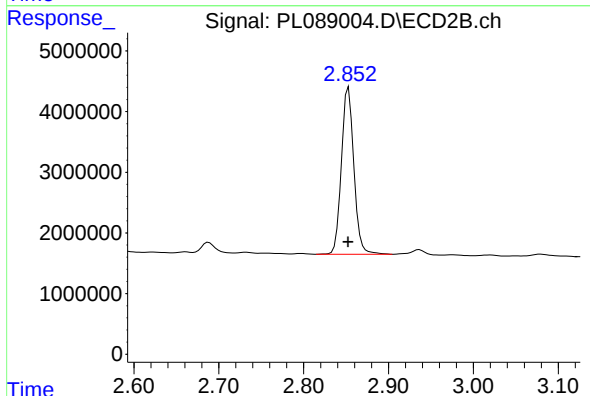


#1 Tetrachloro-m-xylene

R.T.: 2.852 min
Delta R.T.: 0.000 min
Response: 28012219
Conc: 21.02 ng/ml m

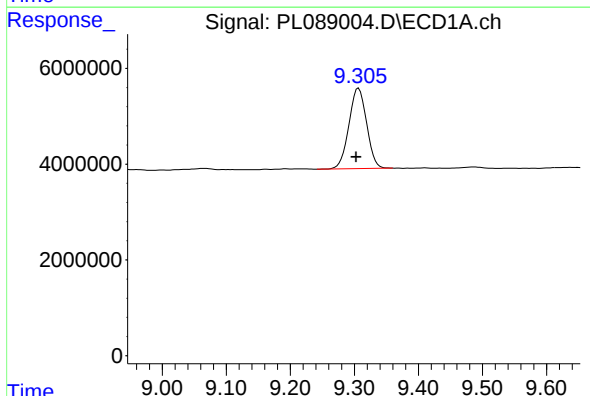

#28 Decachlorobiphenyl

R.T.: 9.307 min
Delta R.T.: 0.004 min
Response: 32279074
Conc: 13.06 ng/ml

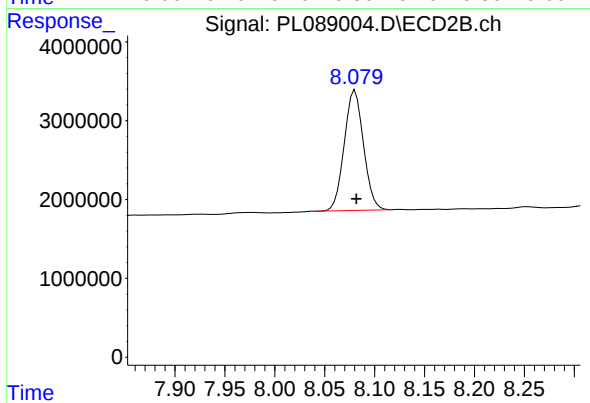

#28 Decachlorobiphenyl

R.T.: 8.080 min
Delta R.T.: -0.001 min
Response: 20419814
Conc: 15.06 ng/ml