

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041224\
 Data File : PL089010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2024 16:43
 Operator : AR\AJ
 Sample : P2038-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-02-040924

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/11/2024
 Supervised By :Ankita Jodhani 04/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 04:29:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.633	2.852	4396667	2724603	1.659m	2.044
28) SA Decachlor...	9.297	8.078	1552401	2492940	0.628m	1.839 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041224\
Data File : PL089010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2024 16:43
Operator : AR\AJ
Sample : P2038-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-02-040924


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/11/2024
Supervised By : Ankita Jodhani 04/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 04:29:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

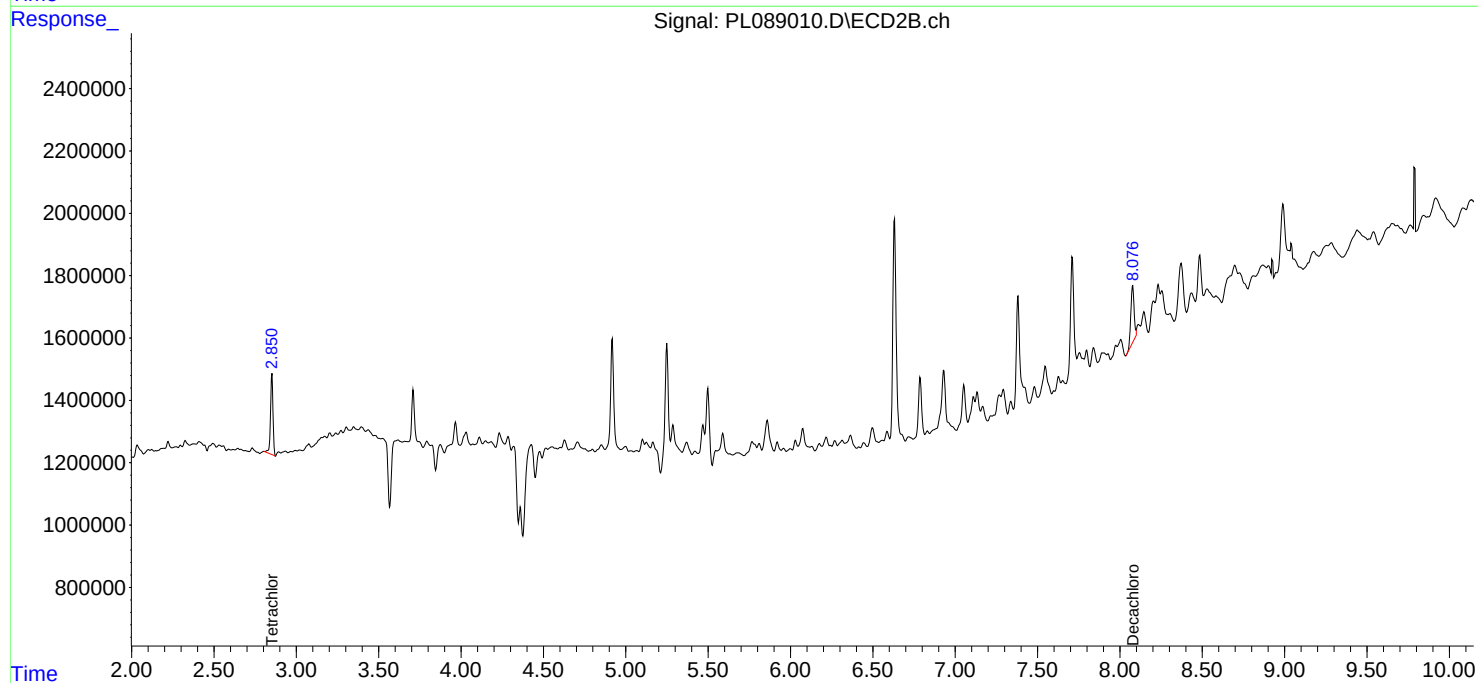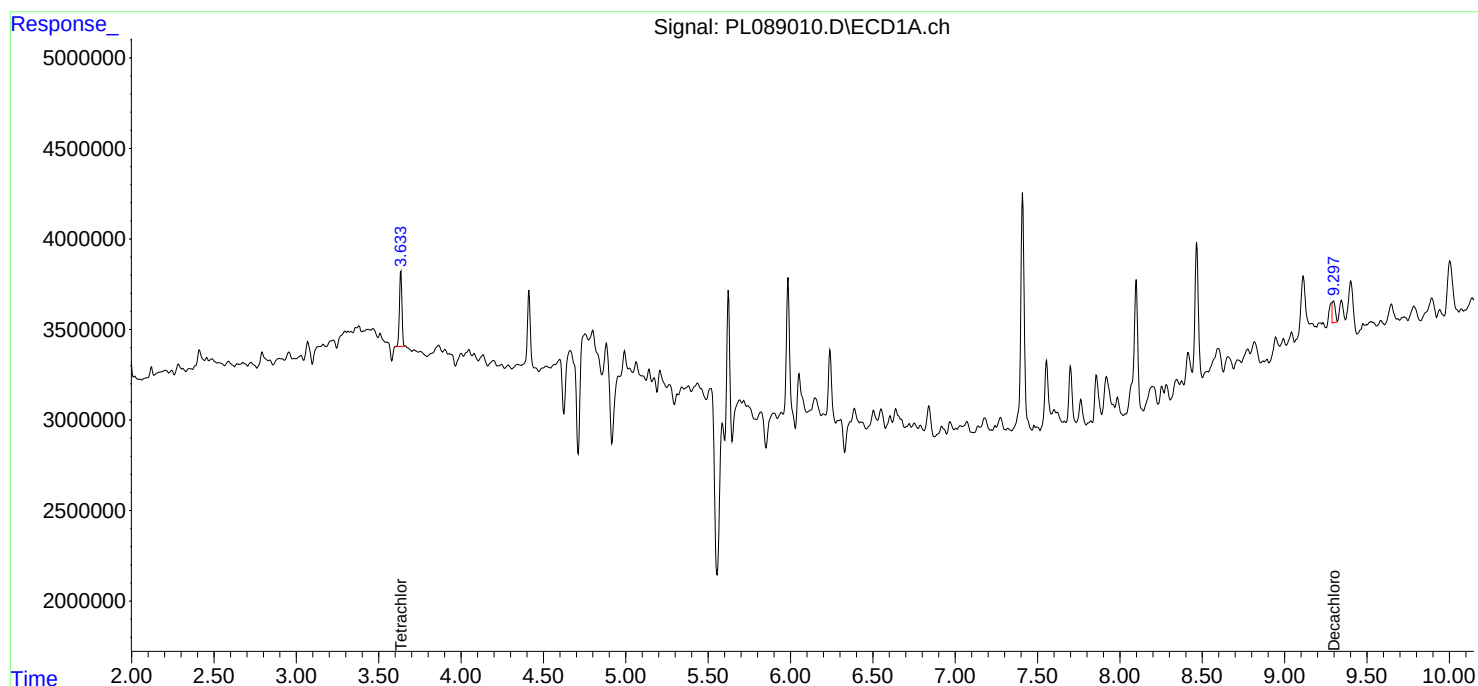

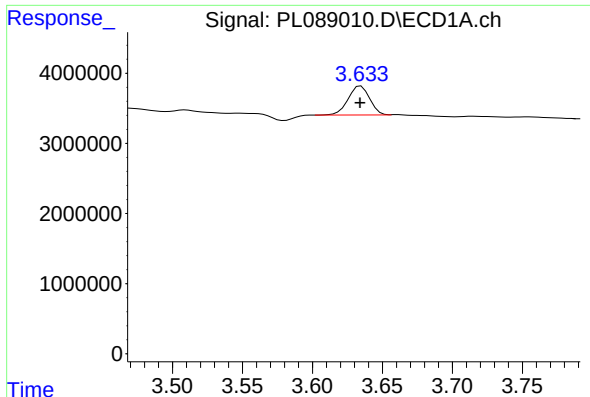


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: 0.000 min
Response: 4396667
Conc: 1.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-040924


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/11/2024
Supervised By :Ankita Jodhani 04/11/2024

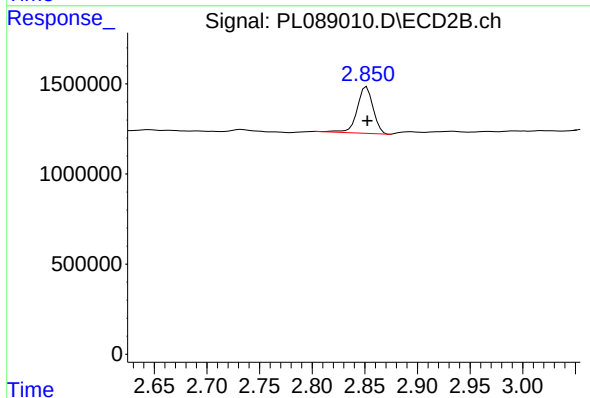


#1 Tetrachloro-m-xylene

R.T.: 2.852 min
Delta R.T.: 0.000 min
Response: 2724603
Conc: 2.04 ng/ml

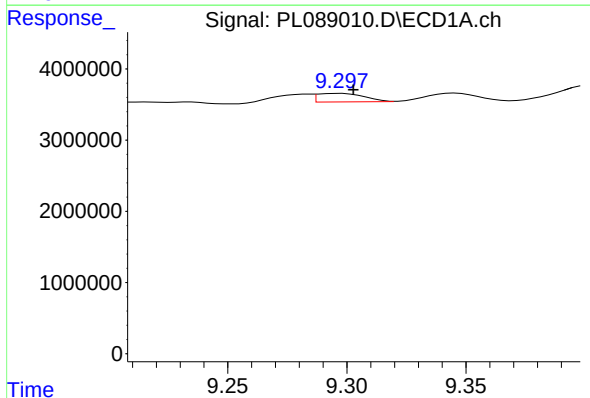

#28 Decachlorobiphenyl

R.T.: 9.297 min
Delta R.T.: -0.006 min
Response: 1552401
Conc: 0.63 ng/ml m

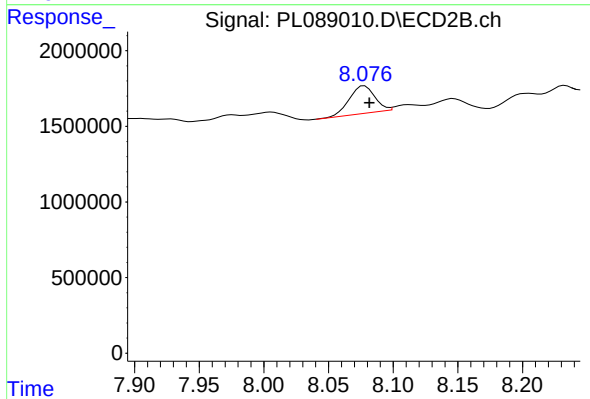

#28 Decachlorobiphenyl

R.T.: 8.078 min
Delta R.T.: -0.004 min
Response: 2492940
Conc: 1.84 ng/ml