

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041224\
 Data File : PL089016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2024 18:34
 Operator : AR\AJ
 Sample : P2025-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TOTE-COMP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/11/2024
 Supervised By :Ankita Jodhani 04/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 04:18:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.633	2.852	56970101	30986232	21.498m	23.250
28) SA Decachlor...	9.299	8.079	31284848	19081075	12.656m	14.072

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041224\
Data File : PL089016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2024 18:34
Operator : AR\AJ
Sample : P2025-03
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TOTE-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/11/2024
Supervised By : Ankita Jodhani 04/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 04:18:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

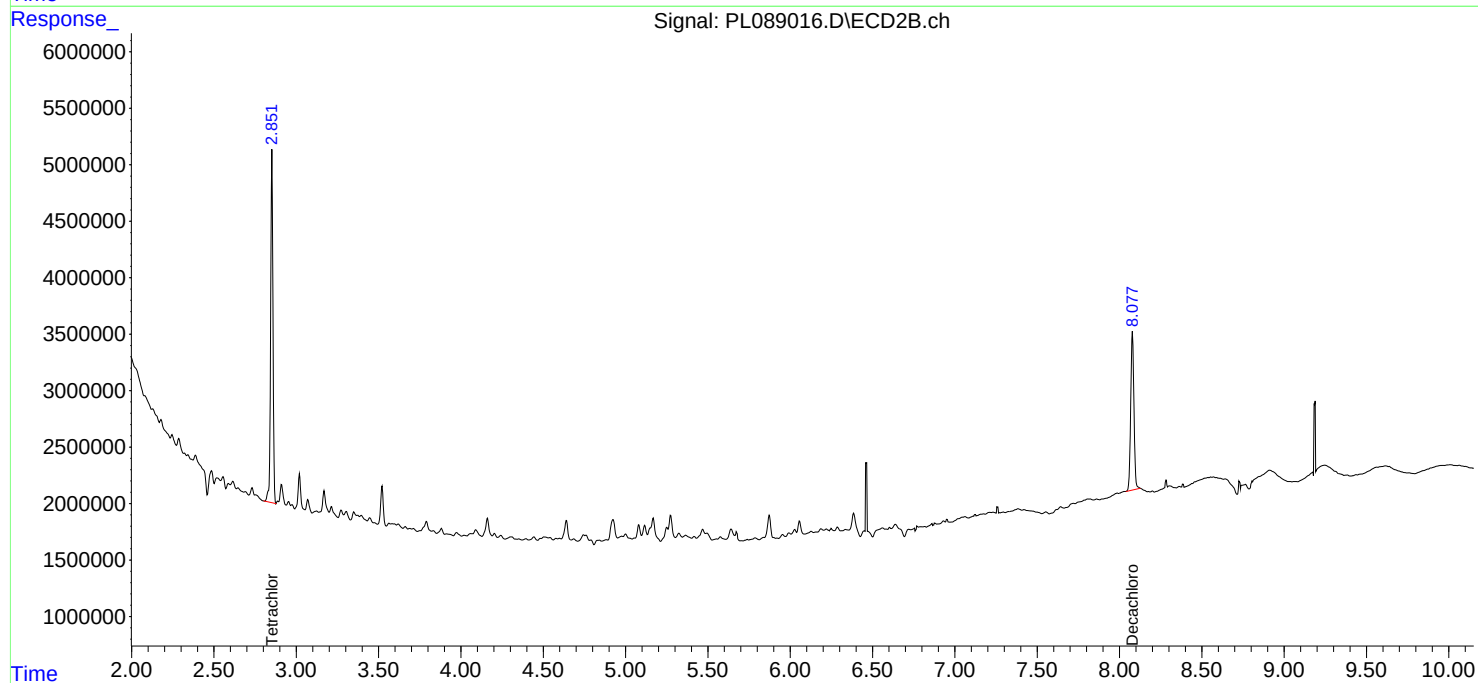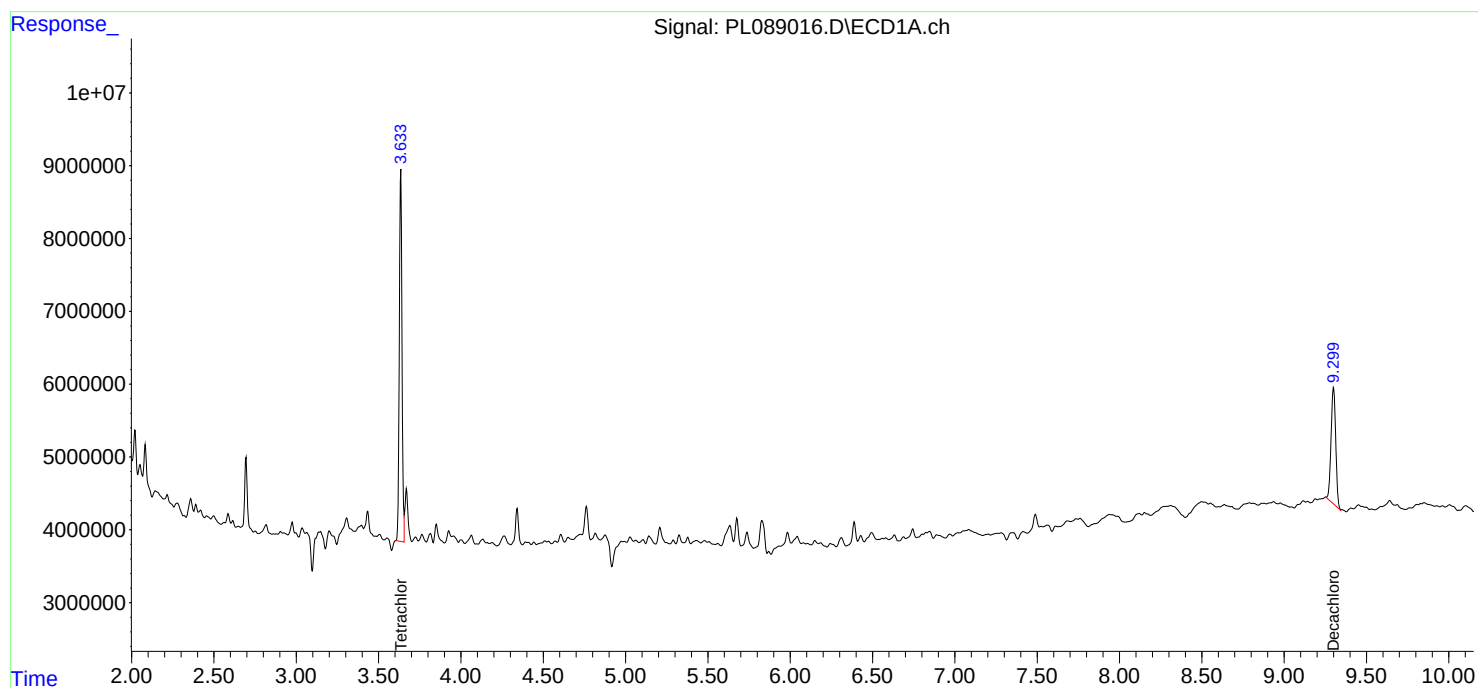

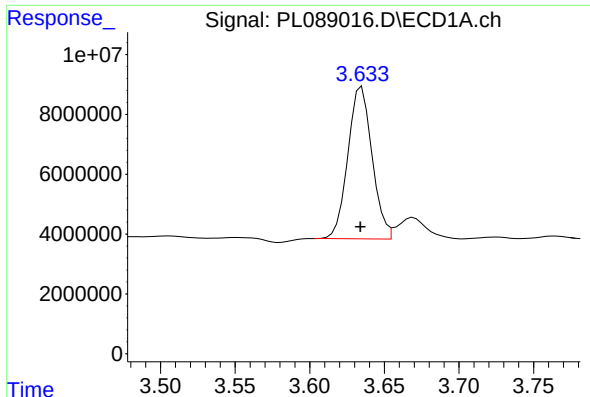


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: 0.000 min
Response: 56970101
Conc: 21.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
TOTE-COMP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/11/2024
Supervised By :Ankita Jodhani 04/11/2024

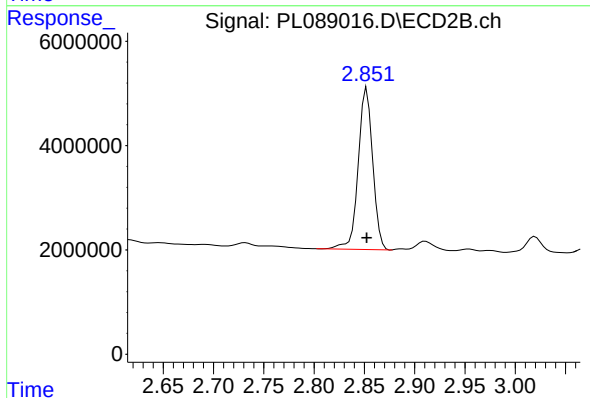


#1 Tetrachloro-m-xylene

R.T.: 2.852 min
Delta R.T.: 0.000 min
Response: 30986232
Conc: 23.25 ng/ml

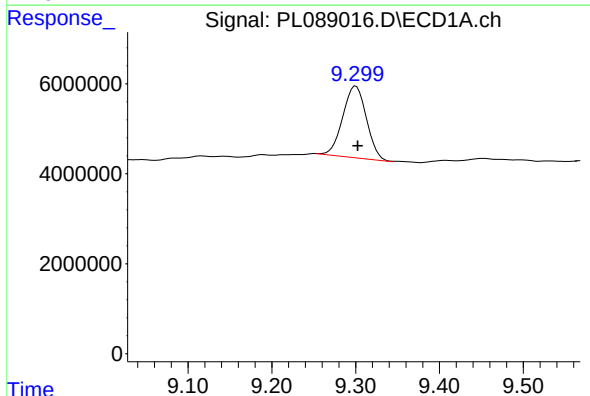

#28 Decachlorobiphenyl

R.T.: 9.299 min
Delta R.T.: -0.004 min
Response: 31284848
Conc: 12.66 ng/ml m

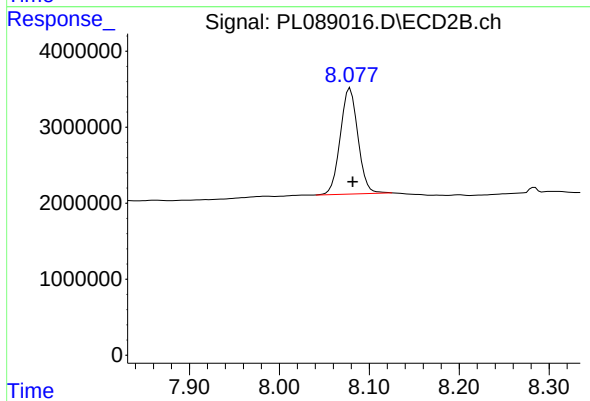

#28 Decachlorobiphenyl

R.T.: 8.079 min
Delta R.T.: -0.003 min
Response: 19081075
Conc: 14.07 ng/ml