

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
 Data File : PL057888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2020 14:44
 Operator : AJ\MA
 Sample : PB128183BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 01:02:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.957	215.7E6	46712152	21.399	21.525
28)	SA Decachlor...	8.206	8.981	204.4E6	46130983	19.824	20.652
Target Compounds							
2)	A alpha-BHC	3.899	0.000	10456481	0	0.602	N.D. #
4)	MA Heptachlor	0.000	5.141	0	105453	N.D.	0.031 #
5)	MB Aldrin	0.000	5.452f	0	71774	N.D.	0.022 #
7)	B delta-BHC	0.000	4.985f	0	2185815	N.D.	2.864 #
8)	B Heptachlo...	0.000	5.802	0	1604533	N.D.	0.594 #
15)	B Endosulfa...	0.000	6.870f	0	745988	N.D.	0.288 #
22)	Mirex	7.333	0.000	157075	0	0.019	N.D. #
23)	Chlordane-1	4.354f	0.000	5135122	0	13.884	N.D. #
24)	Chlordane-2	4.844f	0.000	5329058	0	13.200	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
Data File : PL057888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2020 14:44
Operator : AJ\MA
Sample : PB128183BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 01:02:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

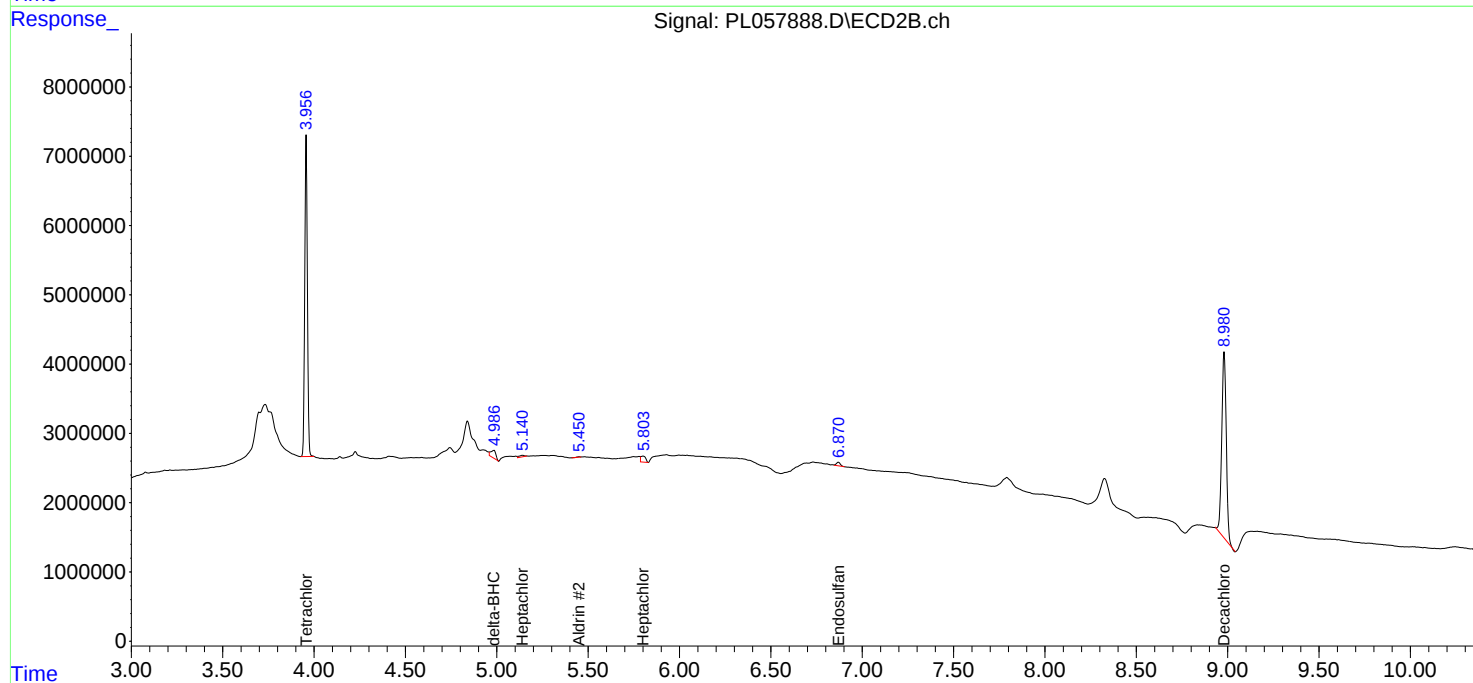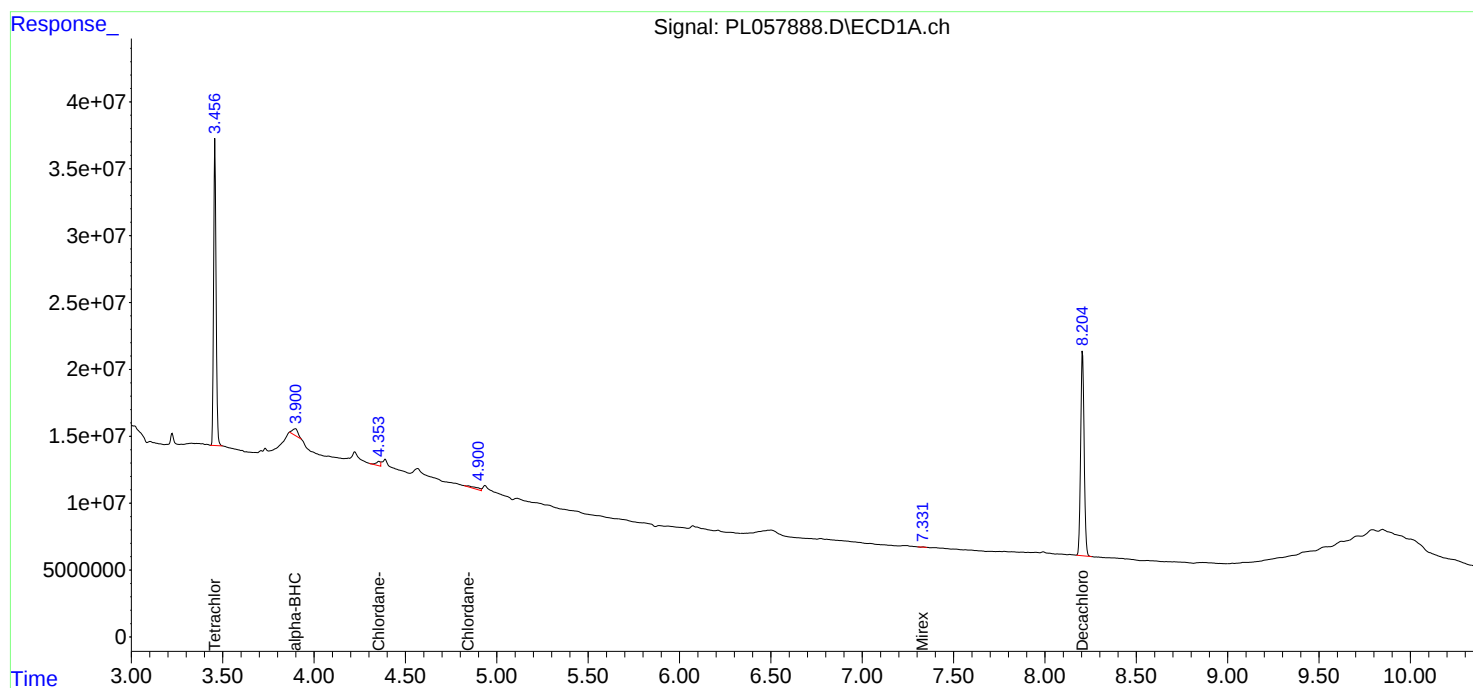


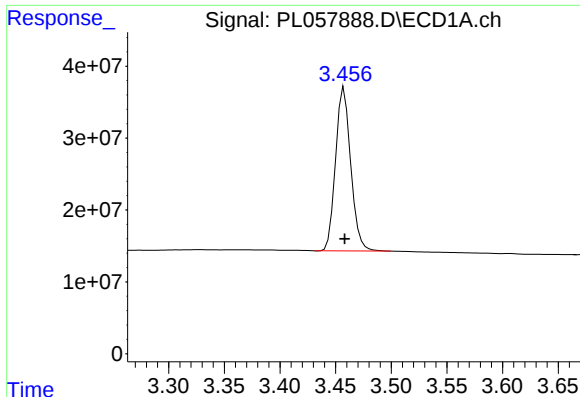

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 215727817
Conc: 21.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

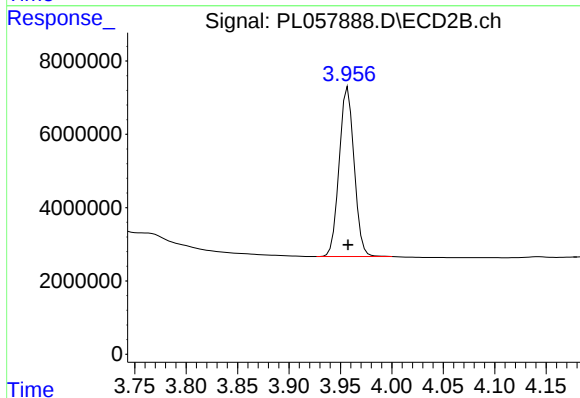


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 46712152
Conc: 21.52 ng/ml

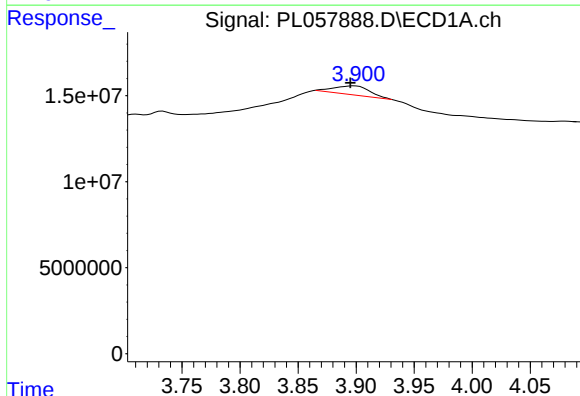


#2 alpha-BHC

R.T.: 3.899 min
Delta R.T.: 0.004 min
Response: 10456481
Conc: 0.60 ng/ml

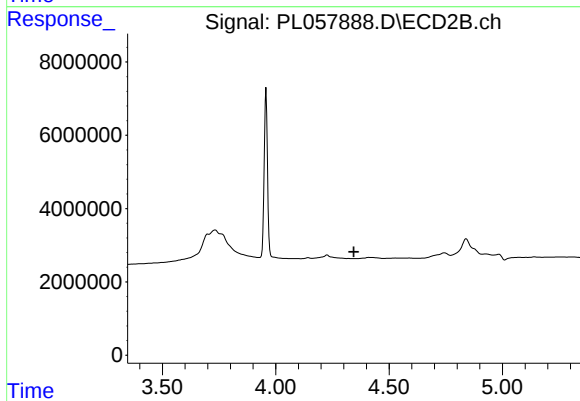

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

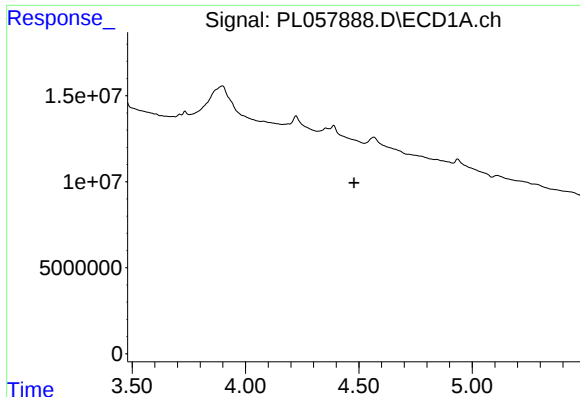

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

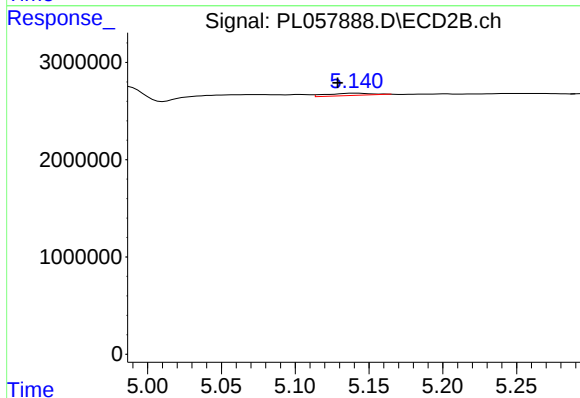


#4 Heptachlor

R.T.: 5.141 min
Delta R.T.: 0.013 min
Response: 105453
Conc: 0.03 ng/ml

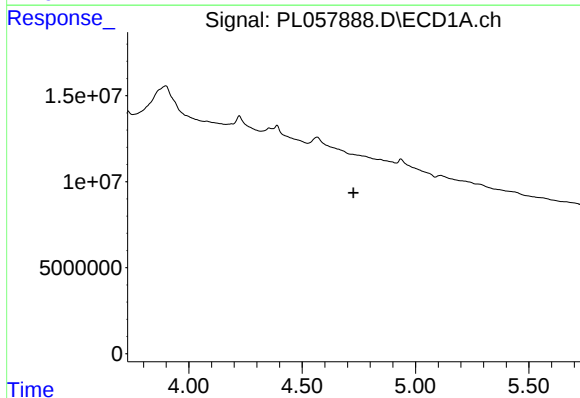


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.727 min
Response: 0
Conc: N.D.

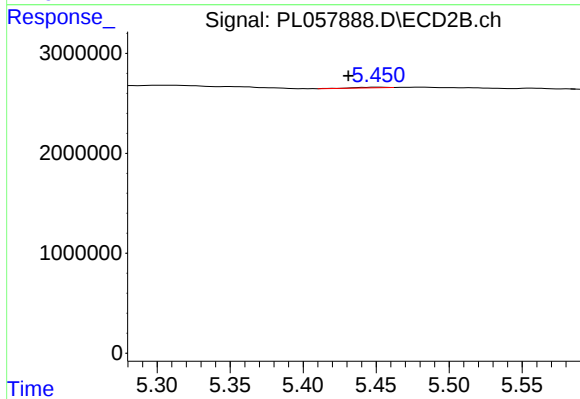

#5 Aldrin


R.T.: 5.452 min
Delta R.T.: 0.021 min
Response: 71774
Conc: 0.02 ng/ml

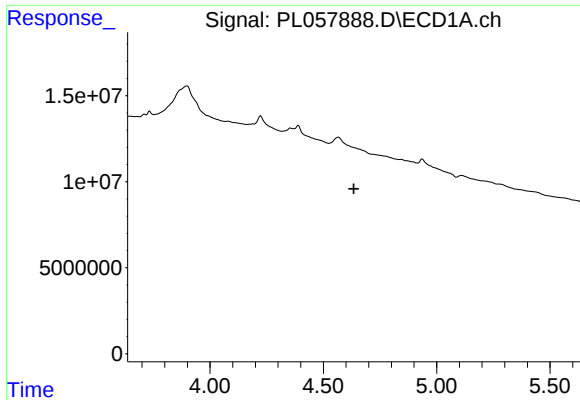

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

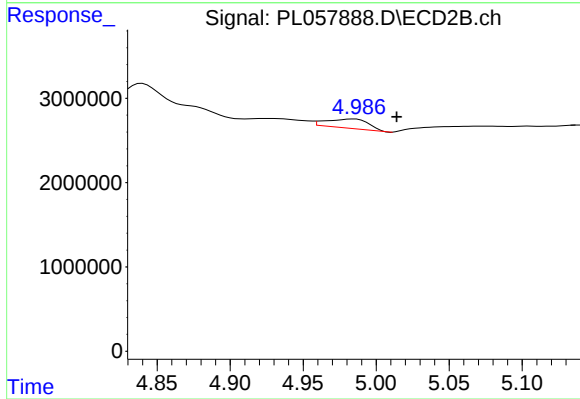


#7 delta-BHC

R.T.: 4.985 min
Delta R.T.: -0.029 min
Response: 2185815
Conc: 2.86 ng/ml

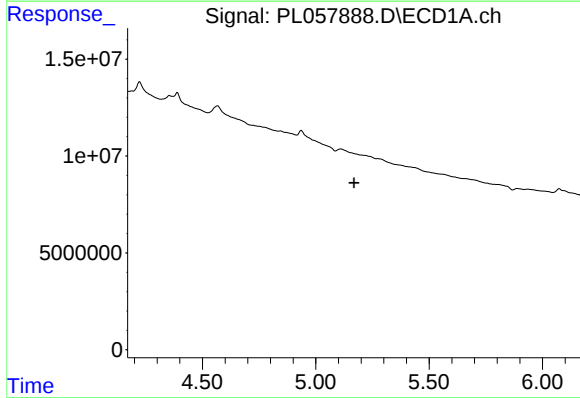


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

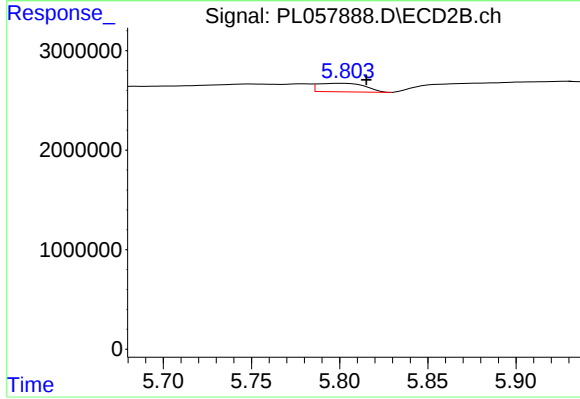

#8 Heptachlor epoxide


R.T.: 5.802 min
Delta R.T.: -0.013 min
Response: 1604533
Conc: 0.59 ng/ml

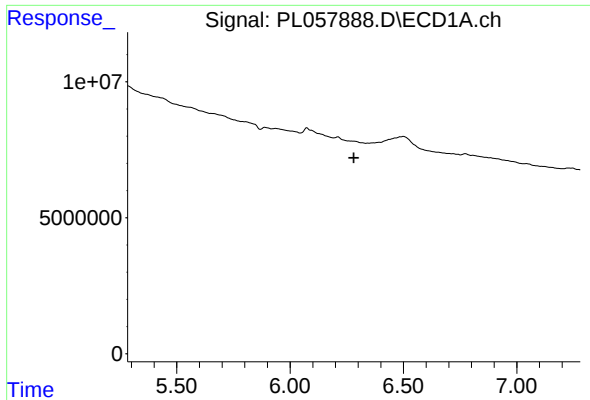

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

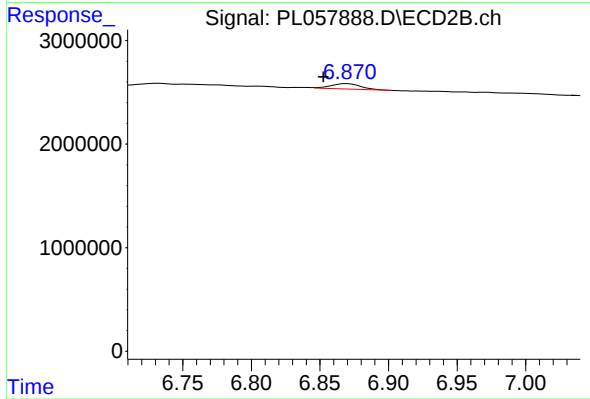


#15 Endosulfan II

R.T.: 6.870 min
Delta R.T.: 0.017 min
Response: 745988
Conc: 0.29 ng/ml

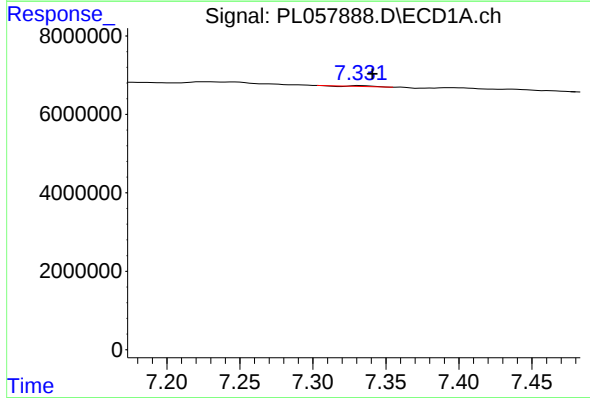


#22 Mirex

R.T.: 7.333 min
Delta R.T.: -0.008 min
Response: 157075
Conc: 0.02 ng/ml

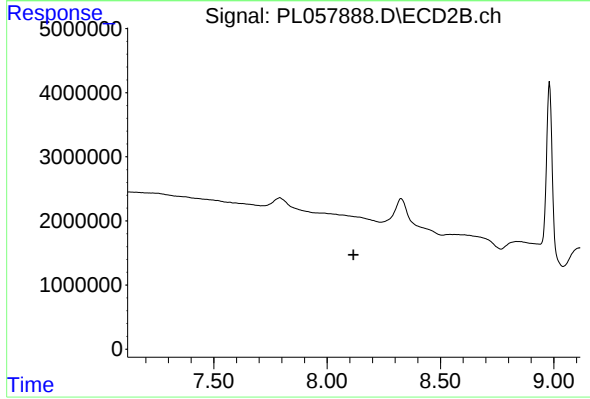

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.117 min
Response: 0
Conc: N.D.

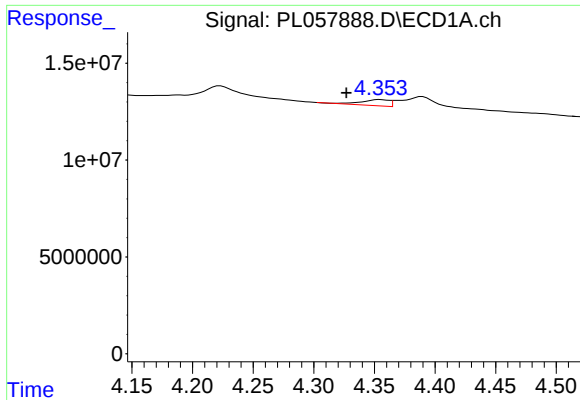

#23 Chlordane-1


R.T.: 4.354 min
Delta R.T.: 0.028 min
Response: 5135122
Conc: 13.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

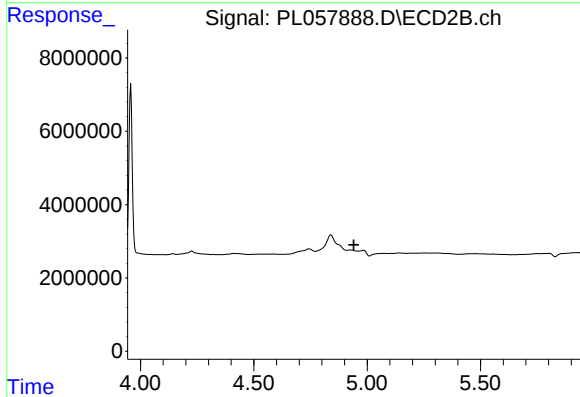


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

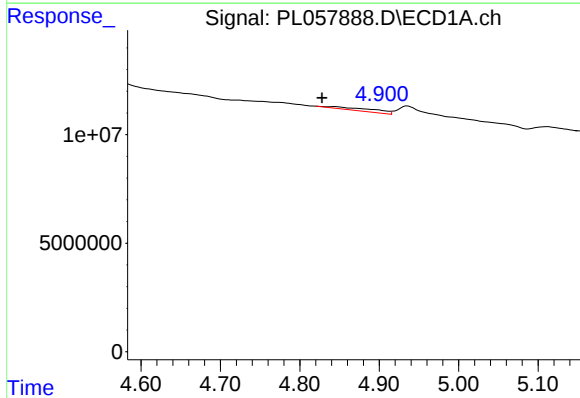


#24 Chlordane-2

R.T.: 4.844 min
Delta R.T.: 0.016 min
Response: 5329058
Conc: 13.20 ng/ml

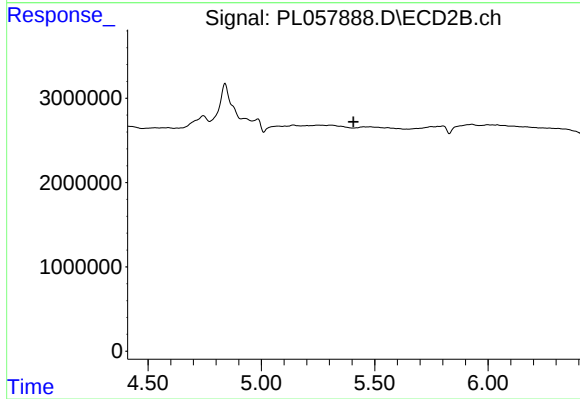

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

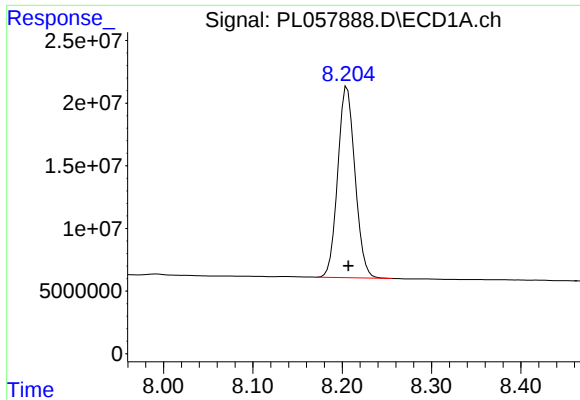

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.001 min
Response: 204351273
Conc: 19.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

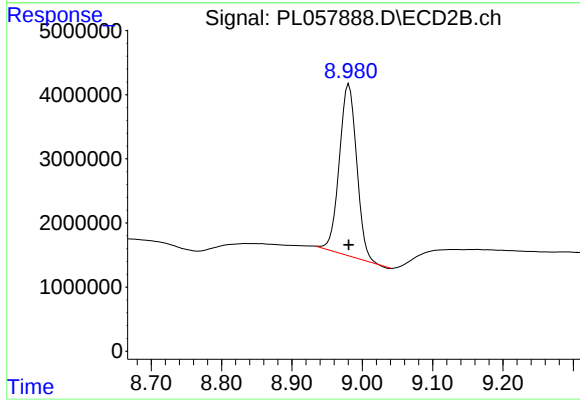

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 46130983
Conc: 20.65 ng/ml