

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
 Data File : PL057892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2020 15:42
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 01:03:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.957	229.4E6	49429030	22.751	22.777
28)	SA Decachlor...	8.206	8.980	216.8E6	48433749	21.034	21.682
Target Compounds							
2)	A alpha-BHC	3.896	0.000	14180193	0	0.816	N.D. #
4)	MA Heptachlor	0.000	5.139	0	270020	N.D.	0.080 #
7)	B delta-BHC	0.000	4.985f	0	2766779	N.D.	3.087 #
8)	B Heptachlo...	0.000	5.806	0	3607106	N.D.	1.336 #
11)	B alpha-Chl...	5.450	0.000	2559091	0	0.192	N.D. #
15)	B Endosulfa...	0.000	6.870f	0	806397	N.D.	0.311 #
19)	B Endosulfa...	6.681f	0.000	79246	0	0.008	N.D. #
23)	Chlordane-1	4.356f	0.000	3719132	0	10.056	N.D. #
26)	Chlordane-4	5.450	0.000	2559091	0	2.460	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
Data File : PL057892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2020 15:42
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 01:03:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

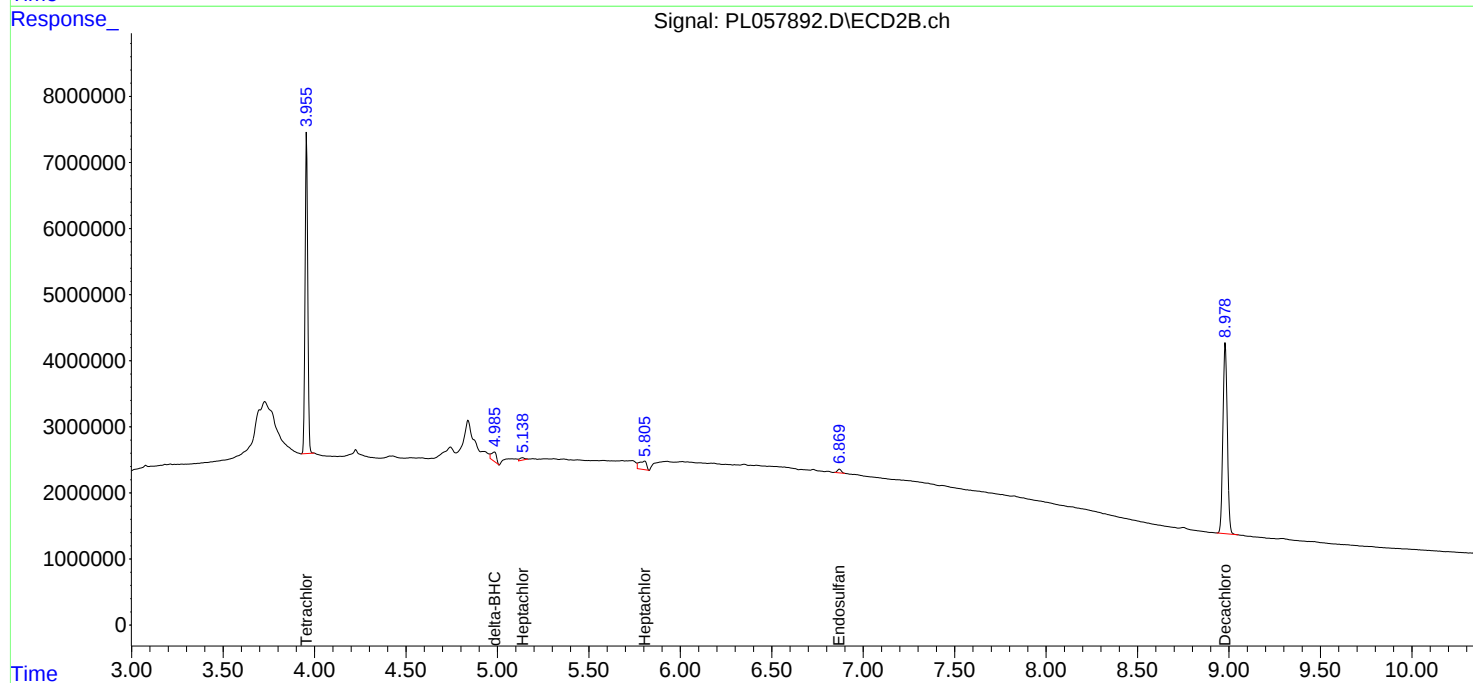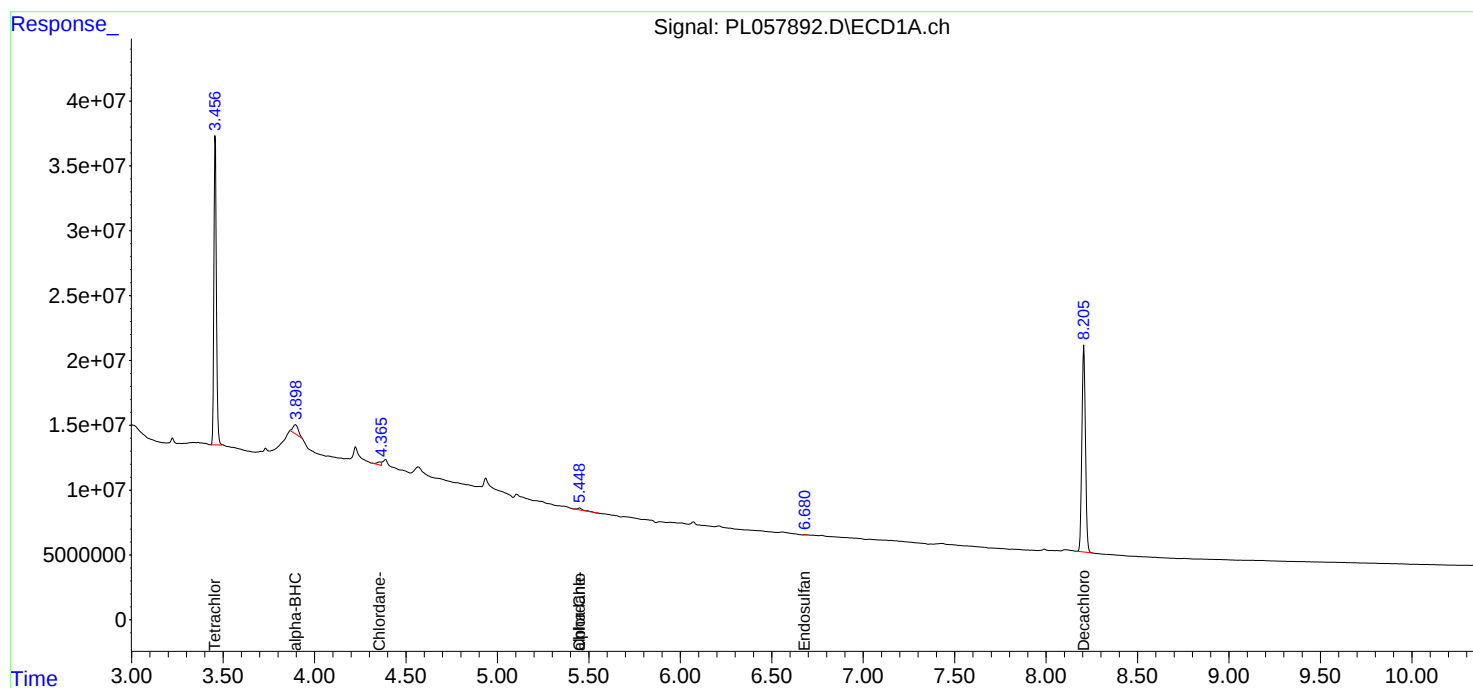


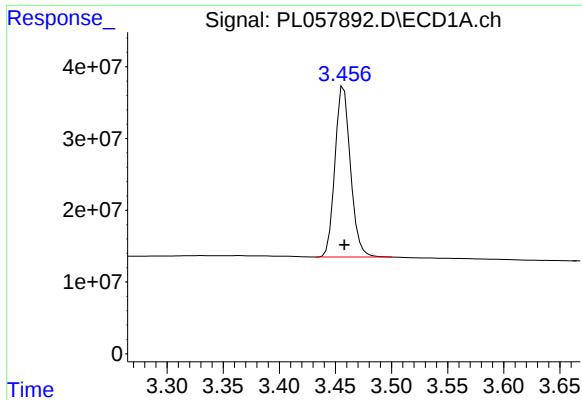

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 229357819
Conc: 22.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

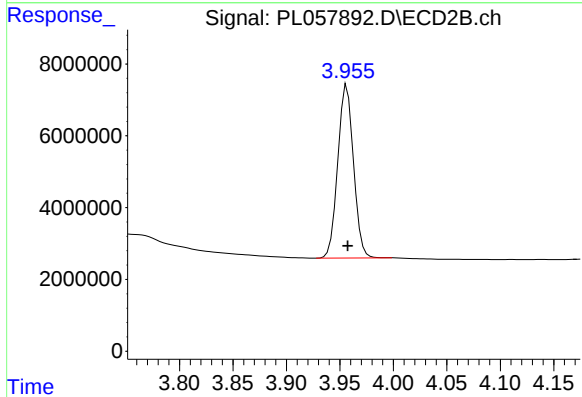


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 49429030
Conc: 22.78 ng/ml

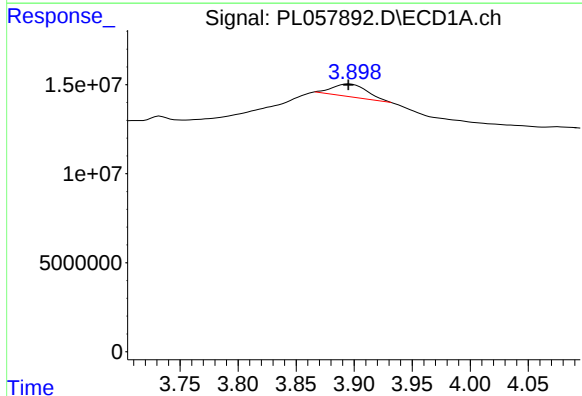


#2 alpha-BHC

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 14180193
Conc: 0.82 ng/ml

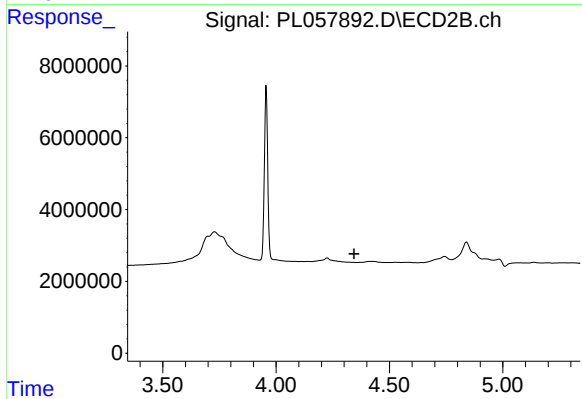

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

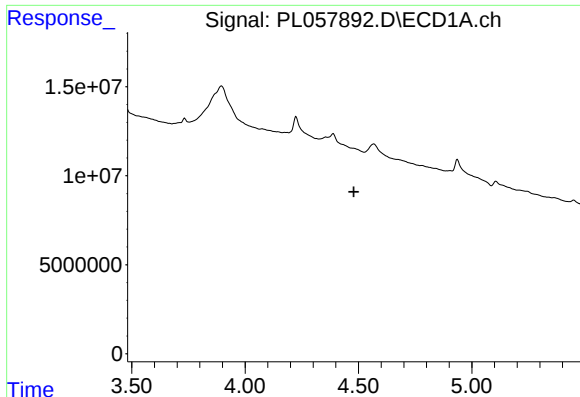

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

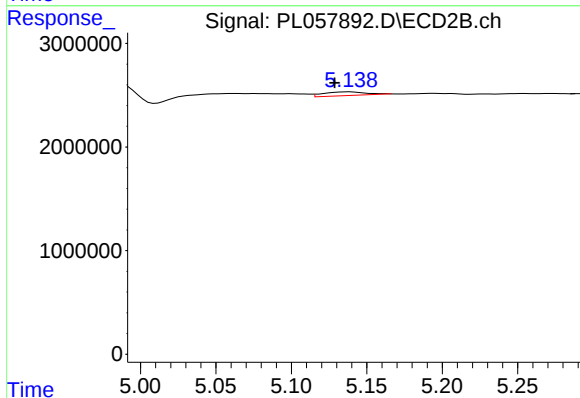


#4 Heptachlor

R.T.: 5.139 min
Delta R.T.: 0.010 min
Response: 270020
Conc: 0.08 ng/ml

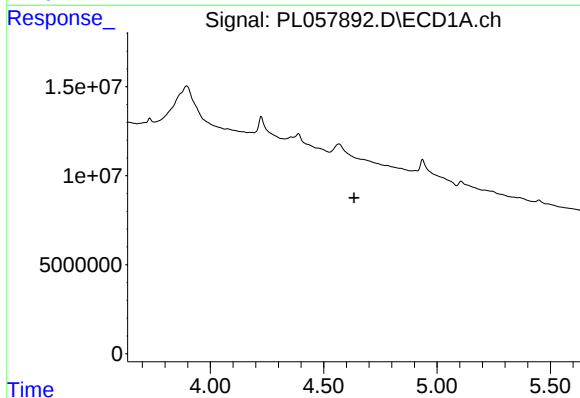


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.634 min
Response: 0
Conc: N.D.

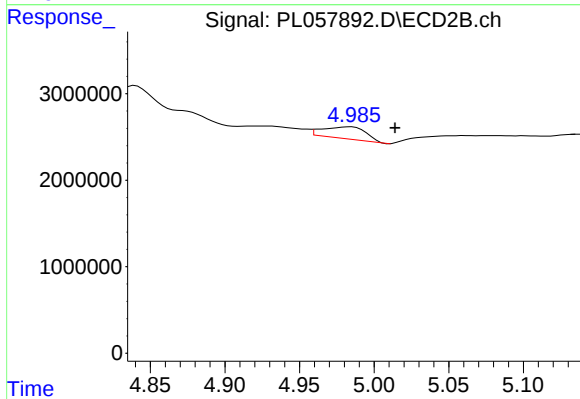

#7 delta-BHC


R.T.: 4.985 min
Delta R.T.: -0.029 min
Response: 2766779
Conc: 3.09 ng/ml

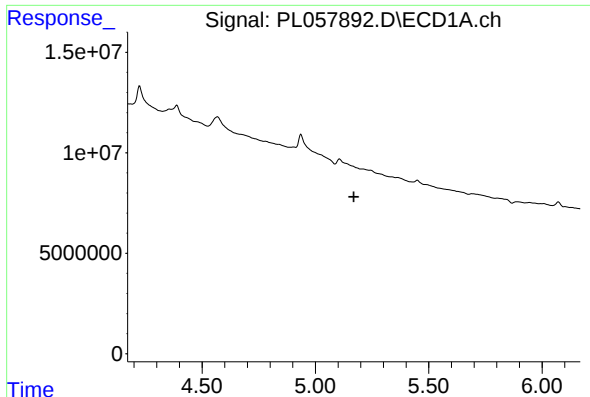

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

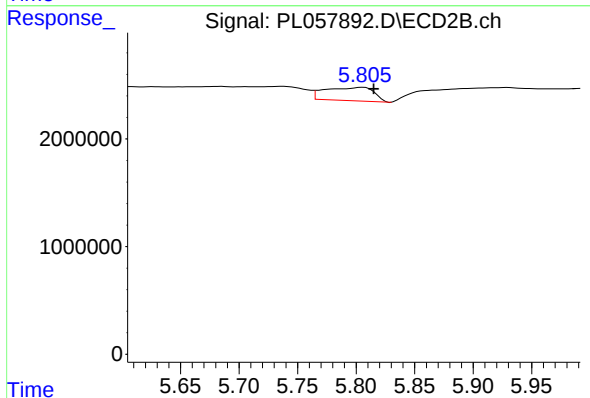


#8 Heptachlor epoxide

R.T.: 5.806 min
Delta R.T.: -0.009 min
Response: 3607106
Conc: 1.34 ng/ml

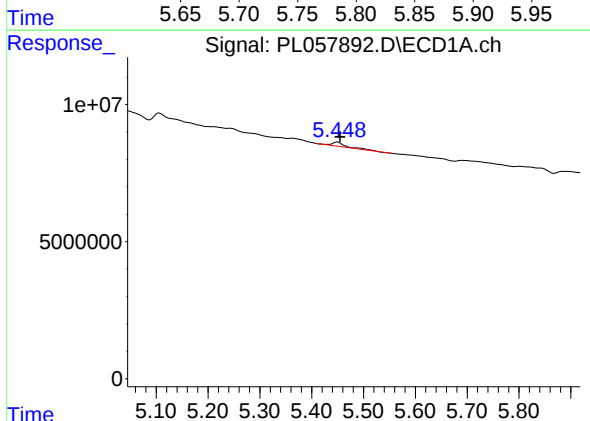


#11 alpha-Chlordane

R.T.: 5.450 min
Delta R.T.: -0.005 min
Response: 2559091
Conc: 0.19 ng/ml

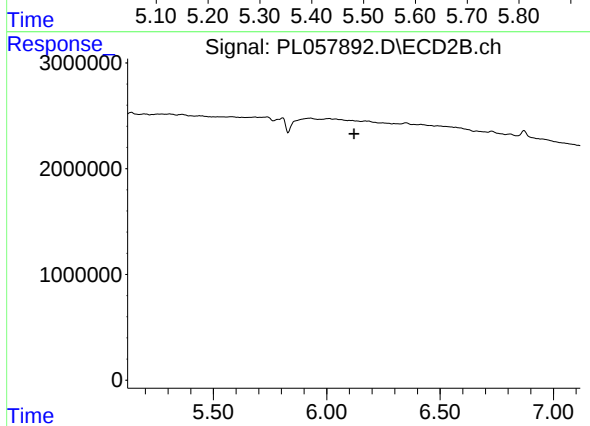

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.120 min
Response: 0
Conc: N.D.

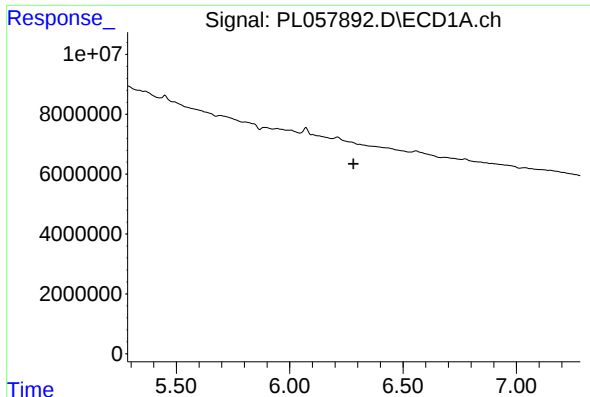

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

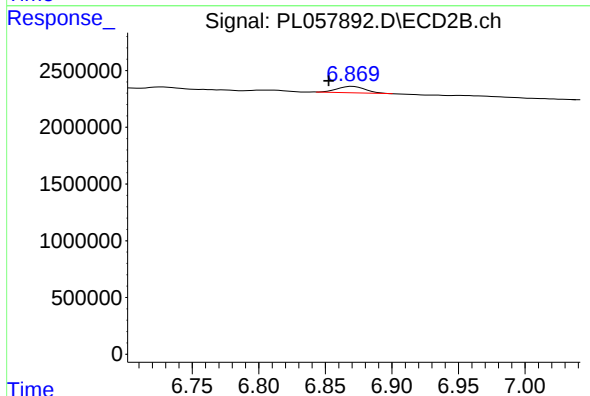


#15 Endosulfan II

R.T.: 6.870 min
Delta R.T.: 0.018 min
Response: 806397
Conc: 0.31 ng/ml

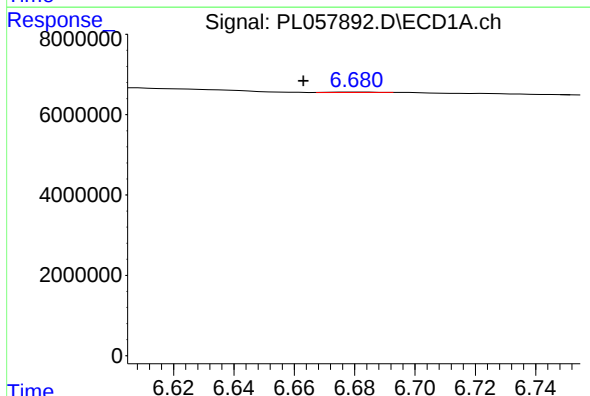


#19 Endosulfan Sulfate

R.T.: 6.681 min
Delta R.T.: 0.018 min
Response: 79246
Conc: 0.01 ng/ml

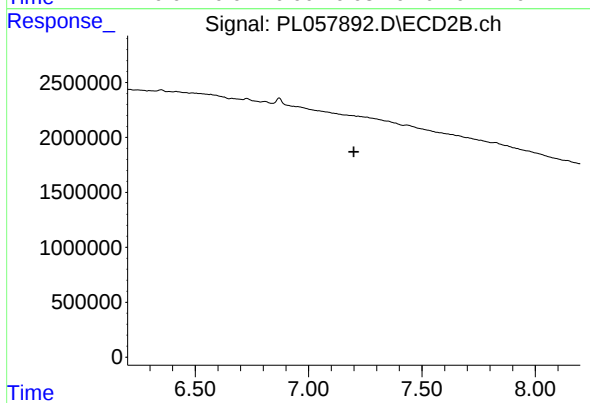

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

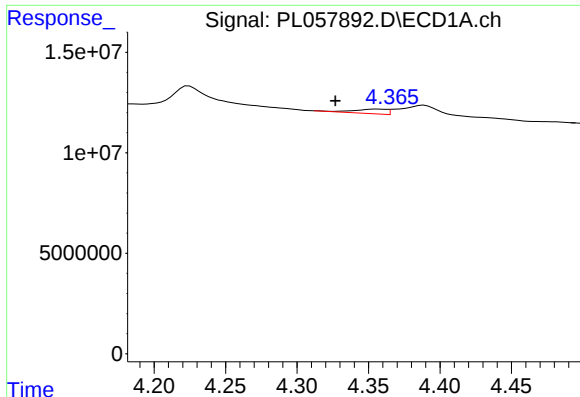

#23 Chlordane-1


R.T.: 4.356 min
Delta R.T.: 0.030 min
Response: 3719132
Conc: 10.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

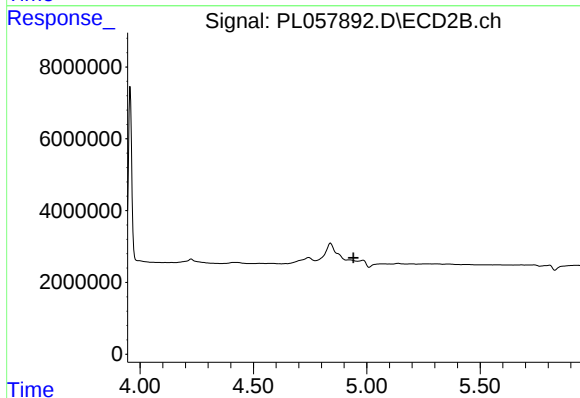


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

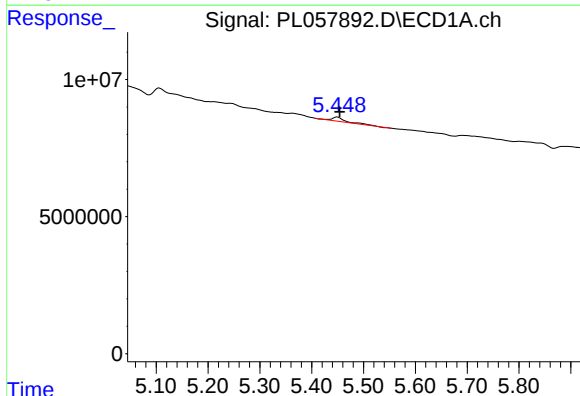


#26 Chlordane-4

R.T.: 5.450 min
Delta R.T.: -0.005 min
Response: 2559091
Conc: 2.46 ng/ml

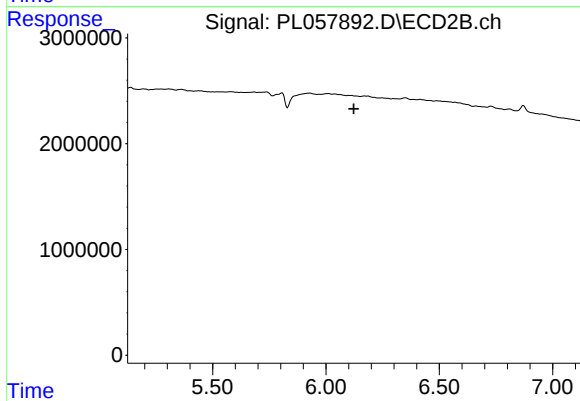

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.123 min
Response: 0
Conc: N.D.

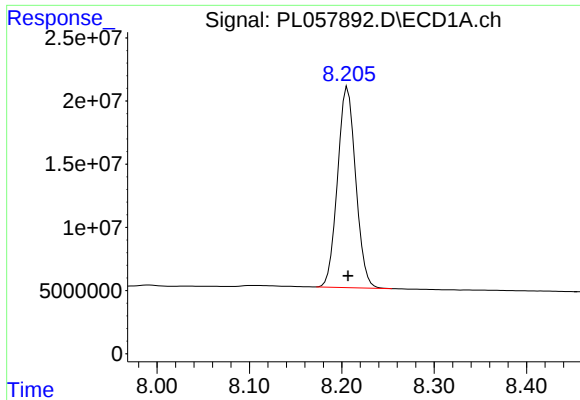

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 216829157
Conc: 21.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

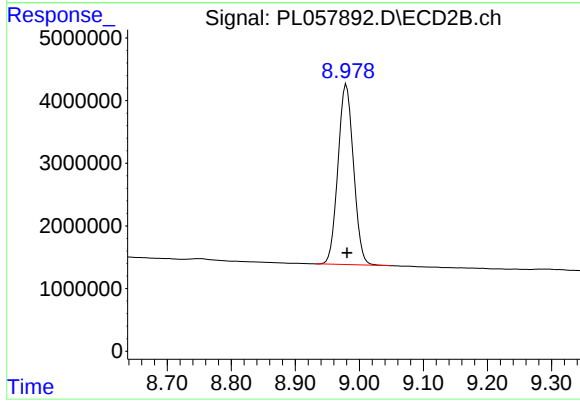

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: -0.001 min
Response: 48433749
Conc: 21.68 ng/ml