

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
 Data File : PL057921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2020 23:02
 Operator : AJ\MA
 Sample : PB128183TB
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 01:10:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	221.5E6	46151643	21.967	21.267
28)	SA Decachlor...	8.203	8.977	217.0E6	46342042	21.050	20.746
Target Compounds							
2)	A alpha-BHC	3.898	0.000	10849575	0	0.625	N.D. #
4)	MA Heptachlor	0.000	5.134	0	1541517	N.D.	0.459 #
8)	B Heptachlo...	0.000	5.808	0	3184259	N.D.	1.179 #
12)	B 4,4'-DDE	5.630	0.000	2868533	0	0.219	N.D. #
14)	MA Endrin	6.009	0.000	1104147	0	0.095	N.D. #
15)	B Endosulfa...	0.000	6.868f	0	622050	N.D.	0.240 #
22)	Mirex	7.364f	0.000	71312	0	0.009	N.D. #
23)	Chlordane-1	4.355f	0.000	4878087	0	13.189	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
Data File : PL057921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2020 23:02
Operator : AJ\MA
Sample : PB128183TB
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 01:10:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

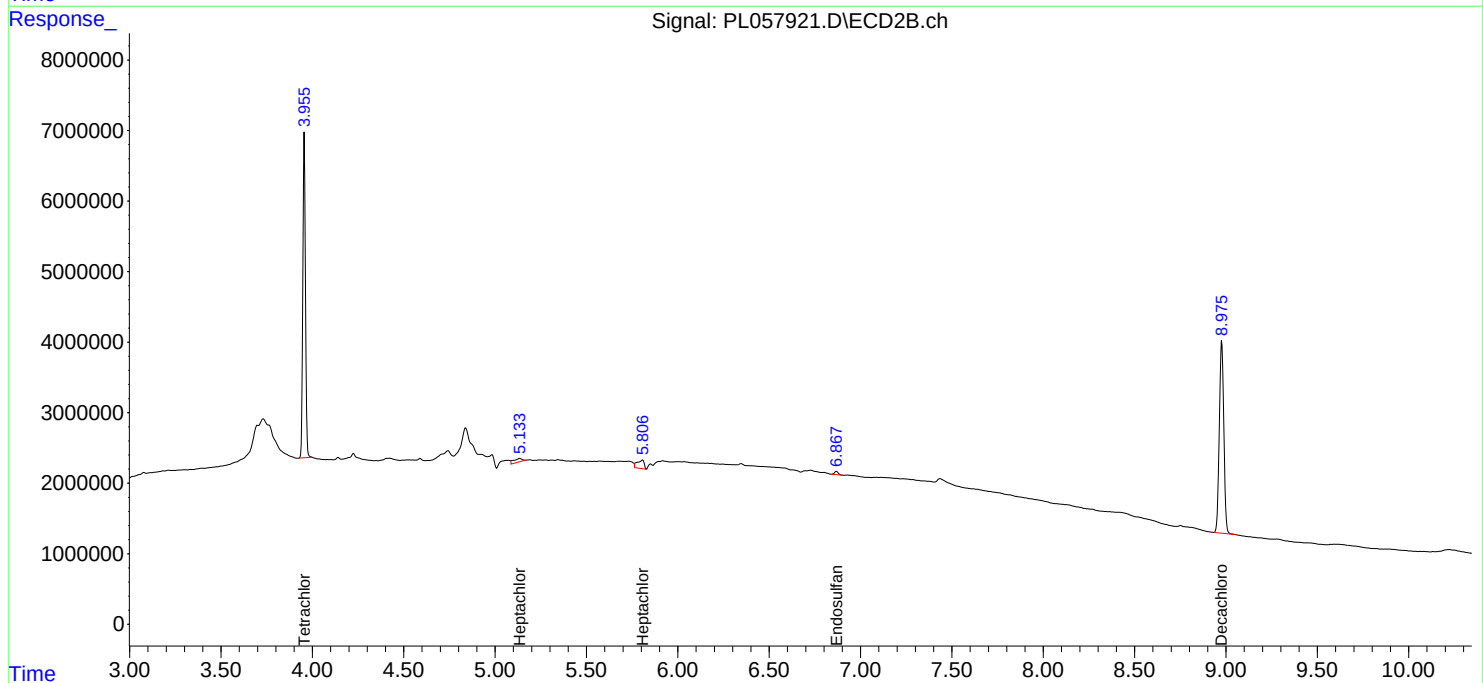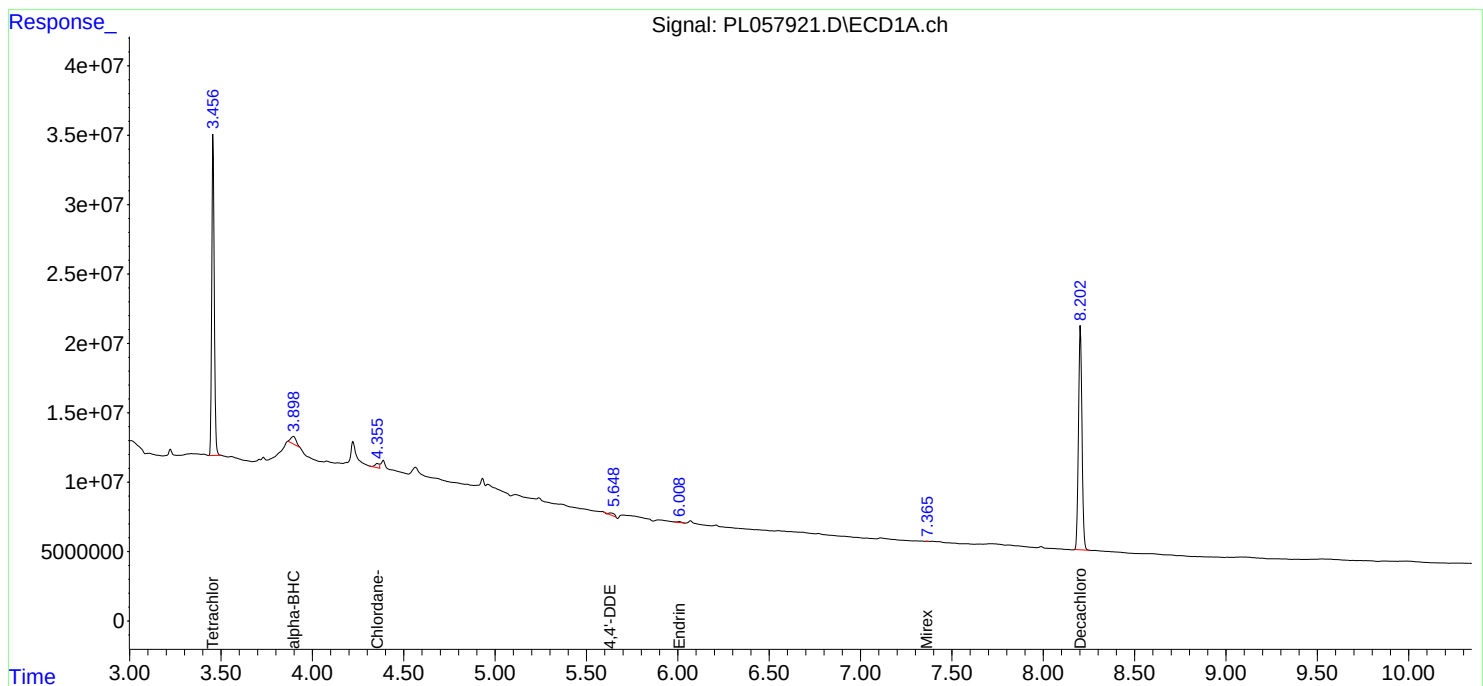


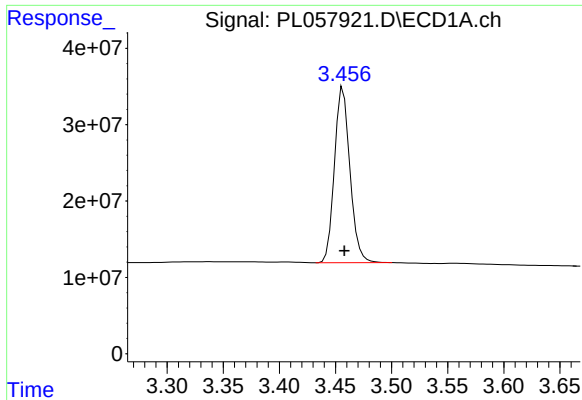

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 221454173
Conc: 21.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

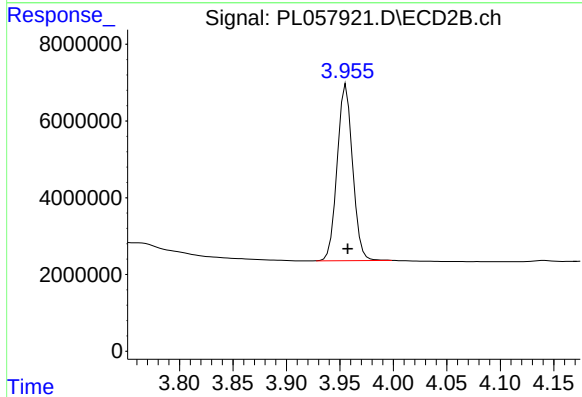


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 46151643
Conc: 21.27 ng/ml

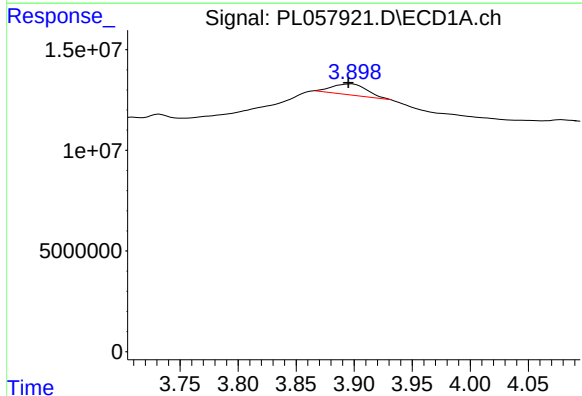


#2 alpha-BHC

R.T.: 3.898 min
Delta R.T.: 0.003 min
Response: 10849575
Conc: 0.62 ng/ml

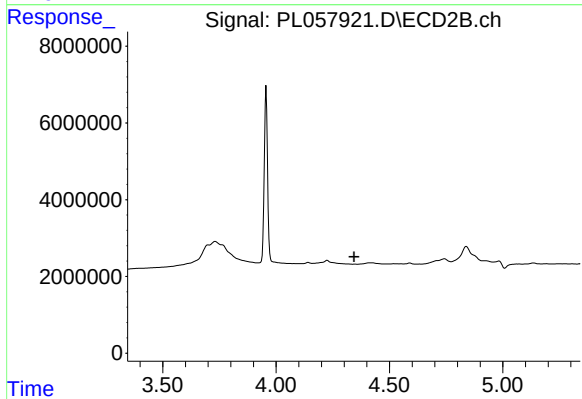

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

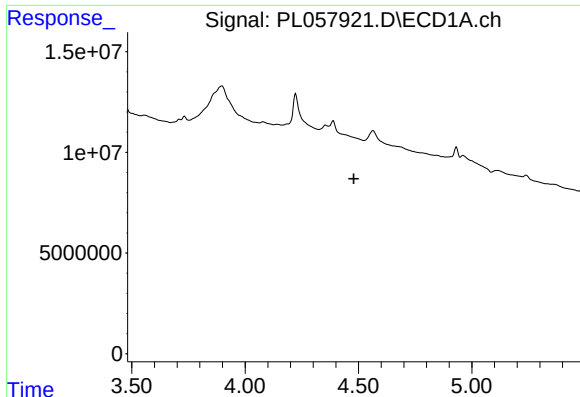

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

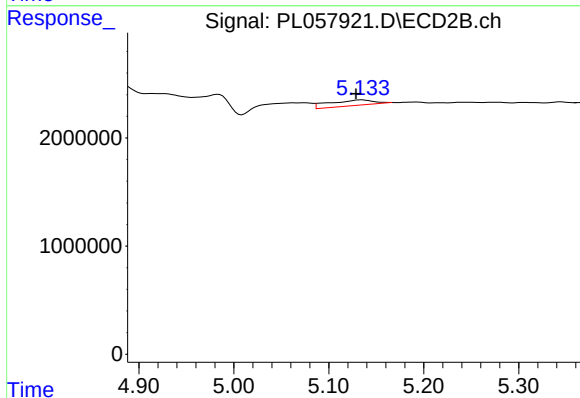


#4 Heptachlor

R.T.: 5.134 min
Delta R.T.: 0.006 min
Response: 1541517
Conc: 0.46 ng/ml

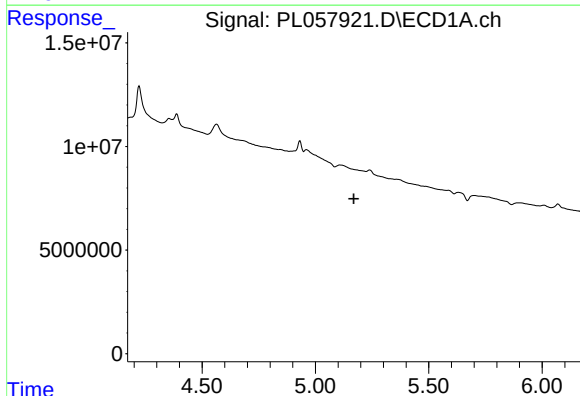


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

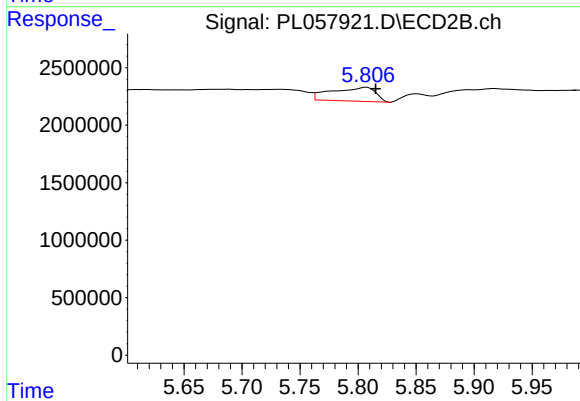

#8 Heptachlor epoxide


R.T.: 5.808 min
Delta R.T.: -0.008 min
Response: 3184259
Conc: 1.18 ng/ml

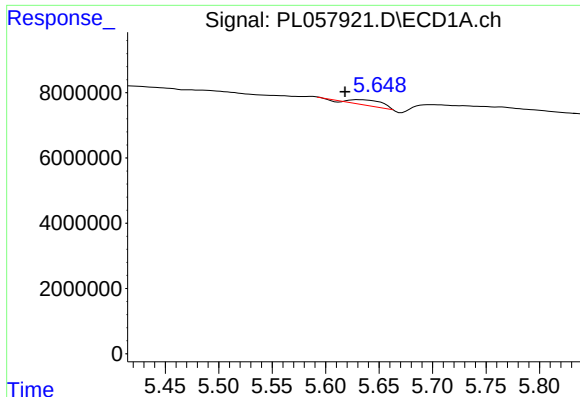

#12 4,4'-DDE


R.T.: 5.630 min
Delta R.T.: 0.012 min
Response: 2868533
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

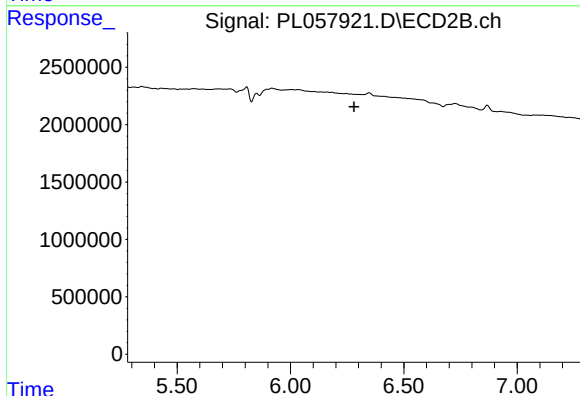


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.280 min
Response: 0
Conc: N.D.

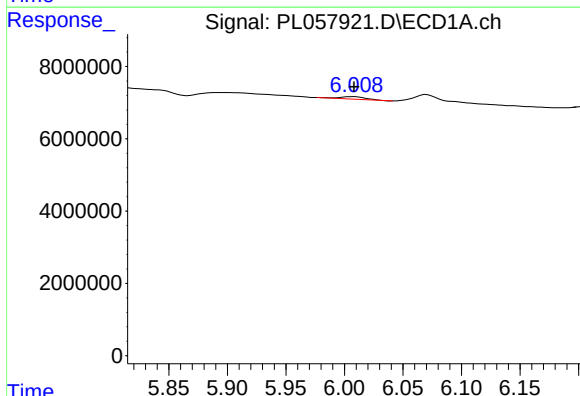


#14 Endrin

R.T.: 6.009 min
Delta R.T.: 0.000 min
Response: 1104147
Conc: 0.09 ng/ml

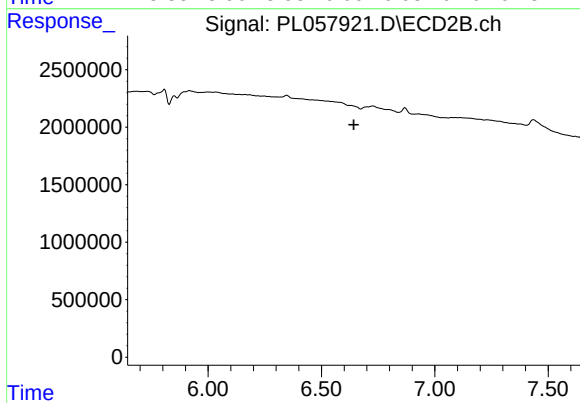

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

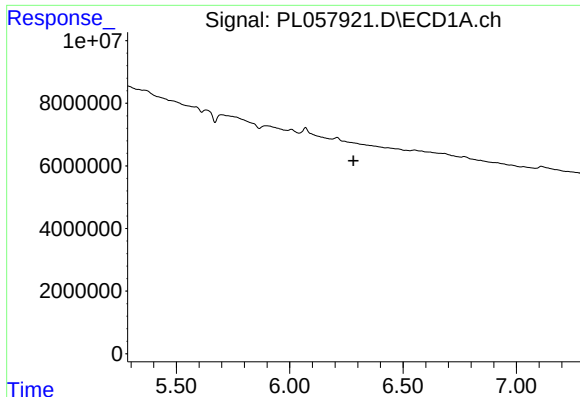

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

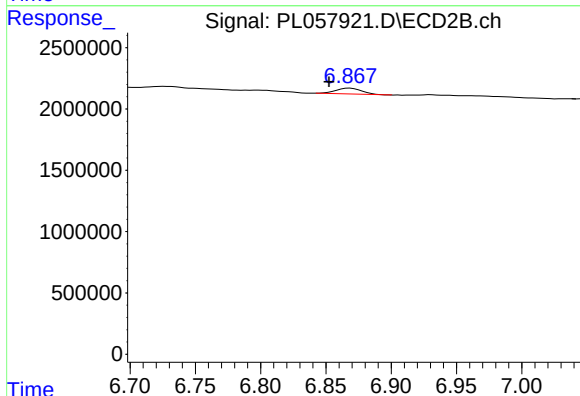


#15 Endosulfan II

R.T.: 6.868 min
Delta R.T.: 0.016 min
Response: 622050
Conc: 0.24 ng/ml

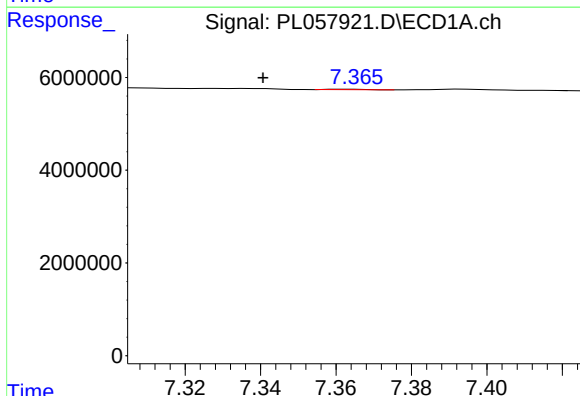


#22 Mirex

R.T.: 7.364 min
Delta R.T.: 0.023 min
Response: 71312
Conc: 0.01 ng/ml

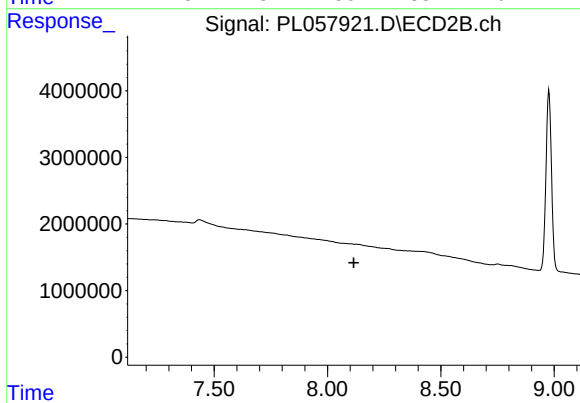

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.117 min
Response: 0
Conc: N.D.

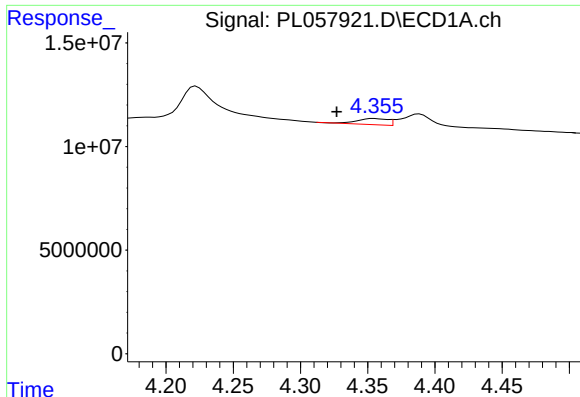

#23 Chlordane-1


R.T.: 4.355 min
Delta R.T.: 0.028 min
Response: 4878087
Conc: 13.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

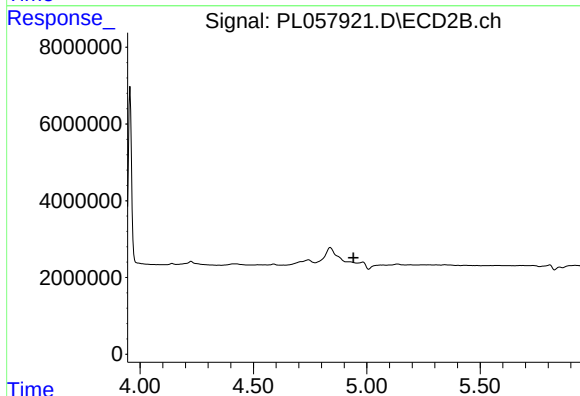


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

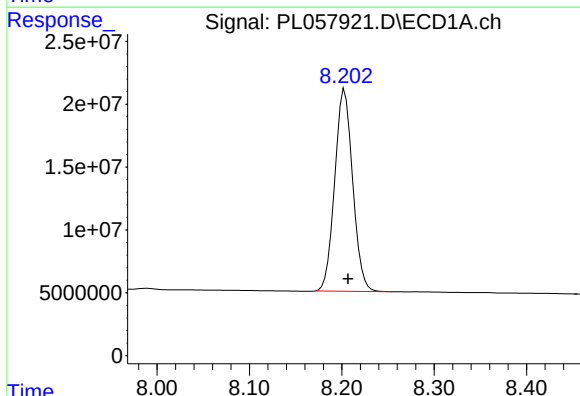

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 216994458
Conc: 21.05 ng/ml

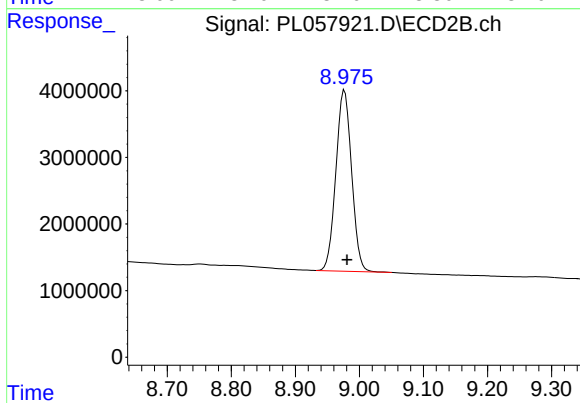

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.004 min
Response: 46342042
Conc: 20.75 ng/ml