

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
 Data File : PL057942.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2020 04:43
 Operator : AJ\MA
 Sample : L2242-04
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 07:17:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	189.5E6	40475044	18.802	18.651
28)	SA Decachlor...	8.203	8.976	186.3E6	38360687	18.071	17.173
Target Compounds							
4)	MA Heptachlor	0.000	5.137	0	633579	N.D.	0.189 #
5)	MB Aldrin	4.715	0.000	1351796	0	0.092	N.D. #
7)	B delta-BHC	0.000	4.986f	0	7250868	N.D.	4.808 #
8)	B Heptachlo...	0.000	5.801	0	4840350	N.D.	1.793 #
10)	B gamma-Chl...	0.000	6.039	0	467779	N.D.	0.144 #
15)	B Endosulfa...	0.000	6.867	0	1251967	N.D.	0.483 #
23)	Chlordane-1	4.331	0.000	2694462	0	7.285	N.D. #
25)	Chlordane-3	0.000	6.039	0	467779	N.D.	1.081 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
Data File : PL057942.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2020 04:43
Operator : AJ\MA
Sample : L2242-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 07:17:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

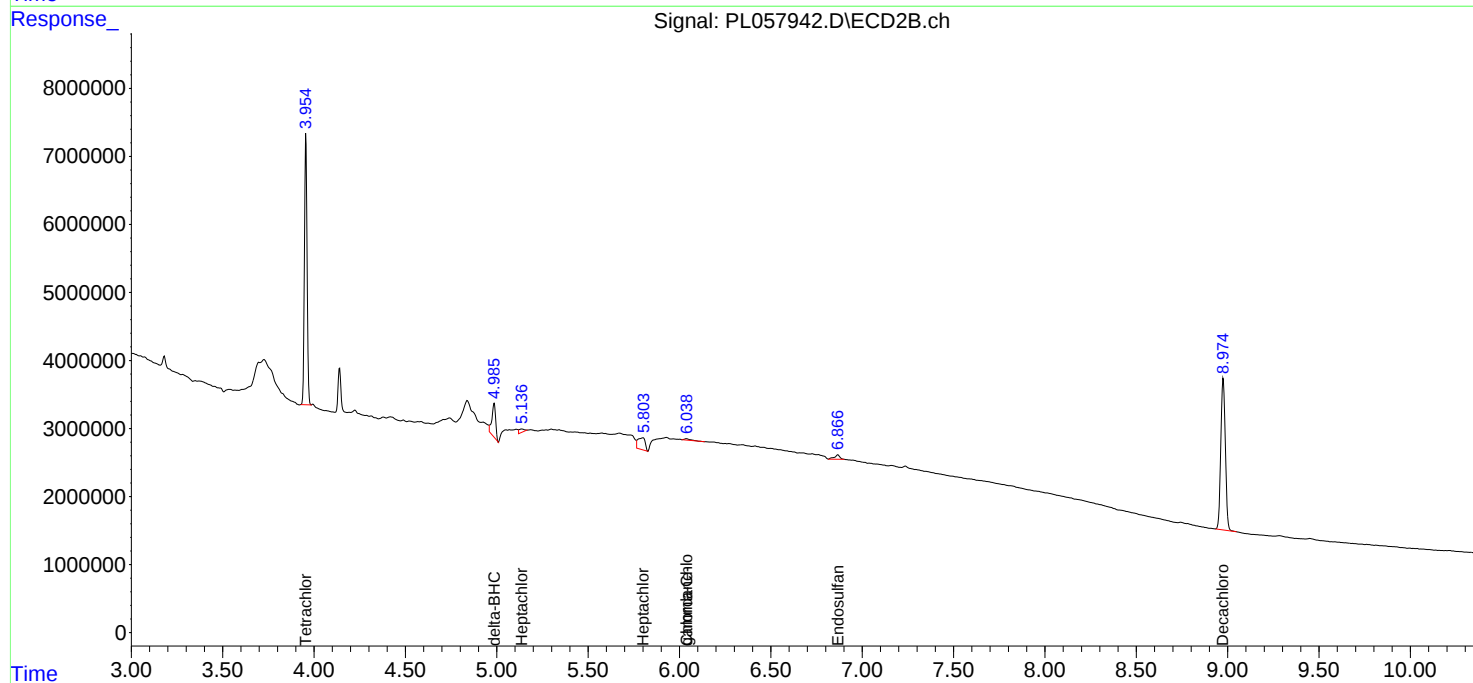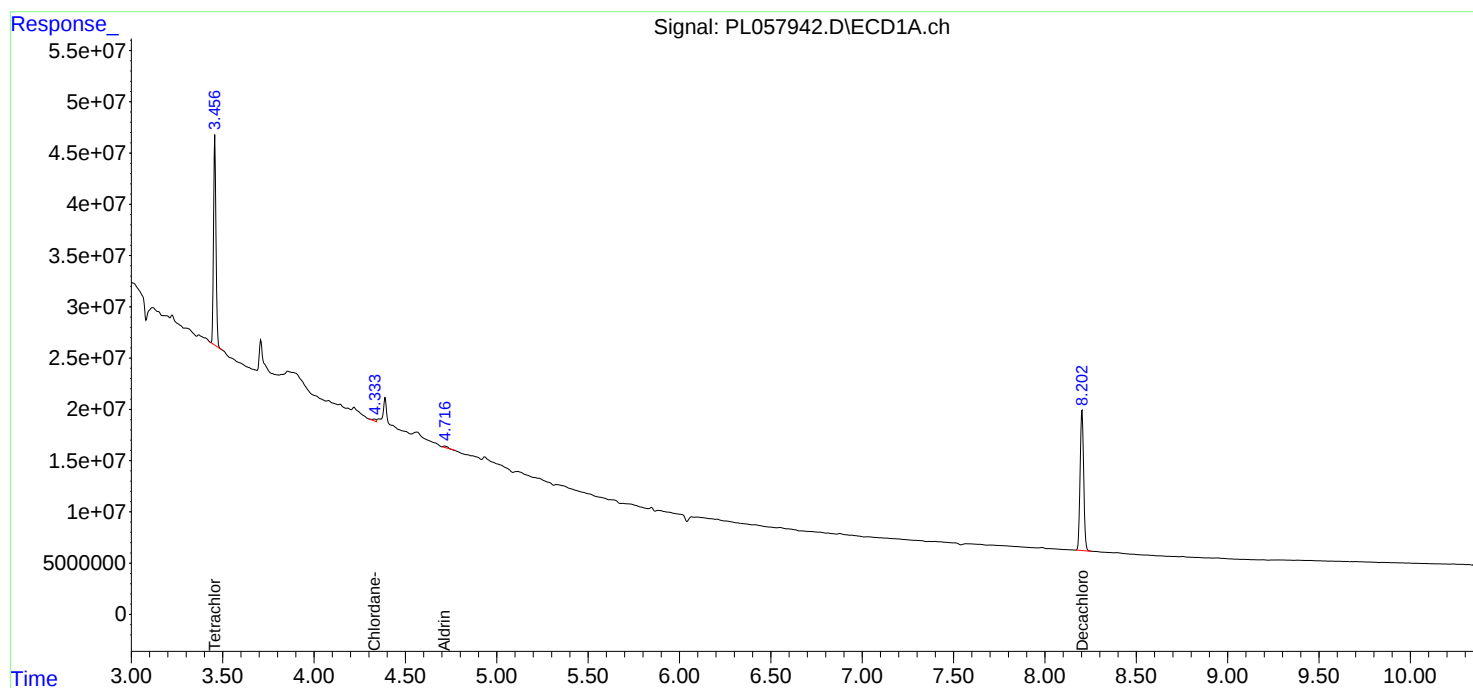


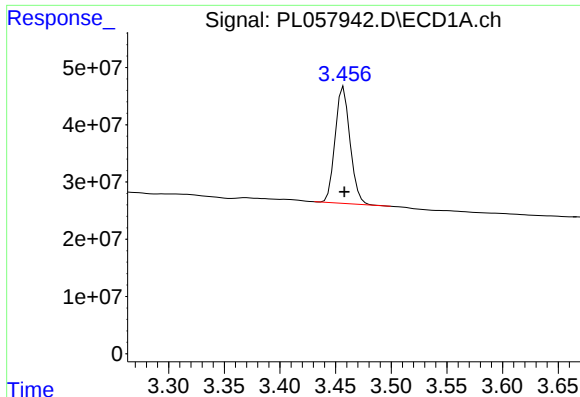

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 189545623
Conc: 18.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

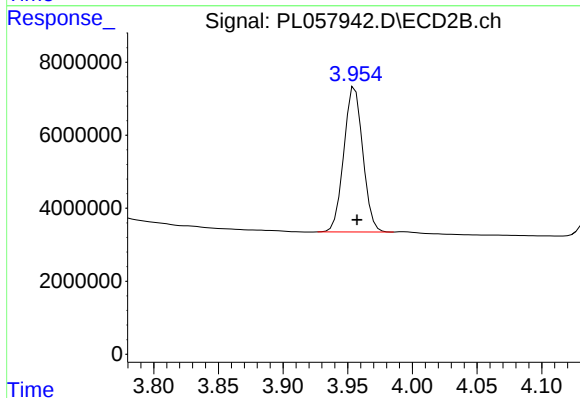


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.002 min
Response: 40475044
Conc: 18.65 ng/ml

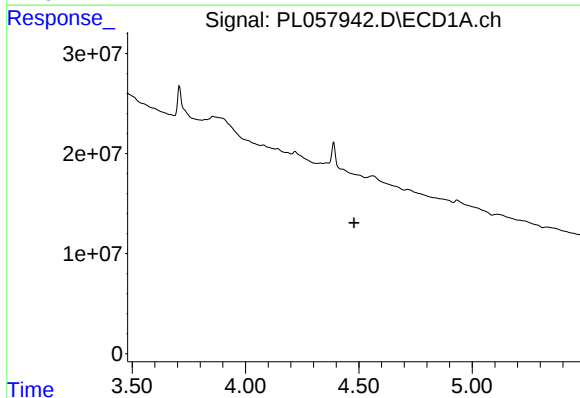


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

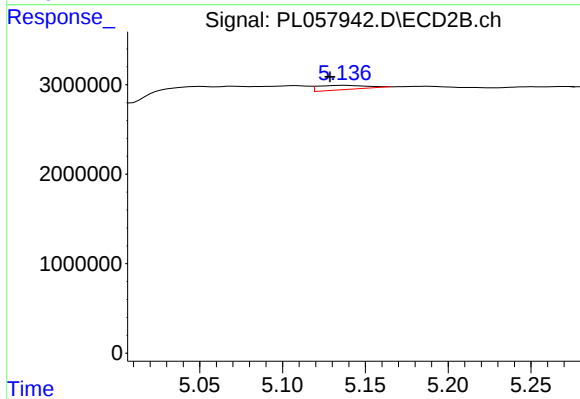

#4 Heptachlor


R.T.: 5.137 min
Delta R.T.: 0.008 min
Response: 633579
Conc: 0.19 ng/ml

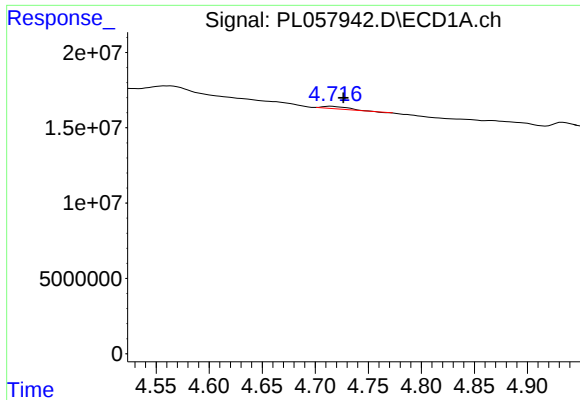

#5 Aldrin


R.T.: 4.715 min
Delta R.T.: -0.012 min
Response: 1351796
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

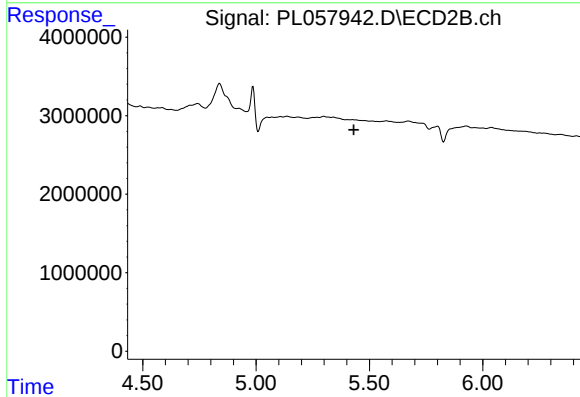


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.431 min
Response: 0
Conc: N.D.

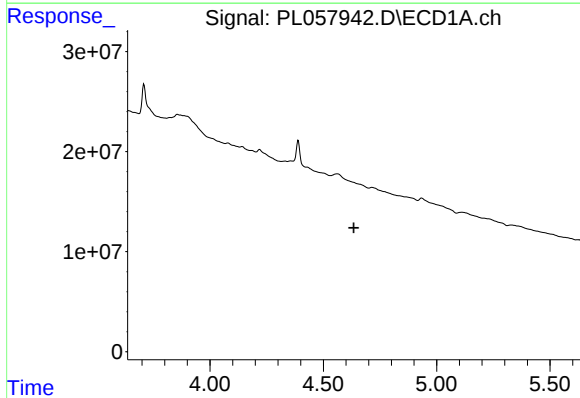


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.634 min
Response: 0
Conc: N.D.

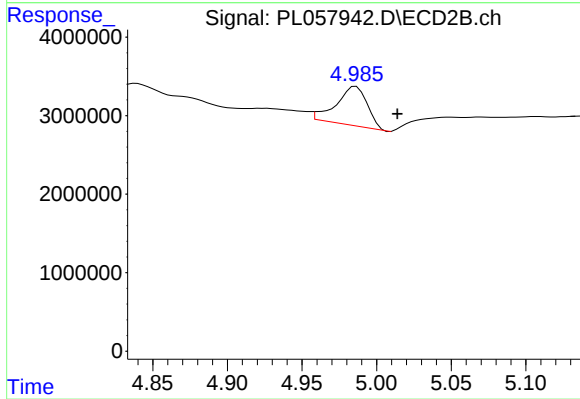

#7 delta-BHC


R.T.: 4.986 min
Delta R.T.: -0.028 min
Response: 7250868
Conc: 4.81 ng/ml

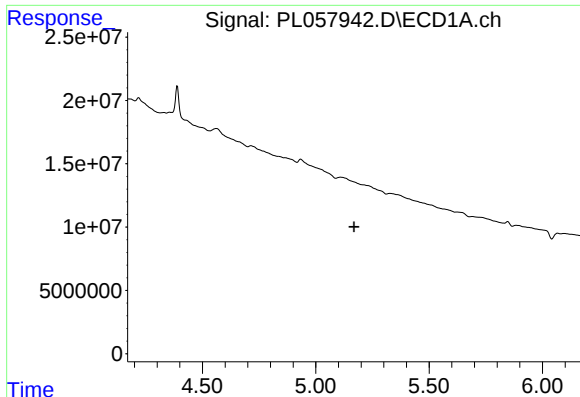

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

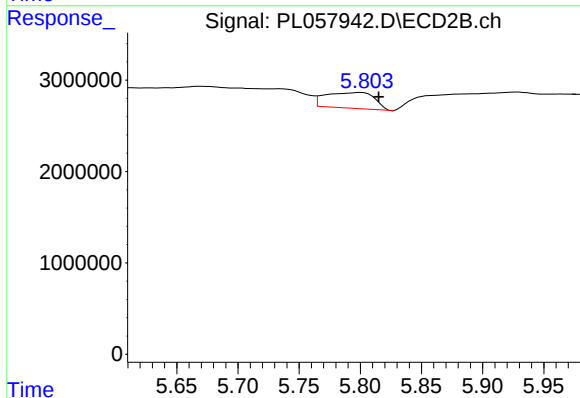


#8 Heptachlor epoxide

R.T.: 5.801 min
Delta R.T.: -0.014 min
Response: 4840350
Conc: 1.79 ng/ml

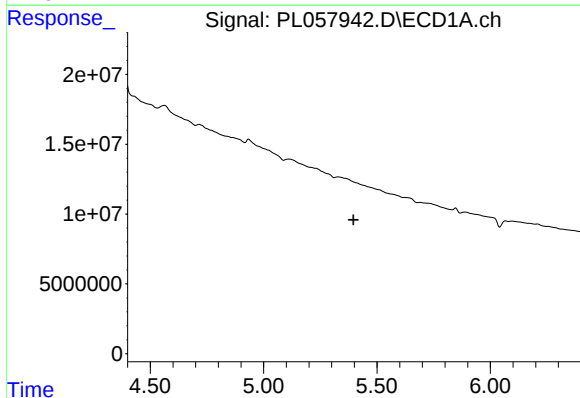


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

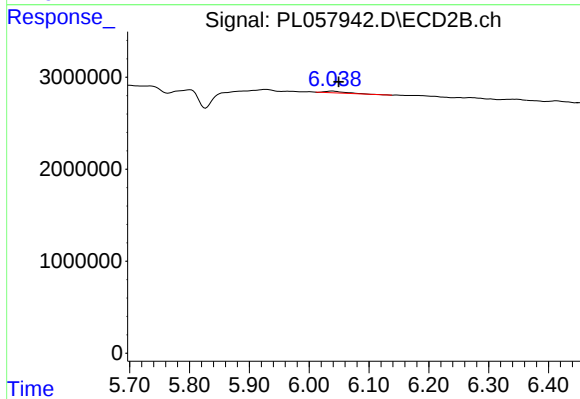

#10 gamma-Chlordane


R.T.: 6.039 min
Delta R.T.: -0.011 min
Response: 467779
Conc: 0.14 ng/ml

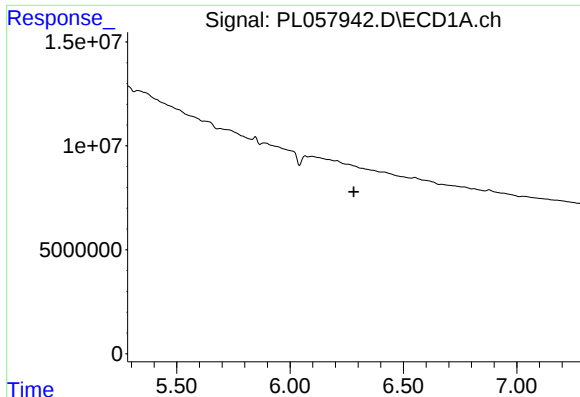

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

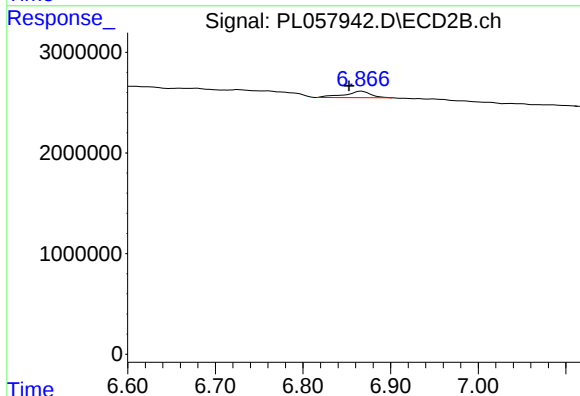


#15 Endosulfan II

R.T.: 6.867 min
Delta R.T.: 0.014 min
Response: 1251967
Conc: 0.48 ng/ml

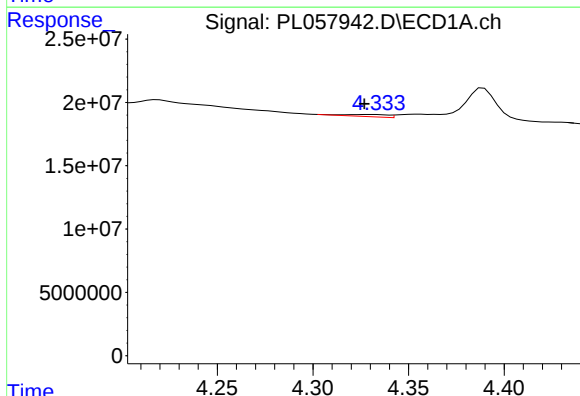


#23 Chlordane-1

R.T.: 4.331 min
Delta R.T.: 0.005 min
Response: 2694462
Conc: 7.29 ng/ml

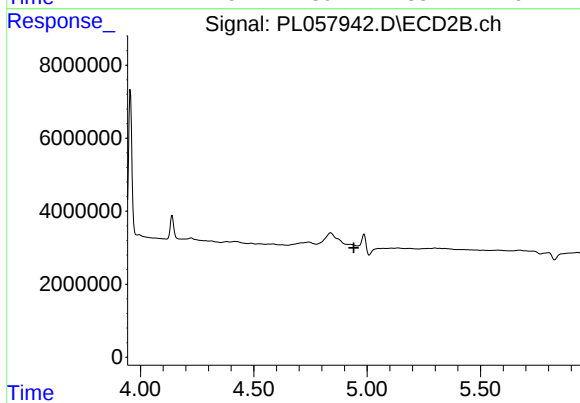

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

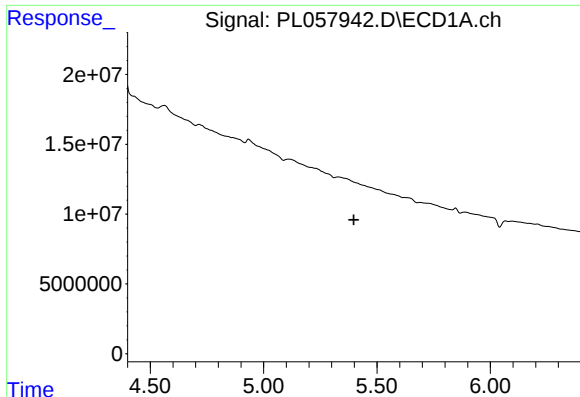

#25 Chlorodane-3


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

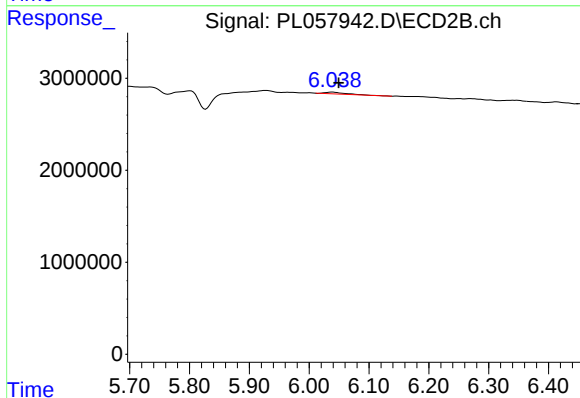


#25 Chlorodane-3

R.T.: 6.039 min
Delta R.T.: -0.010 min
Response: 467779
Conc: 1.08 ng/ml

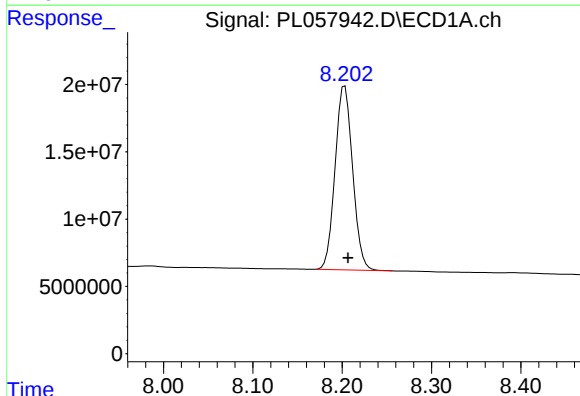

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 186288878
Conc: 18.07 ng/ml

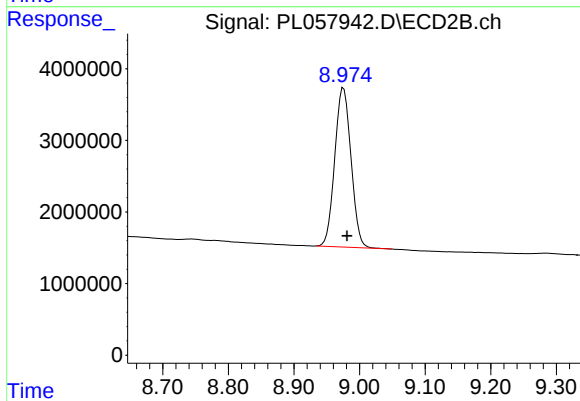

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.005 min
Response: 38360687
Conc: 17.17 ng/ml