

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
 Data File : PL057946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2020 05:40
 Operator : AJ\MA
 Sample : L2244-06
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 07:18:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	188.8E6	40158490	18.724	18.505
28)	SA Decachlor...	8.202	8.976	210.2E6	42752070	20.387	19.139
Target Compounds							
4)	MA Heptachlor	0.000	5.136	0	754776	N.D.	0.225 #
7)	B delta-BHC	0.000	4.984f	0	4127972	N.D.	3.610 #
8)	B Heptachlo...	0.000	5.799f	0	4931340	N.D.	1.826 #
12)	B 4,4'-DDE	0.000	6.252f	0	566132	N.D.	0.191 #
15)	B Endosulfa...	0.000	6.868f	0	367989	N.D.	0.142 #
23)	Chlordane-1	4.323	0.000	2715039	0	7.341	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
Data File : PL057946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2020 05:40
Operator : AJ\MA
Sample : L2244-06
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 07:18:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

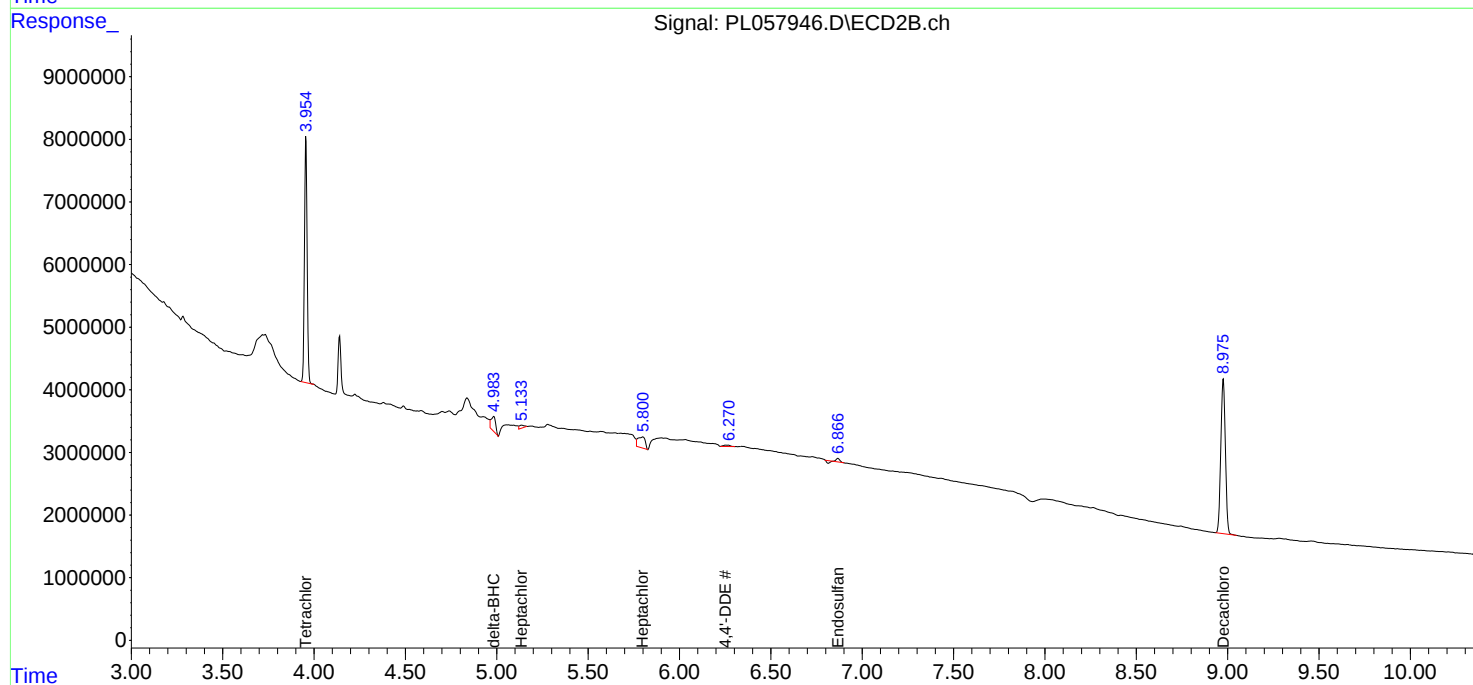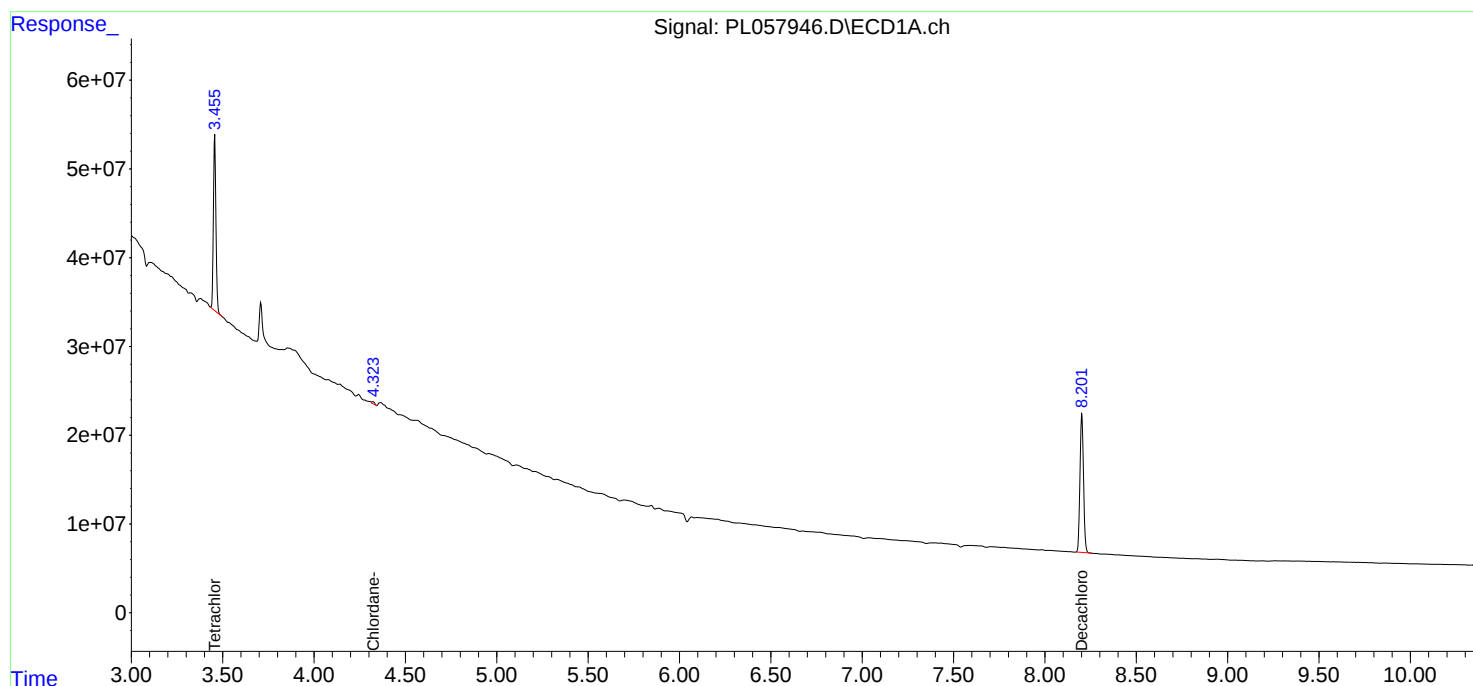


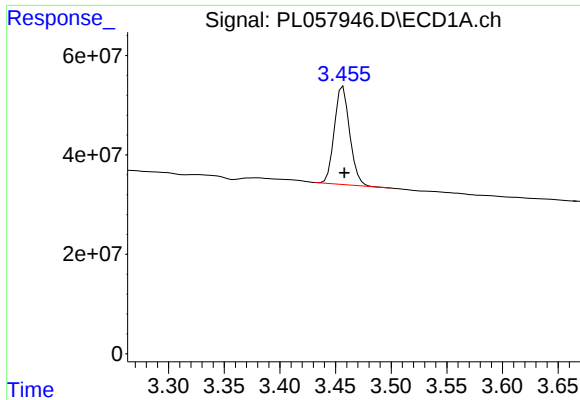

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 188760558
Conc: 18.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

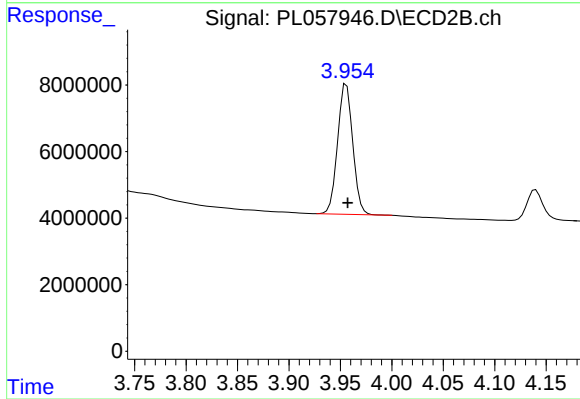


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 40158490
Conc: 18.50 ng/ml

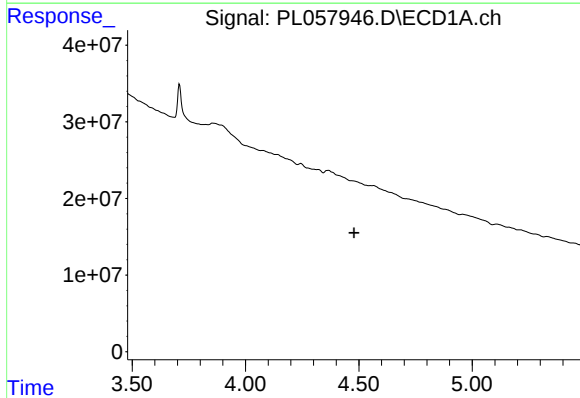


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

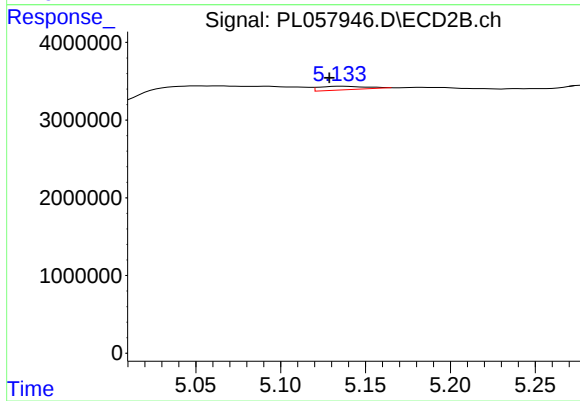

#4 Heptachlor


R.T.: 5.136 min
Delta R.T.: 0.007 min
Response: 754776
Conc: 0.22 ng/ml

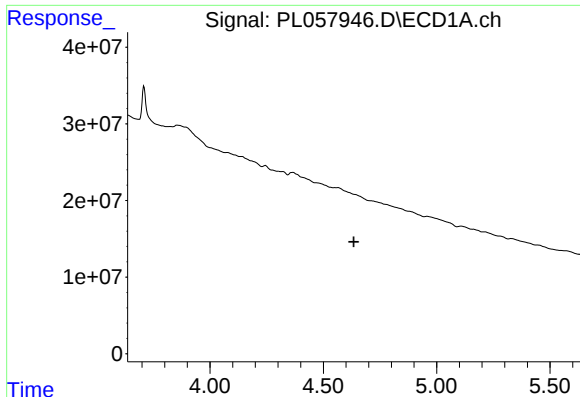

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

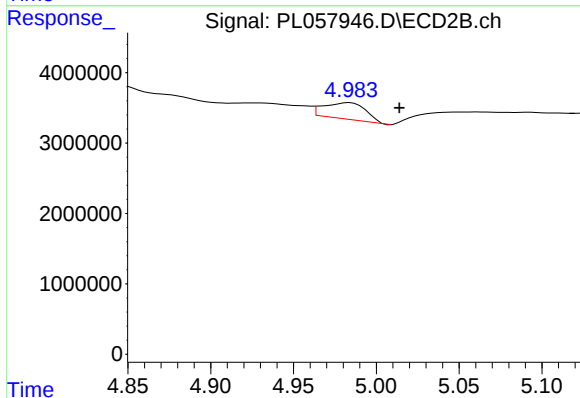


#7 delta-BHC

R.T.: 4.984 min
Delta R.T.: -0.030 min
Response: 4127972
Conc: 3.61 ng/ml

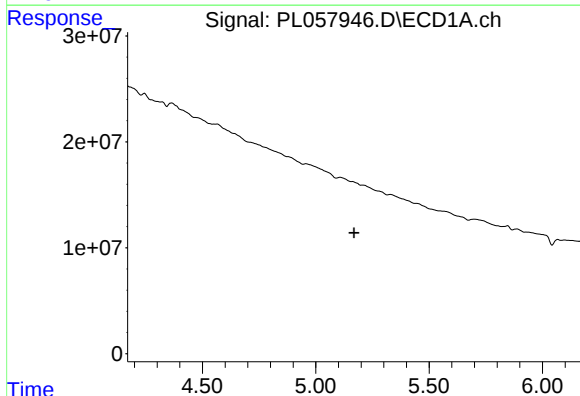


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

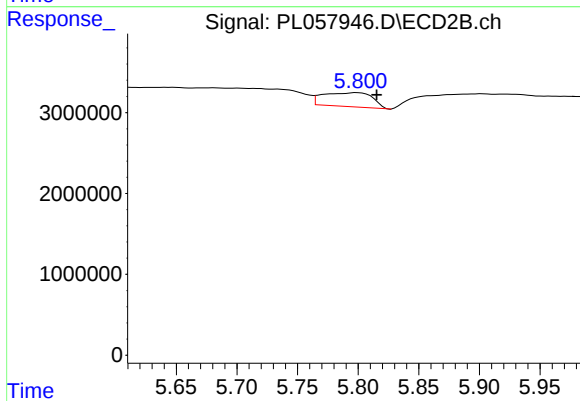

#8 Heptachlor epoxide


R.T.: 5.799 min
Delta R.T.: -0.016 min
Response: 4931340
Conc: 1.83 ng/ml

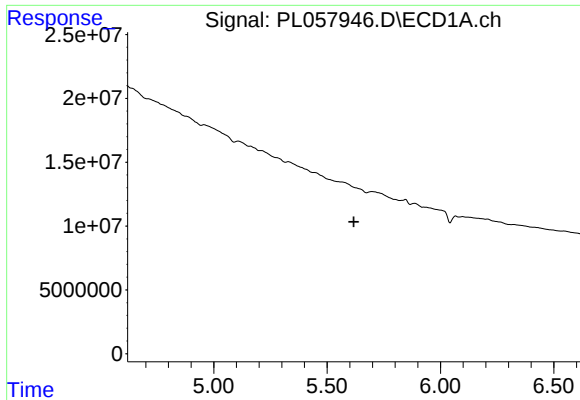

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.618 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

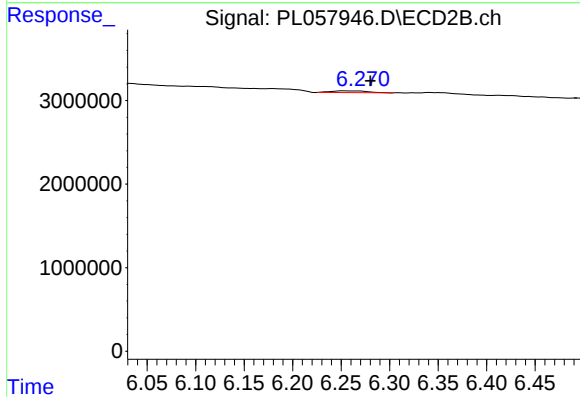


#12 4,4'-DDE

R.T.: 6.252 min
Delta R.T.: -0.028 min
Response: 566132
Conc: 0.19 ng/ml

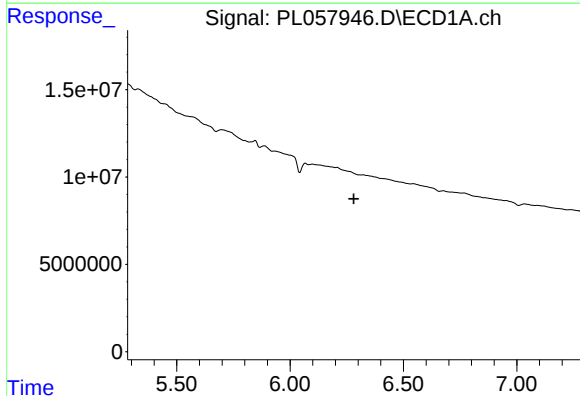


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

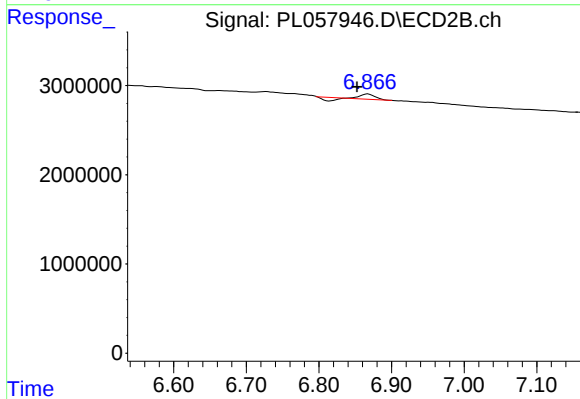

#15 Endosulfan II


R.T.: 6.868 min
Delta R.T.: 0.015 min
Response: 367989
Conc: 0.14 ng/ml

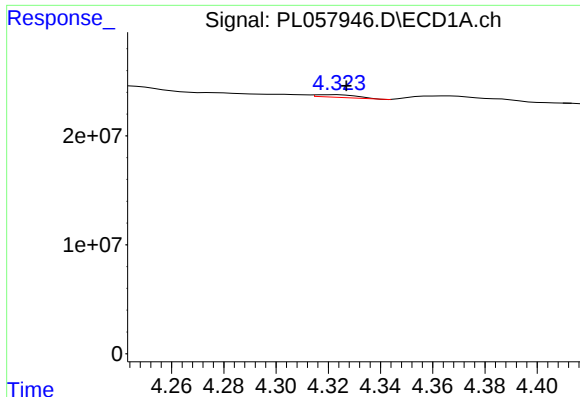

#23 Chlordane-1


R.T.: 4.323 min
Delta R.T.: -0.004 min
Response: 2715039
Conc: 7.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

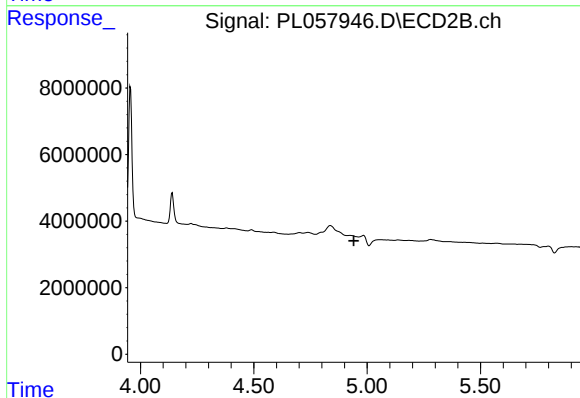


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

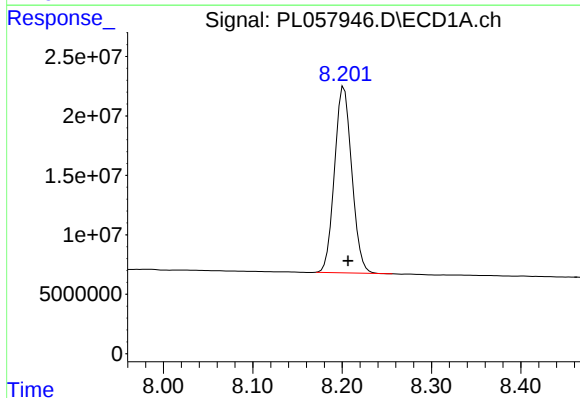

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.005 min
Response: 210163759
Conc: 20.39 ng/ml

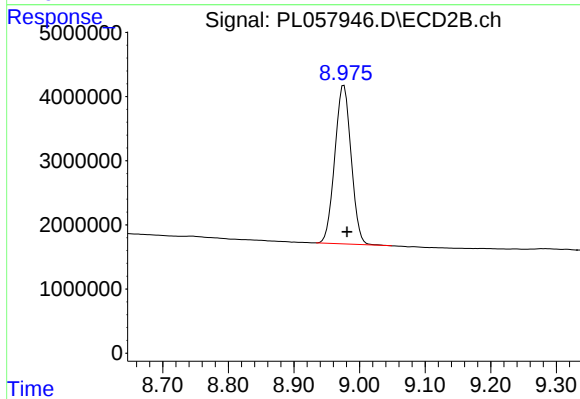

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.005 min
Response: 42752070
Conc: 19.14 ng/ml