

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
 Data File : PL057887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2020 14:30
 Operator : AJ\MA
 Sample : L2197-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RECLAIM-SYSTEM-SLUDGE-SEPA

Manual Integrations
 APPROVED

mohammad
 4/14/2020 1:17:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 01:01:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.956	180.9E6	39761733	17.949m	18.322
28)	SA Decachlor...	8.207	8.980	135.9E6	42646186	13.179m	19.092 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
Data File : PL057887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2020 14:30
Operator : AJ\MA
Sample : L2197-04
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RECLAIM-SYSTEM-SLUDGE-SEPA


Manual Integrations
APPROVED

mohammad
4/14/2020 1:17:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 01:01:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

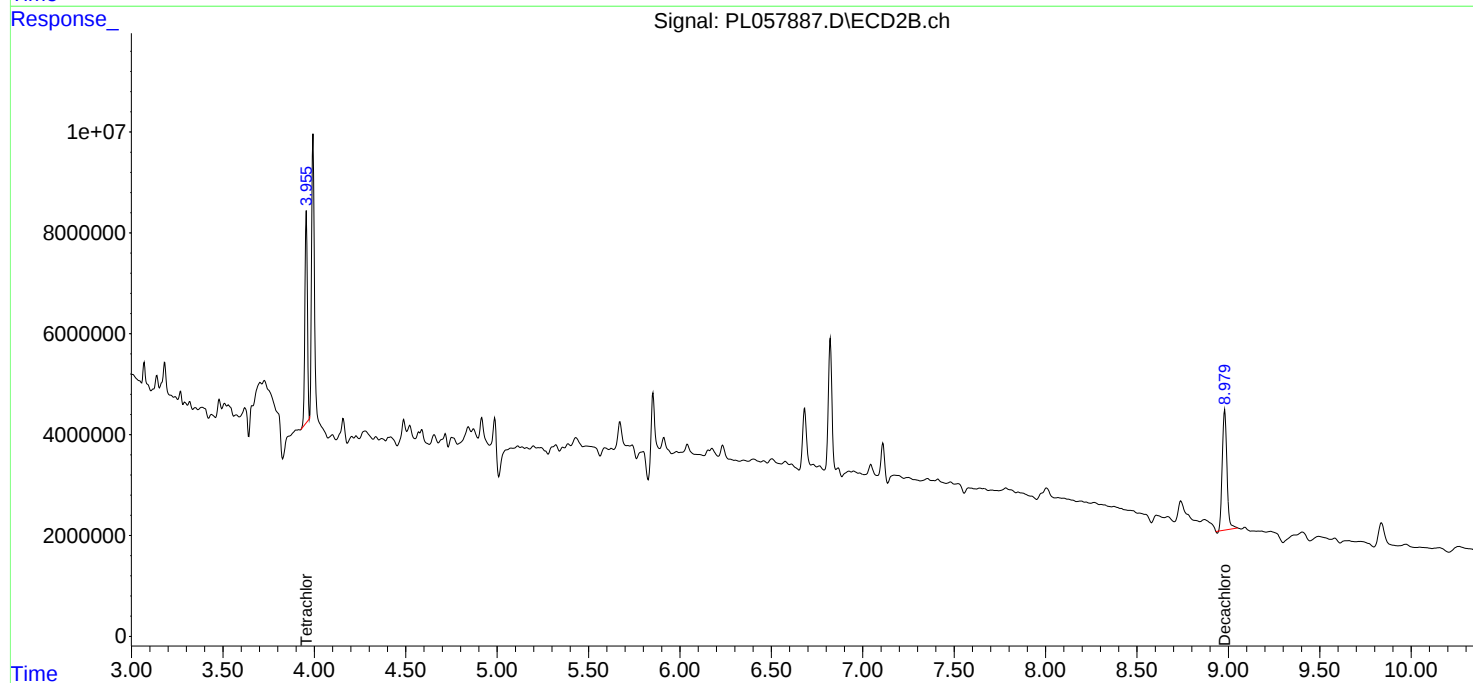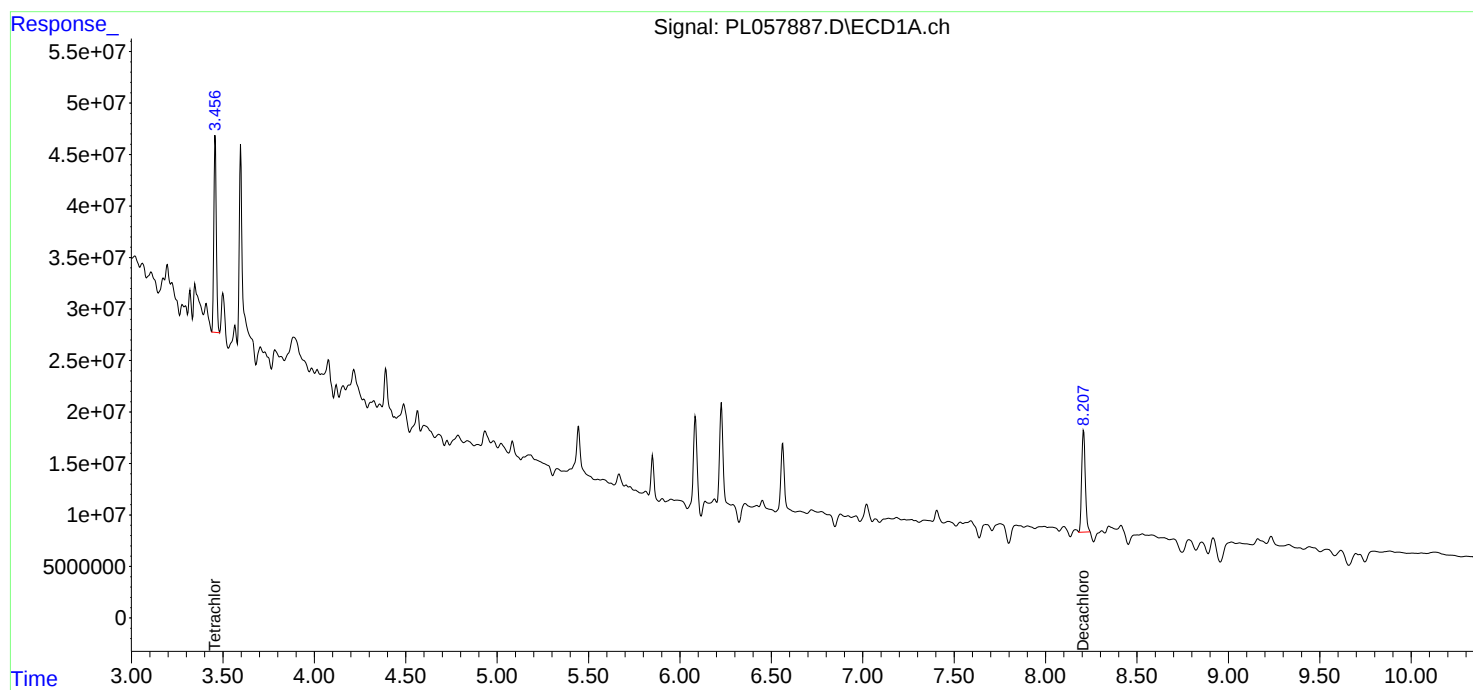

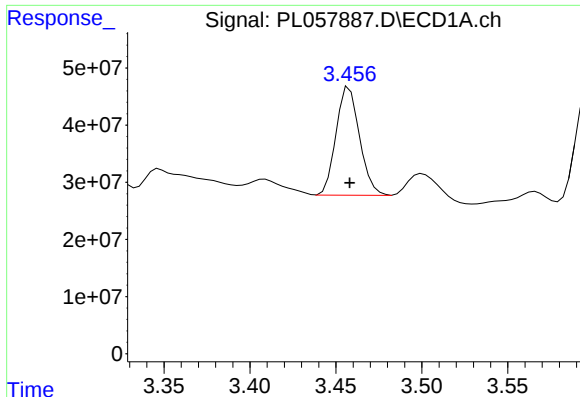


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 180940575
Conc: 17.95 ng/ml m

Instrument :
ECD_L
ClientSampleId :
RECLAIM-SYSTEM-SLUDGE-SEPA


Manual Integrations
APPROVED

mohammad
4/14/2020 1:17:33 PM

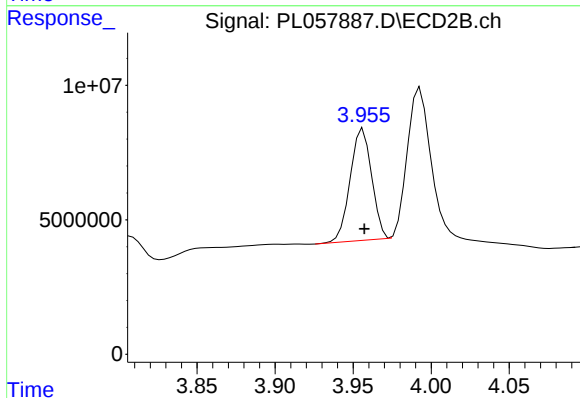


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: 0.000 min
Response: 39761733
Conc: 18.32 ng/ml

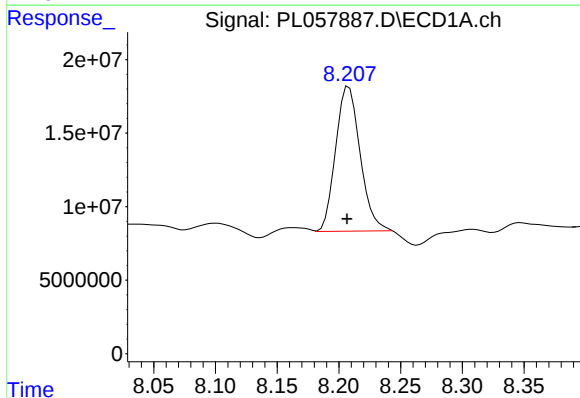

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 135853652
Conc: 13.18 ng/ml m

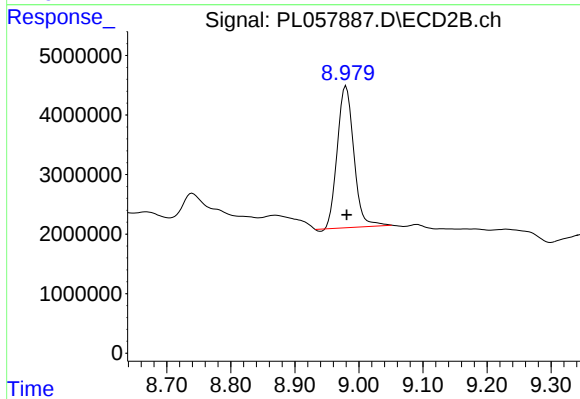

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: 0.000 min
Response: 42646186
Conc: 19.09 ng/ml