

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
 Data File : PL057929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2020 00:56
 Operator : AJ\MA
 Sample : L2230-20
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-12-A

Manual Integrations
 APPROVED

mohammad
 4/14/2020 1:18:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 07:14:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	203.7E6	42797907	20.204	19.721
28)	SA Decachlor...	8.203	8.976	186.6E6	39261759	18.103	17.576
Target Compounds							
10)	B gamma-Chl...	5.395	6.050	9308722	3116186	0.685m	0.962 #
16)	A 4,4'-DDD	6.130	6.762	8391738	3582611	0.840m	1.570m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041320\
Data File : PL057929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2020 00:56
Operator : AJ\MA
Sample : L2230-20
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-12-A


Manual Integrations
APPROVED

mohammad
4/14/2020 1:18:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 07:14:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

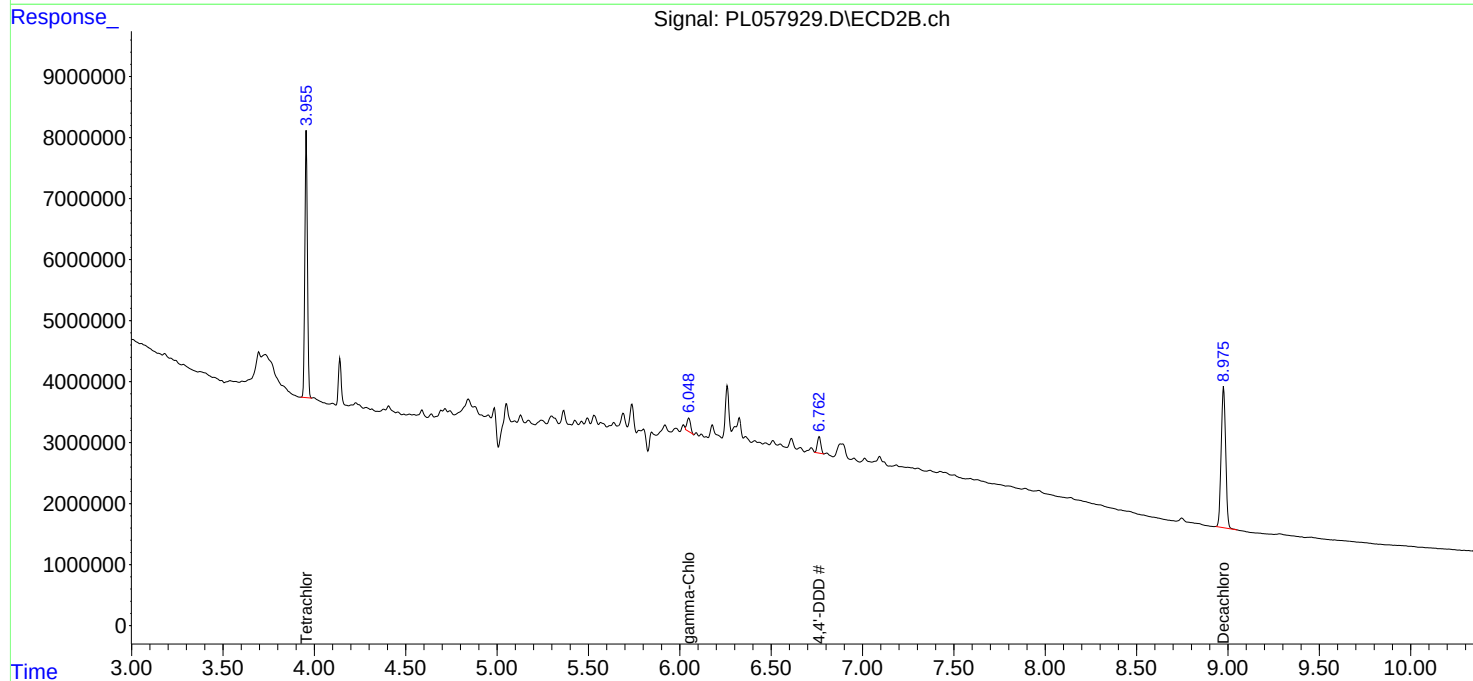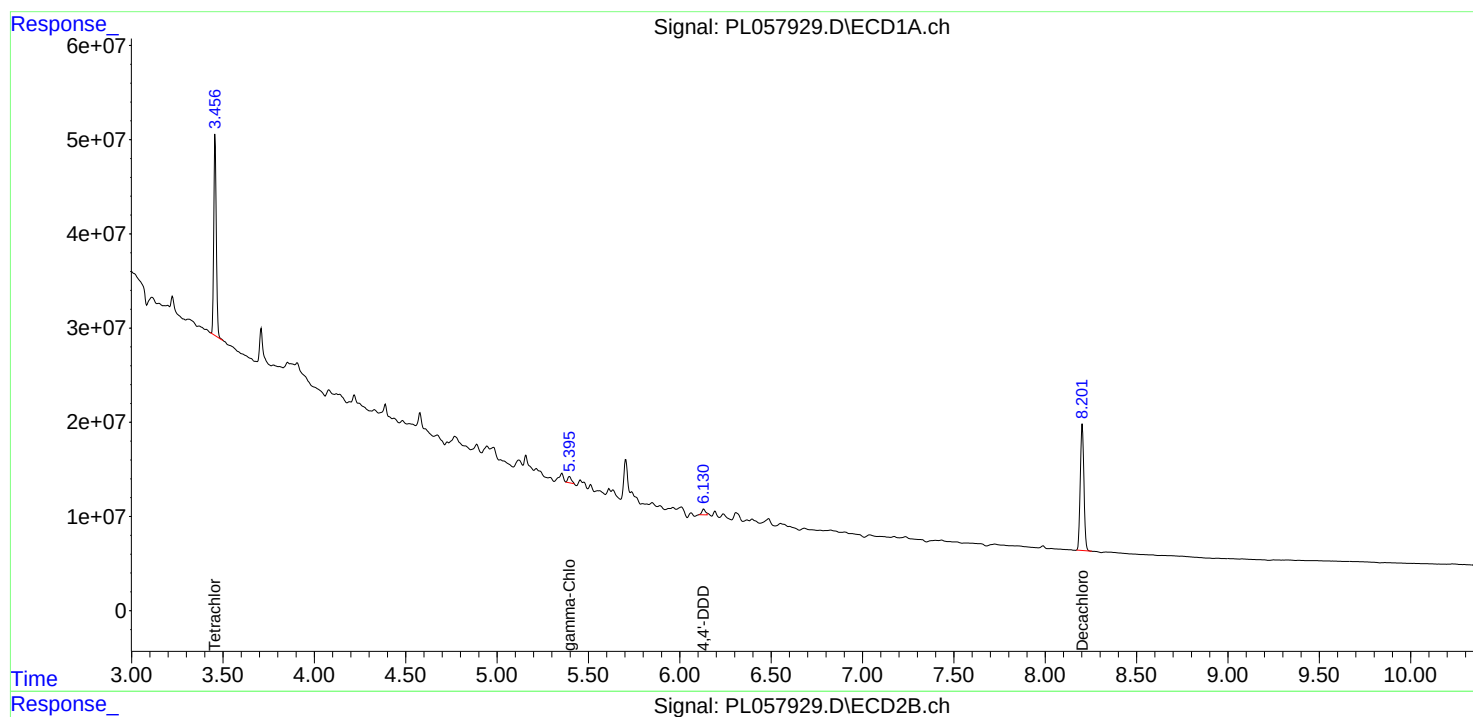

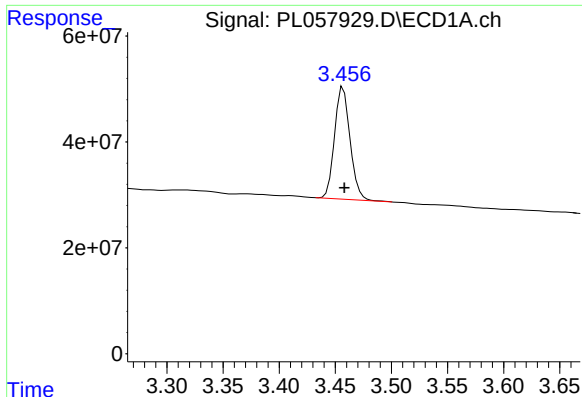


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 203678572
Conc: 20.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-12-A


Manual Integrations
APPROVED

mohammad
4/14/2020 1:18:04 PM

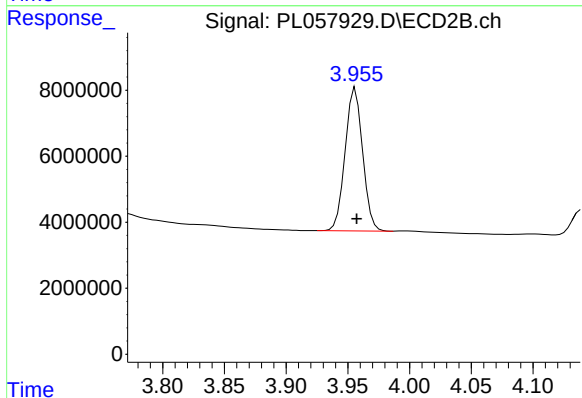


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 42797907
Conc: 19.72 ng/ml

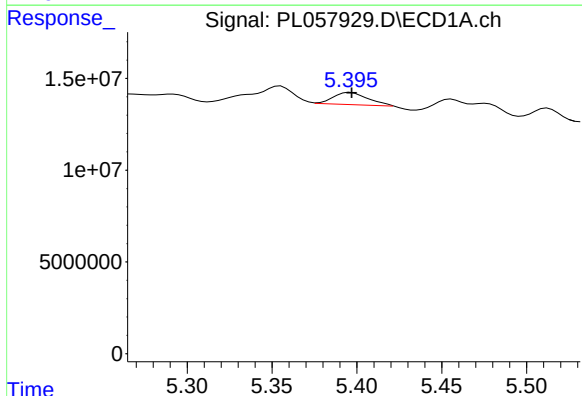


#10 gamma-Chlordane

R.T.: 5.395 min
Delta R.T.: -0.002 min
Response: 9308722
Conc: 0.69 ng/ml m

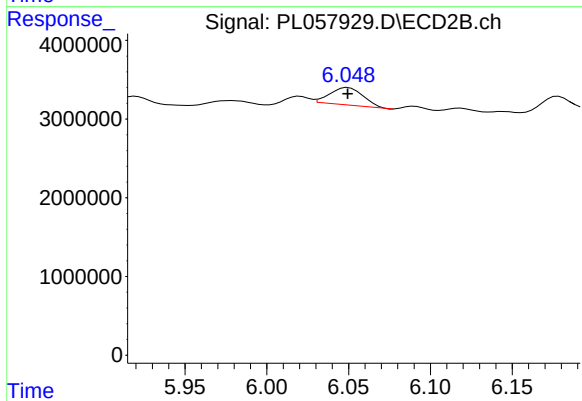

#10 gamma-Chlordane

R.T.: 6.050 min
Delta R.T.: 0.000 min
Response: 3116186
Conc: 0.96 ng/ml

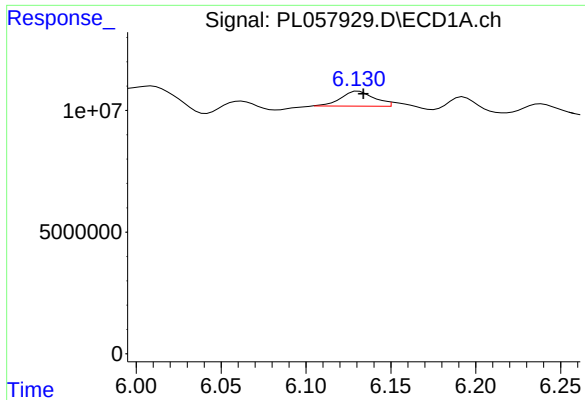


#16 4,4'-DDD

R.T.: 6.130 min
Delta R.T.: -0.004 min
Response: 8391738
Conc: 0.84 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-12-A


Manual Integrations
APPROVED

mohammad
4/14/2020 1:18:04 PM

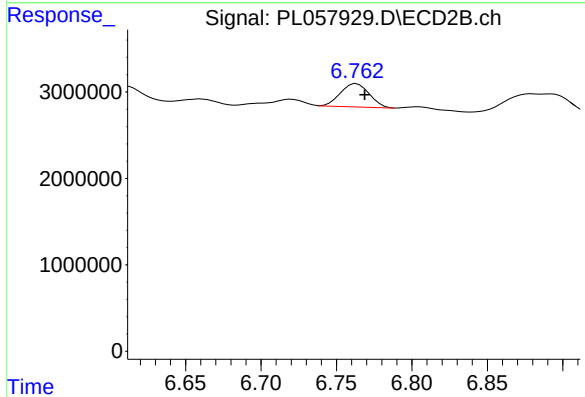


#16 4,4'-DDD

R.T.: 6.762 min
Delta R.T.: -0.007 min
Response: 3582611
Conc: 1.57 ng/ml m

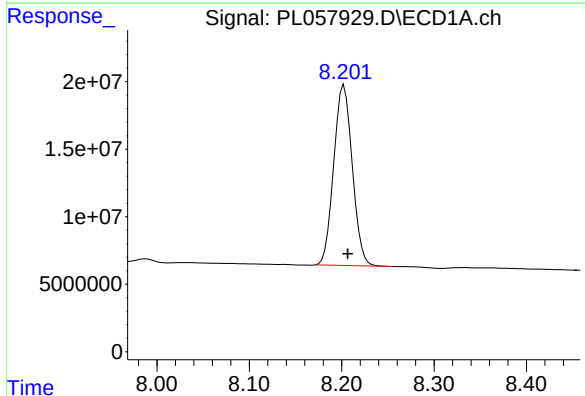

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 186618775
Conc: 18.10 ng/ml

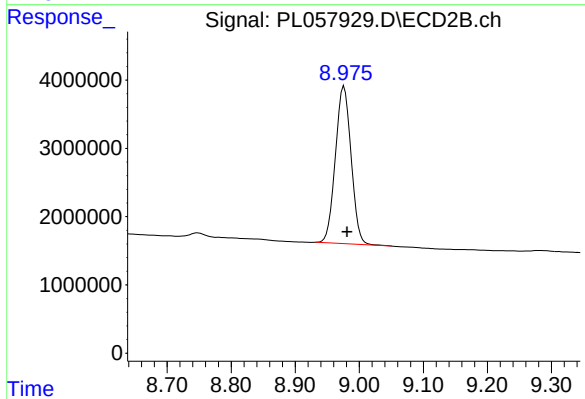

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.005 min
Response: 39261759
Conc: 17.58 ng/ml