

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041323\
 Data File : PL082018.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2023 15:20
 Operator : AR\AJ
 Sample : TOXAPHENE501
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 09:13:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 13 09:07:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.326	2.653	201.7E6	193.0E6	77.617	77.787
27)	SA Decachlor...	8.746	7.768	268.6E6	359.8E6	148.321	151.198
Target Compounds							
22)	Toxaphene-1	5.996	5.187	122.8E6	85818943	7748.865	7848.975
23)	Toxaphene-2	6.813	5.545	482.7E6	104.6E6	7923.366	8241.851
24)	Toxaphene-3	6.900	6.585	348.6E6	593.4E6	7978.209	8172.499
25)	Toxaphene-4	6.996	6.895	210.3E6	371.2E6	7960.772	8128.337
26)	Toxaphene-5	7.679	7.029	252.4E6	205.5E6	7857.328	8380.861

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041323\
Data File : PL082018.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2023 15:20
Operator : AR\AJ
Sample : TOXAPHENE501
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 09:13:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041323CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 13 09:07:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

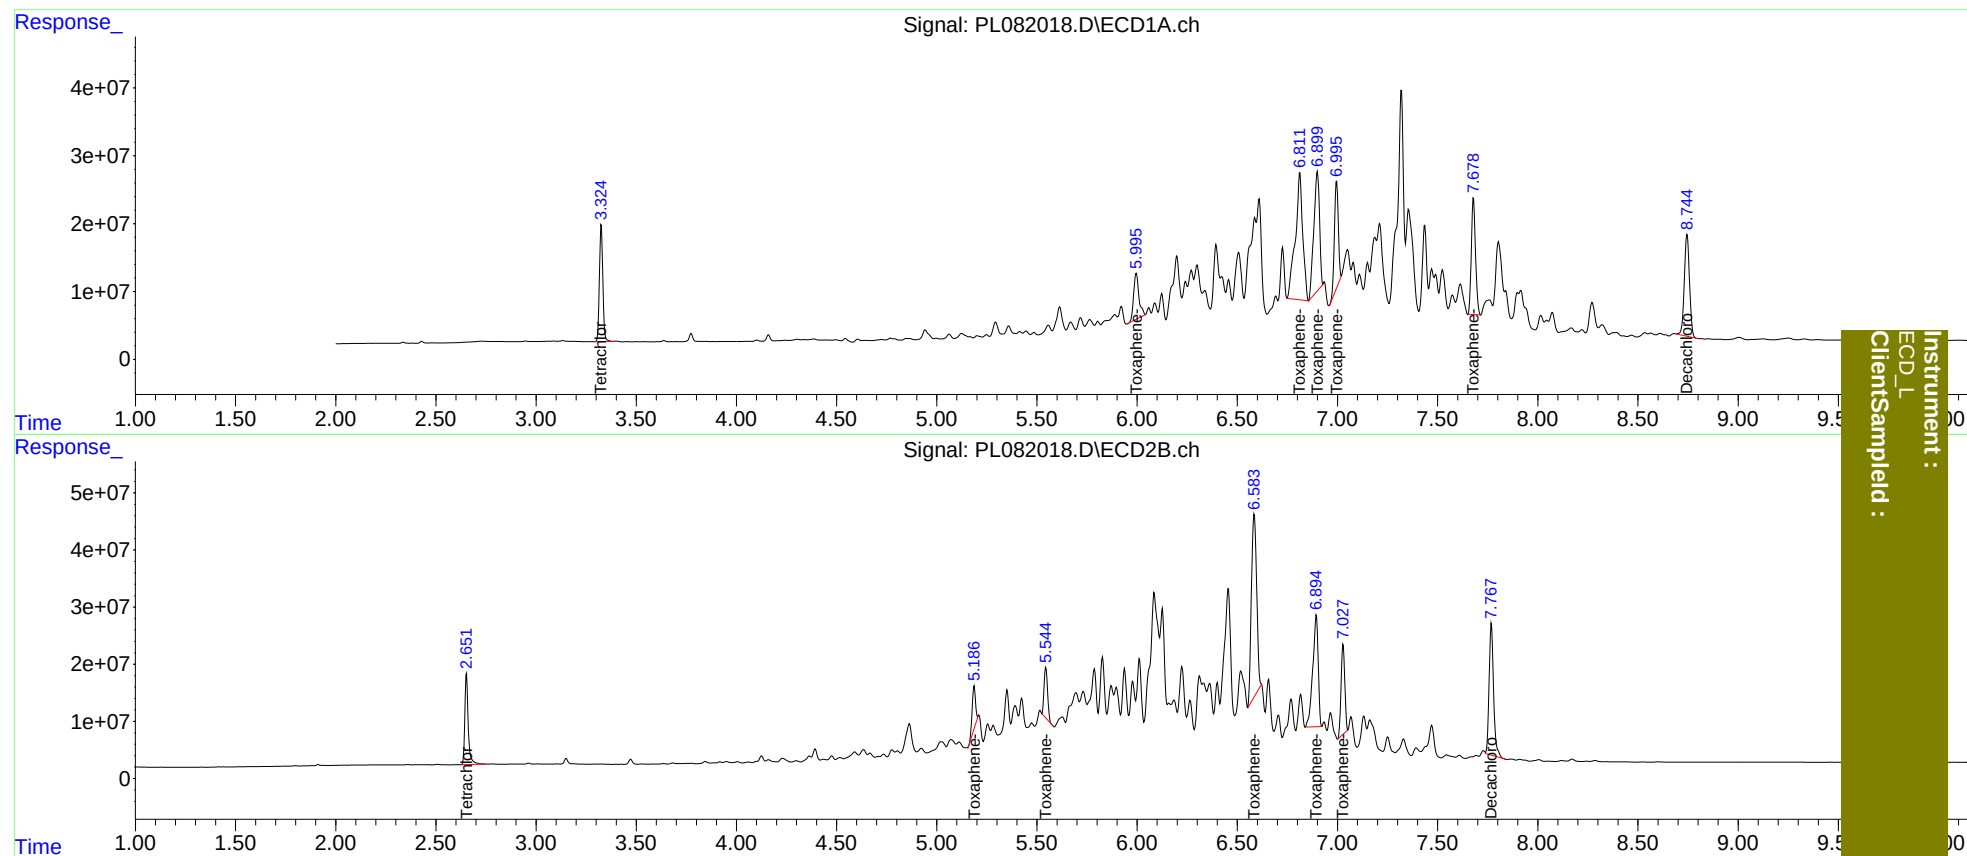

Instrument :
ECD_L
ClientSampled :
PL041323CLP.M Thu Apr 13 09:13:24 2023