

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041323\
 Data File : PL082025.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2023 16:59
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 03:48:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 13 03:40:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	2.653	89580821	87372645	39.687	39.598
27)	SA Decachlor...	8.746	7.767	121.5E6	155.1E6	78.921	78.880
Target Compounds							
2)	A alpha-BHC	3.775	3.151	128.4E6	117.3E6	39.270	39.502
3)	MA gamma-BHC...	4.103	3.478	120.3E6	112.2E6	39.270	39.153
4)	MA Heptachlor	4.681	3.811	116.7E6	112.0E6	39.255	39.228
9)	A Endosulfan I	5.825	4.957	87897830	88304022	39.481	39.448
13)	MA Dieldrin	6.100	5.221	185.8E6	194.5E6	78.759	79.049
14)	MA Endrin	6.327	5.495	164.8E6	172.9E6	78.778	78.927
16)	A 4,4'-DDD	6.471	5.646	139.0E6	135.7E6	78.726	78.980
17)	MA 4,4'-DDT	6.782	5.895	142.9E6	153.4E6	78.723	78.743
20)	A Methoxychlor	7.262	6.475	382.6E6	414.4E6	395.401	395.975

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041323\
Data File : PL082025.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2023 16:59
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 03:48:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041323CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 13 03:40:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

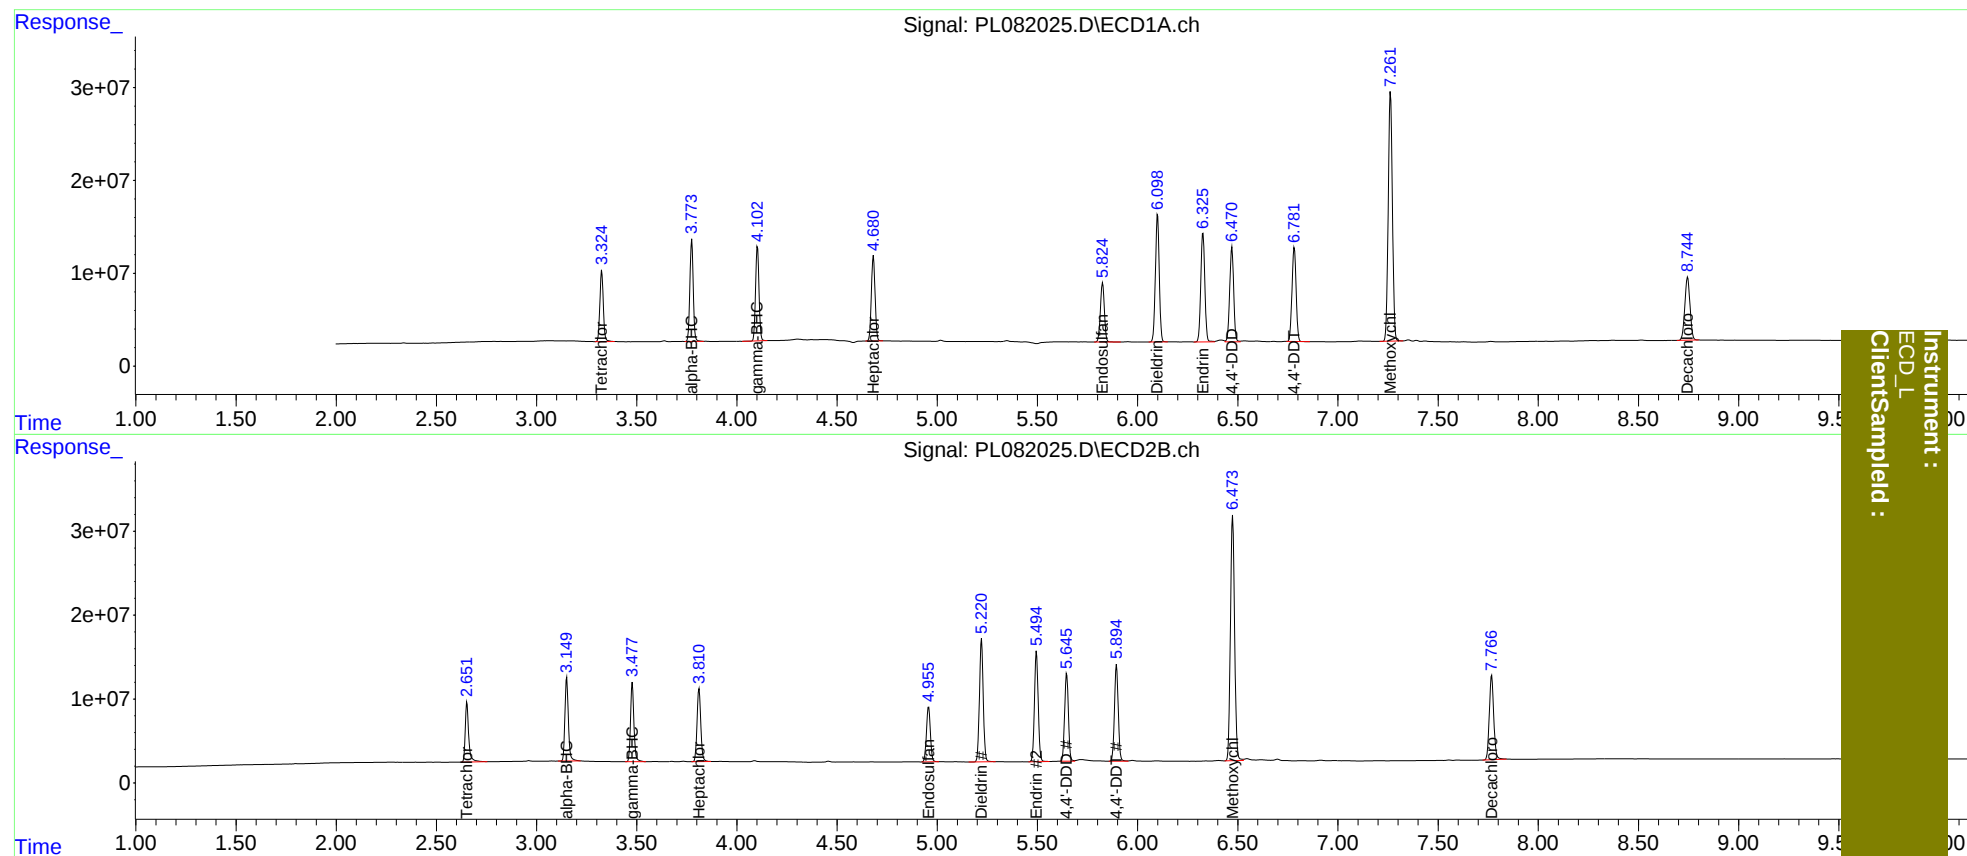

Instrument :
ECD_L
ClientSampled :
PL041323CLP.M Thu Apr 13 03:48:29 2023