

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041323\
 Data File : PL082021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2023 16:03
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA2333

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 03:53:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 13 03:40:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	2.652	23061094	22506896	10.162	10.150
27)	SA Decachlor...	8.745	7.767	34487147	44009428	21.751	21.731
Target Compounds							
2)	A alpha-BHC	3.773	3.150	30958407	27680981	9.608m	9.484
3)	MA gamma-BHC...	4.102	3.477	29380712	27382546	9.689	9.665
4)	MA Heptachlor	4.681	3.810	30083819	28468852	10.091	9.981
9)	A Endosulfan I	5.825	4.957	23246940	22669606	10.328	10.095
13)	MA Dieldrin	6.099	5.221	46302703	47825358	19.722	19.571
14)	MA Endrin	6.327	5.495	40825500	42106208	19.637	19.409
16)	A 4,4'-DDD	6.470	5.647	34867811	31721739	19.815	18.830
17)	MA 4,4'-DDT	6.782	5.895	35808545	36710270	19.789	19.122
20)	A Methoxychlor	7.262	6.475	102.2E6	109.5E6	104.183	103.433

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041323\
 Data File : PL082021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2023 16:03
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 03:53:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041323CLP.M
 Quant Title : GC Extractables
 Qlast Update : Thu Apr 13 03:40:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Signal #2 Phase: ZB-MR1

Signal: PL082021.D\ECD1A.ch

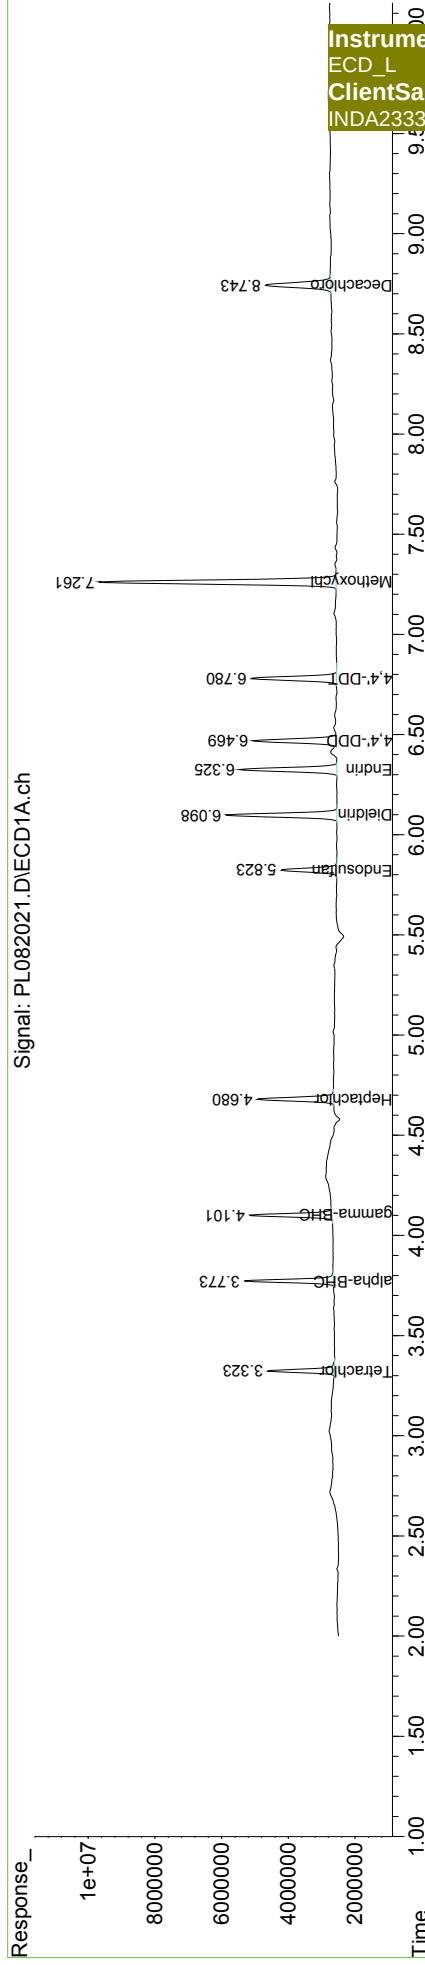

Signal: PL082021.D\ECD2B.ch

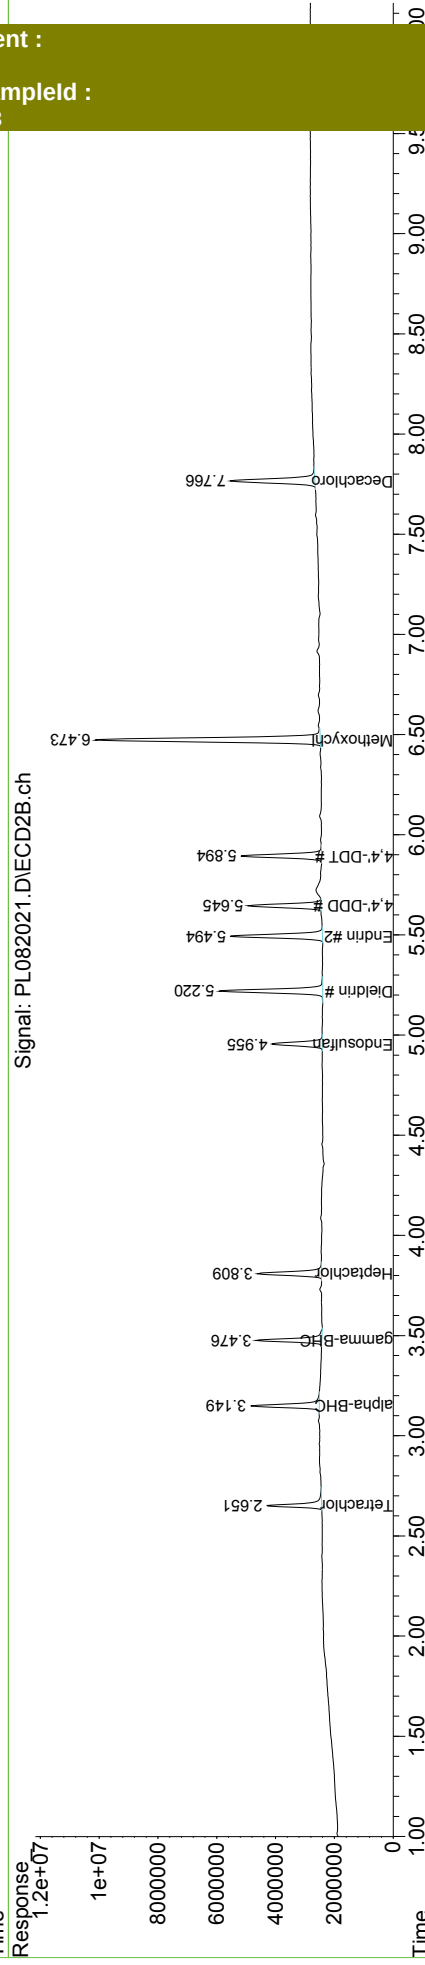

Instrument :
 ECD_1
 ClientSampleId :
 INDA2333