

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041420\
 Data File : PL057982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2020 20:27
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 01:17:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	228.3E6	47743072	22.649	22.000
28)	SA Decachlor...	8.203	8.977	209.2E6	47351963	20.290	21.198
Target Compounds							
2)	A alpha-BHC	3.900	0.000	6177691	0	0.356	N.D. #
4)	MA Heptachlor	0.000	5.139	0	1235405	N.D.	0.368 #
8)	B Heptachlo...	0.000	5.801	0	7030072	N.D.	2.603 #
13)	MA Dieldrin	5.734f	0.000	229120	0	0.018	N.D. #
18)	B Endrin al...	6.447	0.000	707988	0	0.076	N.D. #
23)	Chlordane-1	4.349f	0.000	2429103	0	6.568	N.D. #
24)	Chlordane-2	4.842	0.000	3426627	0	8.488	N.D. #
27)	Chlordane-5	0.000	6.923	0	705854	N.D.	8.279 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041420\
Data File : PL057982.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2020 20:27
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 01:17:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

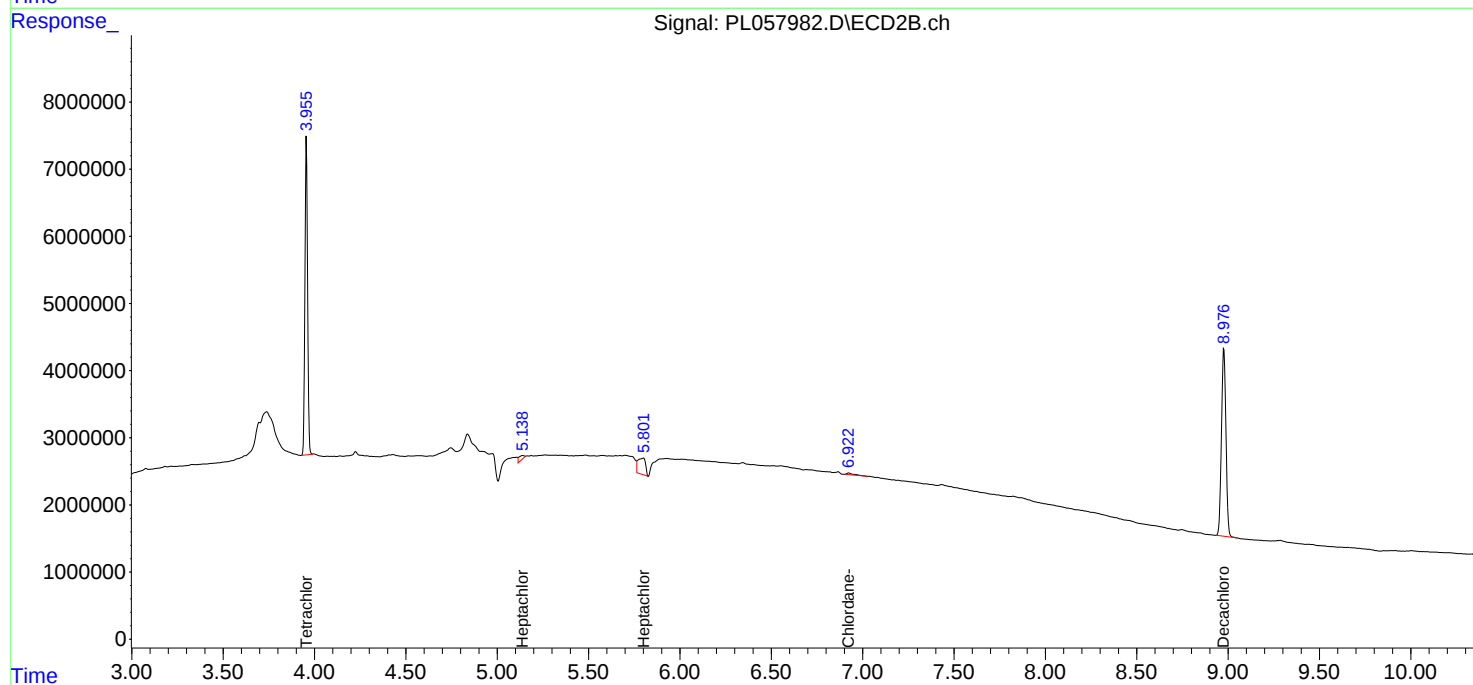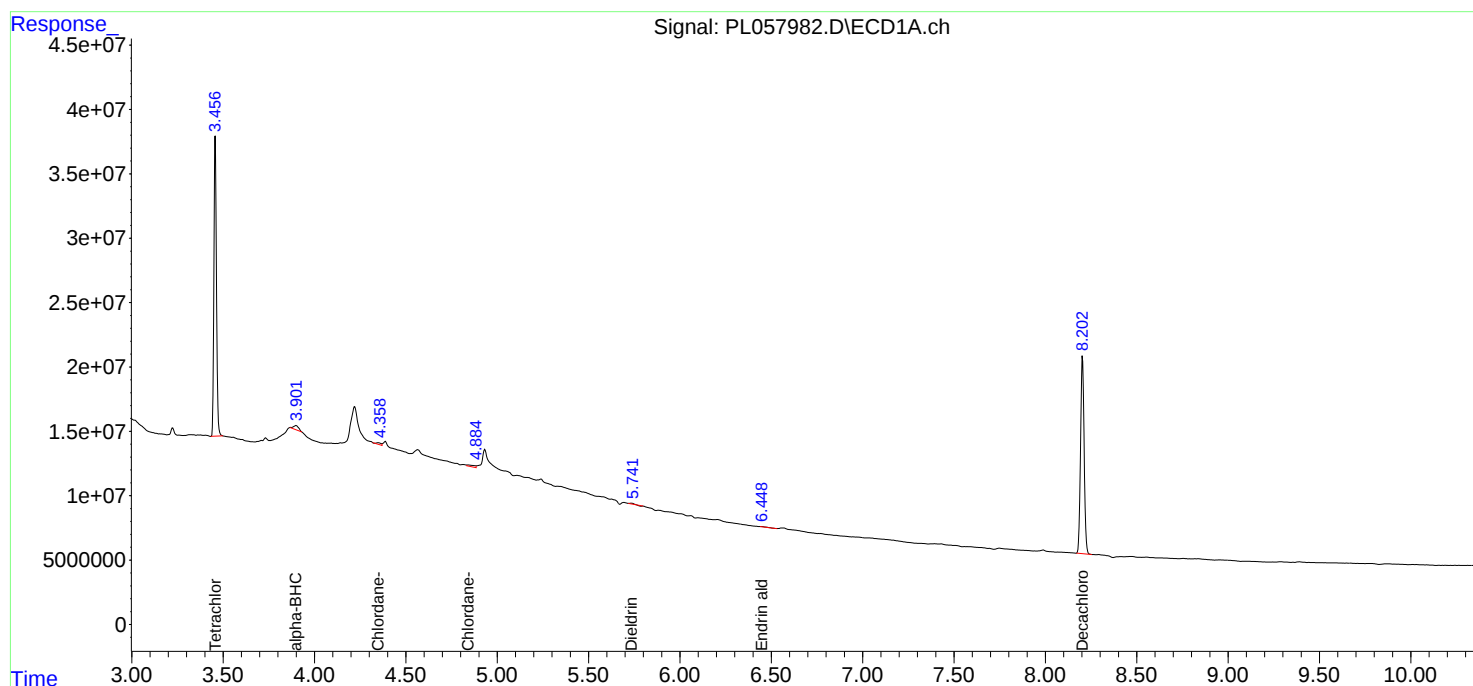


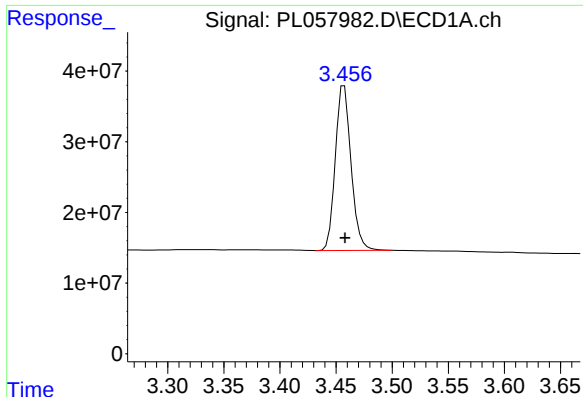

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 228327641
Conc: 22.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

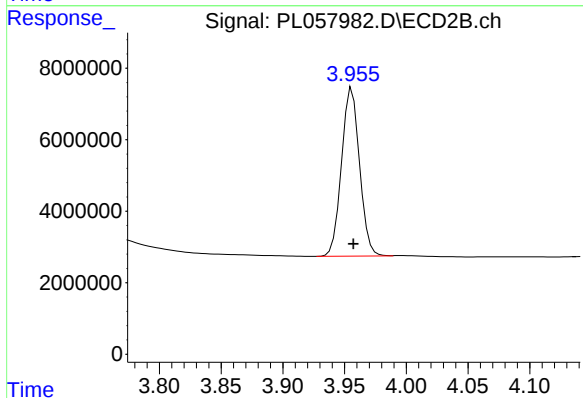


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 47743072
Conc: 22.00 ng/ml

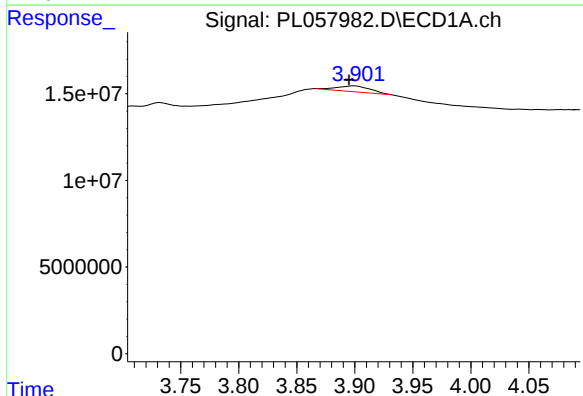


#2 alpha-BHC

R.T.: 3.900 min
Delta R.T.: 0.005 min
Response: 6177691
Conc: 0.36 ng/ml

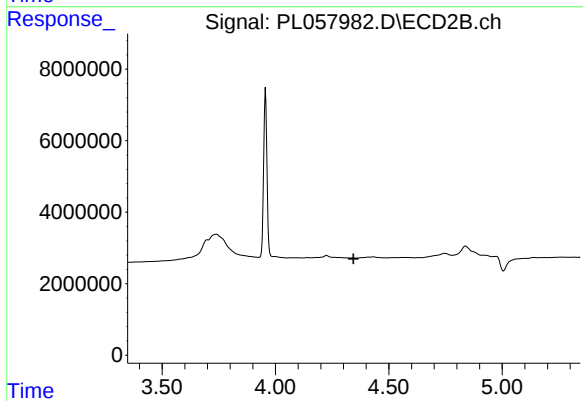

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

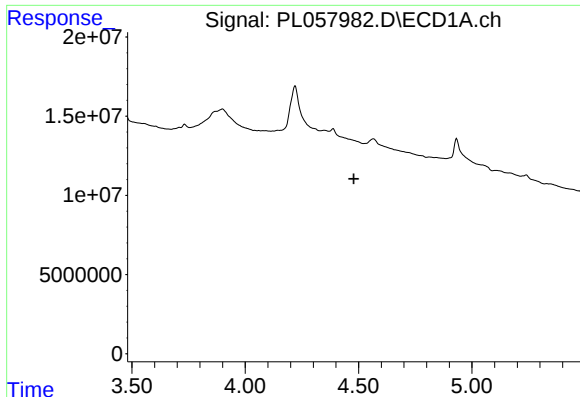

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

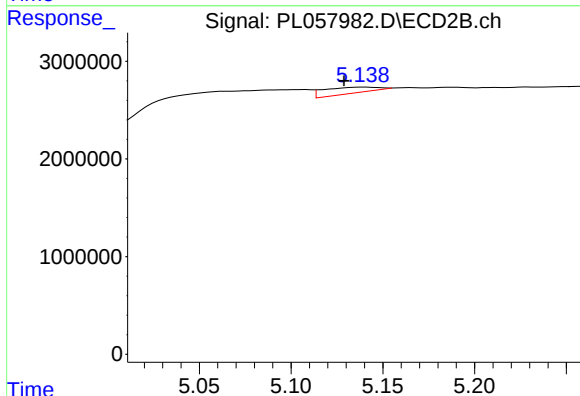


#4 Heptachlor

R.T.: 5.139 min
Delta R.T.: 0.011 min
Response: 1235405
Conc: 0.37 ng/ml

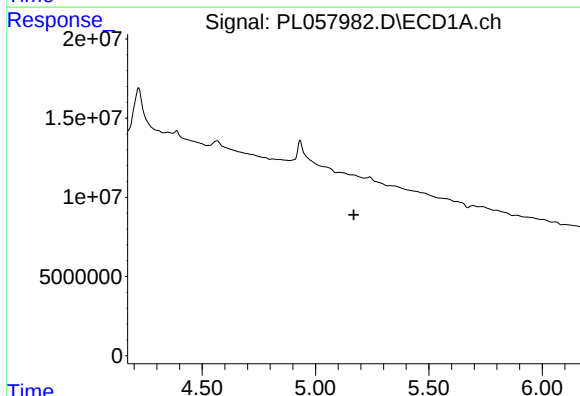


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.169 min
Response: 0
Conc: N.D.

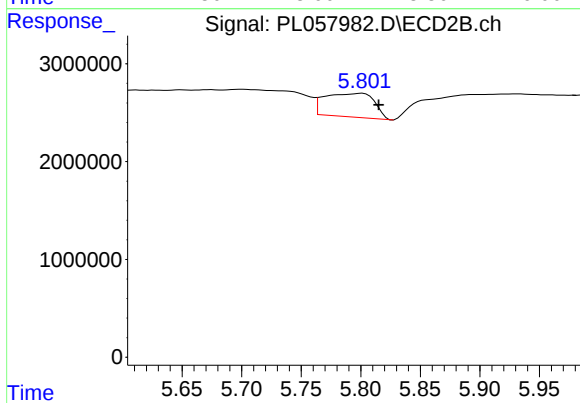

#8 Heptachlor epoxide


R.T.: 5.801 min
Delta R.T.: -0.014 min
Response: 7030072
Conc: 2.60 ng/ml

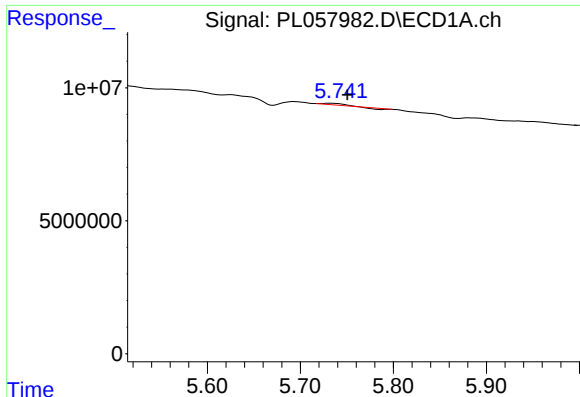

#13 Dieldrin


R.T.: 5.734 min
Delta R.T.: -0.017 min
Response: 229120
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

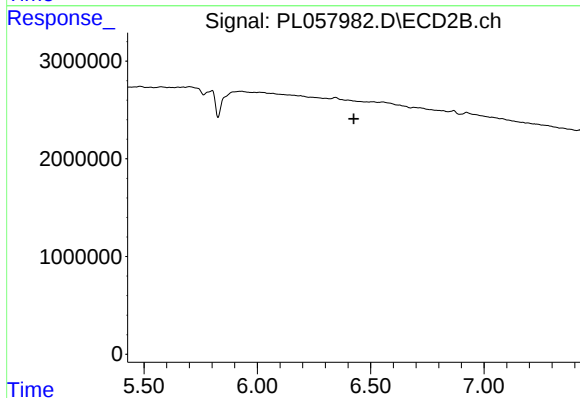


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

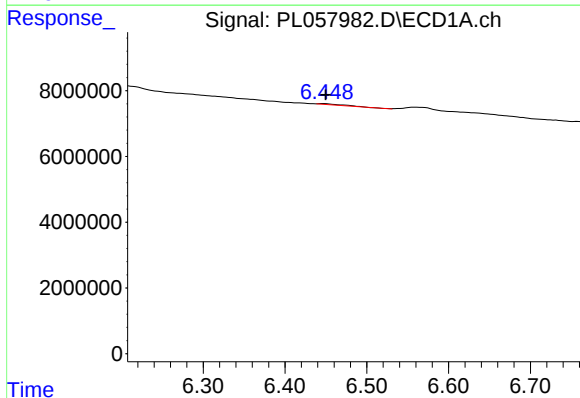


#18 Endrin aldehyde

R.T.: 6.447 min
Delta R.T.: -0.003 min
Response: 707988
Conc: 0.08 ng/ml

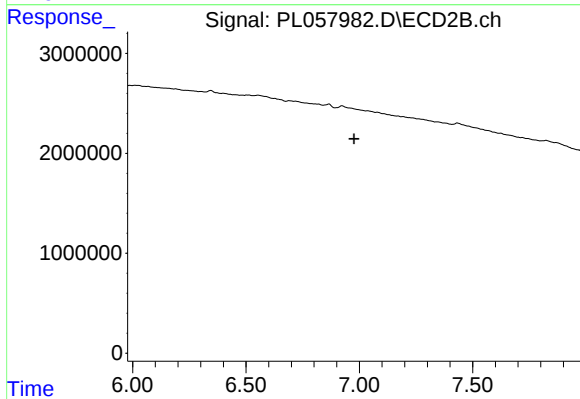

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

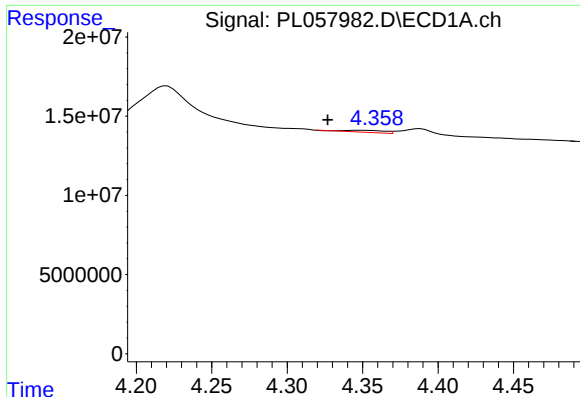

#23 Chlordane-1


R.T.: 4.349 min
Delta R.T.: 0.022 min
Response: 2429103
Conc: 6.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

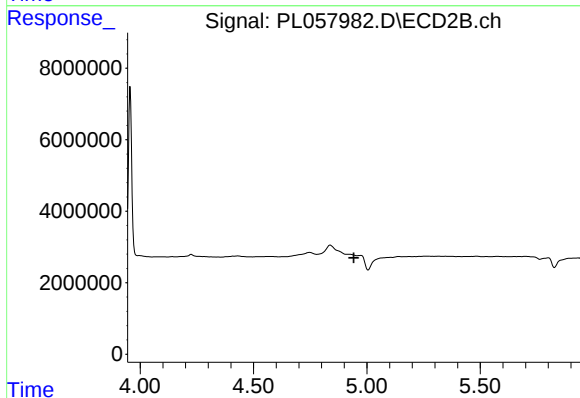


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

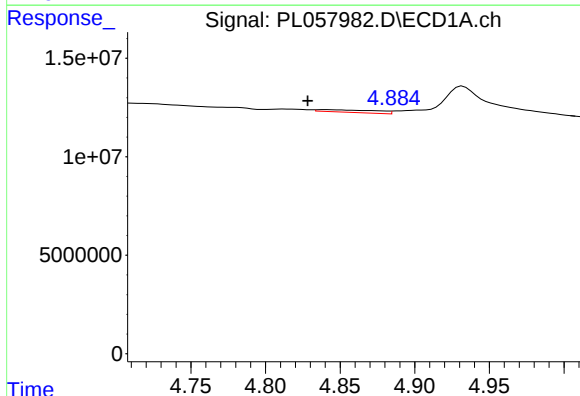


#24 Chlordane-2

R.T.: 4.842 min
Delta R.T.: 0.013 min
Response: 3426627
Conc: 8.49 ng/ml

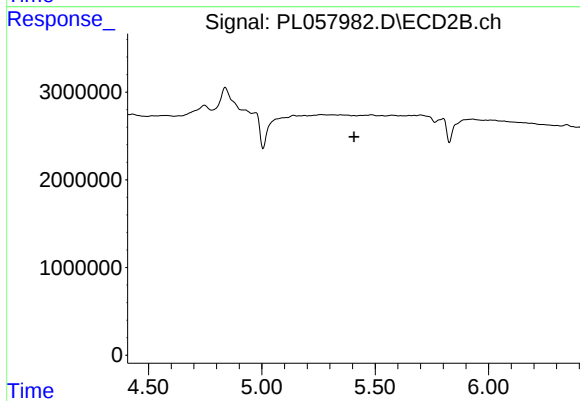

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

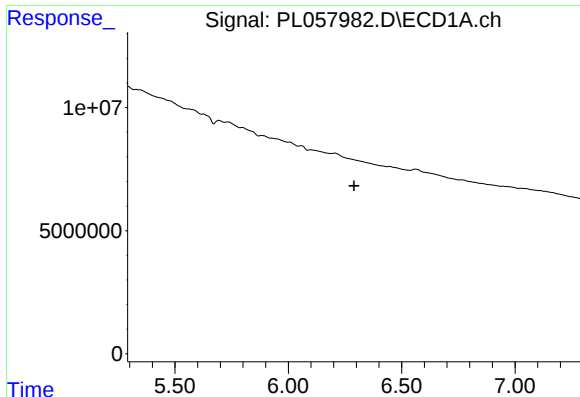

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 6.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

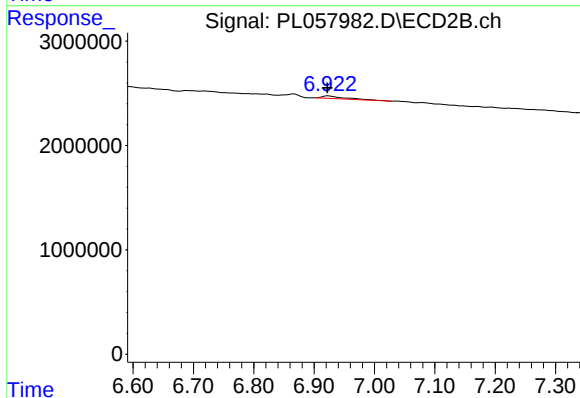


#27 Chlorodane-5

R.T.: 6.923 min
Delta R.T.: 0.000 min
Response: 705854
Conc: 8.28 ng/ml

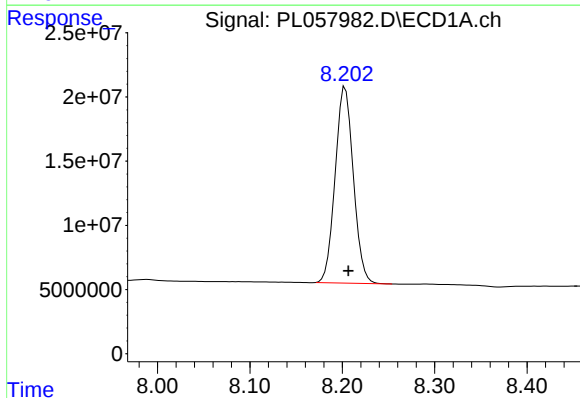

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.003 min
Response: 209153876
Conc: 20.29 ng/ml

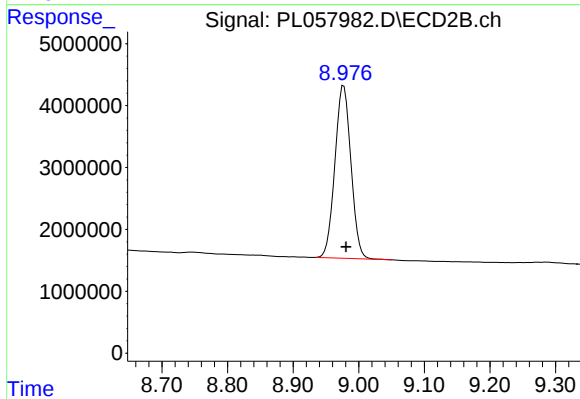

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.004 min
Response: 47351963
Conc: 21.20 ng/ml