

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041420\
 Data File : PL057995.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2020 23:46
 Operator : AJ\MA
 Sample : L2245-40
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 01:21:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.956	209.0E6	45090431	20.734	20.778
28)	SA Decachlor...	8.203	8.977	175.1E6	40543735	16.986	18.150
Target Compounds							
4)	MA Heptachlor	0.000	5.136	0	1586511	N.D.	0.473 #
8)	B Heptachlo...	5.158	5.797f	3406285	6452340	0.253	2.389 #
9)	A Endosulfan I	0.000	6.179	0	466561	N.D.	0.156 #
10)	B gamma-Chl...	5.390	0.000	2003625	0	0.148	N.D. #
12)	B 4,4'-DDE	0.000	6.260f	0	946984	N.D.	0.320 #
15)	B Endosulfa...	0.000	6.870f	0	734727	N.D.	0.283 #
21)	B Endrin ke...	0.000	7.661	0	300056	N.D.	0.121 #
25)	Chlordane-3	5.390	0.000	2003625	0	1.639	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041420\
Data File : PL057995.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2020 23:46
Operator : AJ\MA
Sample : L2245-40
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 01:21:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

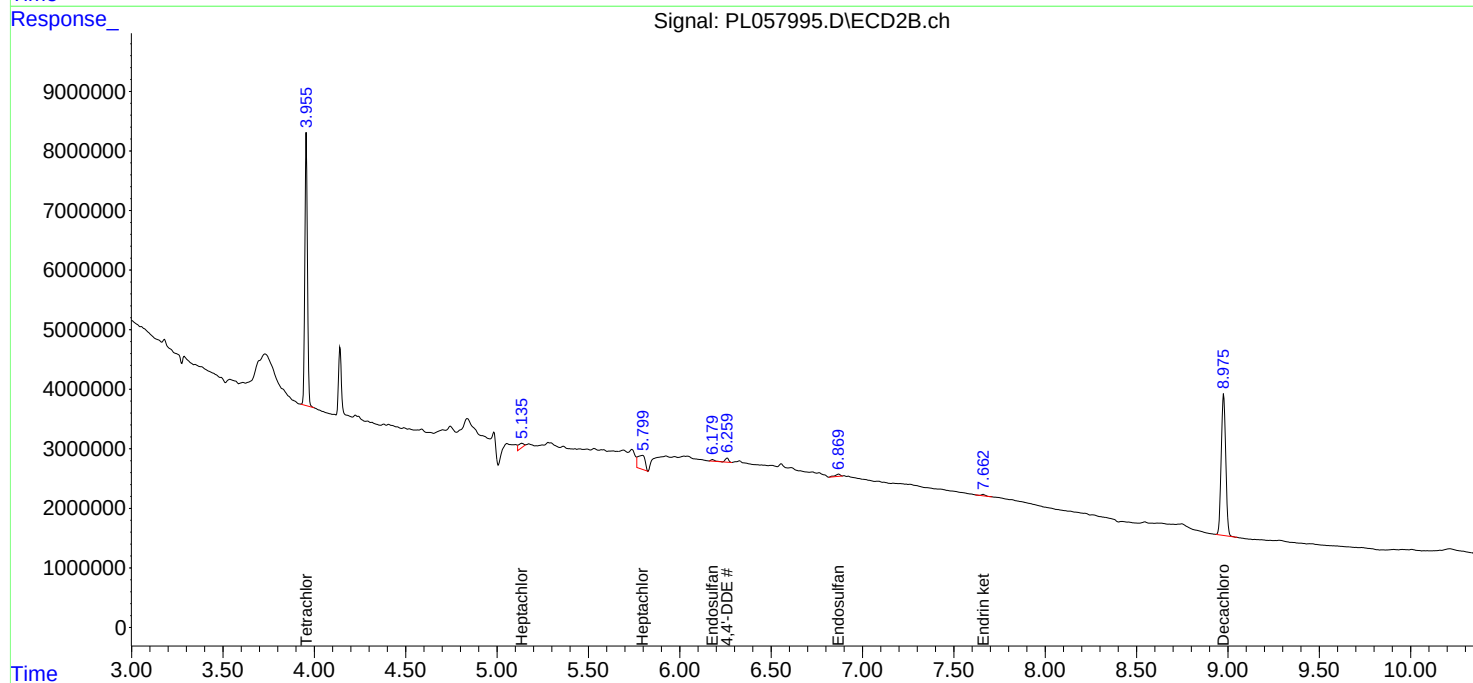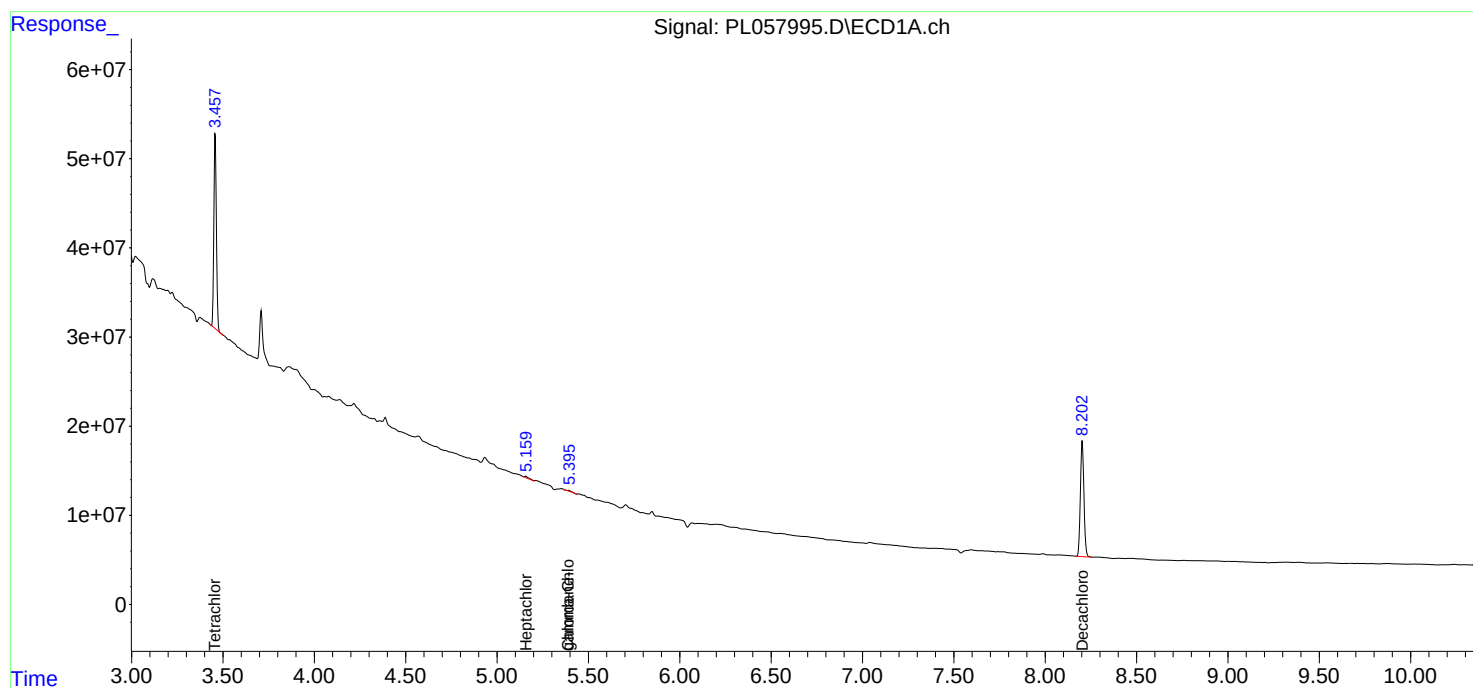


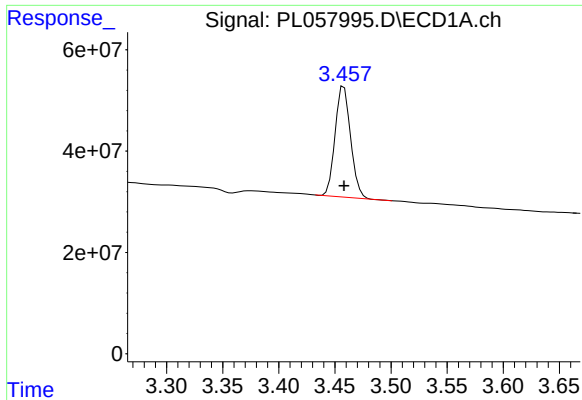

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 209017144
Conc: 20.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

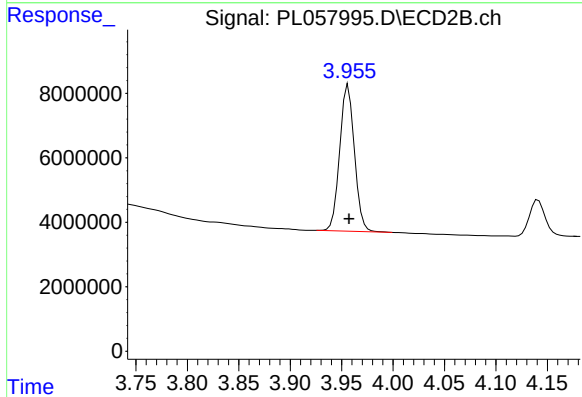


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: 0.000 min
Response: 45090431
Conc: 20.78 ng/ml

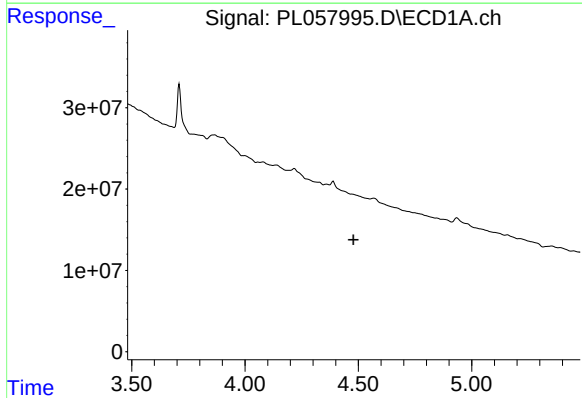


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

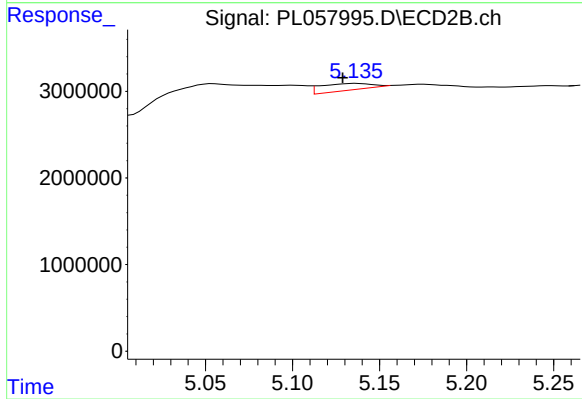

#4 Heptachlor


R.T.: 5.136 min
Delta R.T.: 0.008 min
Response: 1586511
Conc: 0.47 ng/ml

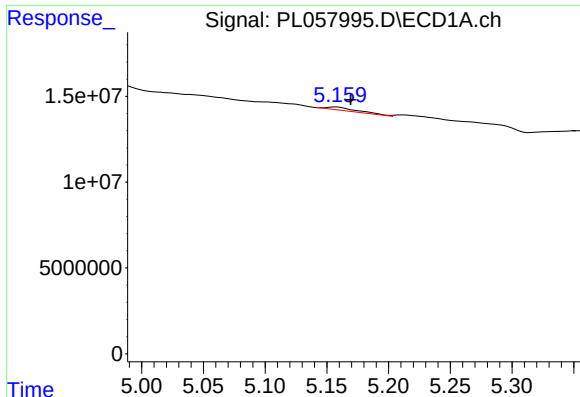

#8 Heptachlor epoxide


R.T.: 5.158 min
Delta R.T.: -0.012 min
Response: 3406285
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

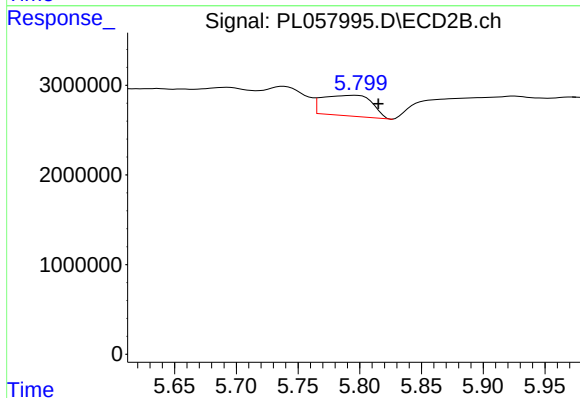


#8 Heptachlor epoxide

R.T.: 5.797 min
Delta R.T.: -0.018 min
Response: 6452340
Conc: 2.39 ng/ml

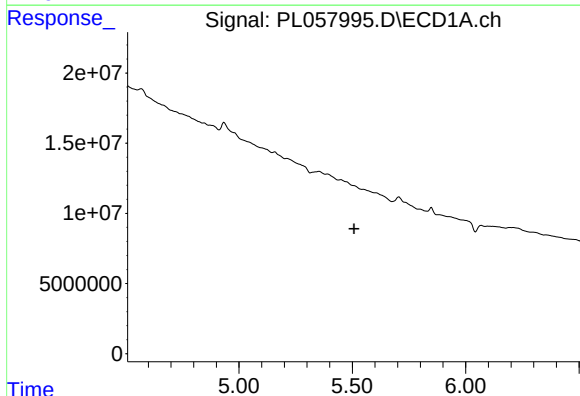


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.508 min
Response: 0
Conc: N.D.

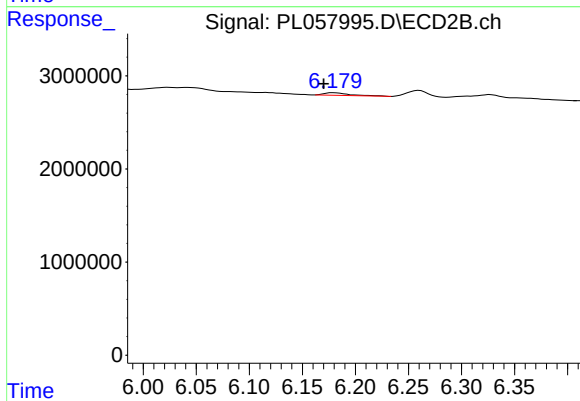

#9 Endosulfan I


R.T.: 6.179 min
Delta R.T.: 0.009 min
Response: 466561
Conc: 0.16 ng/ml

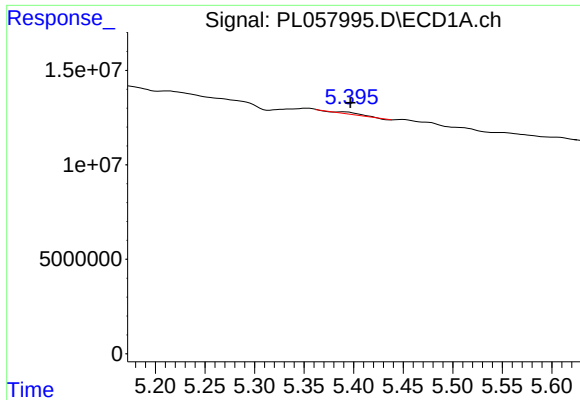

#10 gamma-Chlordane


R.T.: 5.390 min
Delta R.T.: -0.007 min
Response: 2003625
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

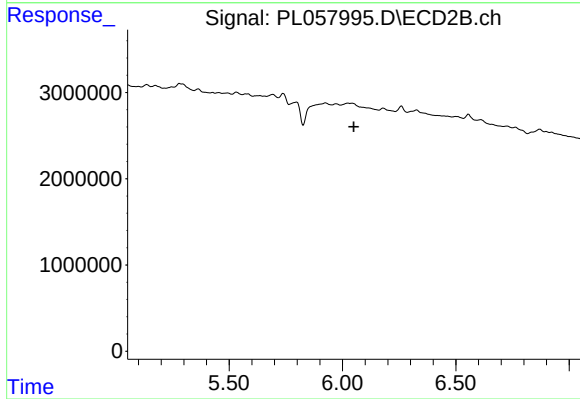


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

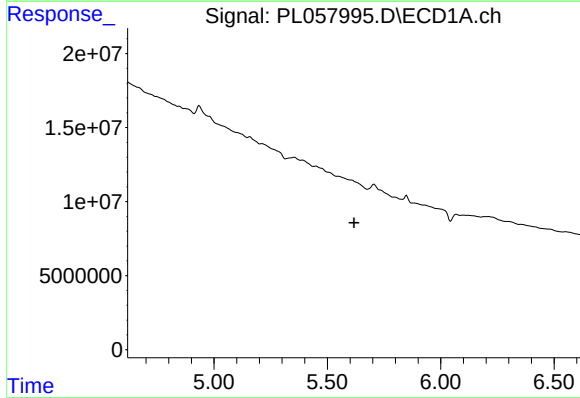


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.618 min
Response: 0
Conc: N.D.

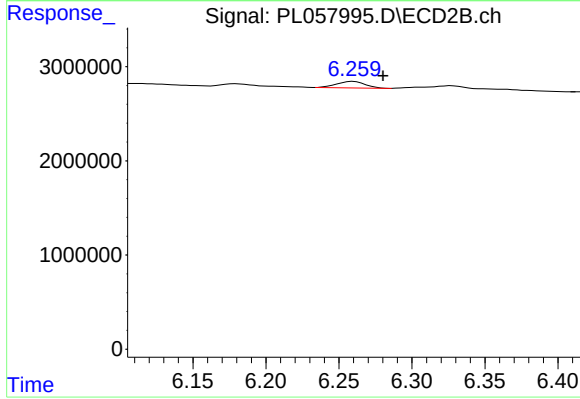

#12 4,4'-DDE


R.T.: 6.260 min
Delta R.T.: -0.020 min
Response: 946984
Conc: 0.32 ng/ml

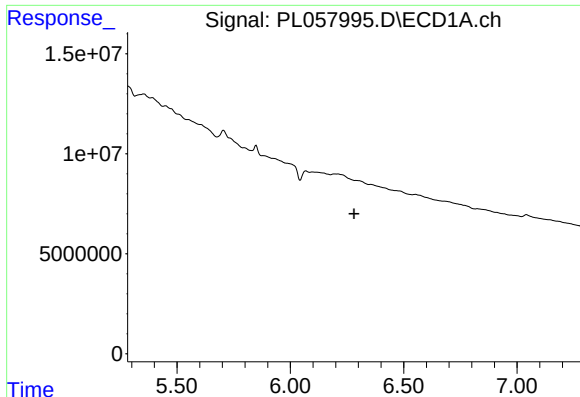

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

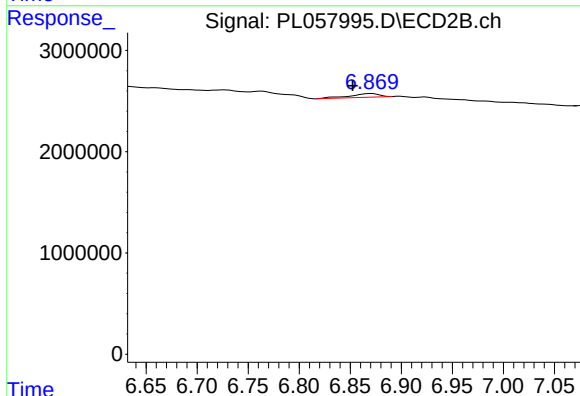


#15 Endosulfan II

R.T.: 6.870 min
Delta R.T.: 0.018 min
Response: 734727
Conc: 0.28 ng/ml

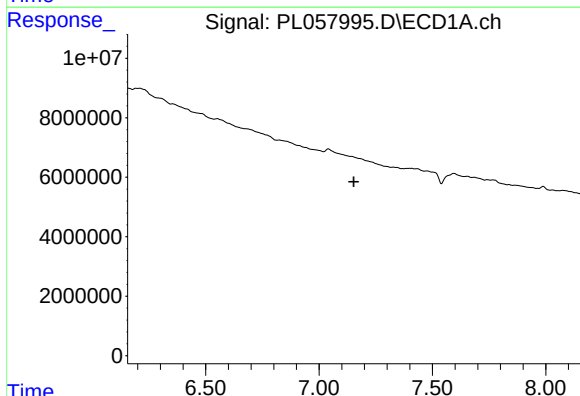


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

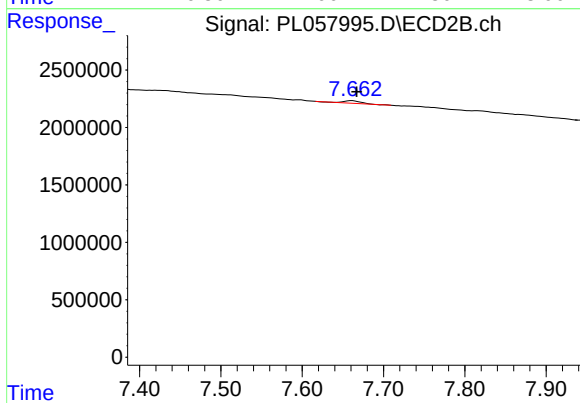

#21 Endrin ketone


R.T.: 7.661 min
Delta R.T.: -0.006 min
Response: 300056
Conc: 0.12 ng/ml

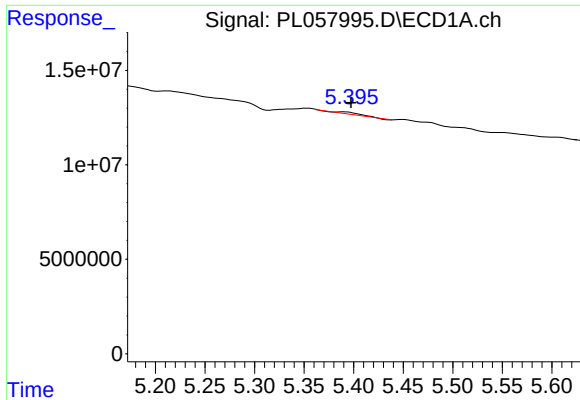

#25 Chlordane-3


R.T.: 5.390 min
Delta R.T.: -0.007 min
Response: 2003625
Conc: 1.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

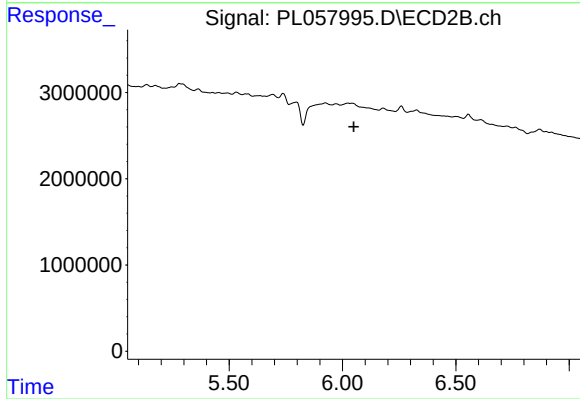


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

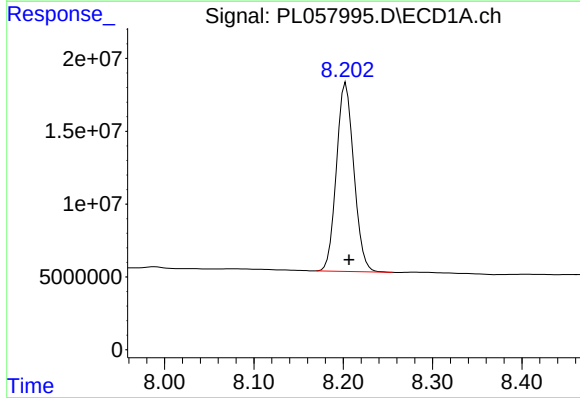

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 175102158
Conc: 16.99 ng/ml

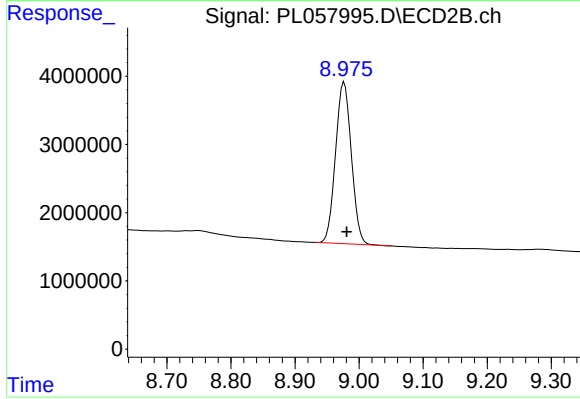

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.004 min
Response: 40543735
Conc: 18.15 ng/ml