

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041420\
 Data File : PL058001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2020 01:12
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 01:52:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.957	229.3E6	48449383	22.743	22.325
28)	SA Decachlor...	8.203	8.977	209.6E6	47310529	20.331	21.180
Target Compounds							
2)	A alpha-BHC	3.898	0.000	6629027	0	0.382	N.D. #
4)	MA Heptachlor	0.000	5.139	0	1518283	N.D.	0.452 #
8)	B Heptachlo...	0.000	5.806	0	6348565	N.D.	2.351 #
12)	B 4,4'-DDE	5.633f	0.000	7788185	0	0.595	N.D. #
14)	MA Endrin	6.009	0.000	3362152	0	0.288	N.D. #
16)	A 4,4'-DDD	6.138	0.000	4573119	0	0.458	N.D. #
23)	Chlordane-1	4.351f	0.000	4724166	0	12.773	N.D. #
24)	Chlordane-2	4.814	0.000	10388242	0	25.732	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041420\
Data File : PL058001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2020 01:12
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 01:52:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

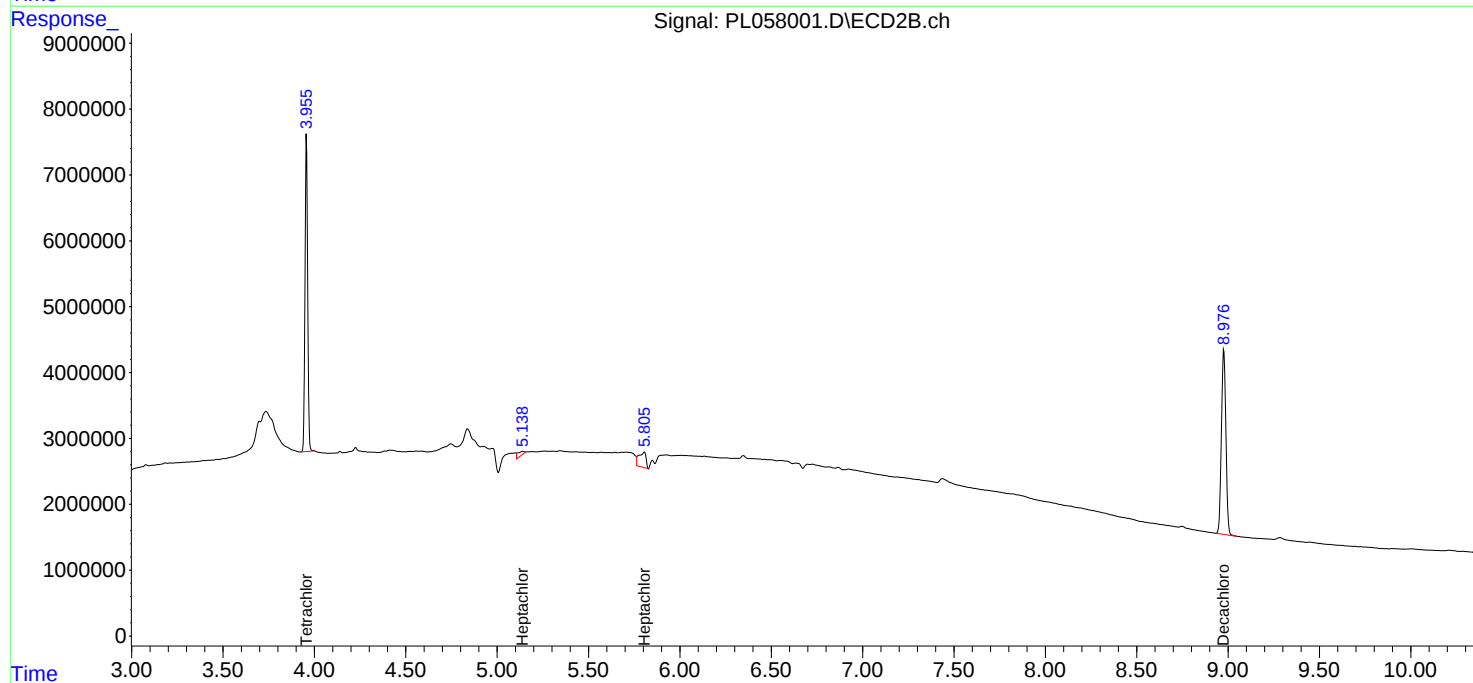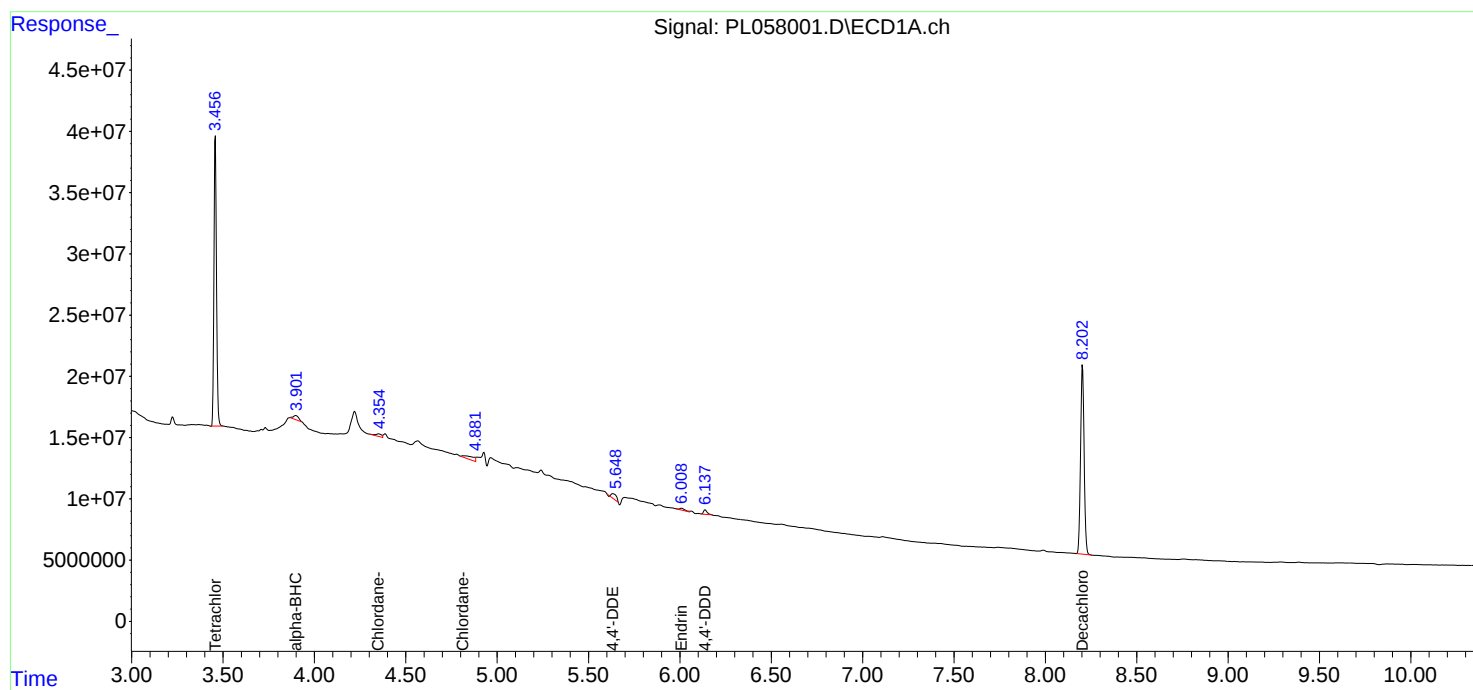


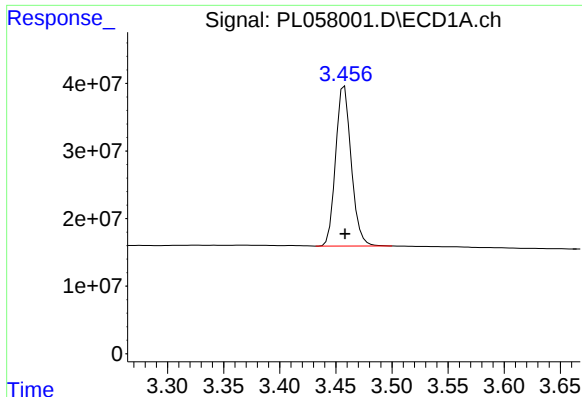

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 229268697
Conc: 22.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

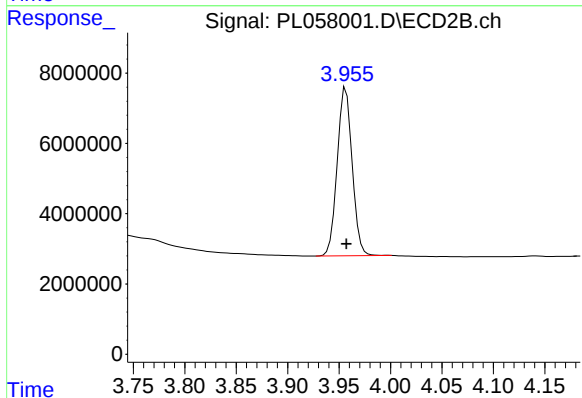


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 48449383
Conc: 22.33 ng/ml

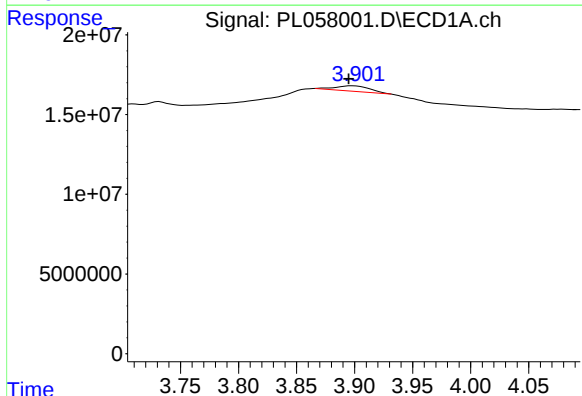


#2 alpha-BHC

R.T.: 3.898 min
Delta R.T.: 0.003 min
Response: 6629027
Conc: 0.38 ng/ml

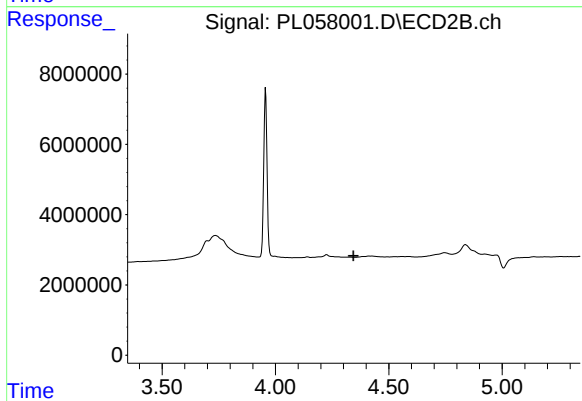

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

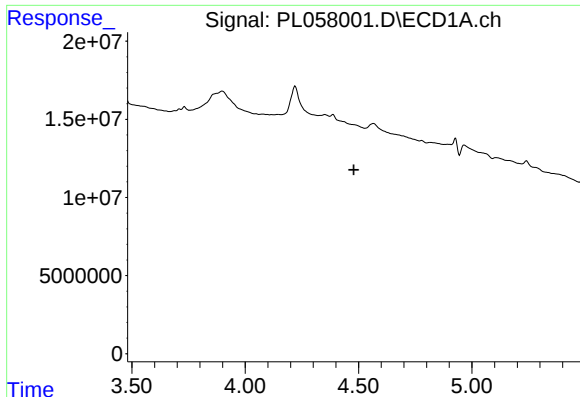

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

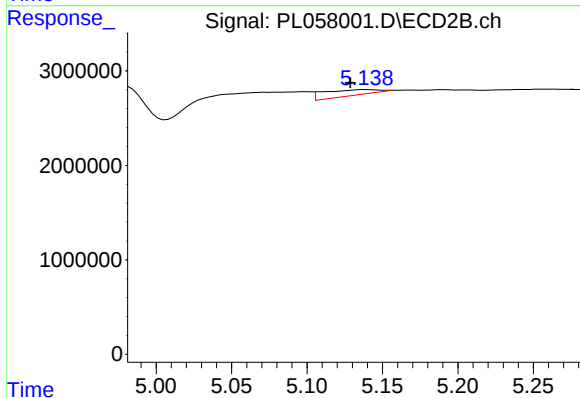


#4 Heptachlor

R.T.: 5.139 min
Delta R.T.: 0.010 min
Response: 1518283
Conc: 0.45 ng/ml

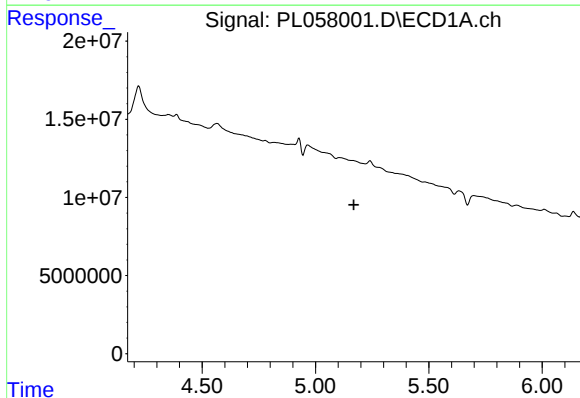


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

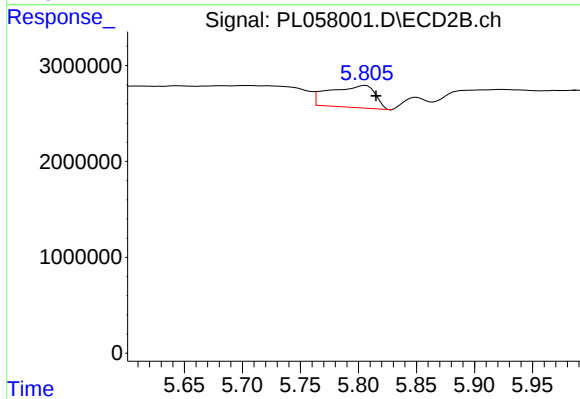

#8 Heptachlor epoxide


R.T.: 5.806 min
Delta R.T.: -0.009 min
Response: 6348565
Conc: 2.35 ng/ml

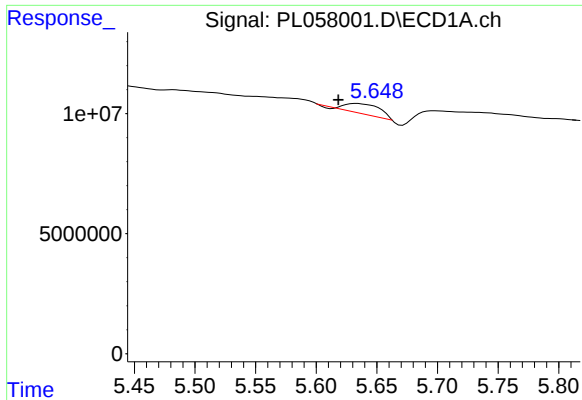

#12 4,4'-DDE


R.T.: 5.633 min
Delta R.T.: 0.015 min
Response: 7788185
Conc: 0.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

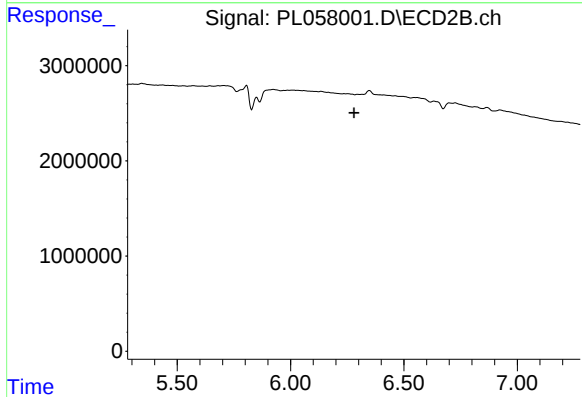


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.280 min
Response: 0
Conc: N.D.

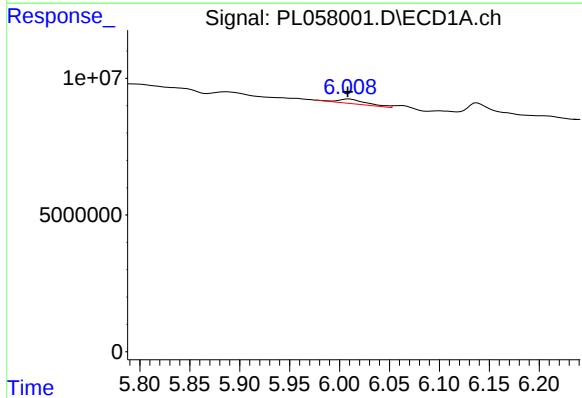


#14 Endrin

R.T.: 6.009 min
Delta R.T.: 0.000 min
Response: 3362152
Conc: 0.29 ng/ml

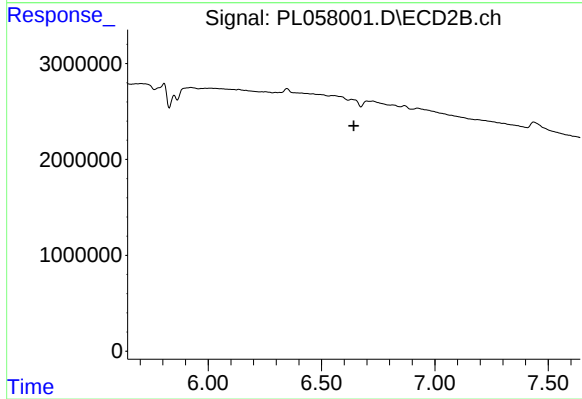

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

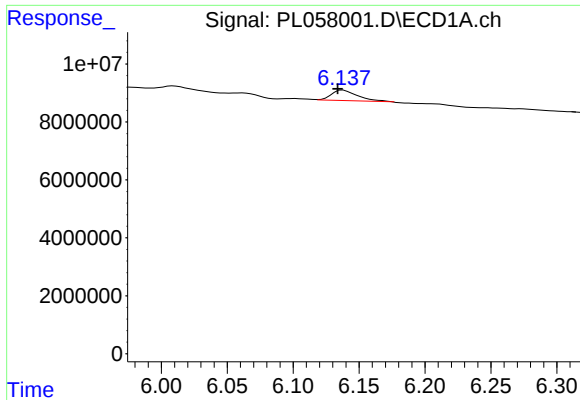

#16 4,4'-DDD


R.T.: 6.138 min
Delta R.T.: 0.004 min
Response: 4573119
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

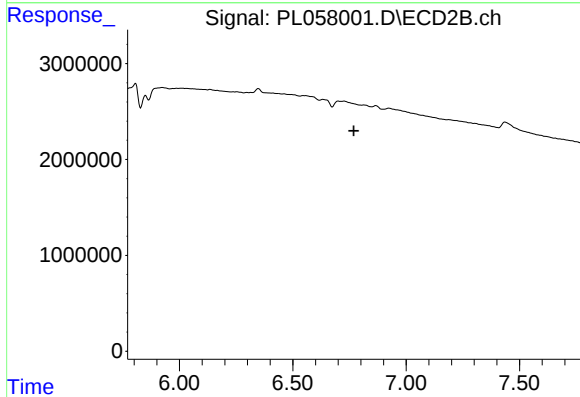


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.769 min
Response: 0
Conc: N.D.

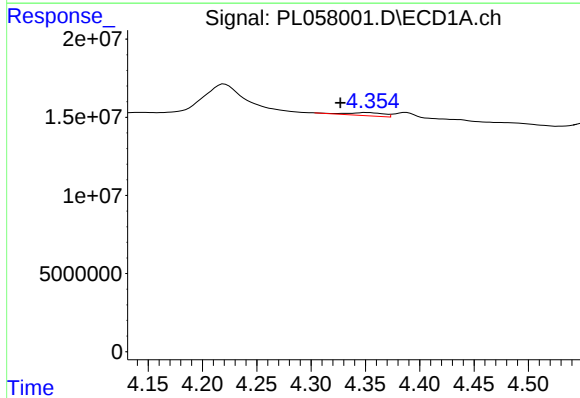


#23 Chlordane-1

R.T.: 4.351 min
Delta R.T.: 0.024 min
Response: 4724166
Conc: 12.77 ng/ml

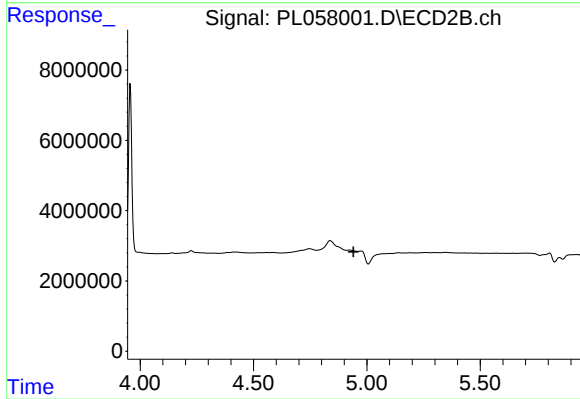

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

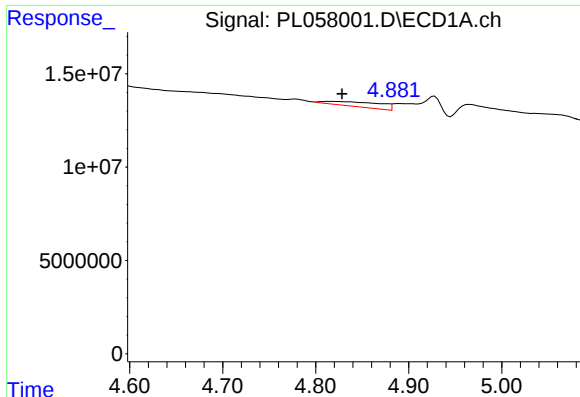

#24 Chlordane-2


R.T.: 4.814 min
Delta R.T.: -0.015 min
Response: 10388242
Conc: 25.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

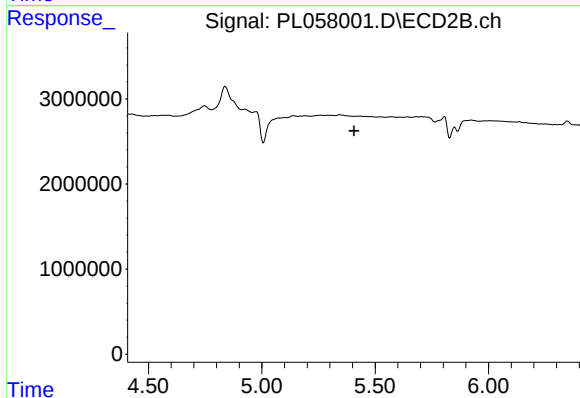


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

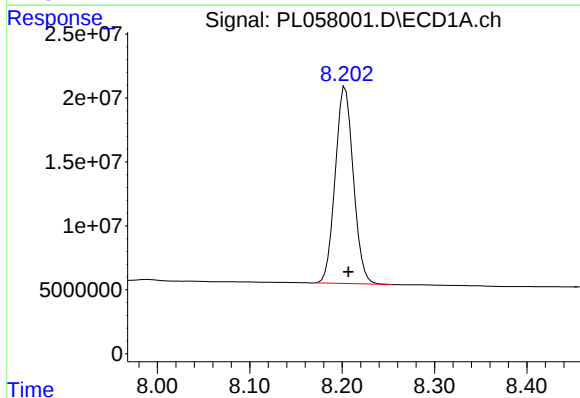

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.003 min
Response: 209584919
Conc: 20.33 ng/ml

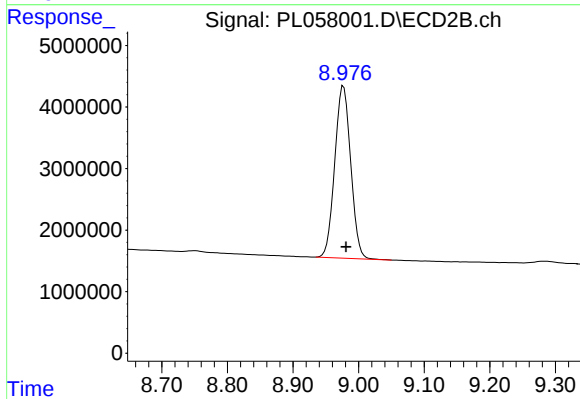

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.004 min
Response: 47310529
Conc: 21.18 ng/ml