

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041420\
 Data File : PL057999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2020 00:43
 Operator : AJ\MA
 Sample : L2245-25
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-21A

Manual Integrations
 APPROVED

mohammad
 4/15/2020 3:32:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 01:23:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.955	190.9E6	41472842	18.933m	19.111m
28)	SA Decachlor...	8.204	8.978	170.2E6	38228667	16.509	17.114
Target Compounds							
10)	B gamma-Chl...	5.395	6.052	39429408	6966505	2.903m	2.150 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041420\
Data File : PL057999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2020 00:43
Operator : AJ\MA
Sample : L2245-25
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-21A


Manual Integrations
APPROVED

mohammad
4/15/2020 3:32:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 01:23:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

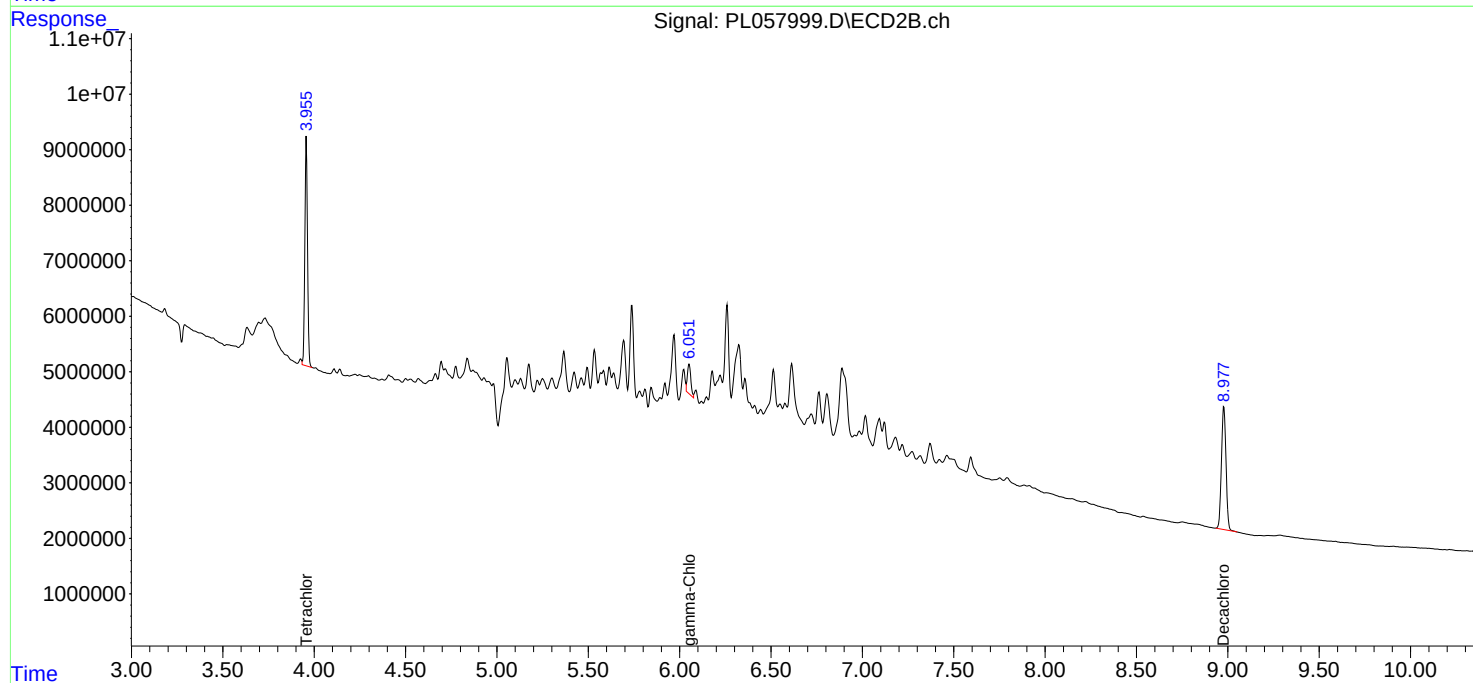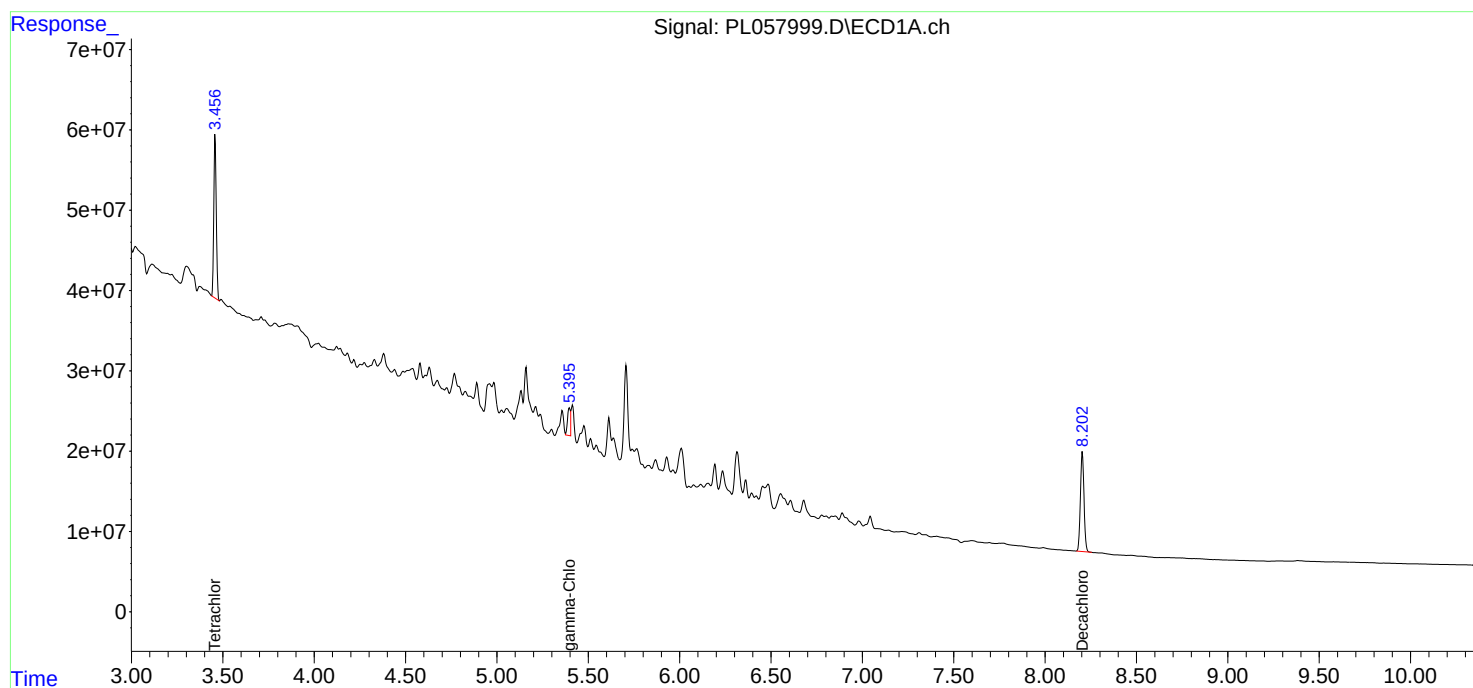

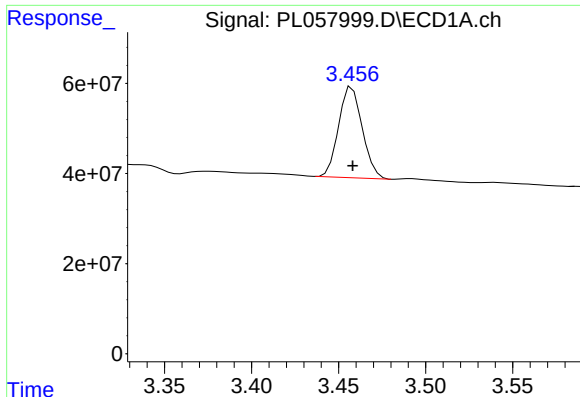


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 190867726
Conc: 18.93 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-21A


Manual Integrations
APPROVED

mohammad
4/15/2020 3:32:01 PM

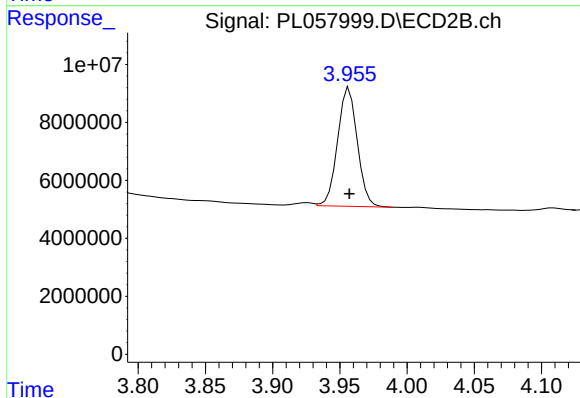


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 41472842
Conc: 19.11 ng/ml m

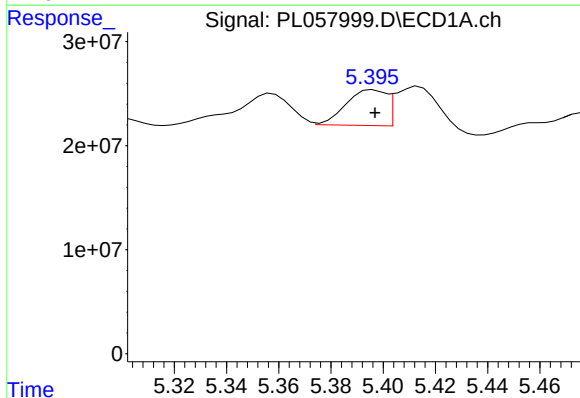


#10 gamma-Chlordane

R.T.: 5.395 min
Delta R.T.: -0.002 min
Response: 39429408
Conc: 2.90 ng/ml m

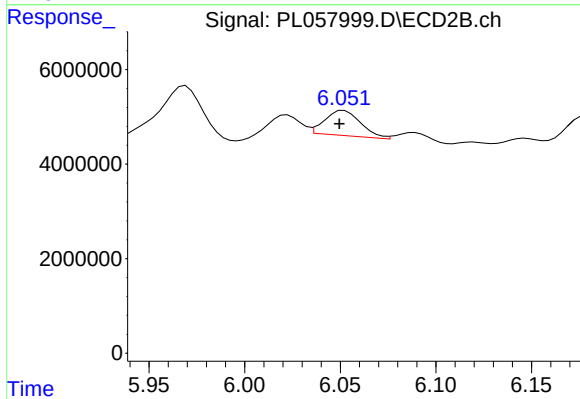

#10 gamma-Chlordane

R.T.: 6.052 min
Delta R.T.: 0.002 min
Response: 6966505
Conc: 2.15 ng/ml

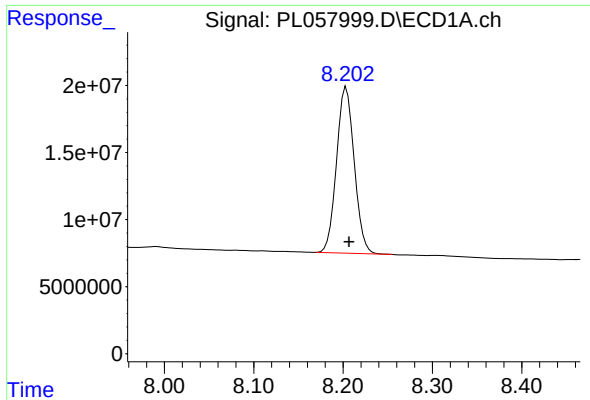


#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 170180803
Conc: 16.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-21A

Manual Integrations
APPROVED

mohammad
4/15/2020 3:32:01 PM

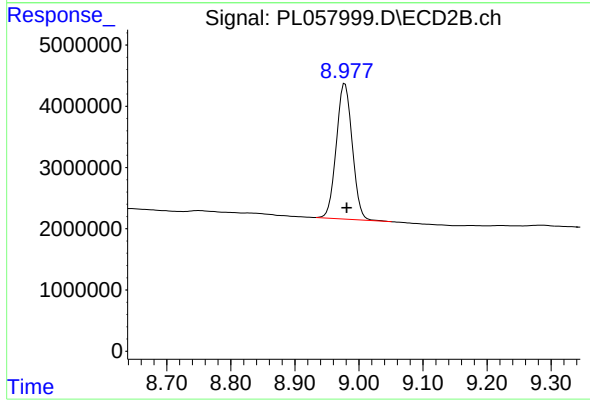

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.003 min
Response: 38228667
Conc: 17.11 ng/ml