

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
 Data File : PL066107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 11:13
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 11:54:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 11:50:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.153	218.9E6	295.7E6	74.167	73.660
28)	SA Decachlor...	8.170	9.351	168.8E6	234.8E6	72.047	73.110
Target Compounds							
23)	Chlordane-1	4.308	5.174	81853170	123.8E6	725.062	730.507
24)	Chlordane-2	4.805	5.651	93147630	123.8E6	716.483	719.832
25)	Chlordane-3	5.368	6.310	269.5E6	494.8E6	740.514	751.658
26)	Chlordane-4	5.426	6.383	231.5E6	581.2E6	744.241	748.071
27)	Chlordane-5	6.251	7.206	104.3E6	101.3E6	736.684	754.631



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
Data File : PL066107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 11:13
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 11:54:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 11:50:27 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

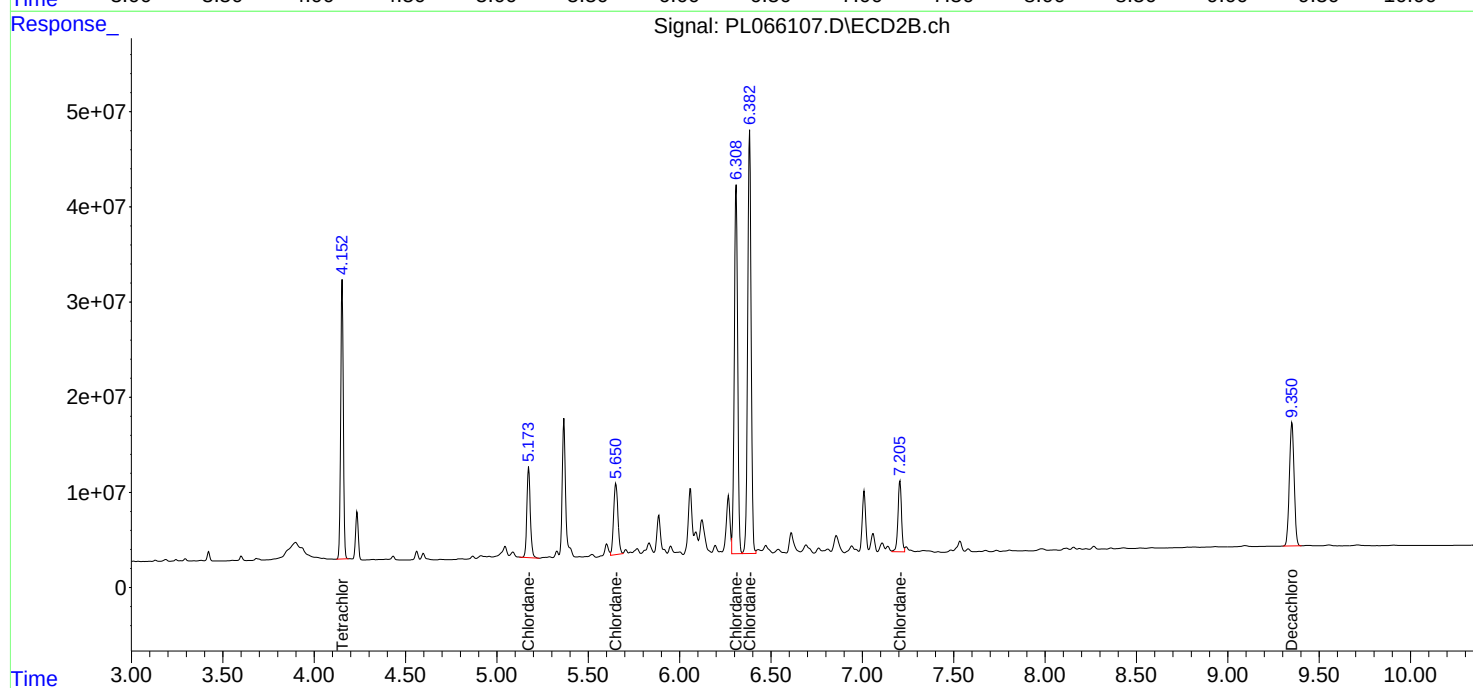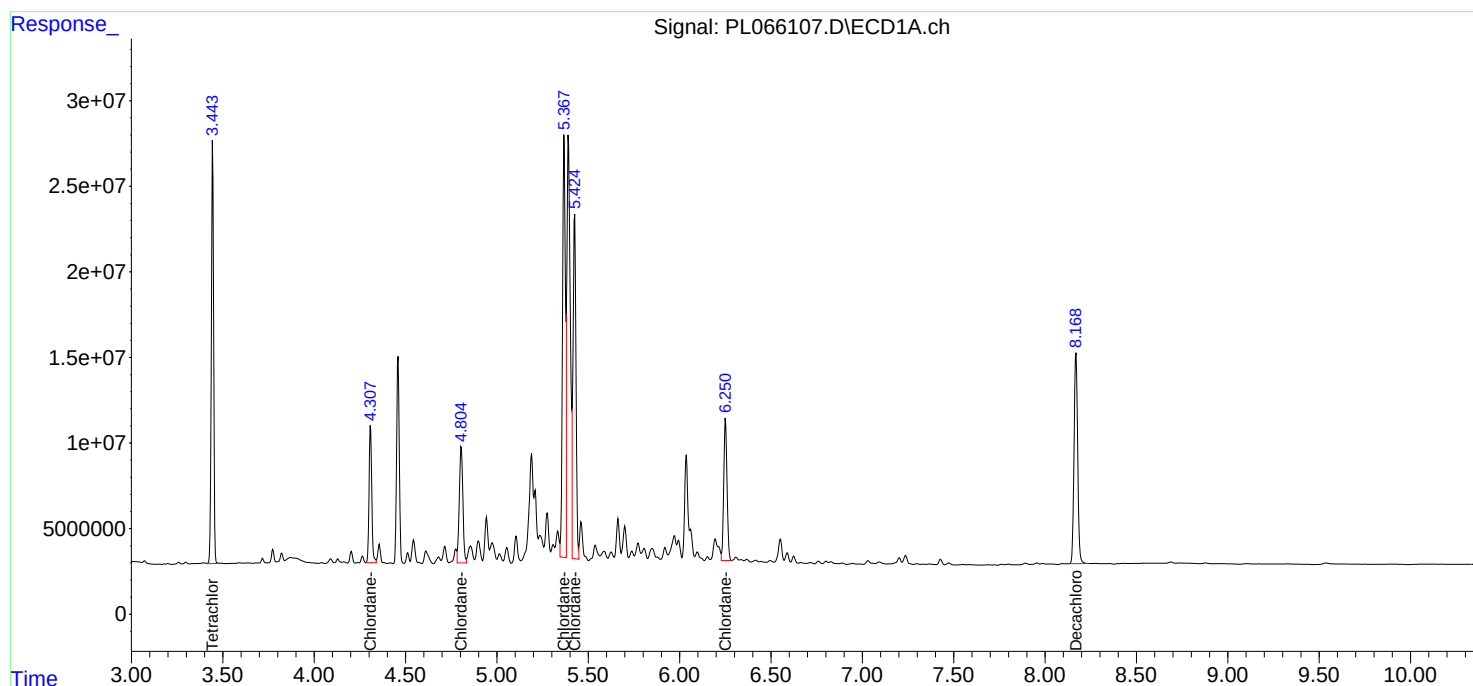


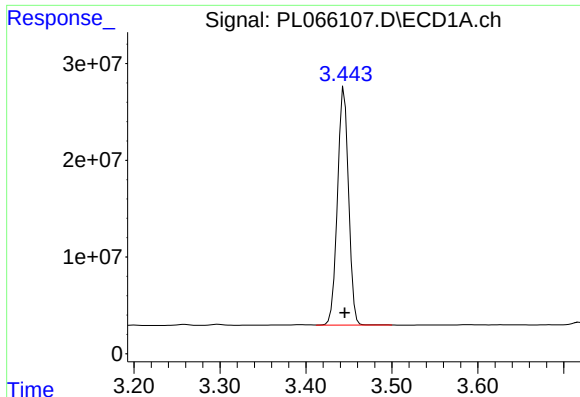

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 218915098
Conc: 74.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

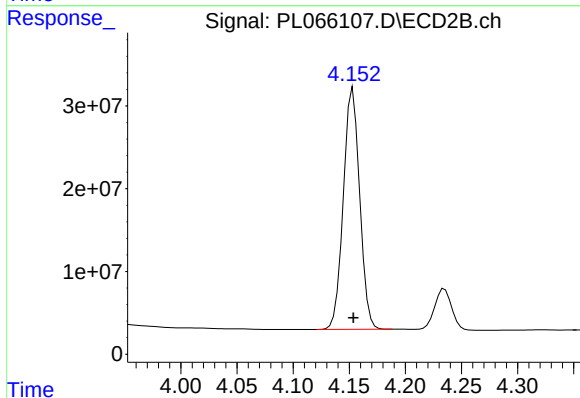


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 295728280
Conc: 73.66 ng/ml

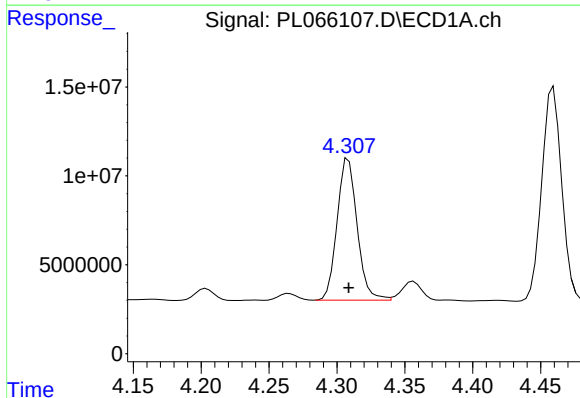


#23 Chlordane-1

R.T.: 4.308 min
Delta R.T.: 0.000 min
Response: 81853170
Conc: 725.06 ng/ml

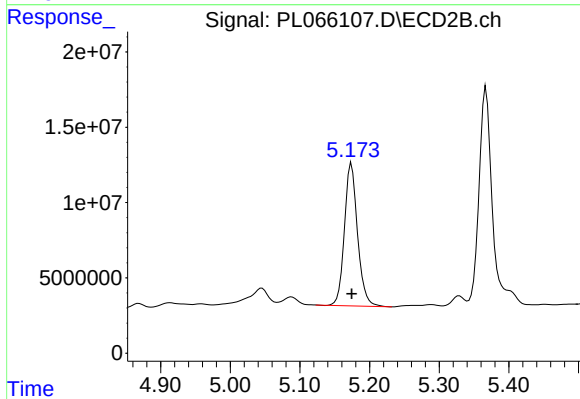

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 123829049
Conc: 730.51 ng/ml

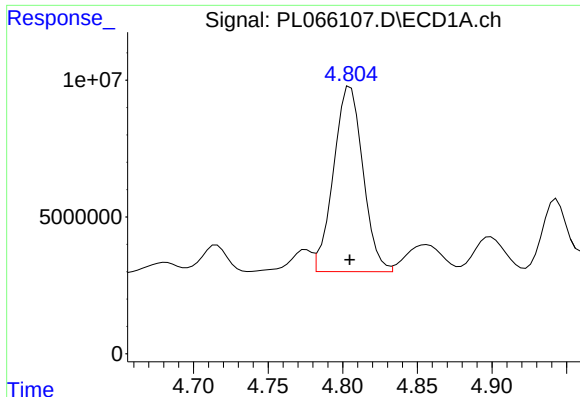

#24 Chlordane-2


R.T.: 4.805 min
Delta R.T.: 0.000 min
Response: 93147630
Conc: 716.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

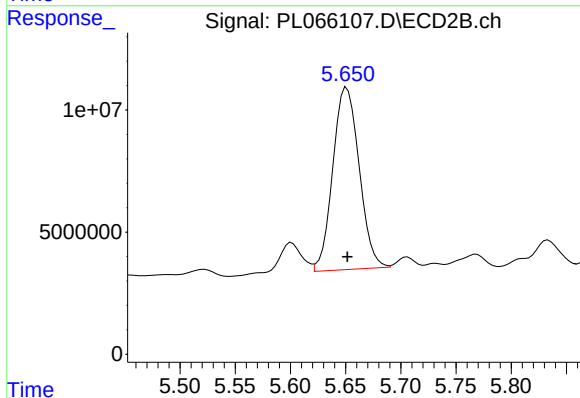


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 123768206
Conc: 719.83 ng/ml

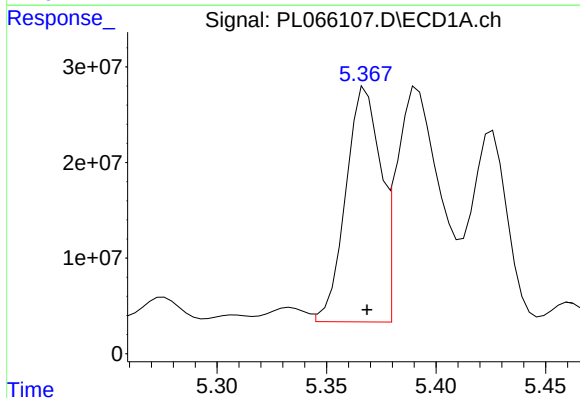


#25 Chlordane-3

R.T.: 5.368 min
Delta R.T.: 0.000 min
Response: 269520564
Conc: 740.51 ng/ml

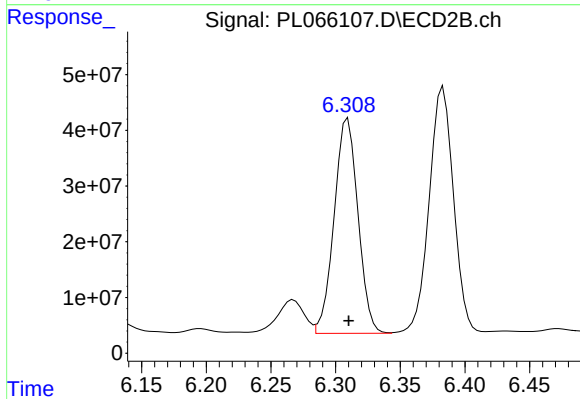

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 494751550
Conc: 751.66 ng/ml

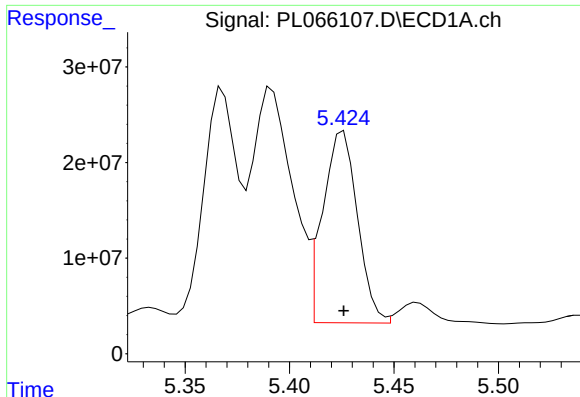

#26 Chlordane-4


R.T.: 5.426 min
Delta R.T.: 0.000 min
Response: 231524212
Conc: 744.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

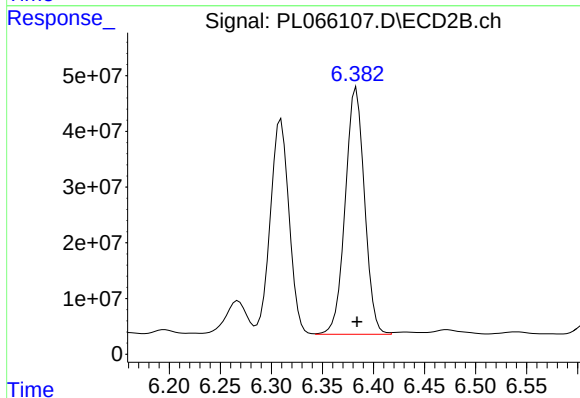


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 581184106
Conc: 748.07 ng/ml

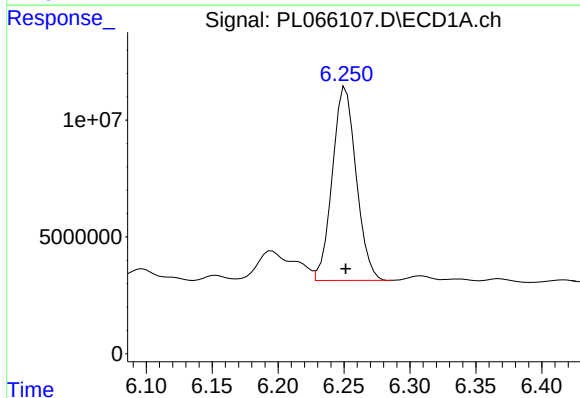


#27 Chlordane-5

R.T.: 6.251 min
Delta R.T.: 0.000 min
Response: 104316651
Conc: 736.68 ng/ml

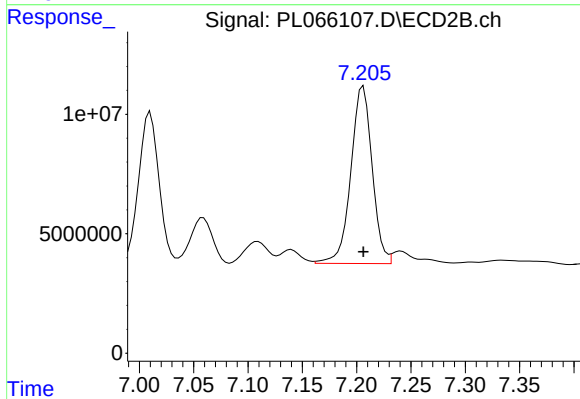

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 101334444
Conc: 754.63 ng/ml

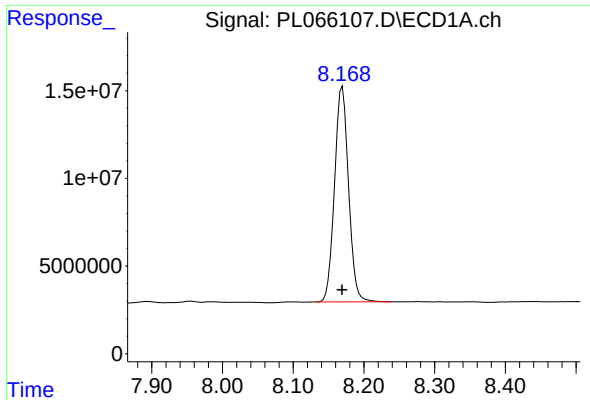

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: 0.000 min
Response: 168845144
Conc: 72.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

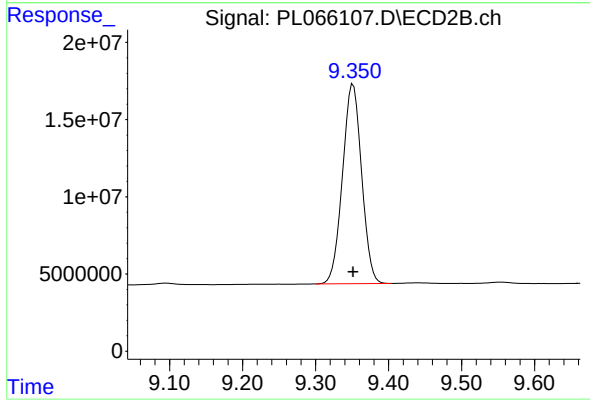

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 234773099
Conc: 73.11 ng/ml