

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
 Data File : PL066151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 23:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 01:21:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.154	50743875	80732493	19.936	20.070
28)	SA Decachlor...	8.170	9.355	40281234	60342579	16.887	18.477
Target Compounds							
2)	A alpha-BHC	3.871	0.000	1336897	0	0.325	N.D. #
4)	MA Heptachlor	0.000	5.352	0	1731780	N.D.	0.311 #
8)	B Heptachlo...	0.000	6.069	0	2507732	N.D.	0.543 #
10)	B gamma-Chl...	0.000	6.314	0	15706021	N.D.	3.441 #
12)	B 4,4'-DDE	0.000	6.549	0	2468696	N.D.	0.596 #
14)	MA Endrin	5.976	0.000	2593884	0	0.744	N.D. #
17)	MA 4,4'-DDT	0.000	7.343	0	4058895	N.D.	1.196 #
21)	B Endrin ke...	0.000	7.972	0	1328021	N.D.	0.361 #
23)	Chlordane-1	4.333f	0.000	2514751	0	21.997	N.D. #
25)	Chlordane-3	0.000	6.314	0	15706021	N.D.	23.886 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
Data File : PL066151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 23:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 01:21:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

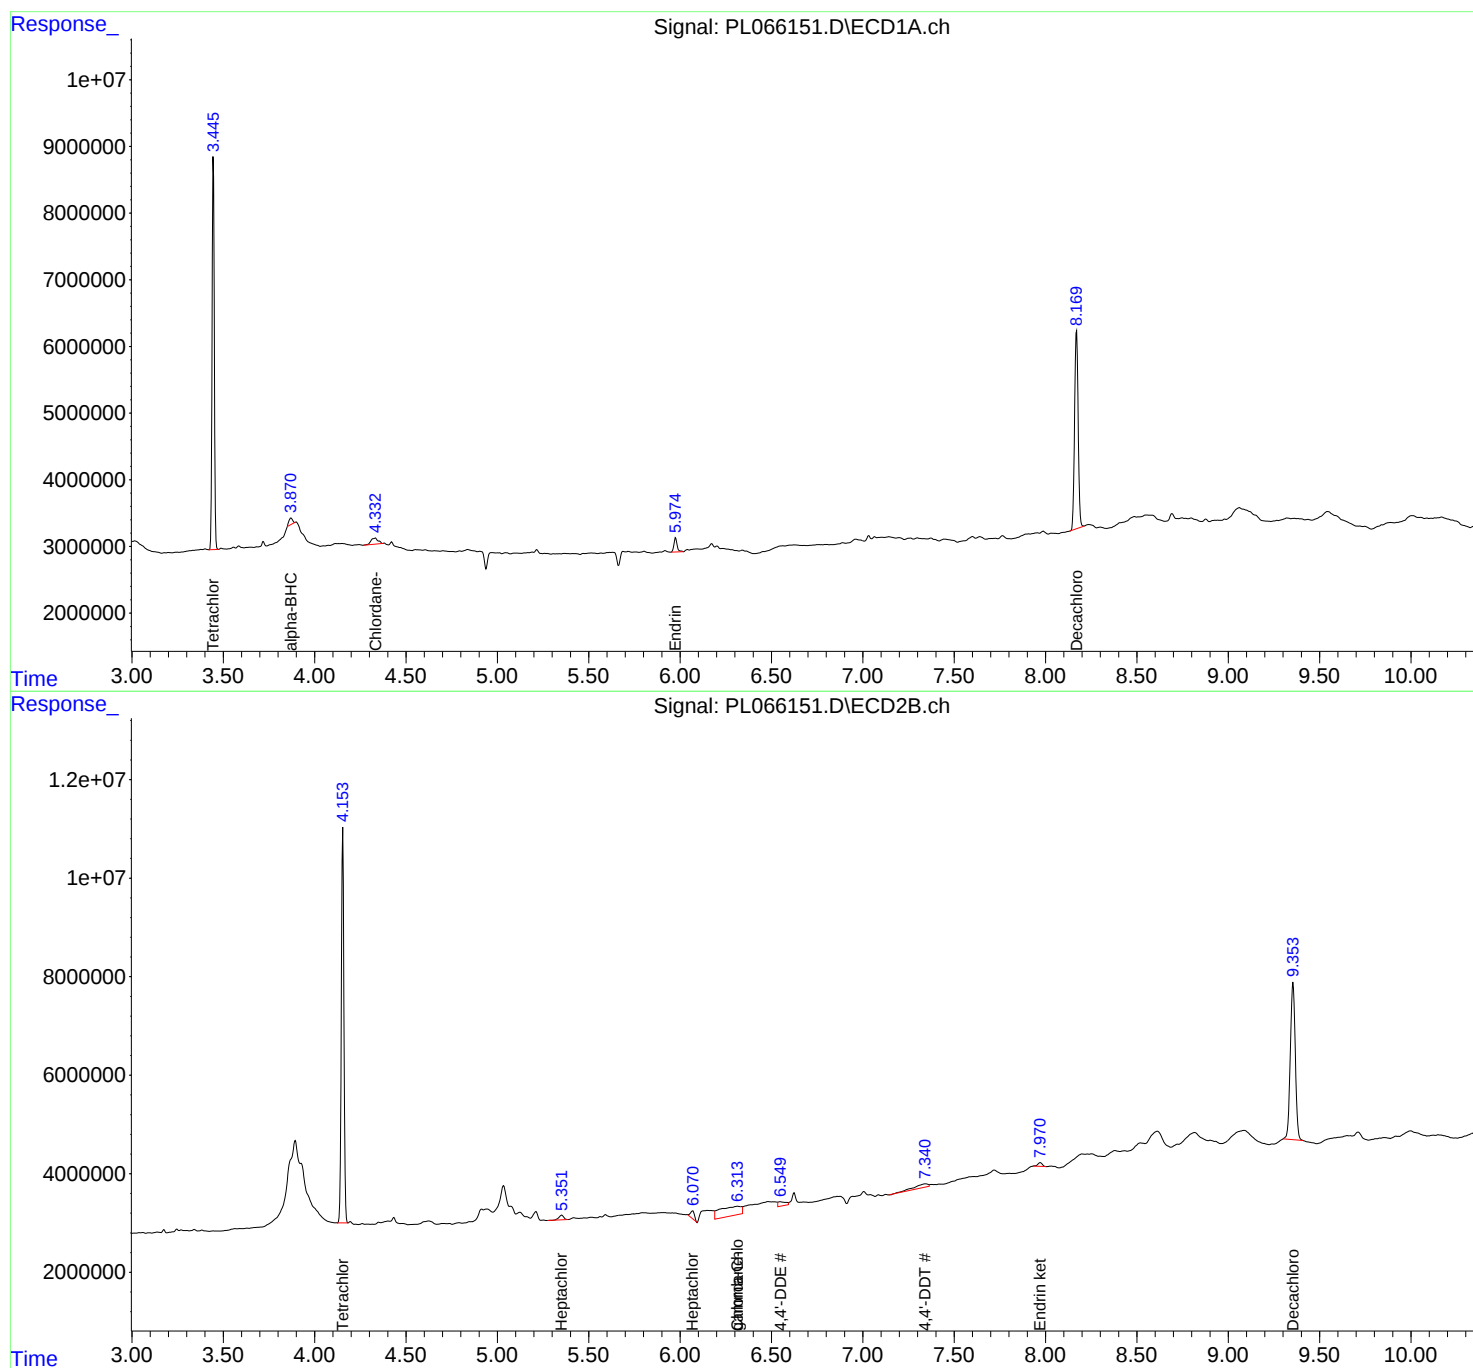


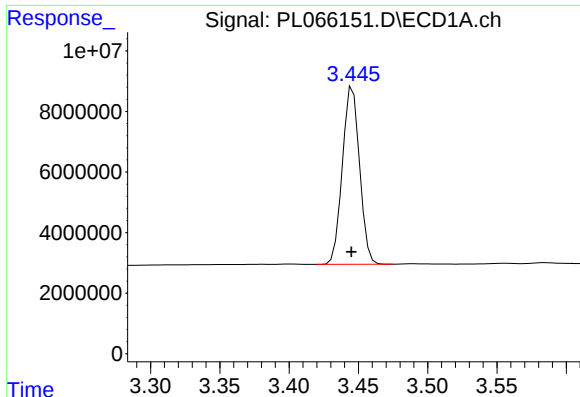

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: 0.000 min
Response: 50743875
Conc: 19.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

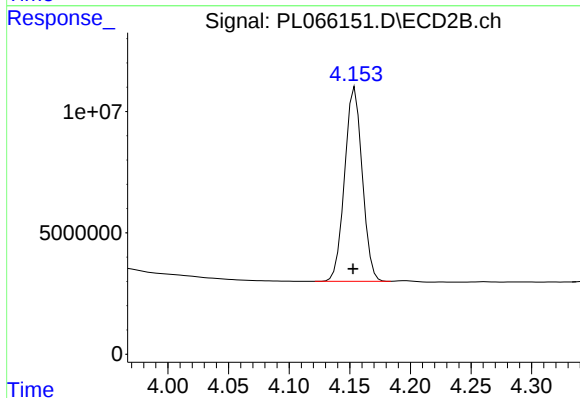


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 80732493
Conc: 20.07 ng/ml

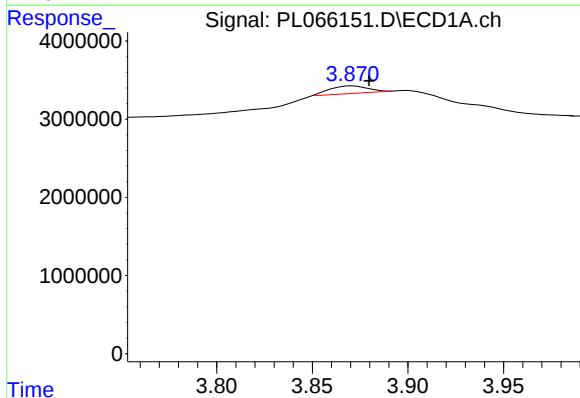


#2 alpha-BHC

R.T.: 3.871 min
Delta R.T.: -0.009 min
Response: 1336897
Conc: 0.32 ng/ml

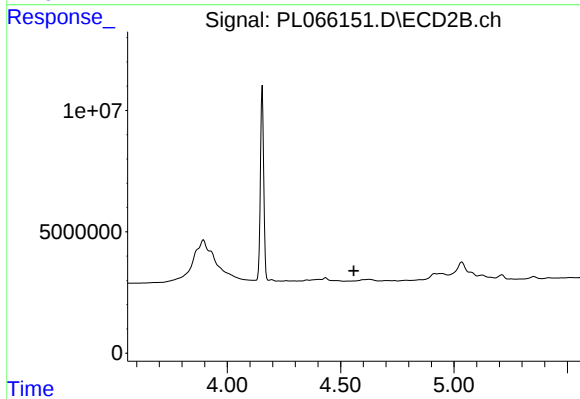

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.558 min
Response: 0
Conc: N.D.

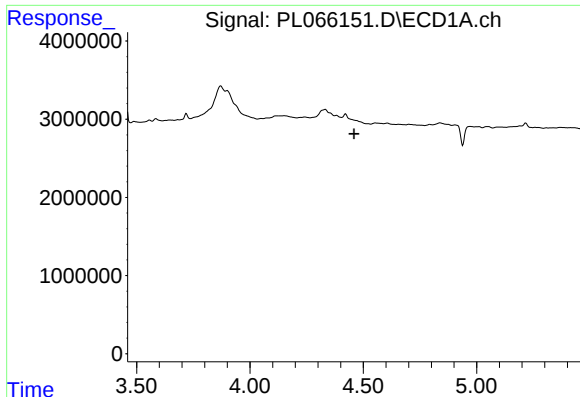

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

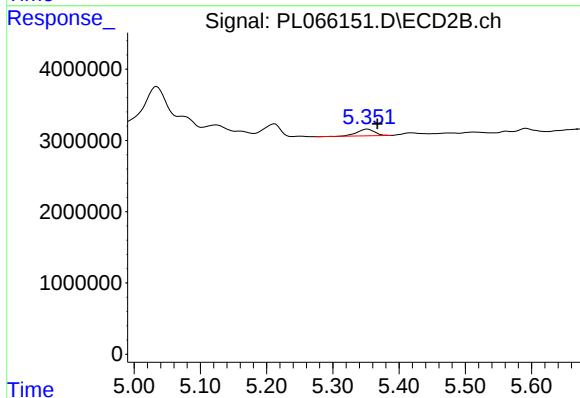


#4 Heptachlor

R.T.: 5.352 min
Delta R.T.: -0.015 min
Response: 1731780
Conc: 0.31 ng/ml

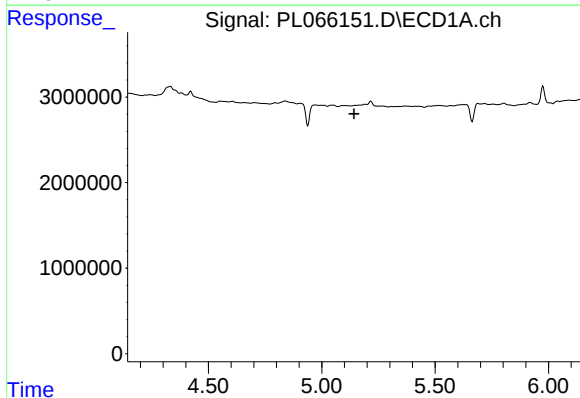


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.143 min
Response: 0
Conc: N.D.

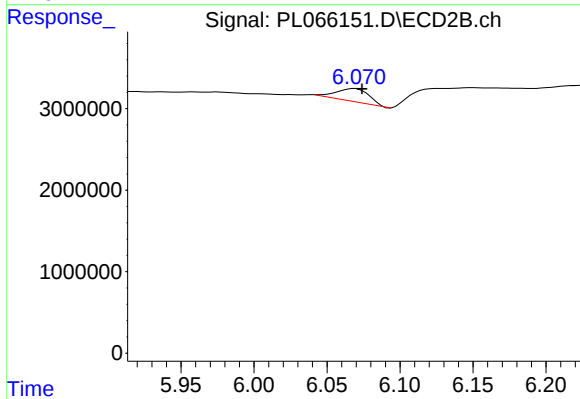

#8 Heptachlor epoxide


R.T.: 6.069 min
Delta R.T.: -0.005 min
Response: 2507732
Conc: 0.54 ng/ml

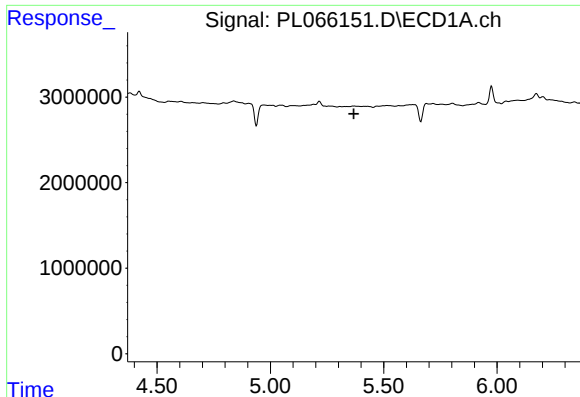

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

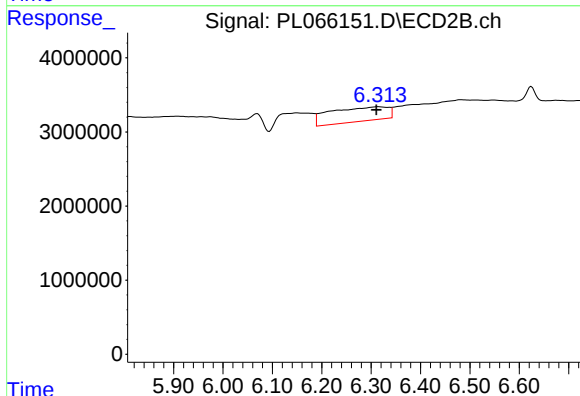


#10 gamma-Chlordane

R.T.: 6.314 min
Delta R.T.: 0.004 min
Response: 15706021
Conc: 3.44 ng/ml

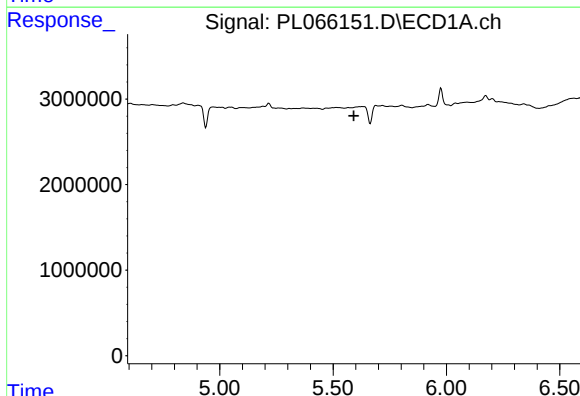


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.591 min
Response: 0
Conc: N.D.

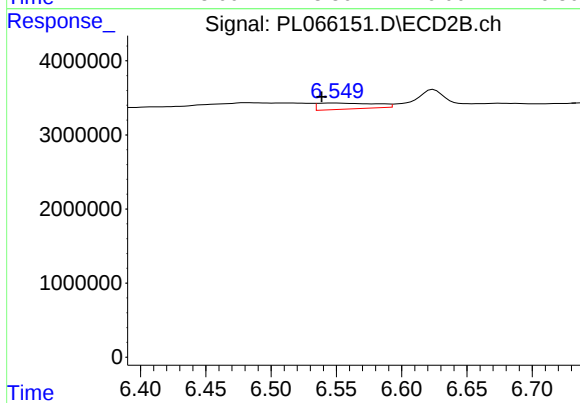

#12 4,4'-DDE


R.T.: 6.549 min
Delta R.T.: 0.011 min
Response: 2468696
Conc: 0.60 ng/ml

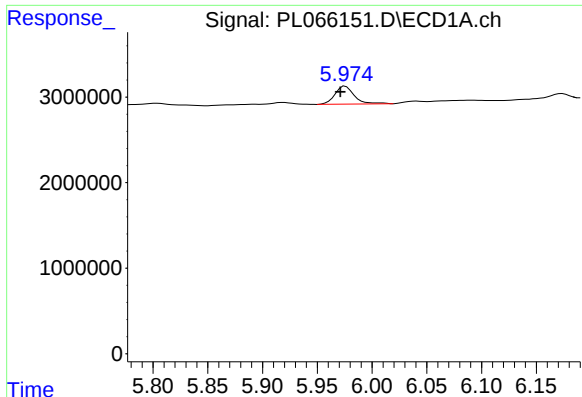

#14 Endrin


R.T.: 5.976 min
Delta R.T.: 0.005 min
Response: 2593884
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

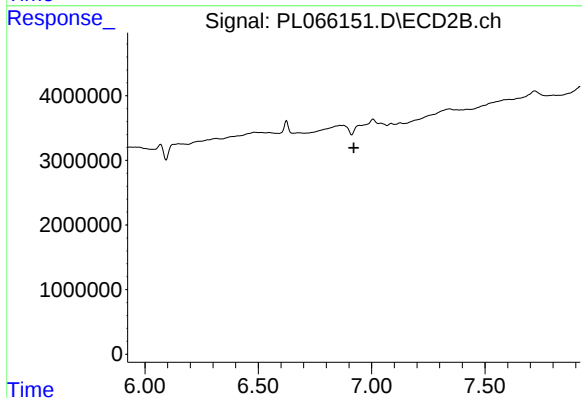


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

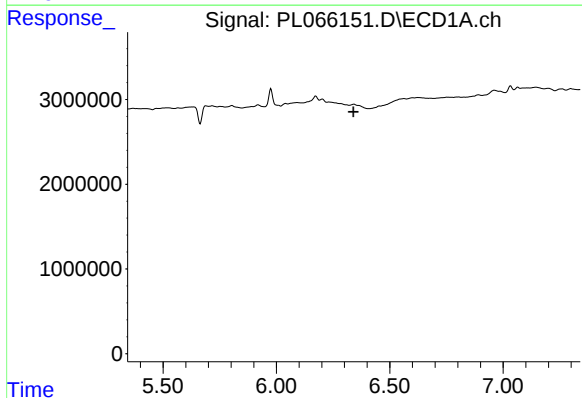


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.341 min
Response: 0
Conc: N.D.

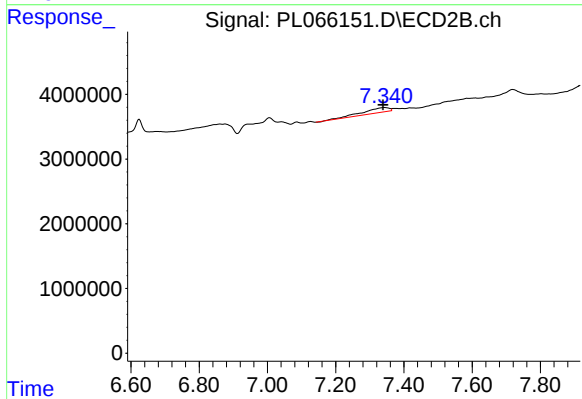

#17 4,4'-DDT


R.T.: 7.343 min
Delta R.T.: 0.004 min
Response: 4058895
Conc: 1.20 ng/ml

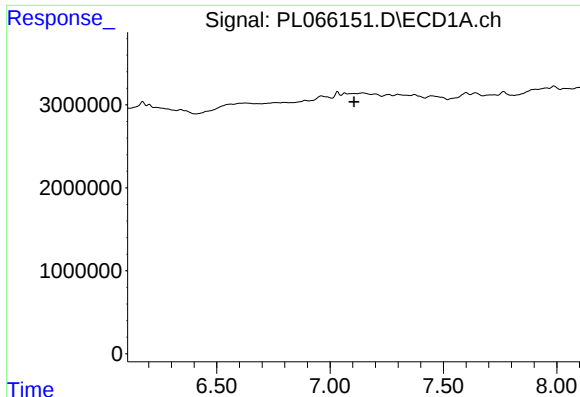

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.105 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

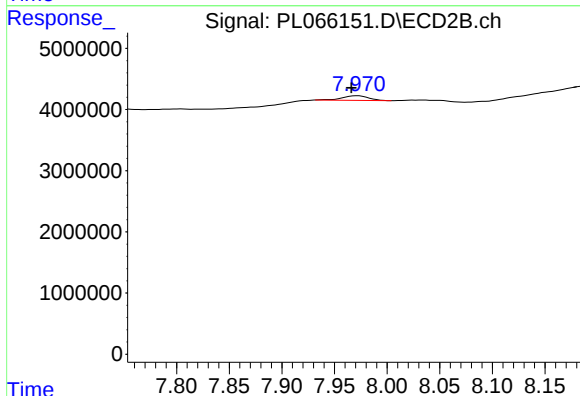


#21 Endrin ketone

R.T.: 7.972 min
Delta R.T.: 0.006 min
Response: 1328021
Conc: 0.36 ng/ml

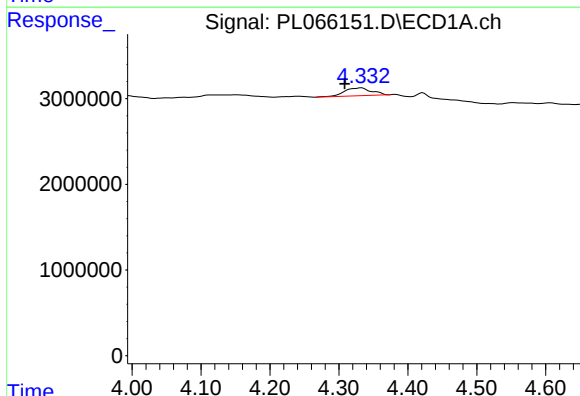


#23 Chlordane-1

R.T.: 4.333 min
Delta R.T.: 0.024 min
Response: 2514751
Conc: 22.00 ng/ml

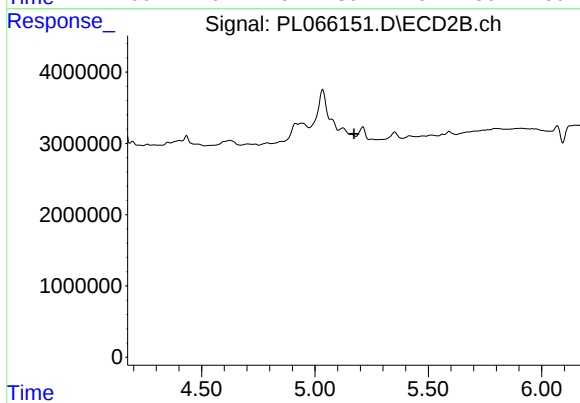

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.173 min
Response: 0
Conc: N.D.

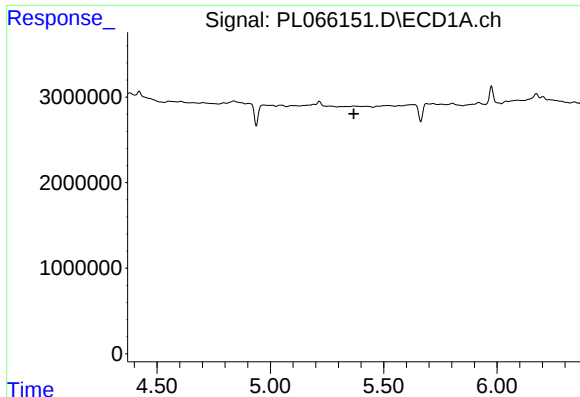

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

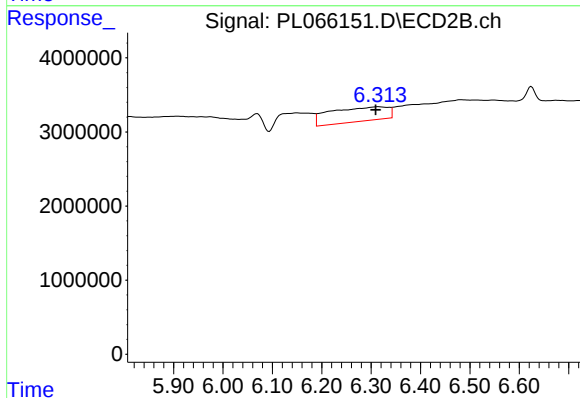


#25 Chlordane-3

R.T.: 6.314 min
Delta R.T.: 0.005 min
Response: 15706021
Conc: 23.89 ng/ml

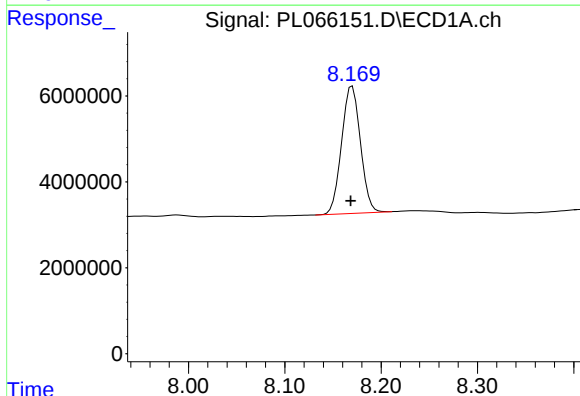

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: 0.002 min
Response: 40281234
Conc: 16.89 ng/ml

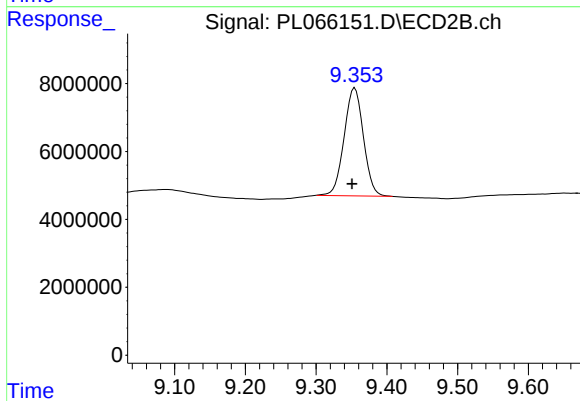

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.004 min
Response: 60342579
Conc: 18.48 ng/ml