

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
 Data File : PL066106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 10:59
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 11:54:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 11:50:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.154	285.4E6	388.0E6	96.690	96.641
28)	SA Decachlor...	8.169	9.351	215.9E6	302.7E6	92.112	94.249
Target Compounds							
23)	Chlordane-1	4.309	5.174	105.5E6	162.3E6	934.251	957.192
24)	Chlordane-2	4.804	5.652	118.7E6	159.6E6	913.008	928.270
25)	Chlordane-3	5.368	6.310	351.1E6	658.7E6	964.633	1000.776
26)	Chlordane-4	5.425	6.384	299.6E6	771.6E6	963.139	993.162
27)	Chlordane-5	6.251	7.206	134.1E6	133.4E6	947.249	993.169



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
Data File : PL066106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 10:59
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 11:54:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 11:50:27 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

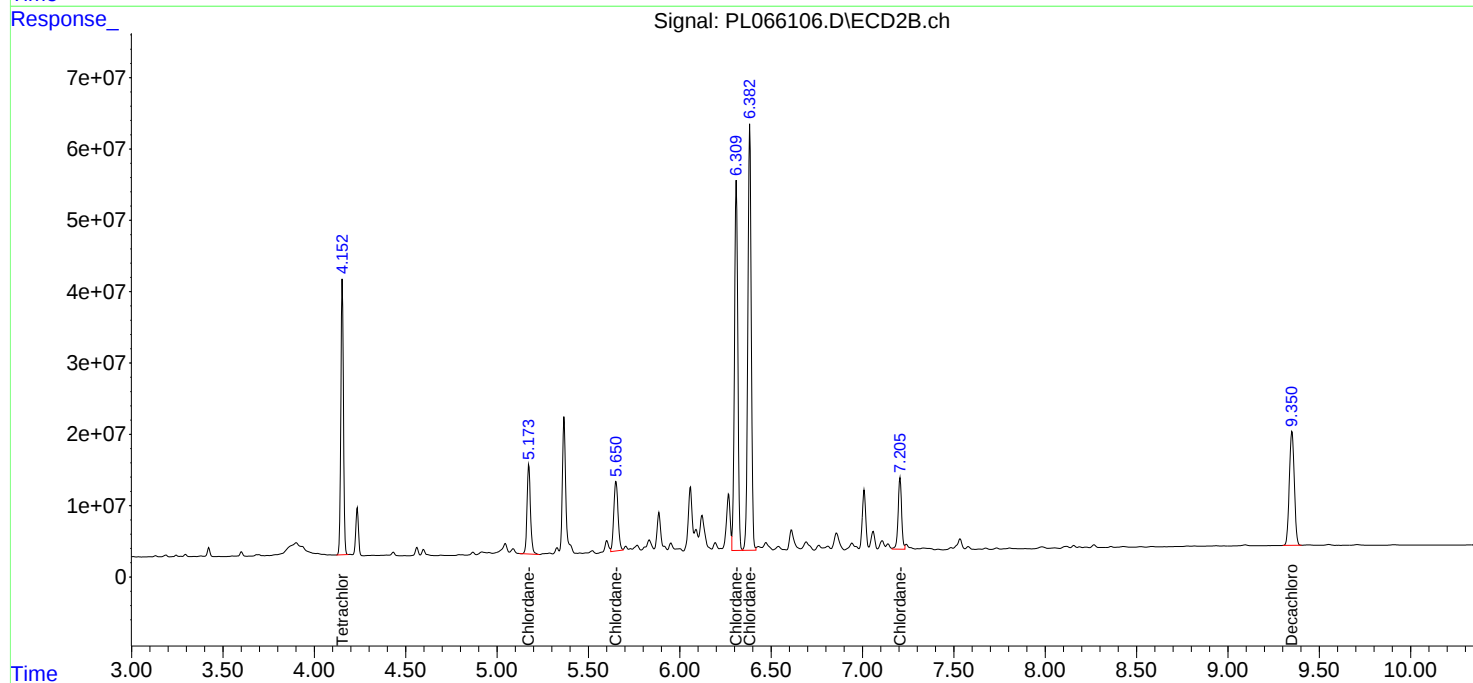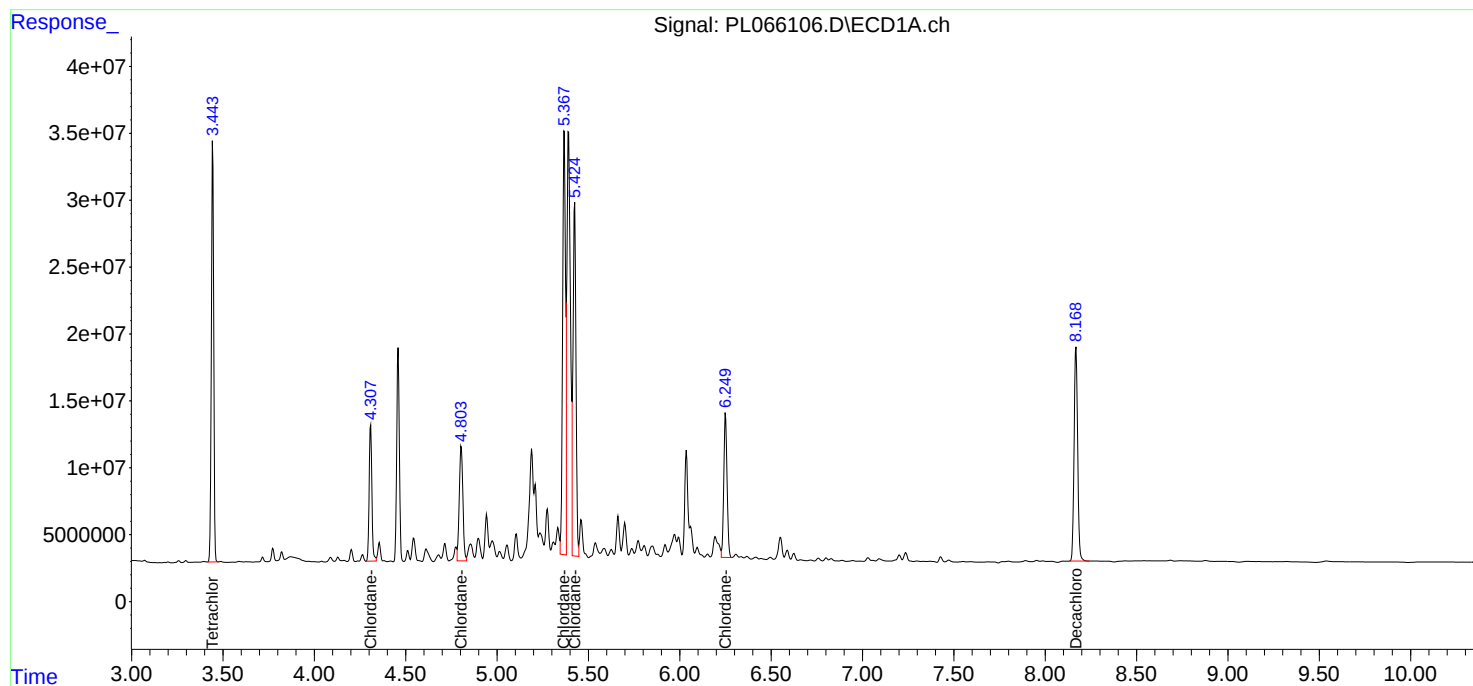


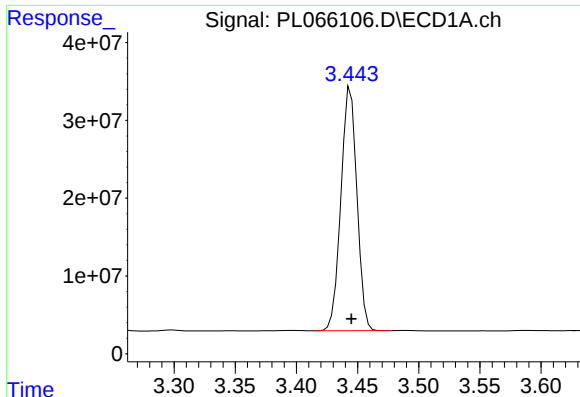

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 285395920
Conc: 96.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

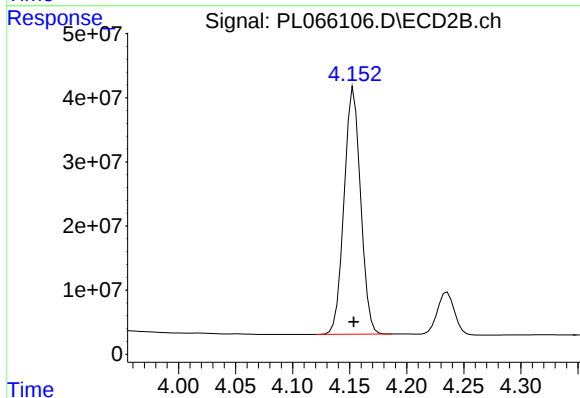


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 387991219
Conc: 96.64 ng/ml

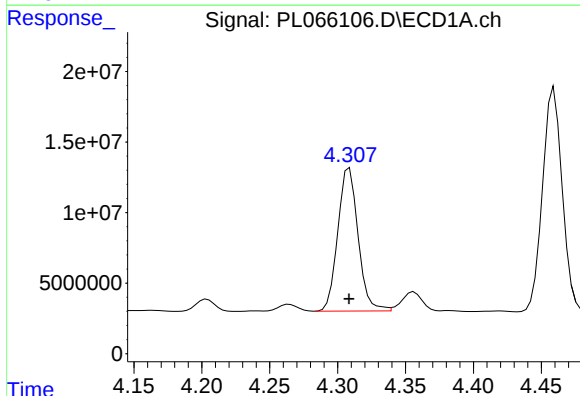


#23 Chlordane-1

R.T.: 4.309 min
Delta R.T.: 0.000 min
Response: 105468838
Conc: 934.25 ng/ml

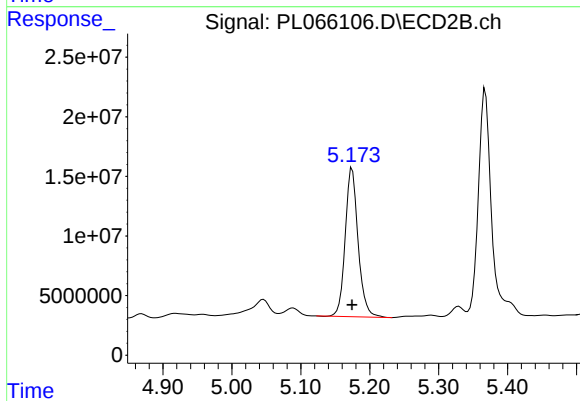

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 162254560
Conc: 957.19 ng/ml

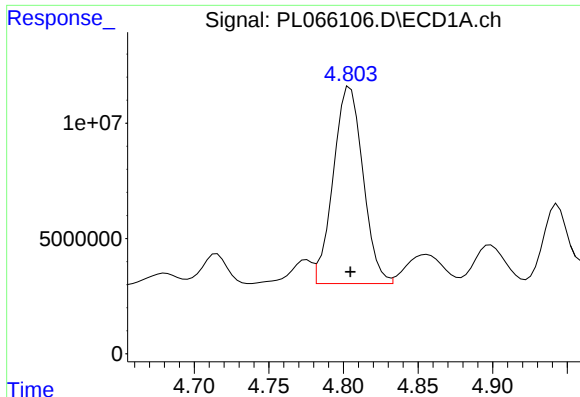

#24 Chlordane-2


R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 118697241
Conc: 913.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

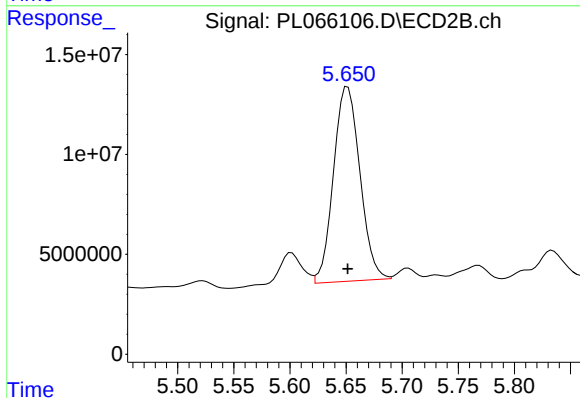


#24 Chlordane-2

R.T.: 5.652 min
Delta R.T.: 0.000 min
Response: 159607109
Conc: 928.27 ng/ml

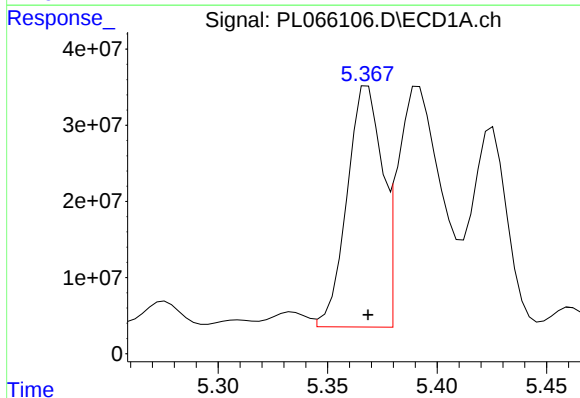


#25 Chlordane-3

R.T.: 5.368 min
Delta R.T.: 0.000 min
Response: 351091713
Conc: 964.63 ng/ml

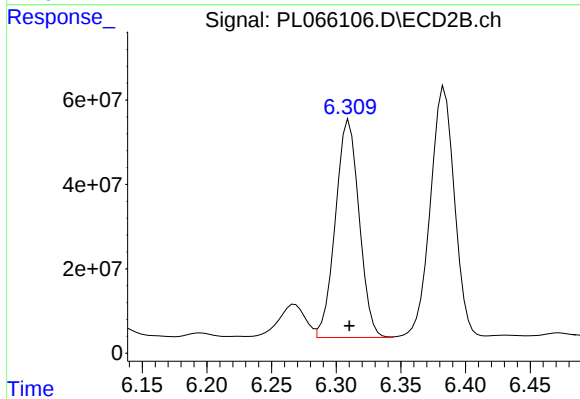

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 658724420
Conc: 1000.78 ng/ml

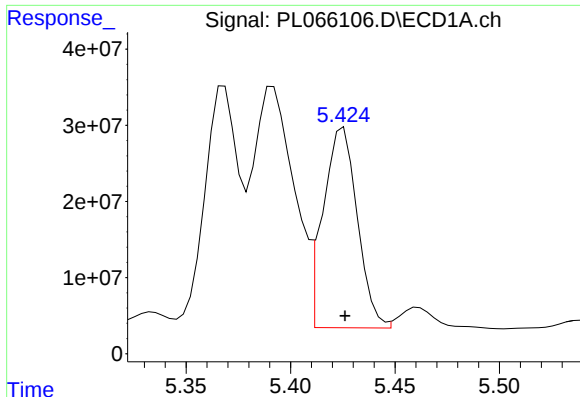

#26 Chlordane-4


R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 299620842
Conc: 963.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

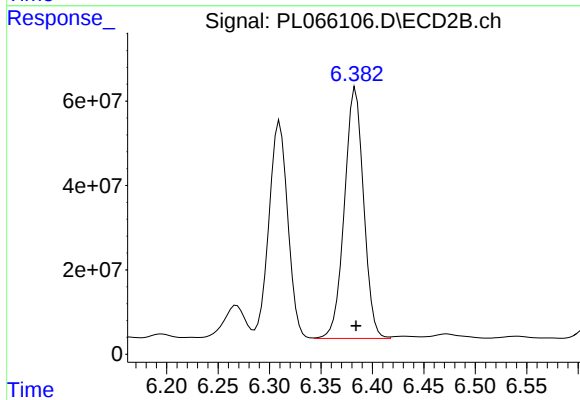


#26 Chlordane-4

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 771597462
Conc: 993.16 ng/ml

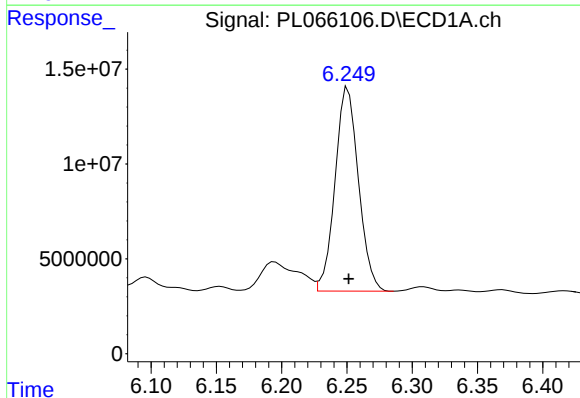


#27 Chlordane-5

R.T.: 6.251 min
Delta R.T.: 0.000 min
Response: 134133223
Conc: 947.25 ng/ml

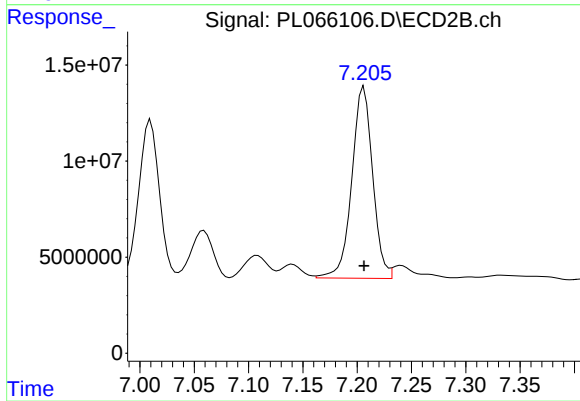

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 133366089
Conc: 993.17 ng/ml

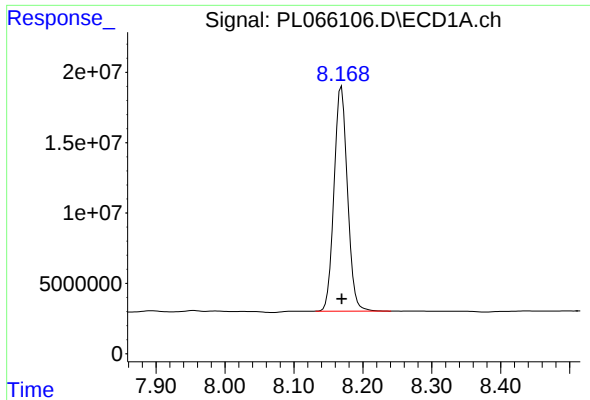

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.000 min
Response: 215866770
Conc: 92.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

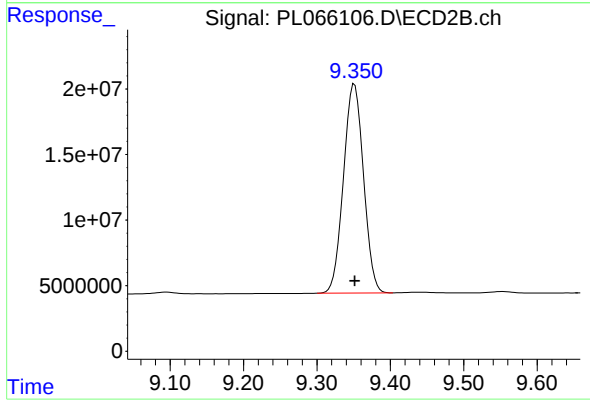

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 302655955
Conc: 94.25 ng/ml