

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
 Data File : PL066108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 11:28
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 11:54:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 11:50:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.154	147.6E6	200.7E6	50.000	50.000
28)	SA Decachlor...	8.169	9.351	117.2E6	160.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.309	5.174	56445641	84755508	500.000	500.000
24)	Chlordane-2	4.805	5.652	65003387	85970227	500.000	500.000
25)	Chlordane-3	5.368	6.310	182.0E6	329.1E6	500.000	500.000
26)	Chlordane-4	5.426	6.384	155.5E6	388.5E6	500.000	500.000
27)	Chlordane-5	6.251	7.206	70801465	67141697	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
Data File : PL066108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 11:28
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 11:54:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 11:50:27 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

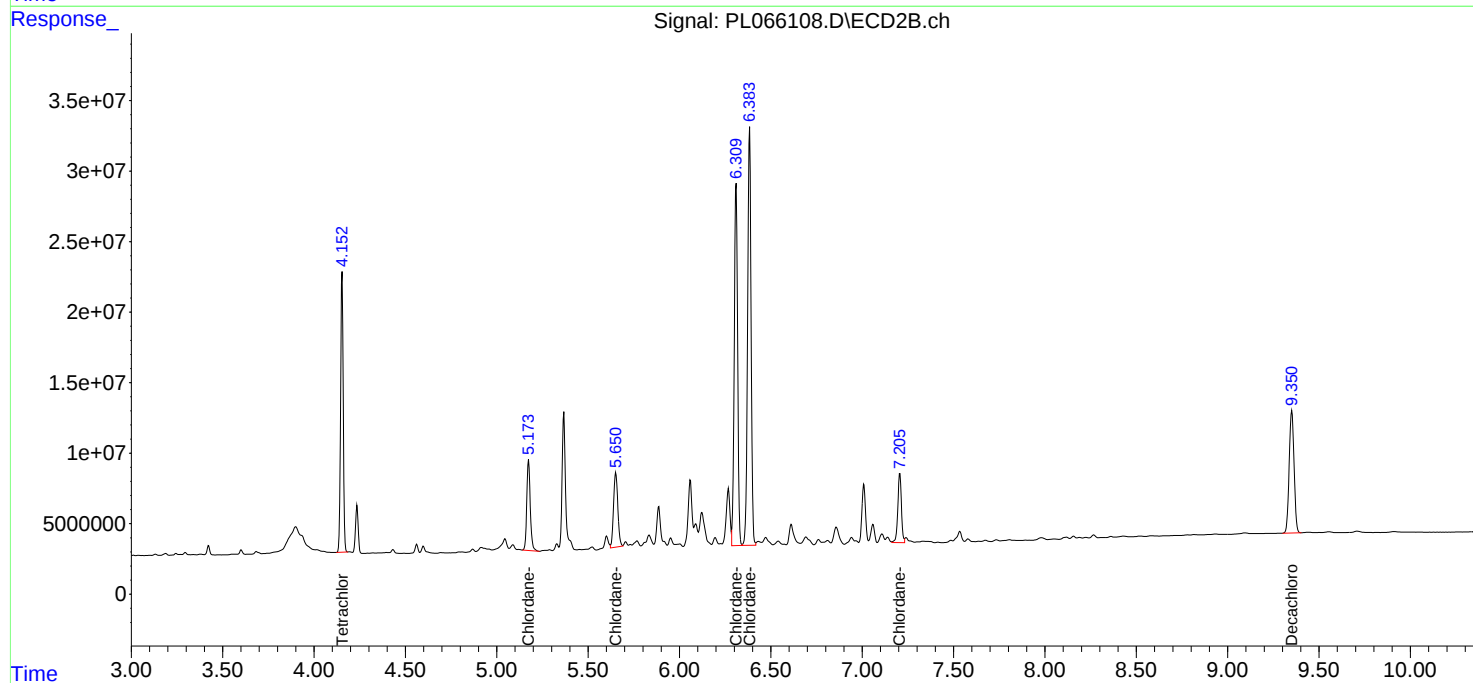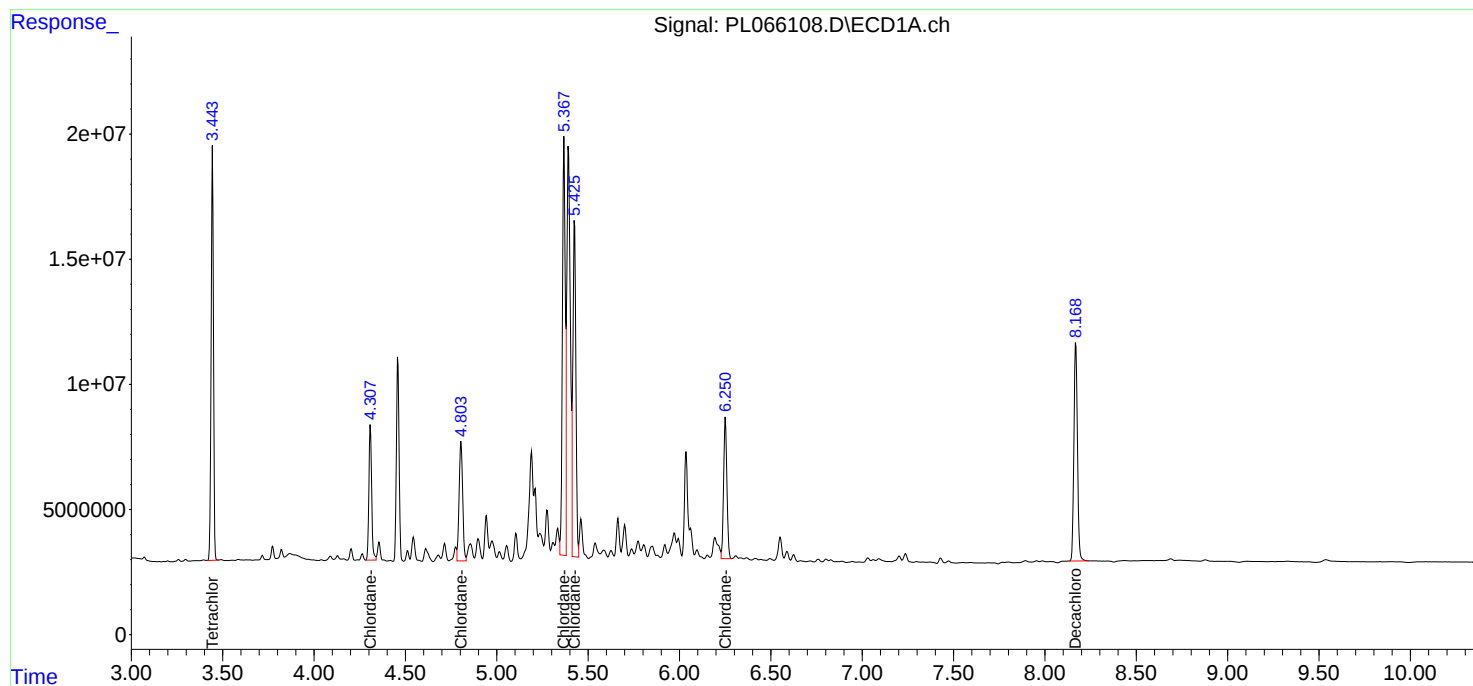


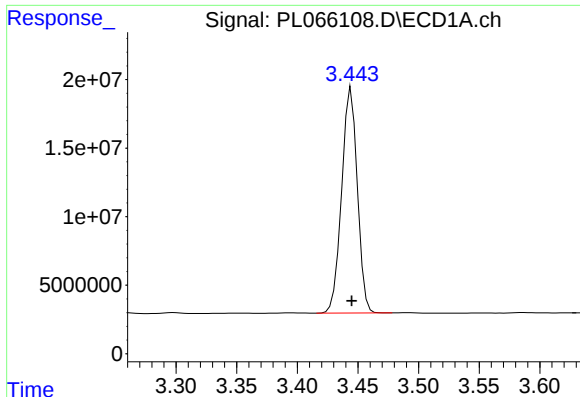

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 147583524
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

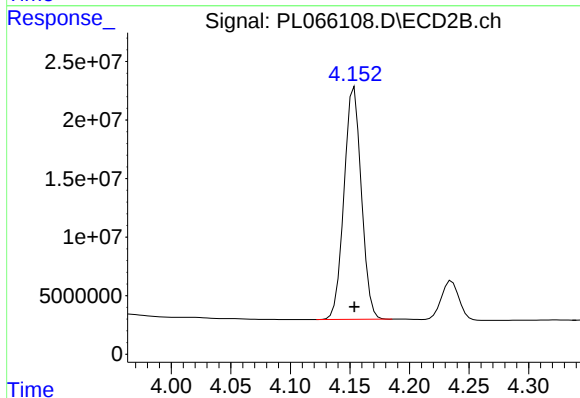


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 200739046
Conc: 50.00 ng/ml

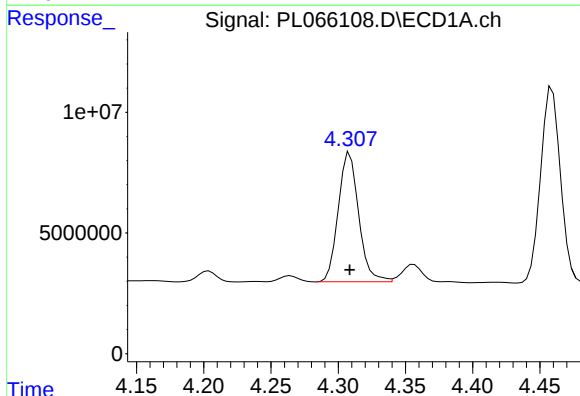


#23 Chlordane-1

R.T.: 4.309 min
Delta R.T.: 0.000 min
Response: 56445641
Conc: 500.00 ng/ml

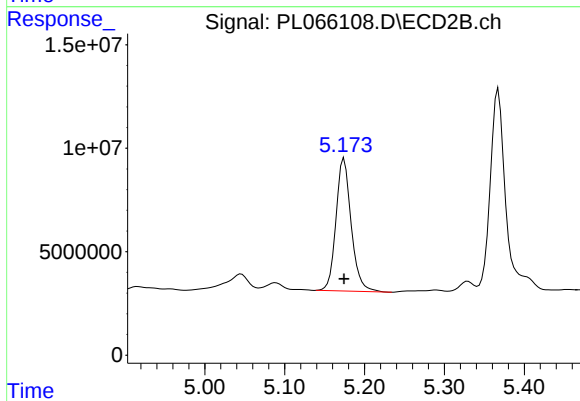

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 84755508
Conc: 500.00 ng/ml

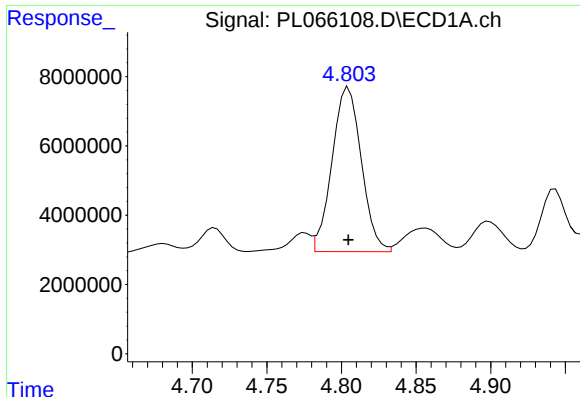

#24 Chlordane-2


R.T.: 4.805 min
Delta R.T.: 0.000 min
Response: 65003387
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

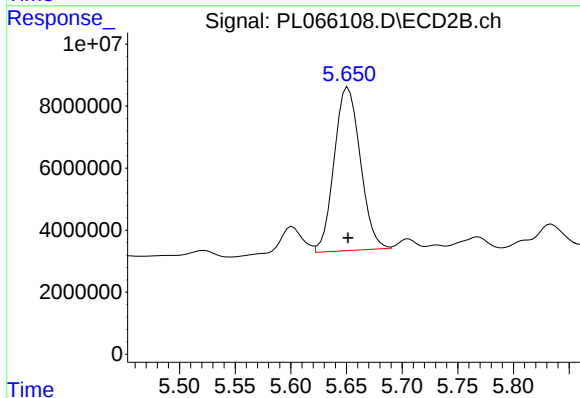


#24 Chlordane-2

R.T.: 5.652 min
Delta R.T.: 0.000 min
Response: 85970227
Conc: 500.00 ng/ml

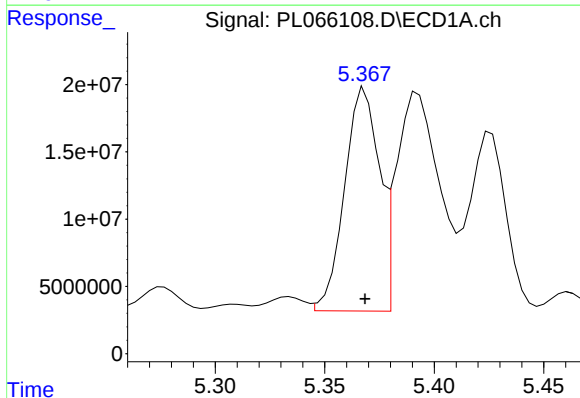


#25 Chlordane-3

R.T.: 5.368 min
Delta R.T.: 0.000 min
Response: 181982090
Conc: 500.00 ng/ml

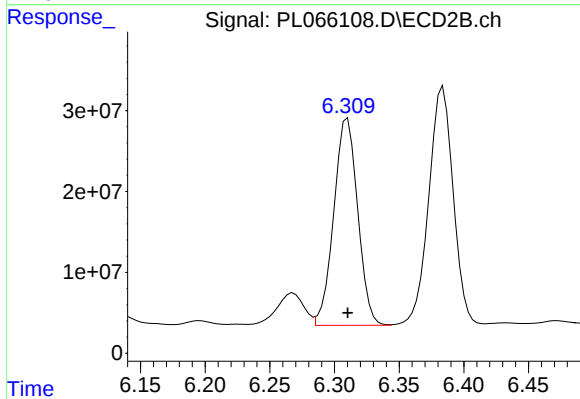

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 329106689
Conc: 500.00 ng/ml

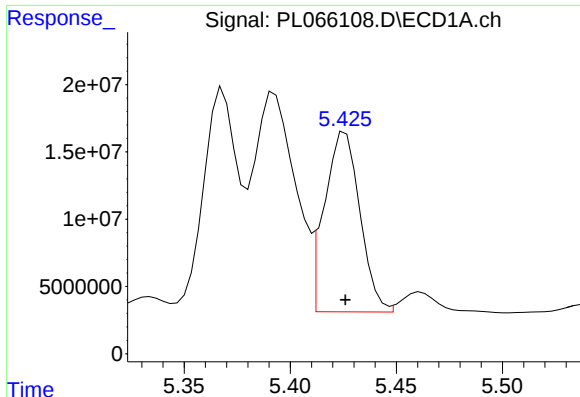

#26 Chlordane-4


R.T.: 5.426 min
Delta R.T.: 0.000 min
Response: 155543912
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

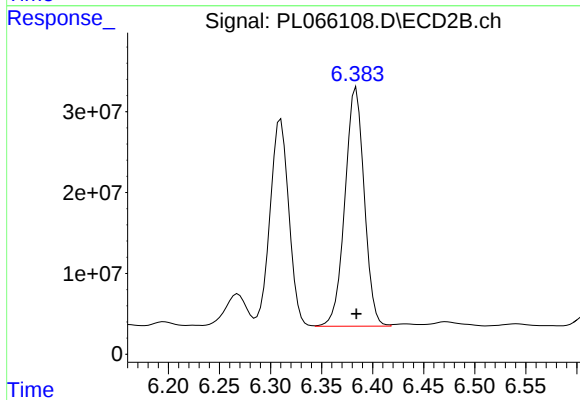


#26 Chlordane-4

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 388455104
Conc: 500.00 ng/ml

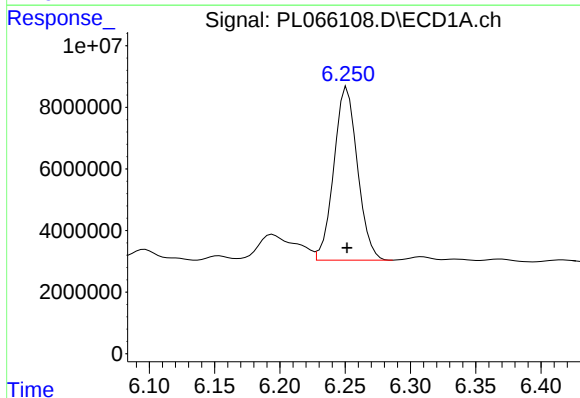


#27 Chlordane-5

R.T.: 6.251 min
Delta R.T.: 0.000 min
Response: 70801465
Conc: 500.00 ng/ml

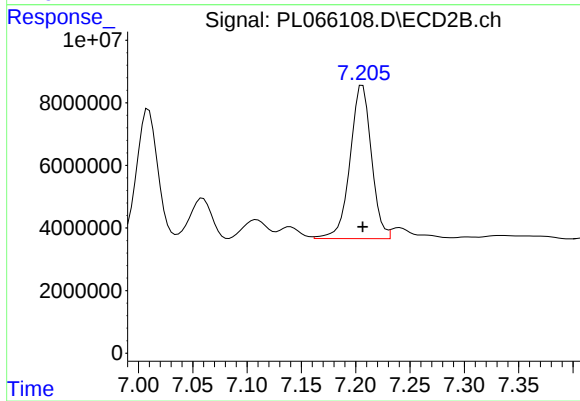

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 67141697
Conc: 500.00 ng/ml

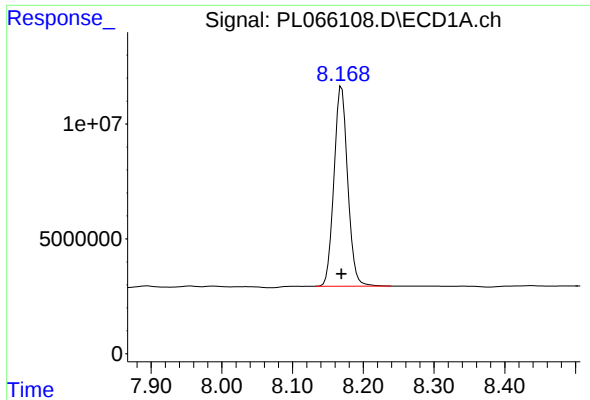

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.000 min
Response: 117176378
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

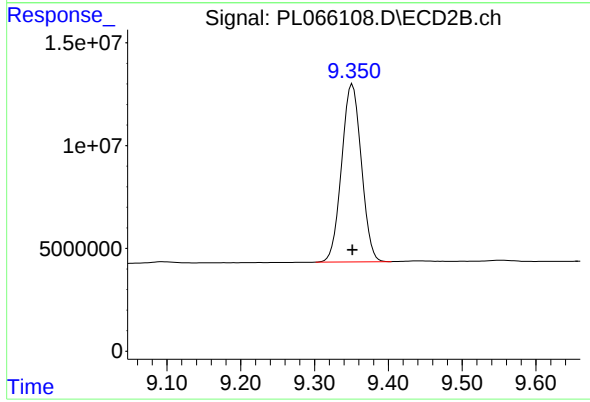

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 160562432
Conc: 50.00 ng/ml