

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
 Data File : PL066110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 11:56
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 12:07:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 11:50:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.153	15472611	20250154	5.242	5.044
28)	SA Decachlor...	8.169	9.351	13800445	17634700	5.889	5.492
Target Compounds							
23)	Chlordane-1	4.308	5.173	6327269	9587219	56.047	56.558
24)	Chlordane-2	4.805	5.650	7774061	10179222	59.797	59.202
25)	Chlordane-3	5.368	6.309	19296222	33193234	53.017	50.429
26)	Chlordane-4	5.425	6.383	17212092	41048150	55.329	52.835
27)	Chlordane-5	6.251	7.206	7499812	6711398	52.964	49.979


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
Data File : PL066110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 11:56
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 12:07:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 11:50:27 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

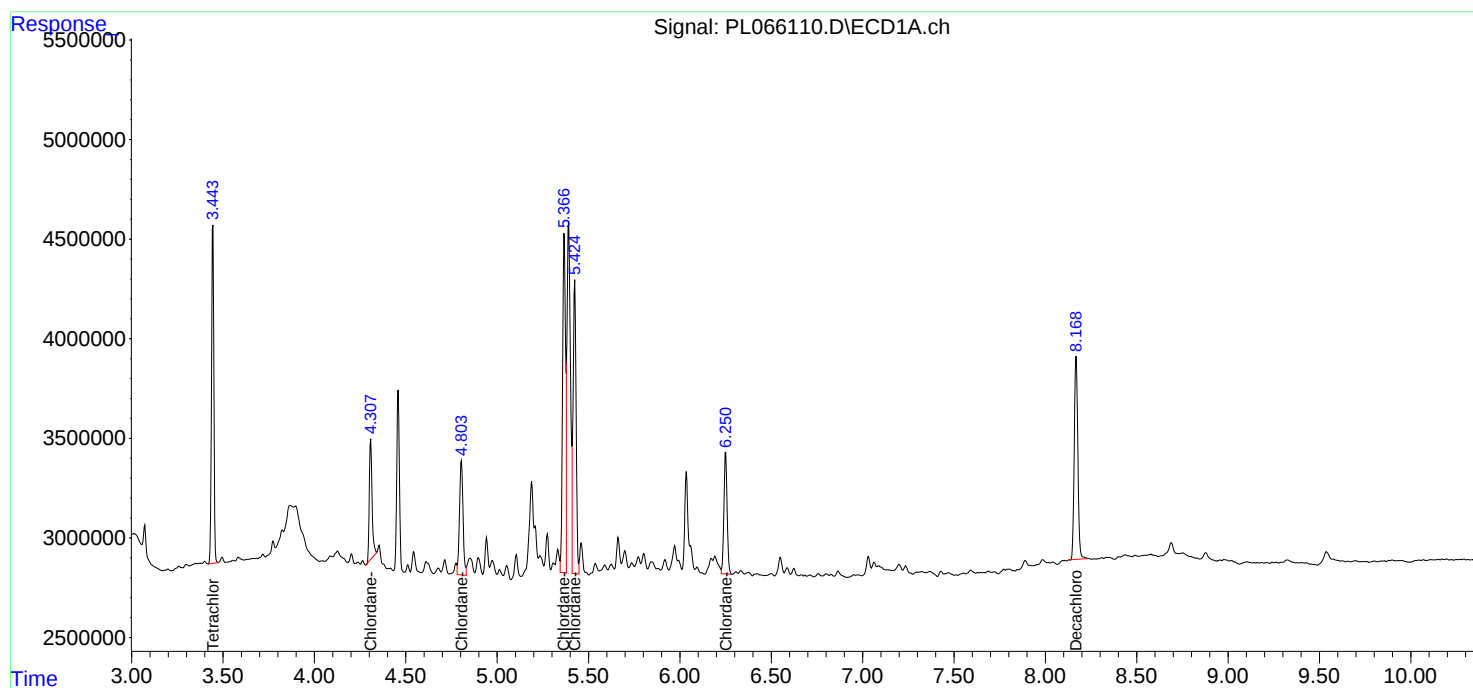


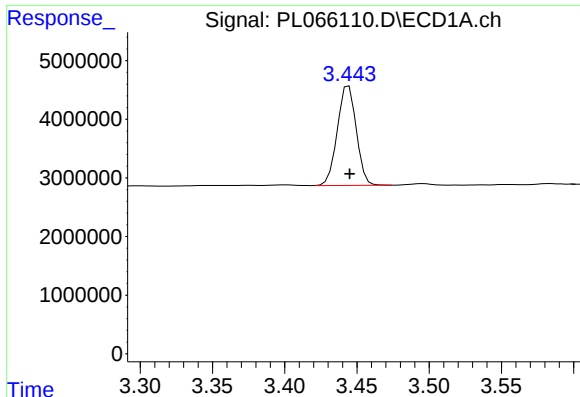

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 15472611
Conc: 5.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

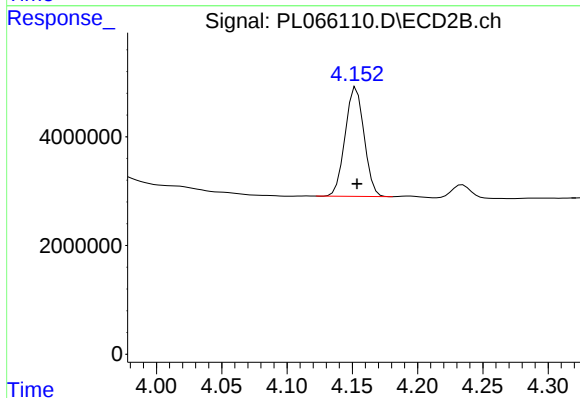


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 20250154
Conc: 5.04 ng/ml

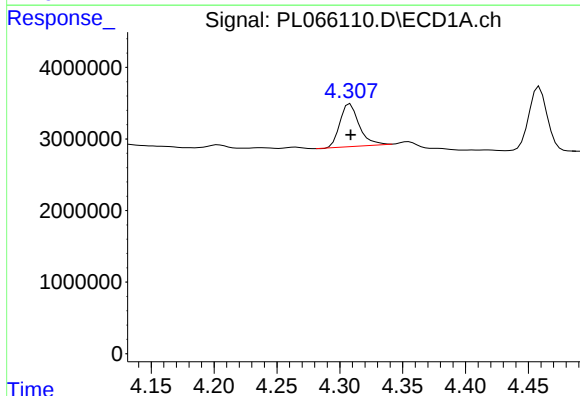


#23 Chlordane-1

R.T.: 4.308 min
Delta R.T.: 0.000 min
Response: 6327269
Conc: 56.05 ng/ml

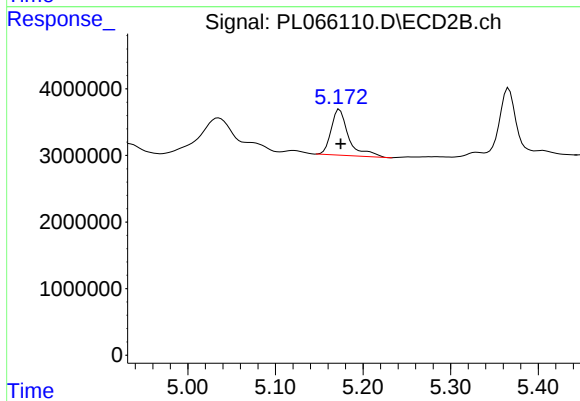

#23 Chlordane-1


R.T.: 5.173 min
Delta R.T.: -0.001 min
Response: 9587219
Conc: 56.56 ng/ml

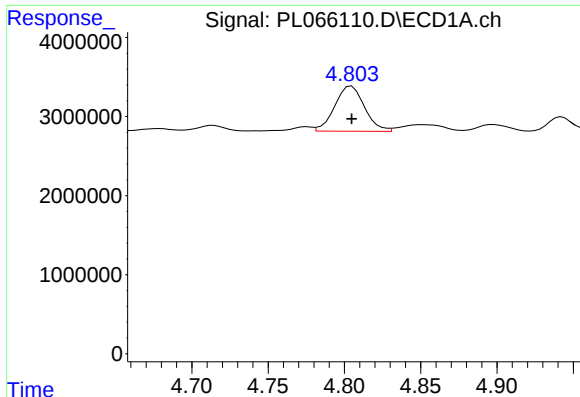

#24 Chlordane-2


R.T.: 4.805 min
Delta R.T.: 0.000 min
Response: 7774061
Conc: 59.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

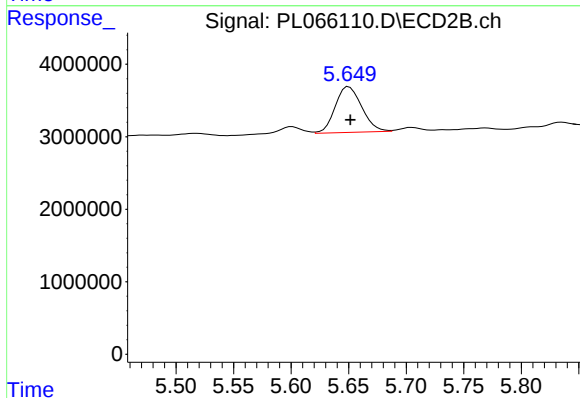


#24 Chlordane-2

R.T.: 5.650 min
Delta R.T.: -0.001 min
Response: 10179222
Conc: 59.20 ng/ml

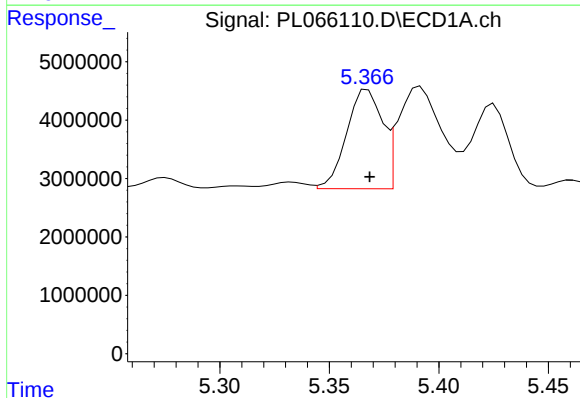


#25 Chlordane-3

R.T.: 5.368 min
Delta R.T.: 0.000 min
Response: 19296222
Conc: 53.02 ng/ml

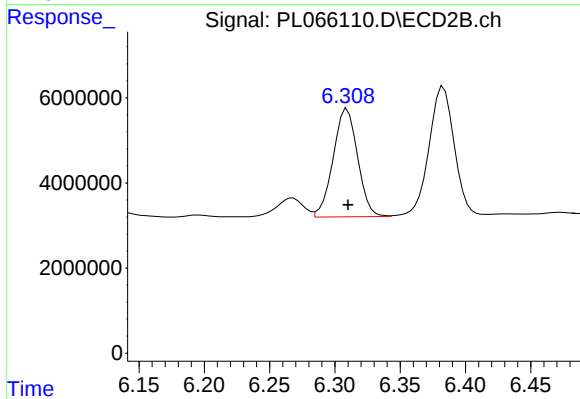

#25 Chlordane-3


R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 33193234
Conc: 50.43 ng/ml

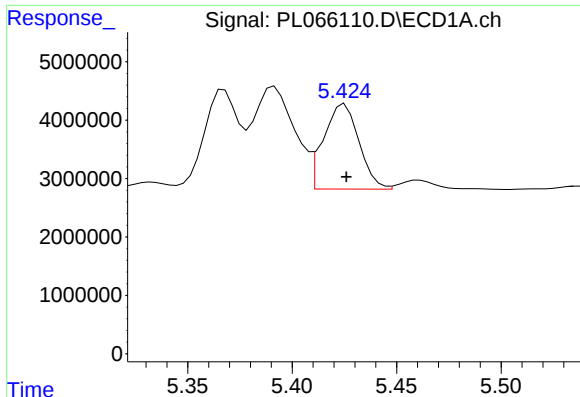

#26 Chlordane-4


R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 17212092
Conc: 55.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

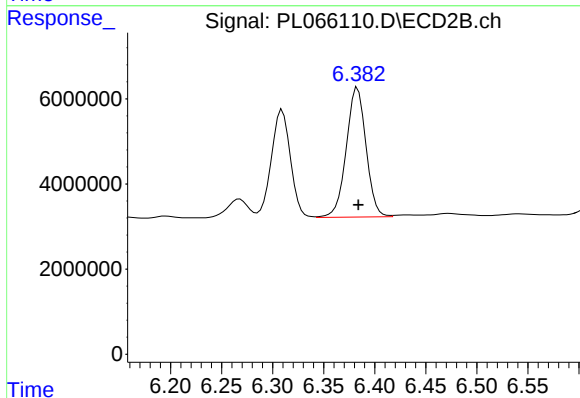


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 41048150
Conc: 52.84 ng/ml

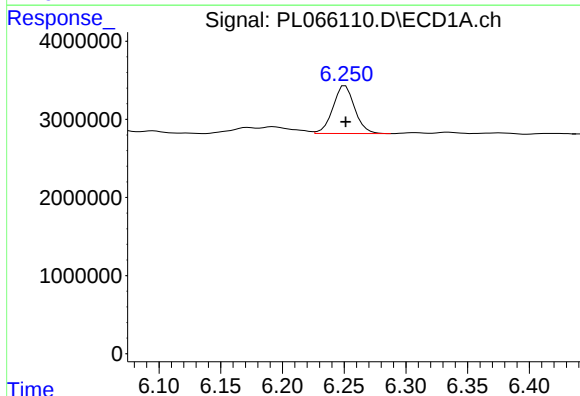


#27 Chlordane-5

R.T.: 6.251 min
Delta R.T.: 0.000 min
Response: 7499812
Conc: 52.96 ng/ml

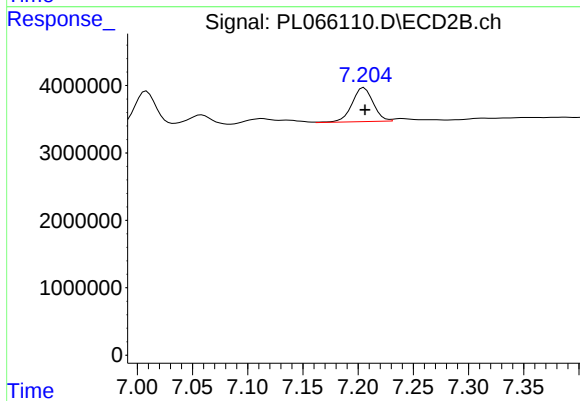

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 6711398
Conc: 49.98 ng/ml

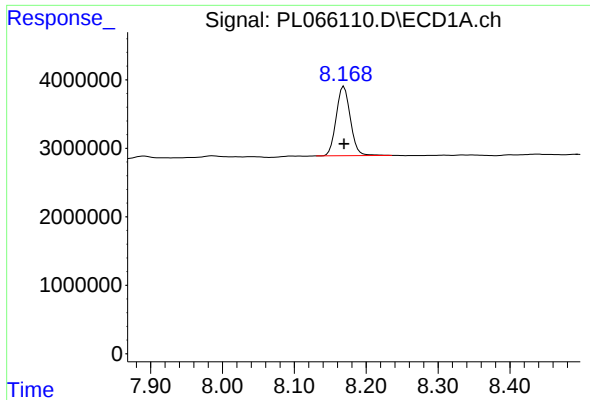

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.000 min
Response: 13800445
Conc: 5.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

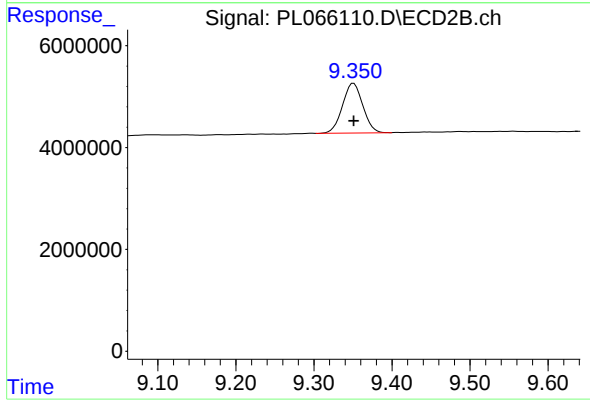

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 17634700
Conc: 5.49 ng/ml