

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
 Data File : PL066117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 13:36
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL041421

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 15:35:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:34:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.153	147.3E6	200.3E6	49.951	50.508
28)	SA Decachlor...	8.169	9.351	116.9E6	162.4E6	49.168	50.201
Target Compounds							
23)	Chlordane-1	4.308	5.173	56329488	85479308	492.732	497.169
24)	Chlordane-2	4.805	5.651	64677113	87066142	486.244	494.890
25)	Chlordane-3	5.368	6.310	177.1E6	337.5E6	487.179	513.332
26)	Chlordane-4	5.425	6.383	154.3E6	402.9E6	489.065	512.907
27)	Chlordane-5	6.251	7.206	71125543	68207313	503.431	508.906



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
Data File : PL066117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 13:36
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL041421

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 15:35:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:34:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

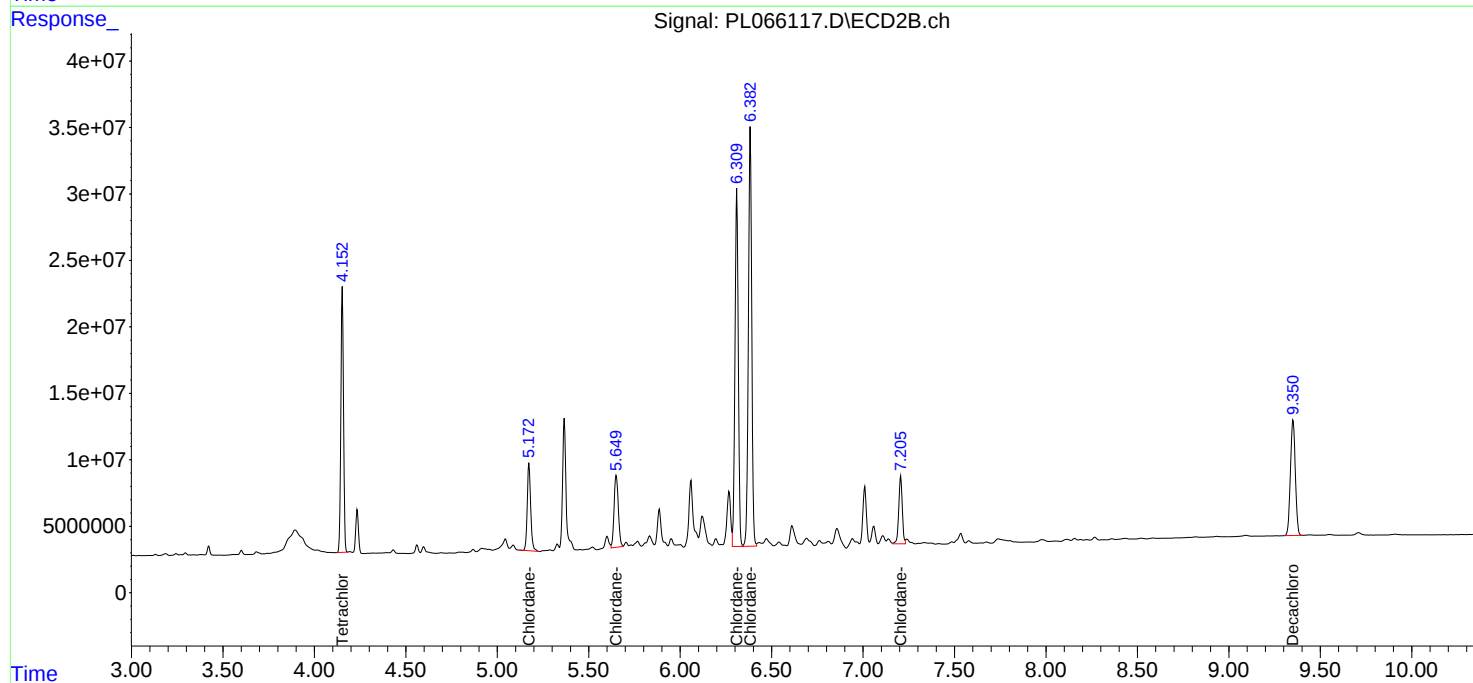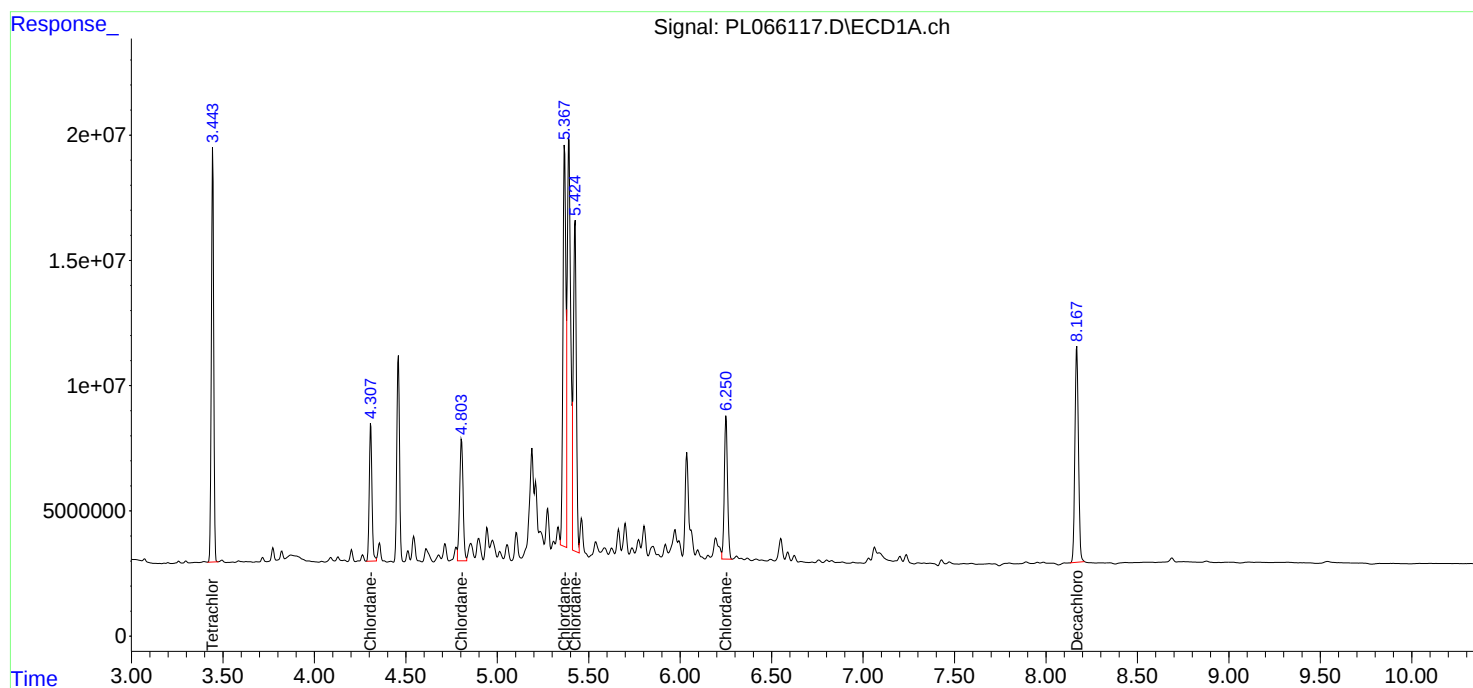


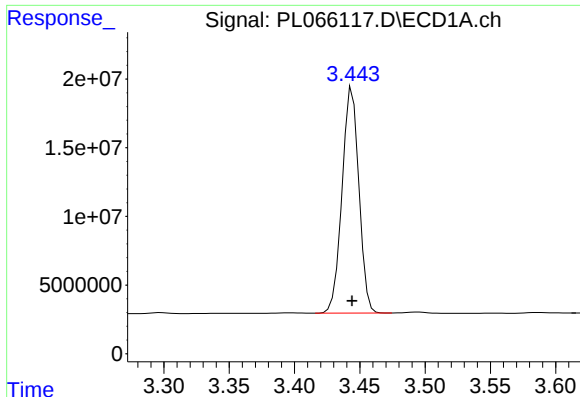

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 147256549
Conc: 49.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL041421

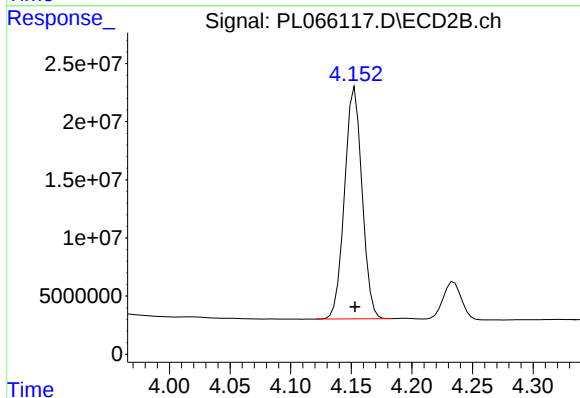


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 200322424
Conc: 50.51 ng/ml

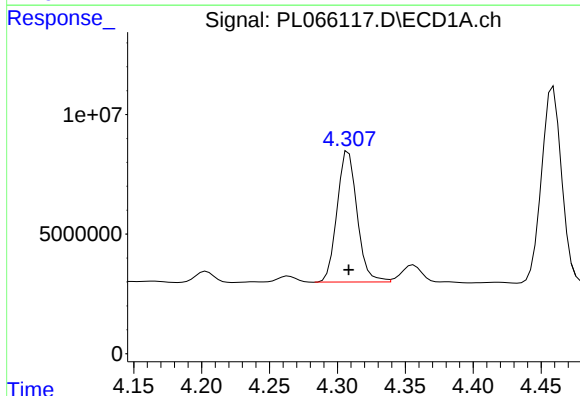


#23 Chlordane-1

R.T.: 4.308 min
Delta R.T.: 0.000 min
Response: 56329488
Conc: 492.73 ng/ml

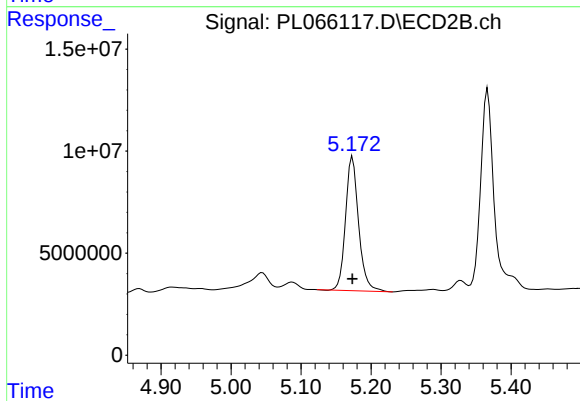

#23 Chlordane-1


R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 85479308
Conc: 497.17 ng/ml

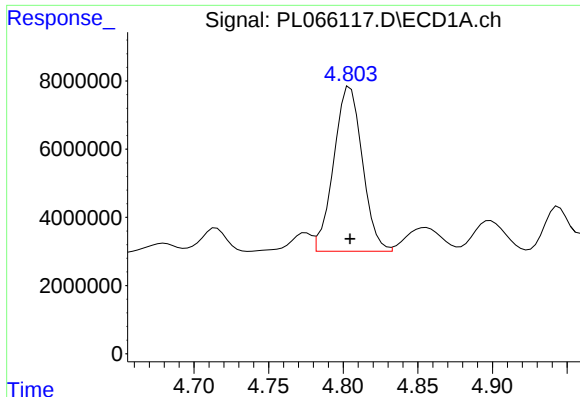

#24 Chlordane-2


R.T.: 4.805 min
Delta R.T.: 0.000 min
Response: 64677113
Conc: 486.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL041421

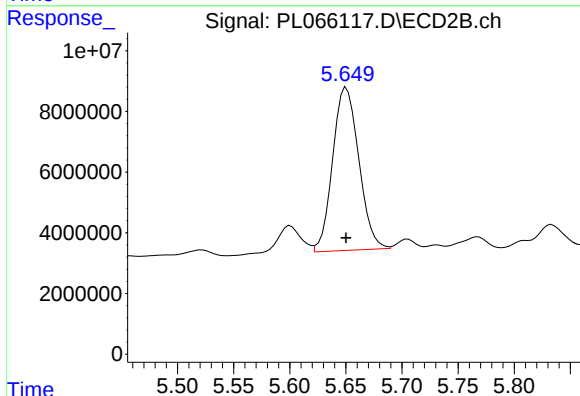


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 87066142
Conc: 494.89 ng/ml

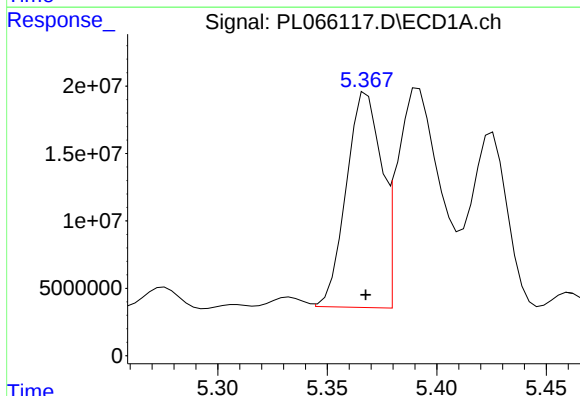


#25 Chlordane-3

R.T.: 5.368 min
Delta R.T.: 0.000 min
Response: 177068369
Conc: 487.18 ng/ml

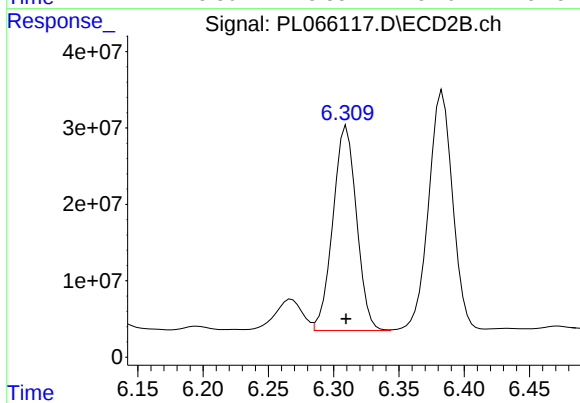

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 337531391
Conc: 513.33 ng/ml

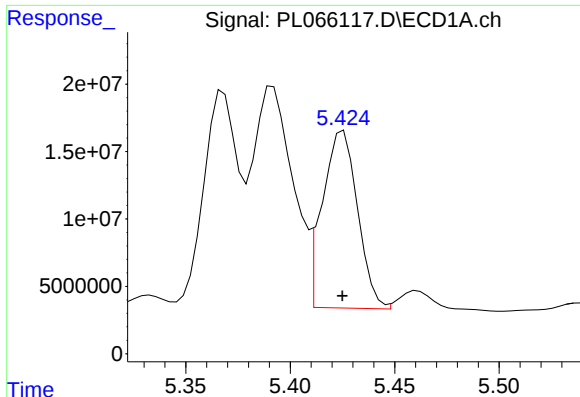

#26 Chlordane-4


R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 154305942
Conc: 489.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL041421

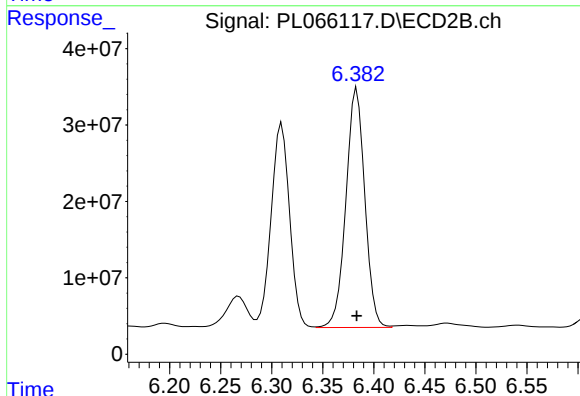


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 402911293
Conc: 512.91 ng/ml

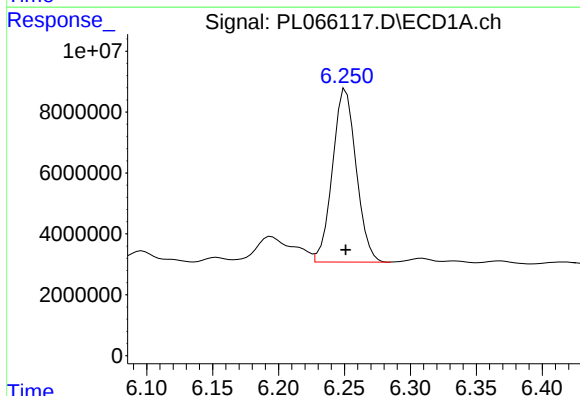


#27 Chlordane-5

R.T.: 6.251 min
Delta R.T.: 0.000 min
Response: 71125543
Conc: 503.43 ng/ml

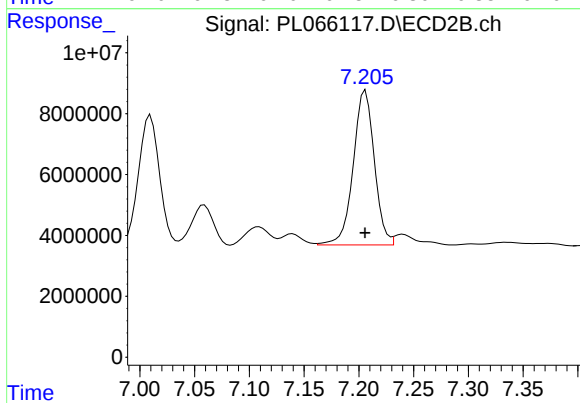

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 68207313
Conc: 508.91 ng/ml

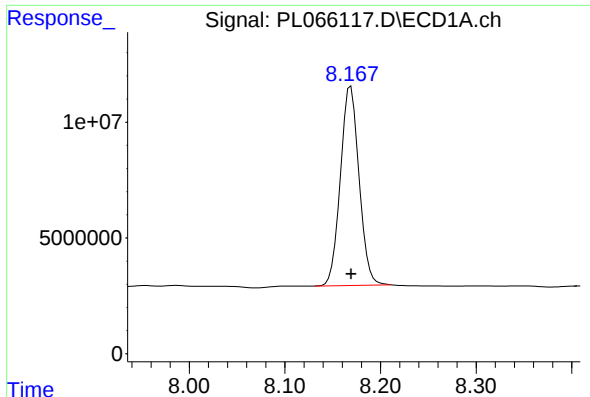

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.000 min
Response: 116879432
Conc: 49.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL041421

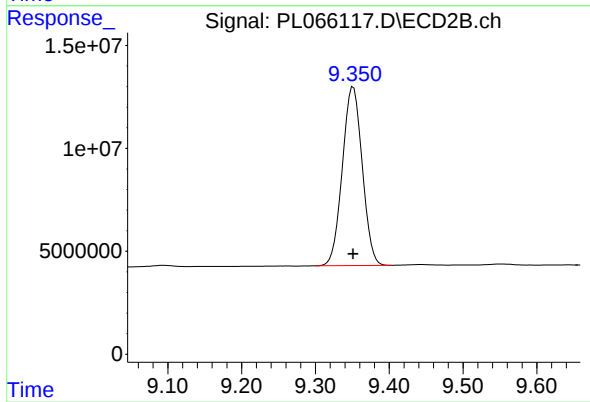

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 162437132
Conc: 50.20 ng/ml