

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
 Data File : PL066124.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 15:36
 Operator : AR\AJ
 Sample : M1998-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-3A

Manual Integrations
 APPROVED

Ankita
 4/15/2021 12:07:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 01:13:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.153	29038907	45966232	11.409	11.427
28)	SA Decachlor...	8.170	9.352	34246460	49578665	14.357	15.181
Target Compounds							
12)	B 4,4'-DDE	5.591	6.540	151.5E6	211.5E6	40.616	51.102 #
17)	MA 4,4'-DDT	6.338	7.339	40311303	26534497	12.647m	7.822 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
Data File : PL066124.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 15:36
Operator : AR\AJ
Sample : M1998-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-3A


Manual Integrations
APPROVED

Ankita
4/15/2021 12:07:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 01:13:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

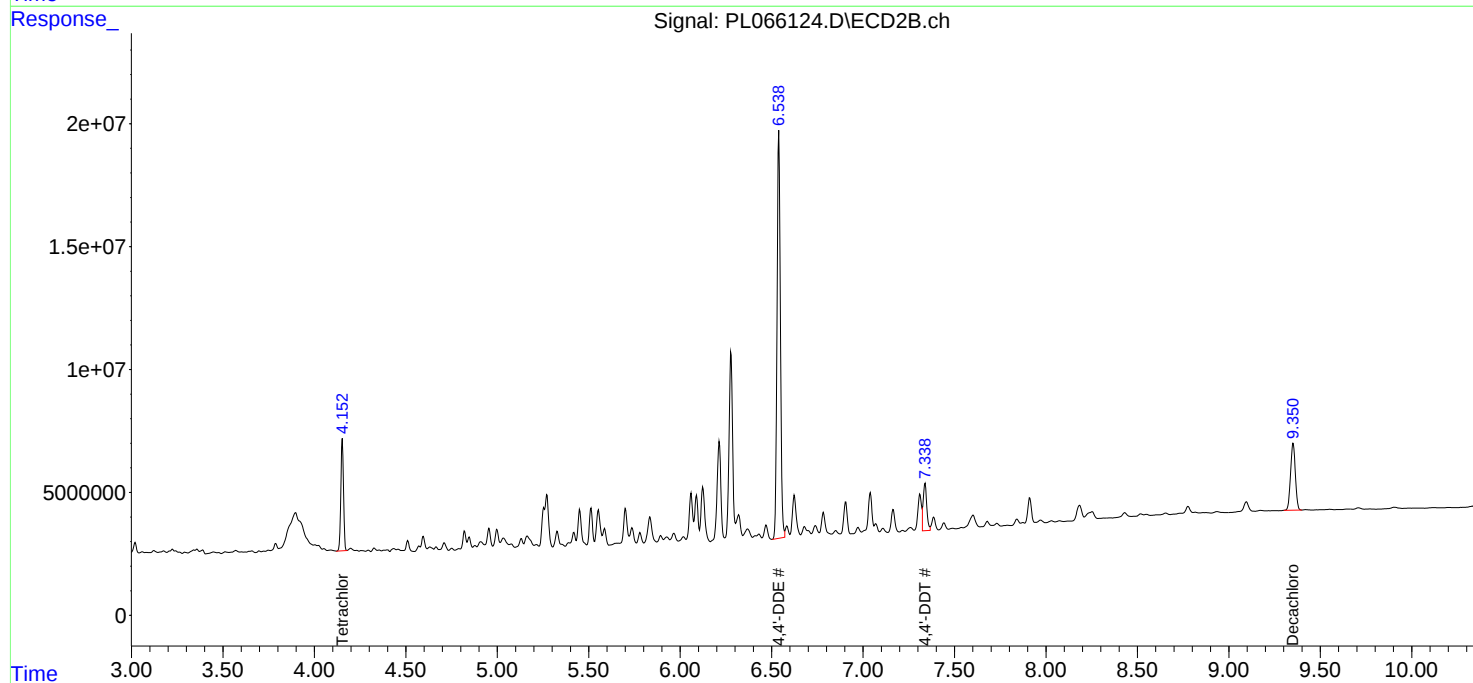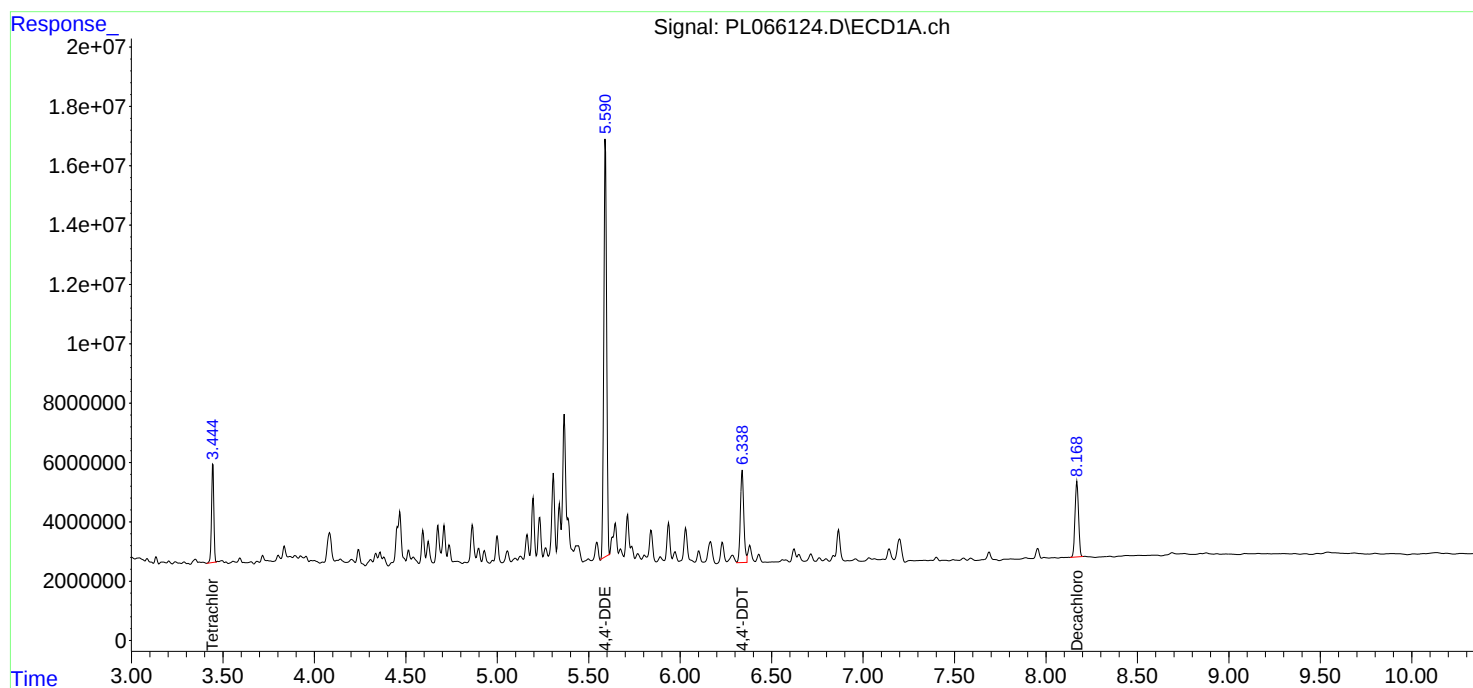

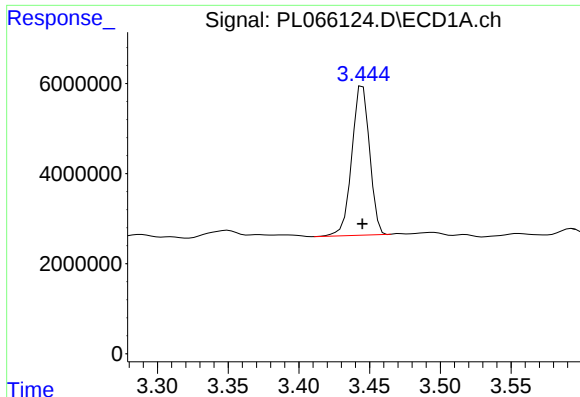


#1 Tetrachloro-m-xylene

R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 29038907
Conc: 11.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-3A


Manual Integrations
APPROVED

Ankita
4/15/2021 12:07:42 PM

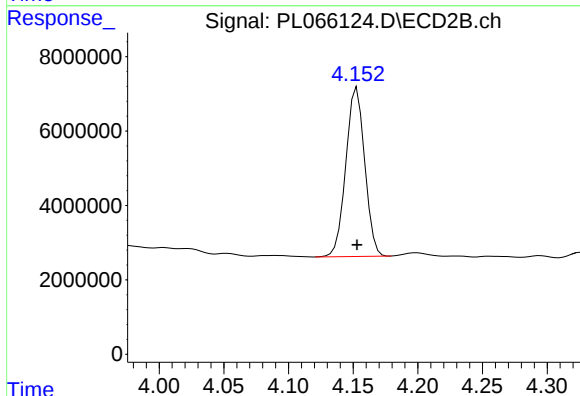


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 45966232
Conc: 11.43 ng/ml

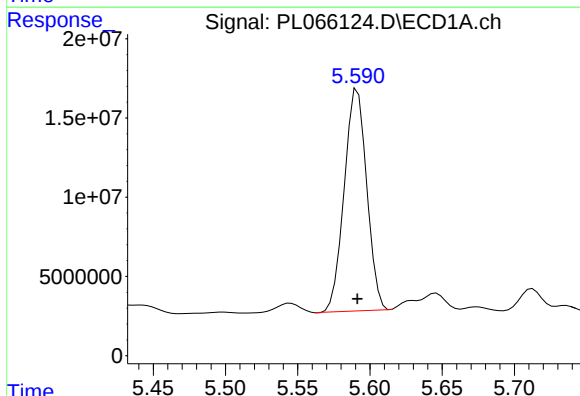


#12 4,4'-DDE

R.T.: 5.591 min
Delta R.T.: 0.000 min
Response: 151502193
Conc: 40.62 ng/ml

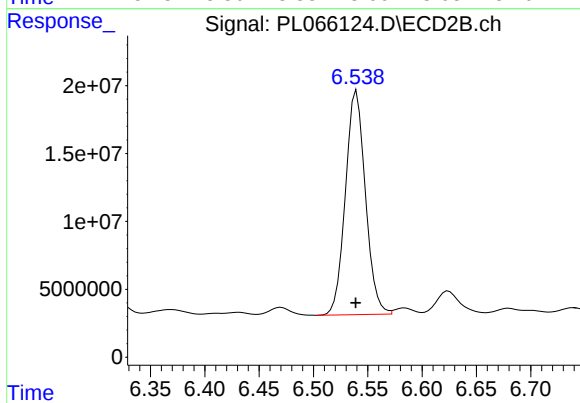

#12 4,4'-DDE

R.T.: 6.540 min
Delta R.T.: 0.000 min
Response: 211516839
Conc: 51.10 ng/ml

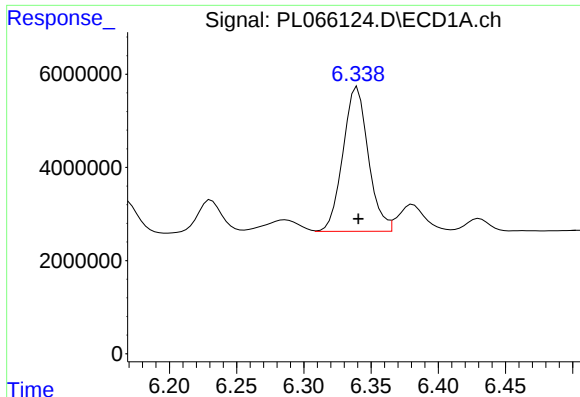


#17 4,4'-DDT

R.T.: 6.338 min
Delta R.T.: -0.002 min
Response: 40311303
Conc: 12.65 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-3A


Manual Integrations
APPROVED

Ankita
4/15/2021 12:07:42 PM

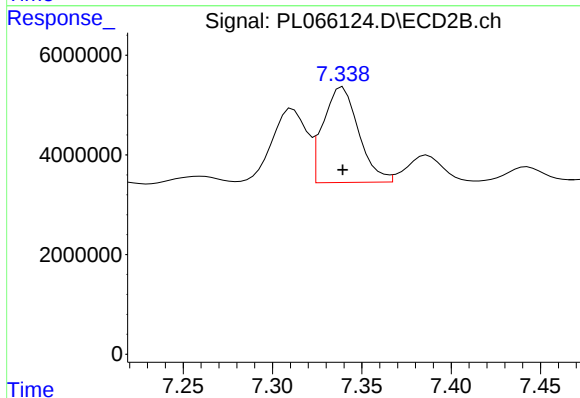


#17 4,4'-DDT

R.T.: 7.339 min
Delta R.T.: 0.000 min
Response: 26534497
Conc: 7.82 ng/ml

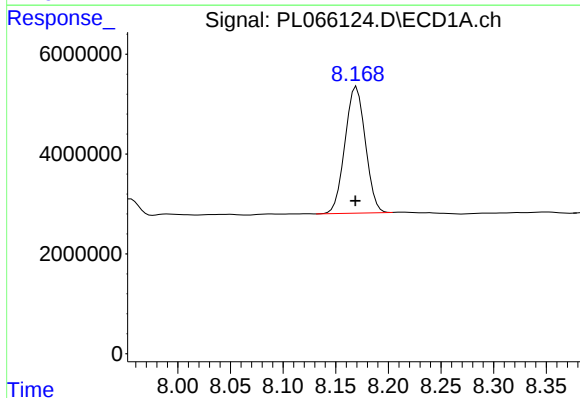

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: 0.001 min
Response: 34246460
Conc: 14.36 ng/ml

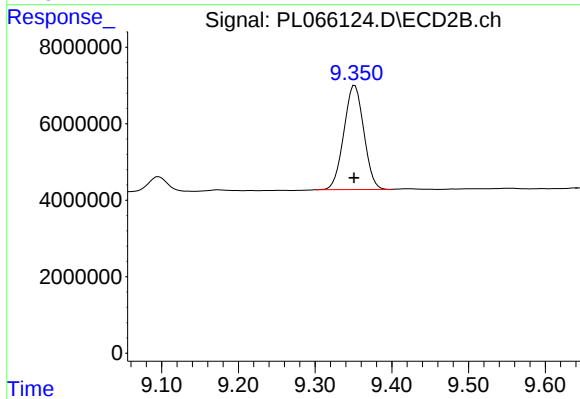

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.001 min
Response: 49578665
Conc: 15.18 ng/ml