

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
 Data File : PL066131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 17:16
 Operator : AR\AJ
 Sample : M2025-11
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 130-SB-1

Manual Integrations
 APPROVED

Ankita
 4/15/2021 12:07:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 01:15:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.154	54588991	82395778	21.447m	20.483
28)	SA Decachlor...	8.170	9.351	47170541	70703250	19.776	21.649
Target Compounds							
12)	B 4,4'-DDE	5.590	6.539	6987856	5228469	1.873	1.263 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041421\
Data File : PL066131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 17:16
Operator : AR\AJ
Sample : M2025-11
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
130-SB-1


Manual Integrations
APPROVED

Ankita
4/15/2021 12:07:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 01:15:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

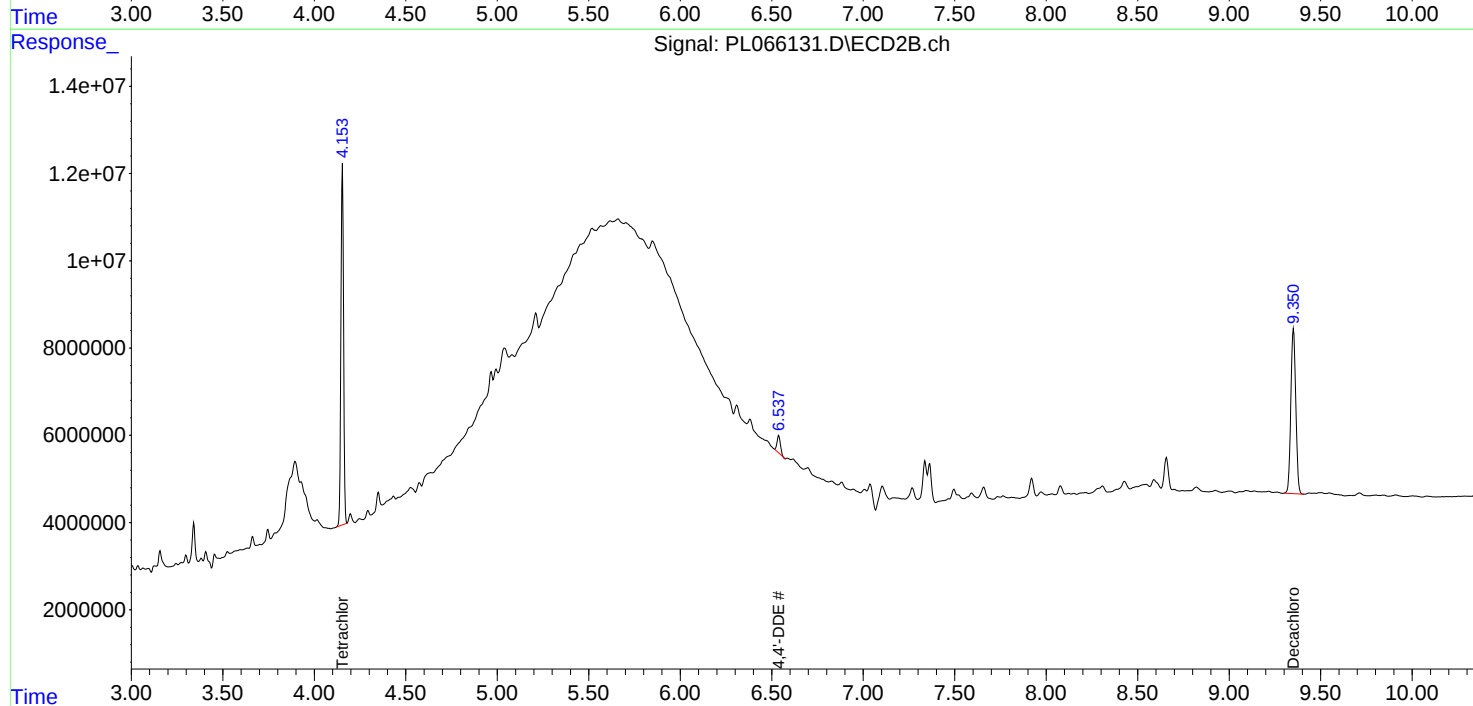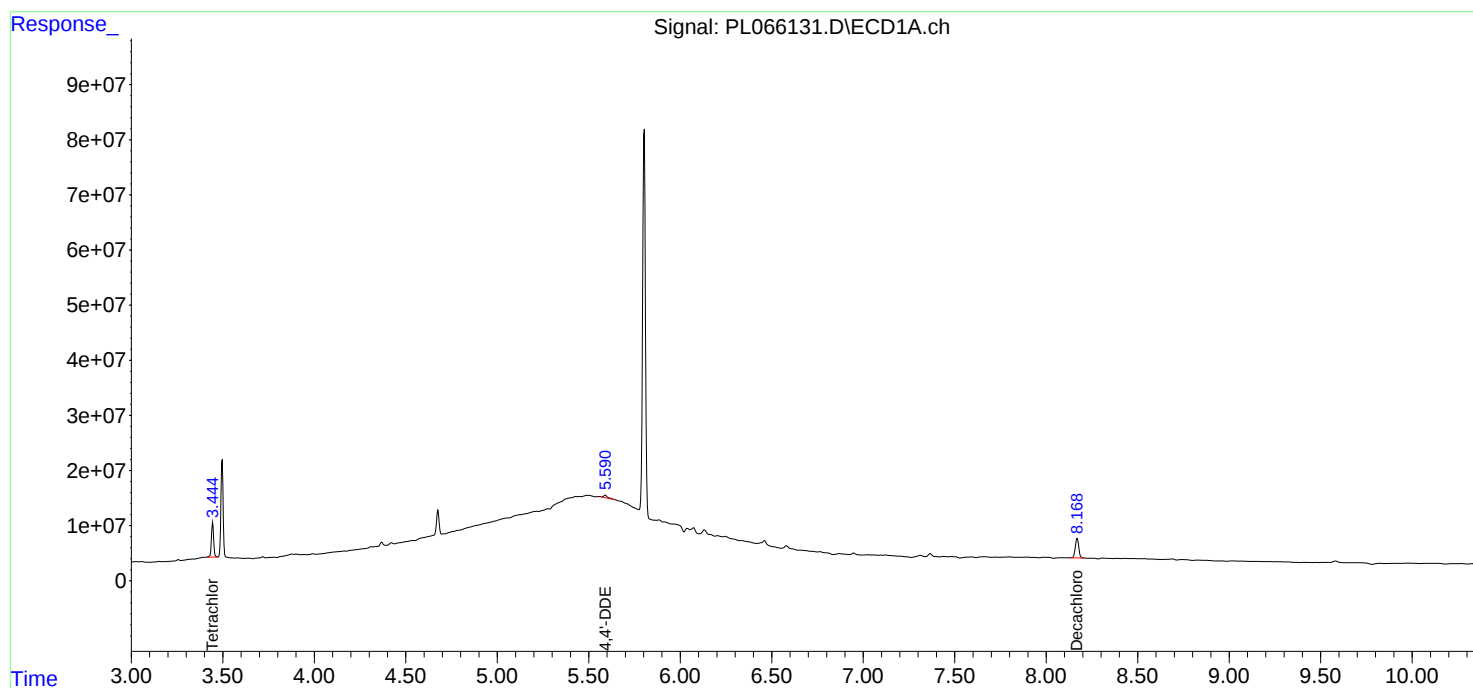

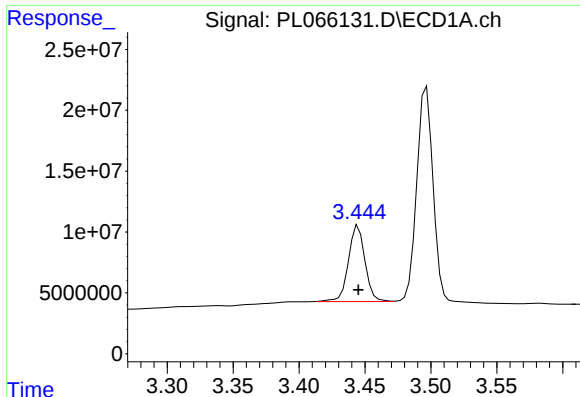


#1 Tetrachloro-m-xylene

R.T.: 3.444 min
Delta R.T.: -0.001 min
Response: 54588991
Conc: 21.45 ng/ml m

Instrument :
ECD_L
ClientSampleId :
130-SB-1


Manual Integrations
APPROVED

Ankita
4/15/2021 12:07:49 PM

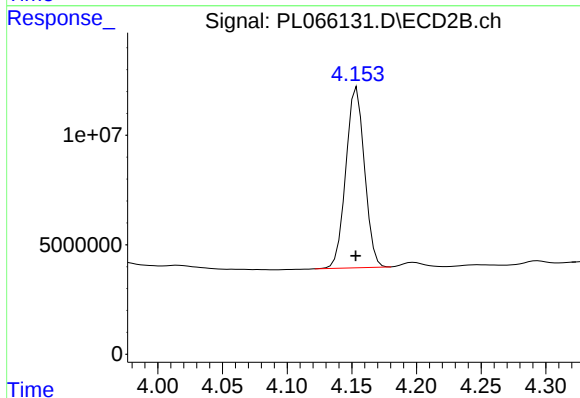


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 82395778
Conc: 20.48 ng/ml

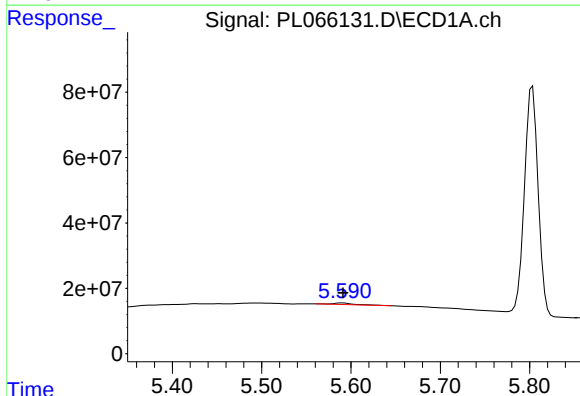


#12 4,4'-DDE

R.T.: 5.590 min
Delta R.T.: 0.000 min
Response: 6987856
Conc: 1.87 ng/ml

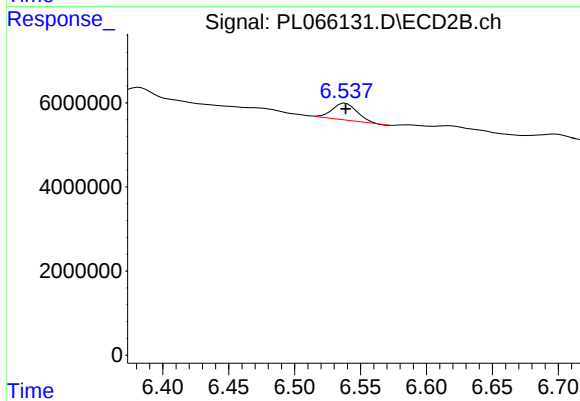

#12 4,4'-DDE

R.T.: 6.539 min
Delta R.T.: 0.000 min
Response: 5228469
Conc: 1.26 ng/ml

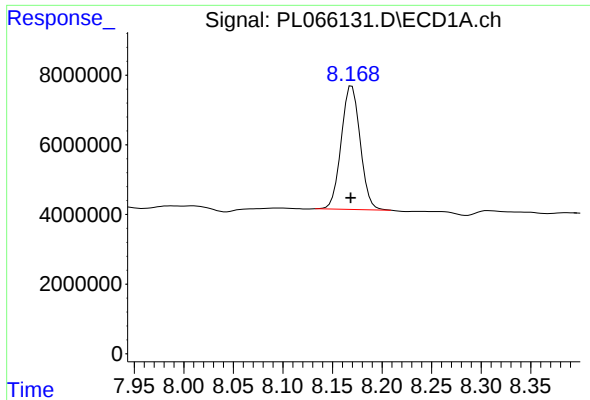


#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: 0.001 min
Response: 47170541
Conc: 19.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
130-SB-1

Manual Integrations
APPROVED

Ankita
4/15/2021 12:07:49 PM

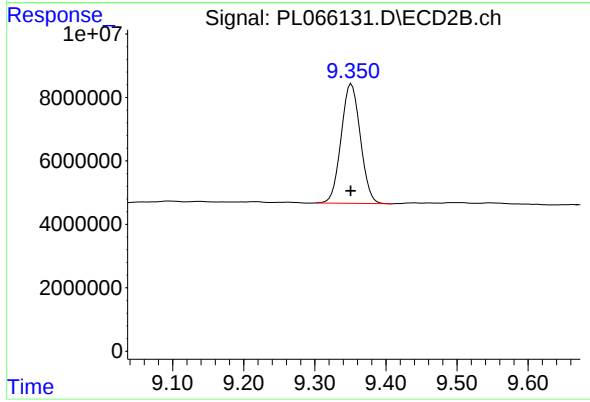

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 70703250
Conc: 21.65 ng/ml