

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041422\
 Data File : PL074051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2022 12:38
 Operator : AR\AJ
 Sample : N2367-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-05-041122

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/15/2022
 Supervised By : mohammad ahmed 04/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 14:56:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.637	5.491	4564366	22028968	14.126m	12.355
2) SA Decachlor...	10.412	11.336	7266749	25788502	13.974	14.600

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041422\
Data File : PL074051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2022 12:38
Operator : AR\AJ
Sample : N2367-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
AU-05-041122


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/15/2022
Supervised By : mohammad ahmed 04/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 14:56:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

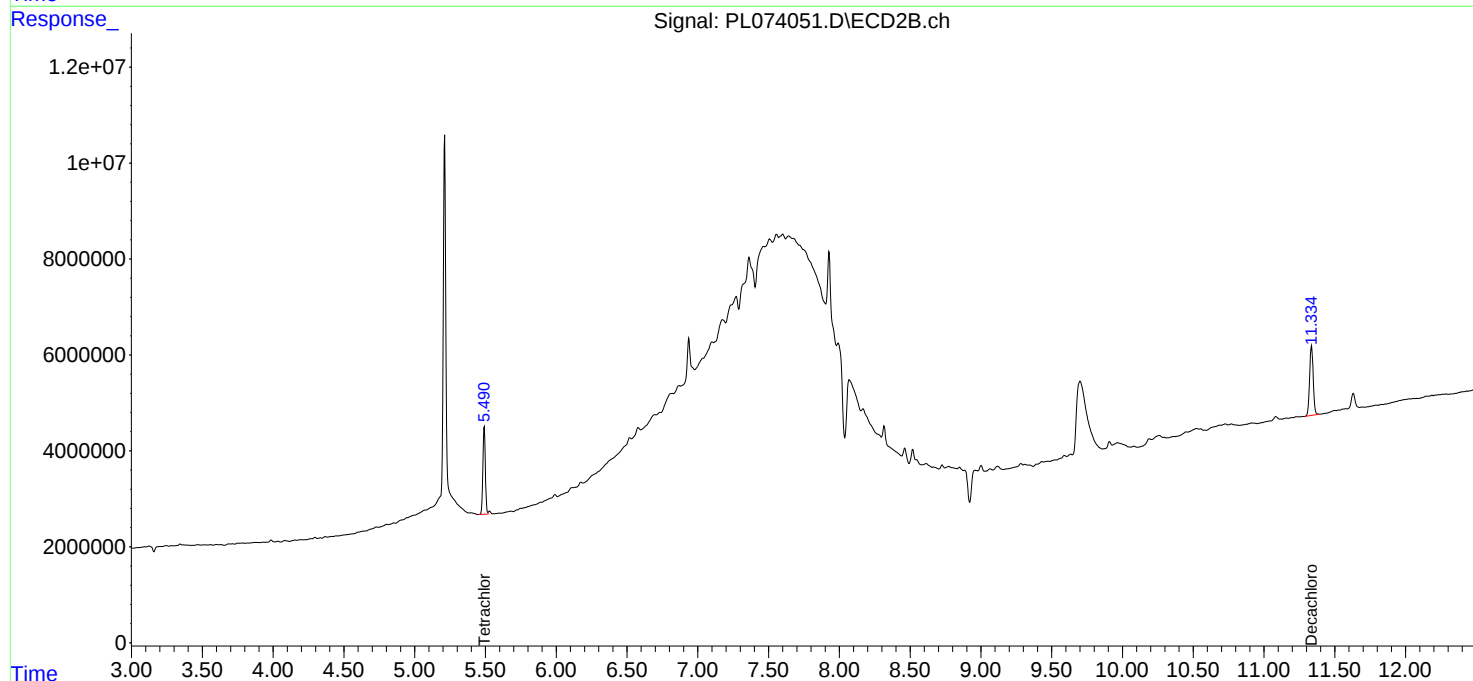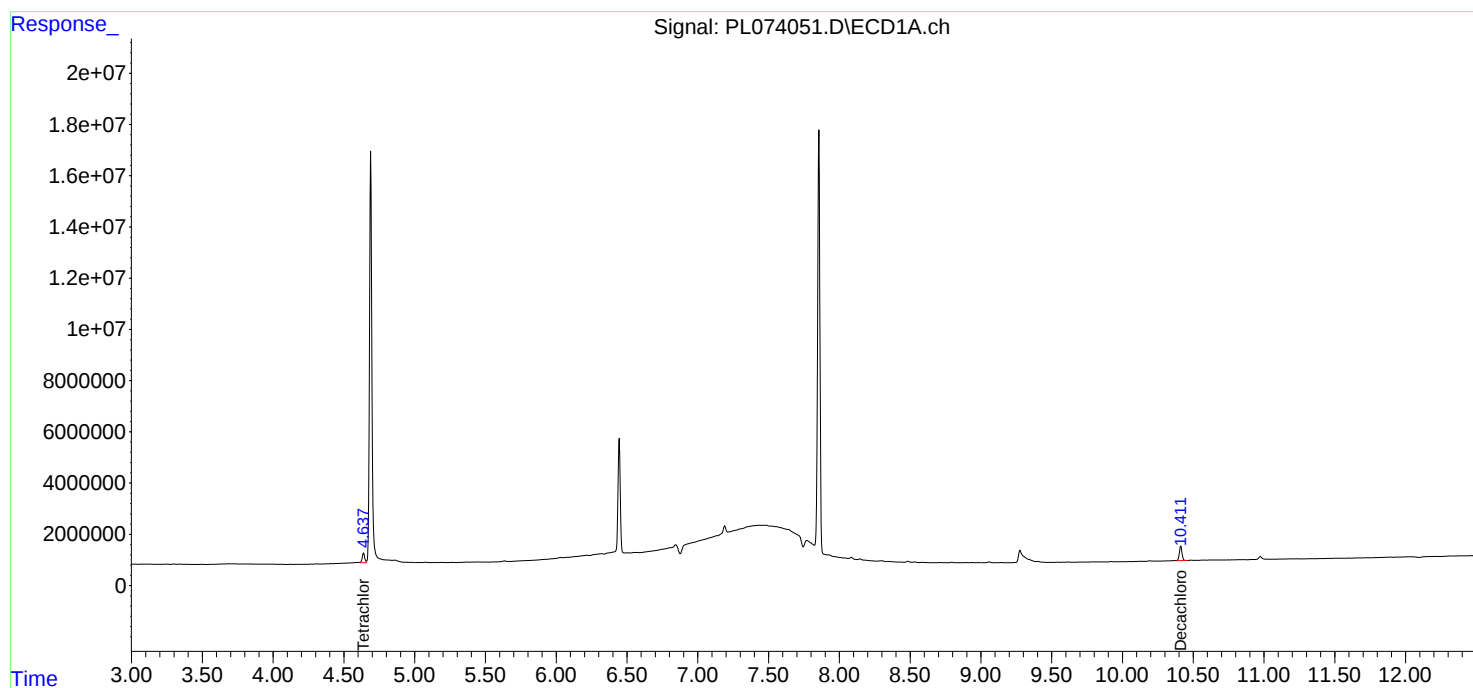

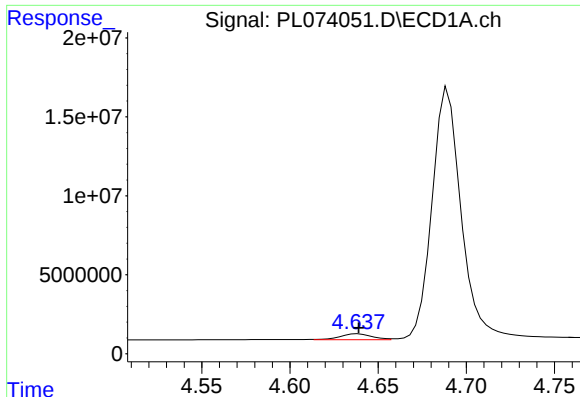


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: -0.002 min
Response: 4564366
Conc: 14.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-041122


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/15/2022
Supervised By :mohammad ahmed 04/18/2022

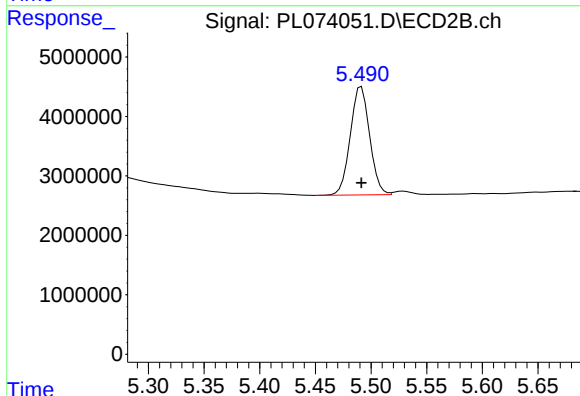


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 22028968
Conc: 12.36 ng/ml

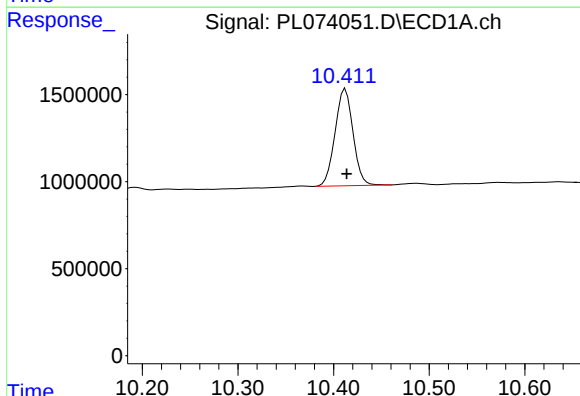

#28 Decachlorobiphenyl

R.T.: 10.412 min
Delta R.T.: -0.002 min
Response: 7266749
Conc: 13.97 ng/ml

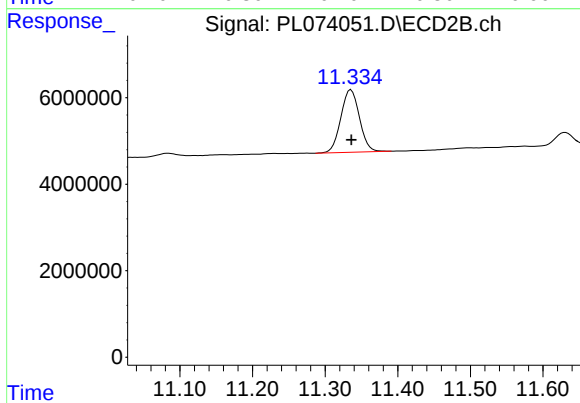

#28 Decachlorobiphenyl

R.T.: 11.336 min
Delta R.T.: 0.000 min
Response: 25788502
Conc: 14.60 ng/ml